

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102022\
 Data File : BG055221.D
 Acq On : 20 Oct 2022 15:47
 Operator : CG/JU
 Sample : N5186-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TEXAS-SP-1019

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	3	6	19	rVB	1646196	2576012	71.44%	12.204%
2	3.623	53	57	64	rBV	127534	158734	4.40%	0.752%
3	3.758	74	80	91	rVB	226175	294307	8.16%	1.394%
4	4.633	224	229	235	rBV	30628	43771	1.21%	0.207%
5	4.821	256	261	267	rVB	43510	60902	1.69%	0.289%
6	4.886	267	272	278	rBV	32121	45218	1.25%	0.214%
7	5.291	333	341	343	rBV	65028	104442	2.90%	0.495%
8	5.326	343	347	355	rVB	366464	542256	15.04%	2.569%
9	5.802	421	428	442	rBV	1179403	1897489	52.62%	8.989%
10	7.424	695	704	718	rBV	1057453	1853770	51.41%	8.782%
11	8.282	843	850	857	rBV	197109	328485	9.11%	1.556%
12	9.457	1042	1050	1063	rVB	759516	1370639	38.01%	6.493%
13	11.114	1324	1332	1340	rBV	283479	503357	13.96%	2.385%
14	13.523	1735	1742	1750	rBV	1750738	2825969	78.37%	13.388%
15	14.898	1969	1976	1985	rVB	431601	660374	18.31%	3.128%
16	16.378	2220	2228	2243	rBV	1305948	2042376	56.64%	9.676%
17	17.630	2435	2441	2453	rVB	498625	739668	20.51%	3.504%
18	20.209	2873	2880	2886	rBV	2695574	3605905	100.00%	17.083%
19	21.913	3163	3170	3178	rBV	421281	712530	19.76%	3.376%
20	25.326	3741	3751	3762	rVB2	251574	742496	20.59%	3.517%




Sum of corrected areas: 21108700

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102022\
Data File : BG055221.D
Acq On : 20 Oct 2022 15:47
Operator : CG/JU
Sample : N5186-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEXAS-SP-1019

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

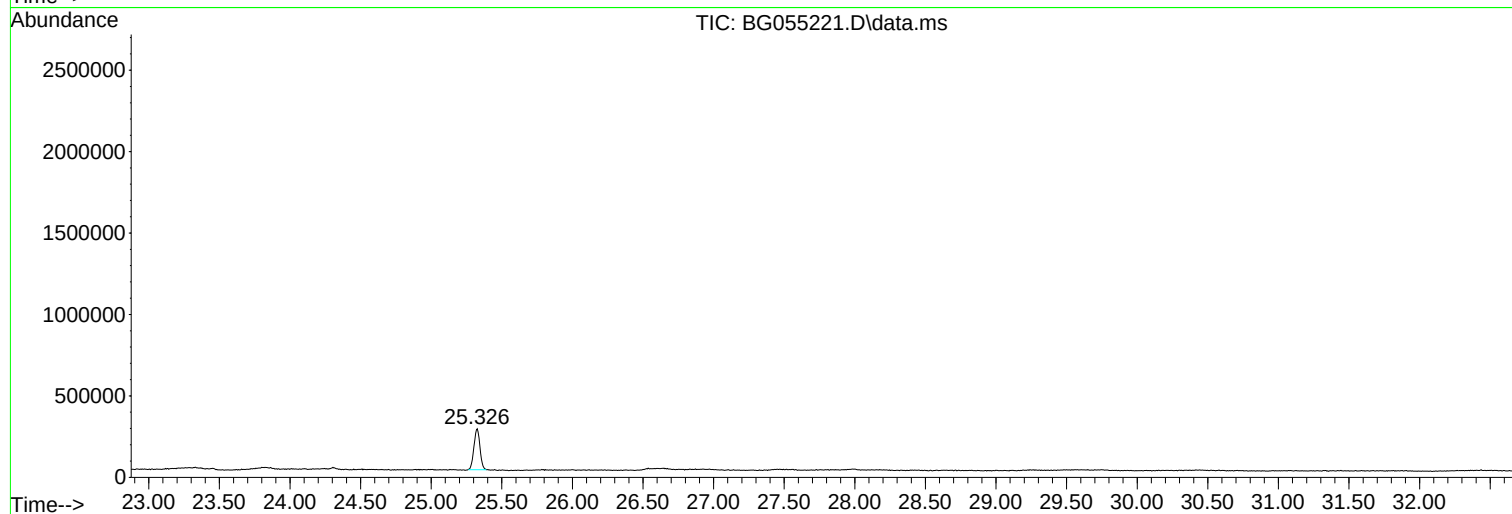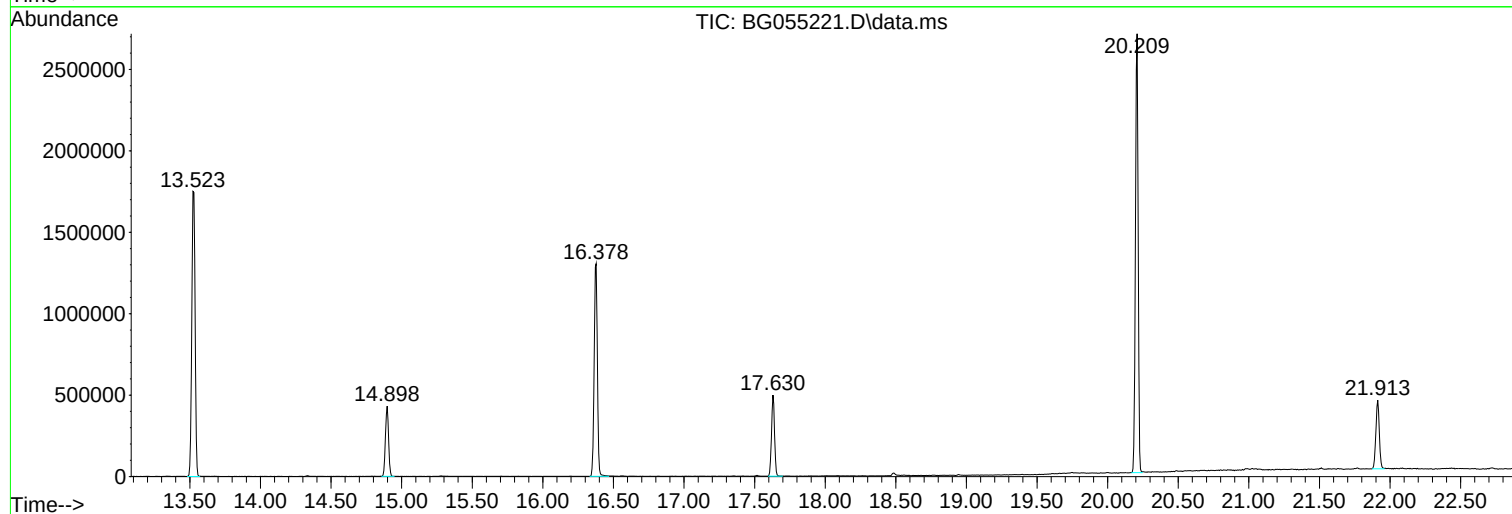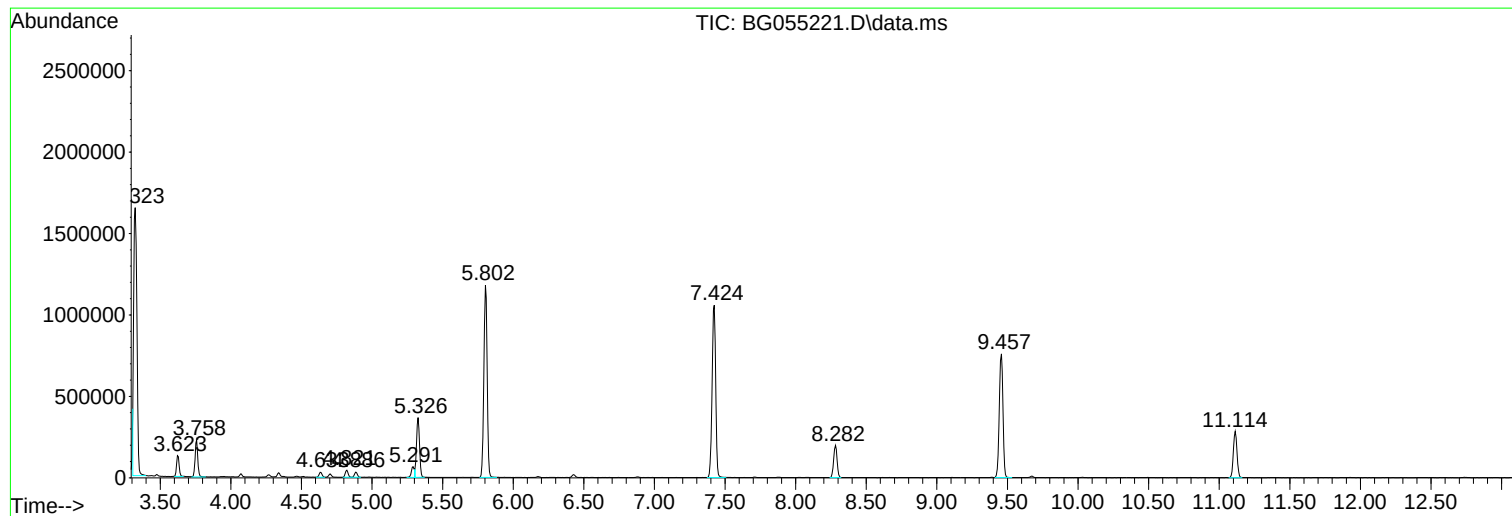

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102022\
Data File : BG055221.D
Acq On : 20 Oct 2022 15:47
Operator : CG/JU
Sample : N5186-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEXAS-SP-1019

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102022\
Data File : BG055221.D
Acq On : 20 Oct 2022 15:47
Operator : CG/JU
Sample : N5186-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEXAS-SP-1019

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------