
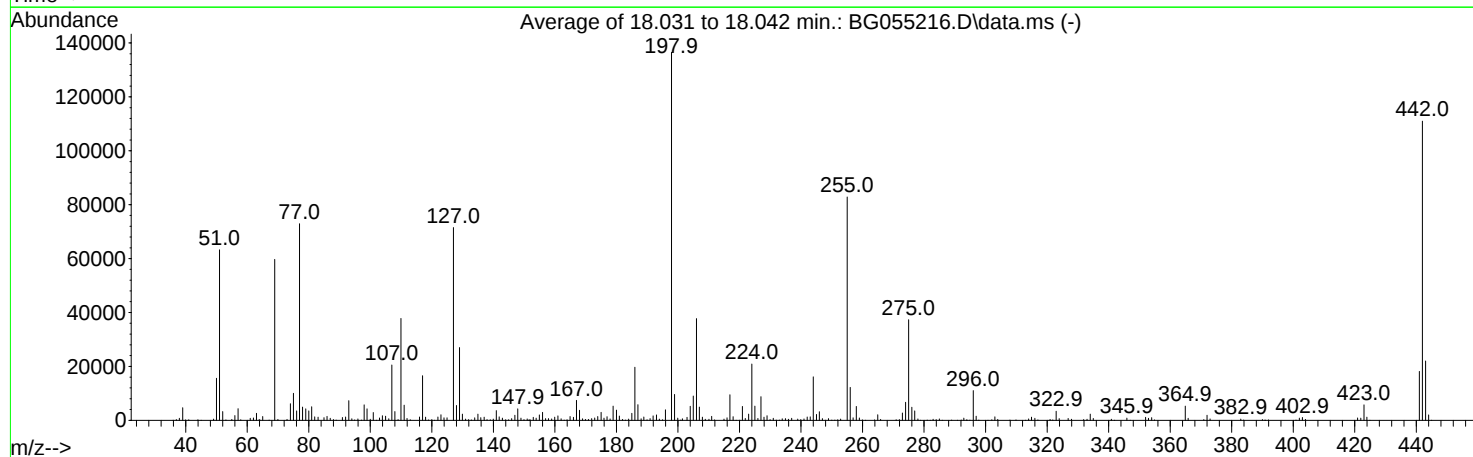


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102022\
 Data File : BG055216.D
 Acq On : 20 Oct 2022 10:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 20 09:21:42 2022

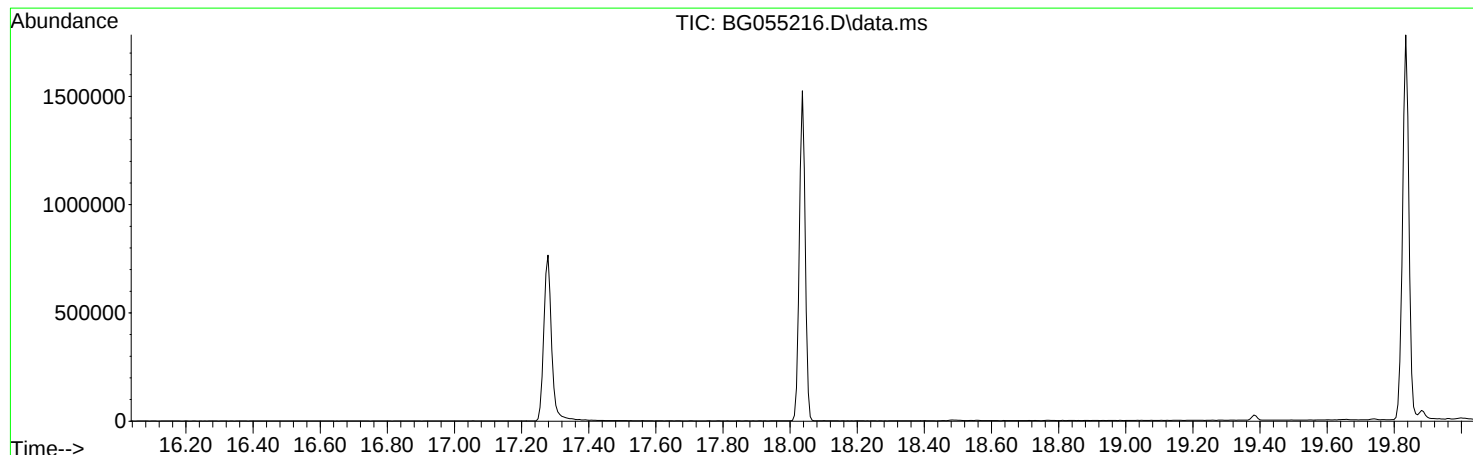




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	63261	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.8	59723	PASS
70	69	0.00	2	0.6	330	PASS
127	198	10	80	52.4	71499	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136499	PASS
199	198	5	9	7.0	9602	PASS
275	198	10	60	27.3	37307	PASS
365	198	1	100	3.8	5245	PASS
441	198	0.01	100	13.3	18112	PASS
442	442	50	100	100.0	110992	PASS
443	442	15	24	19.8	22002	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102022\
 Data File : BG055216.D
 Acq On : 20 Oct 2022 10:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 20 11:04:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 20 09:21:42 2022
 Response via : Initial Calibration

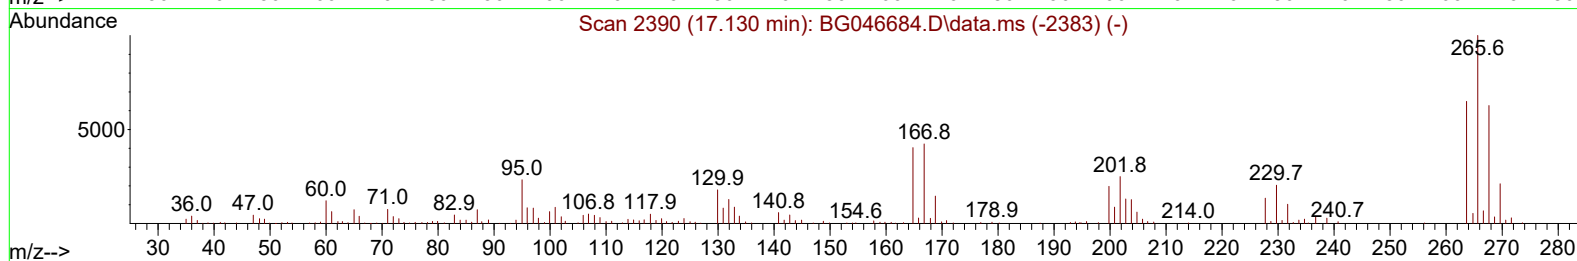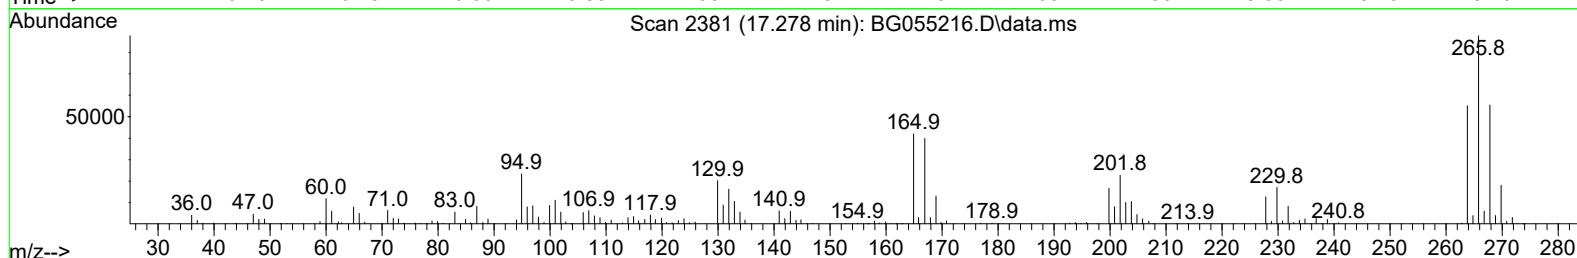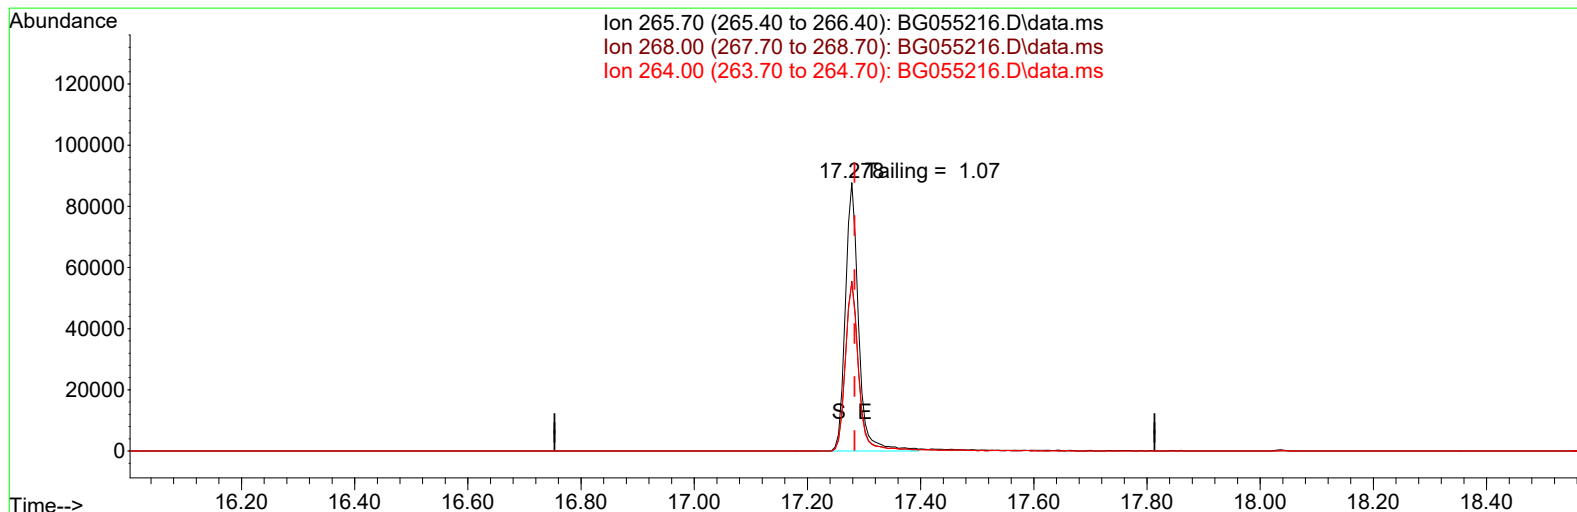

TIC: BG055216.D\data.ms

(70) Pentachlorophenol (C)

17.278min (-0.005) 32922.02 ng




response 142910

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.70	63.19
264.00	63.90	62.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102022\
 Data File : BG055216.D
 Acq On : 20 Oct 2022 10:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 20 11:04:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 20 09:21:42 2022
 Response via : Initial Calibration

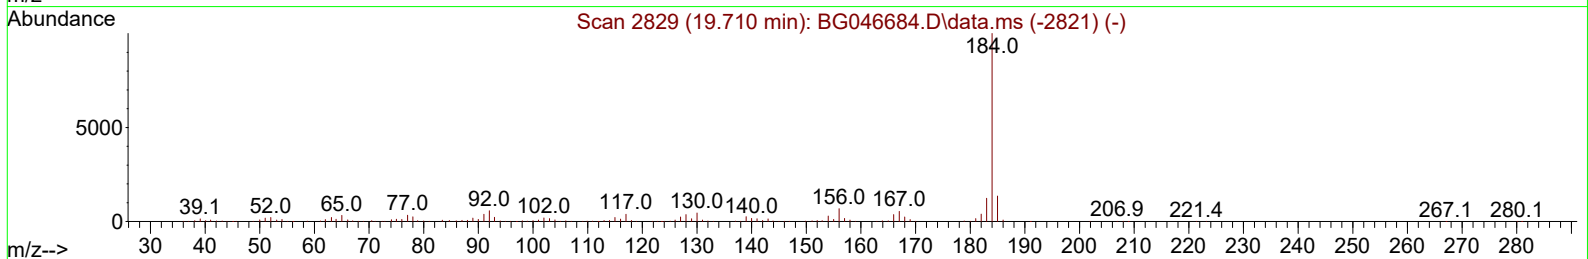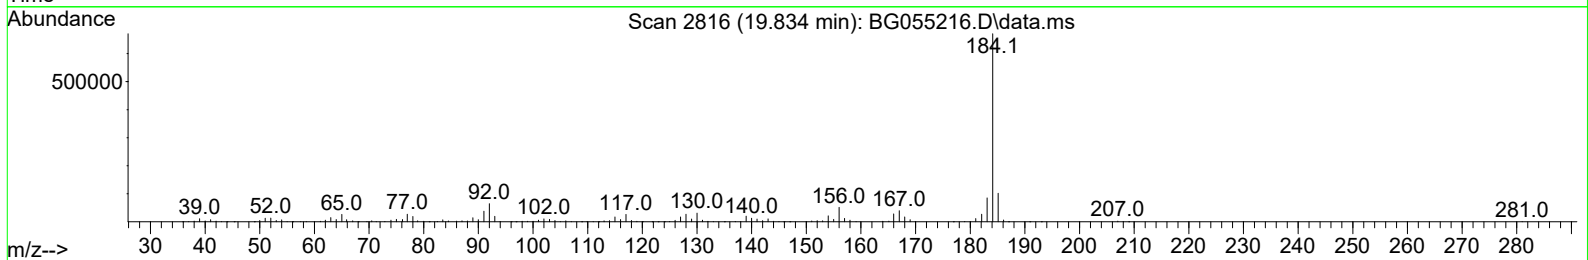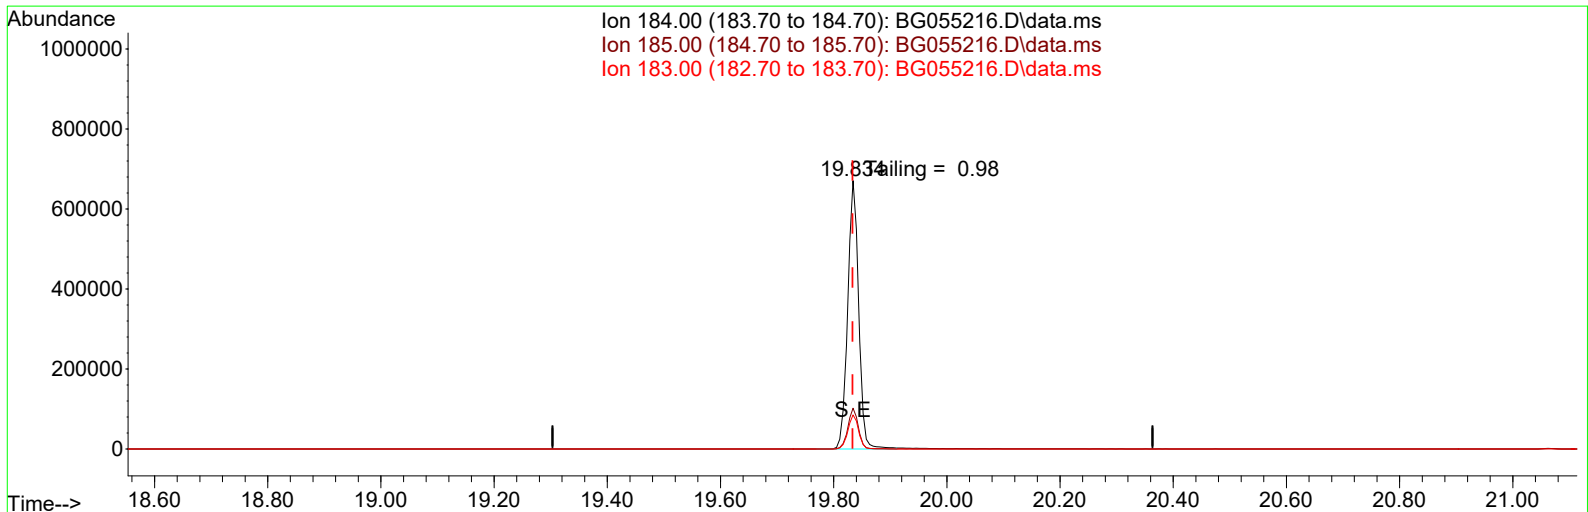

TIC: BG055216.D\data.ms

(77) Benzidine

19.834min (+ 0.001) 0.00 ng

response 910202

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.21
183.00	12.20	12.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2022	BNA_G	<u>BG055216.D</u>
Compound Name	Response	Retention Time
DDT	425193	21.068
DDD	8595	20.61
DDE	354	20.116
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8949	434142	2.06

Instrument :
BNA_G
ClientSampleId :
DFTPP