
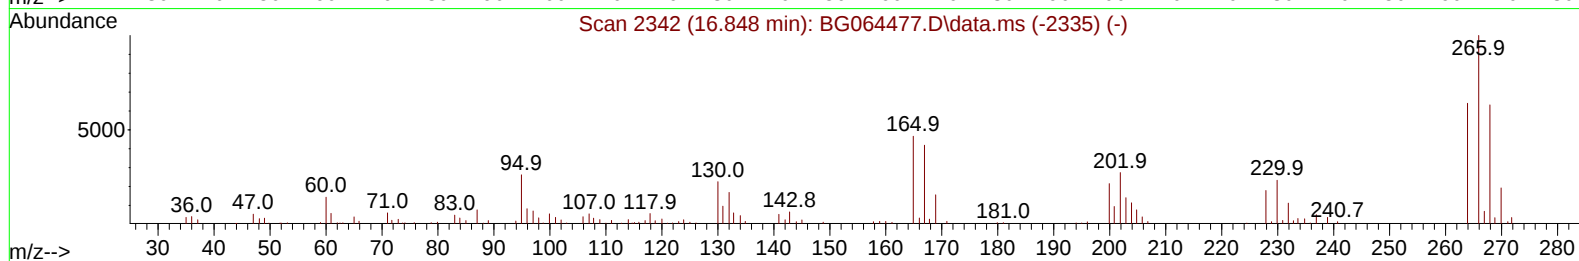
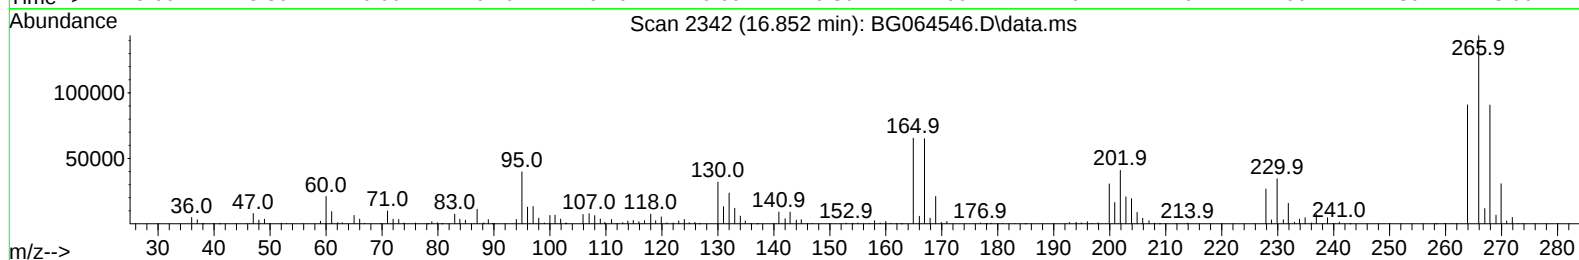


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102025\
Data File : BG064546.D
Acq On : 20 Oct 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 15:49:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

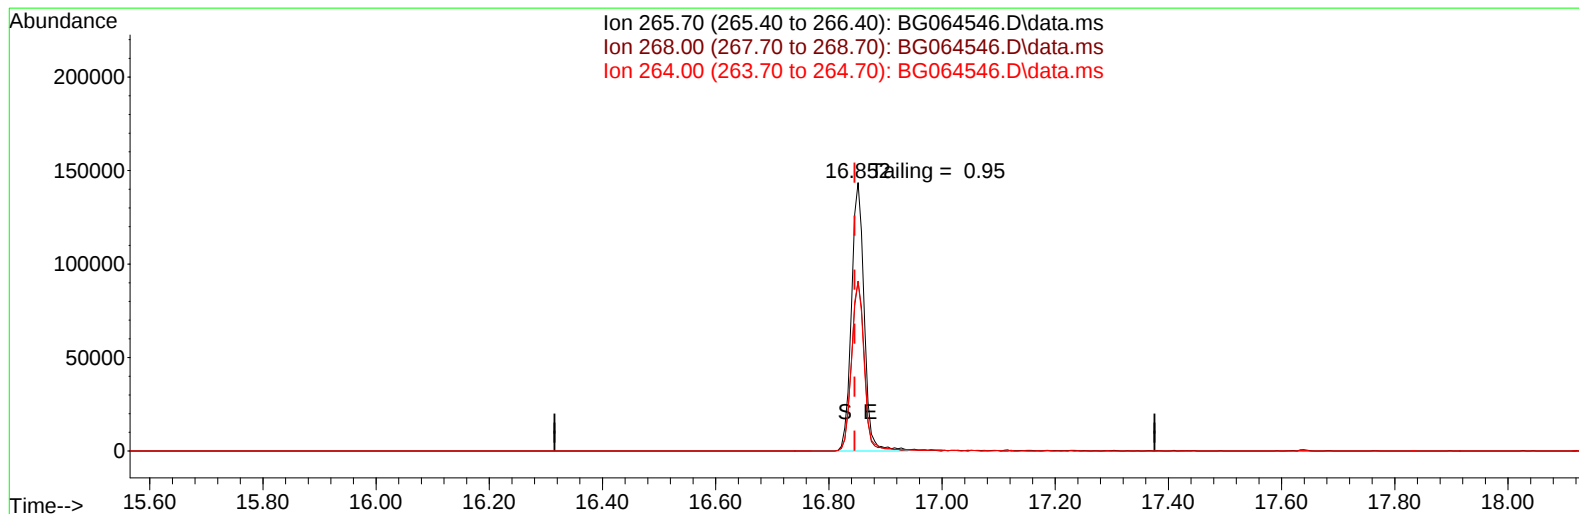

TIC: BG064546.D\data.ms

(70) Pentachlorophenol (C)




16.852min (+ 0.006) 508135.96 ng

response 224037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.21
264.00	64.00	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102025\
Data File : BG064546.D
Acq On : 20 Oct 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 15:49:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

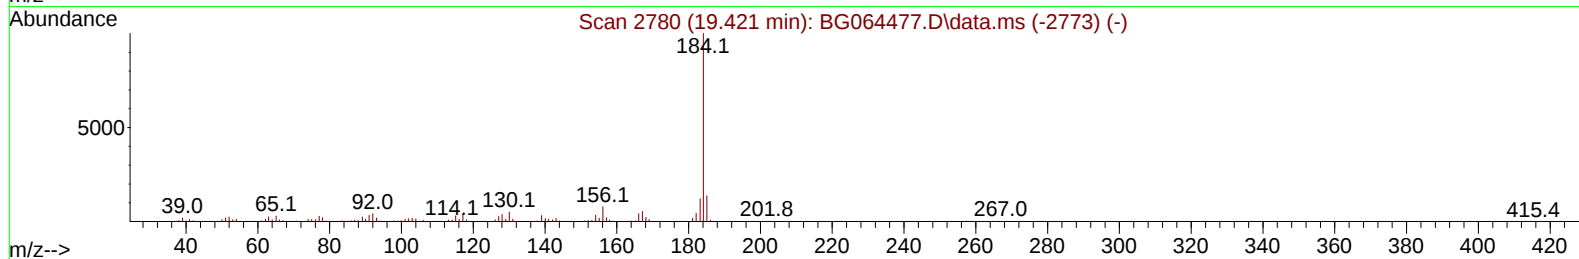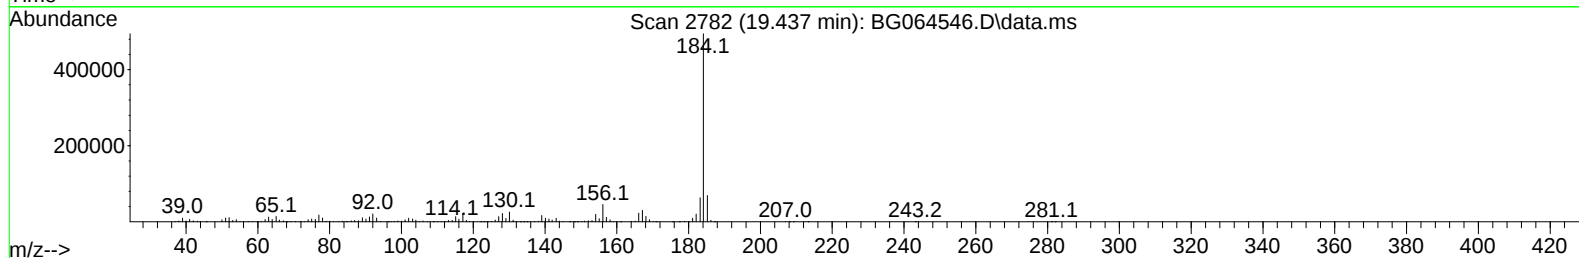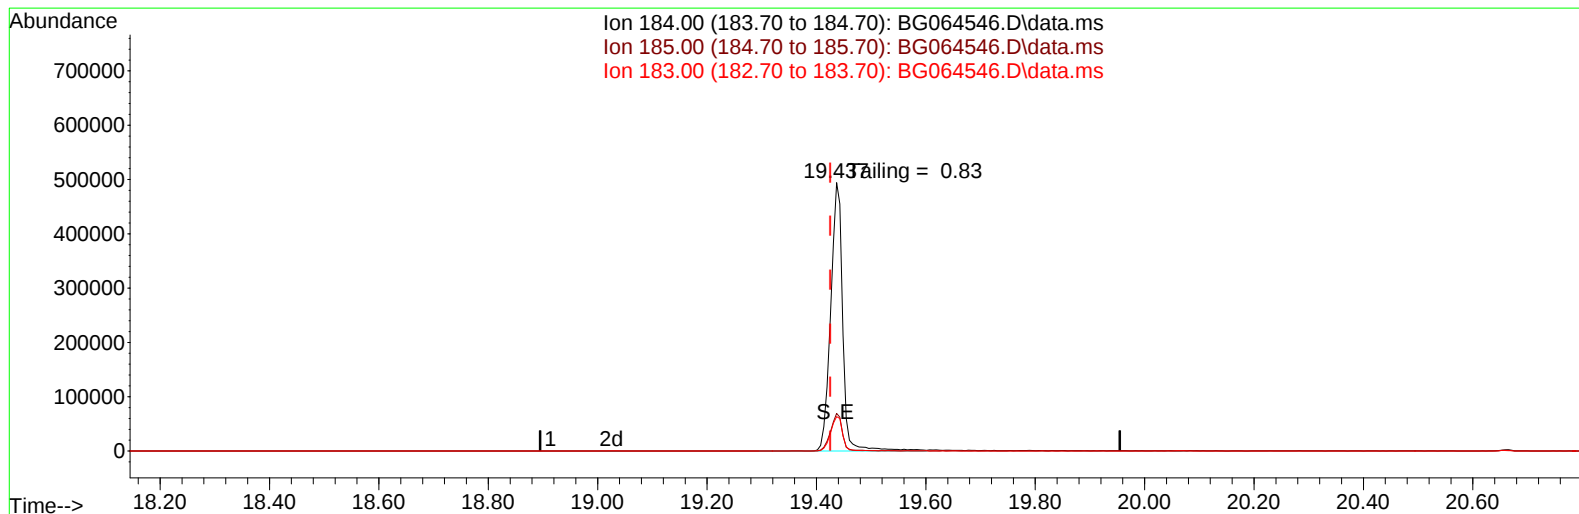

TIC: BG064546.D\data.ms

(77) Benzidine

19.437min (+ 0.012) 4548.02 ng m

response 771146

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.01
183.00	12.20	12.84
0.00	0.00	0.00