


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102025\
Data File : BG064546.D
Acq On : 20 Oct 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 02 16:40:42 2025

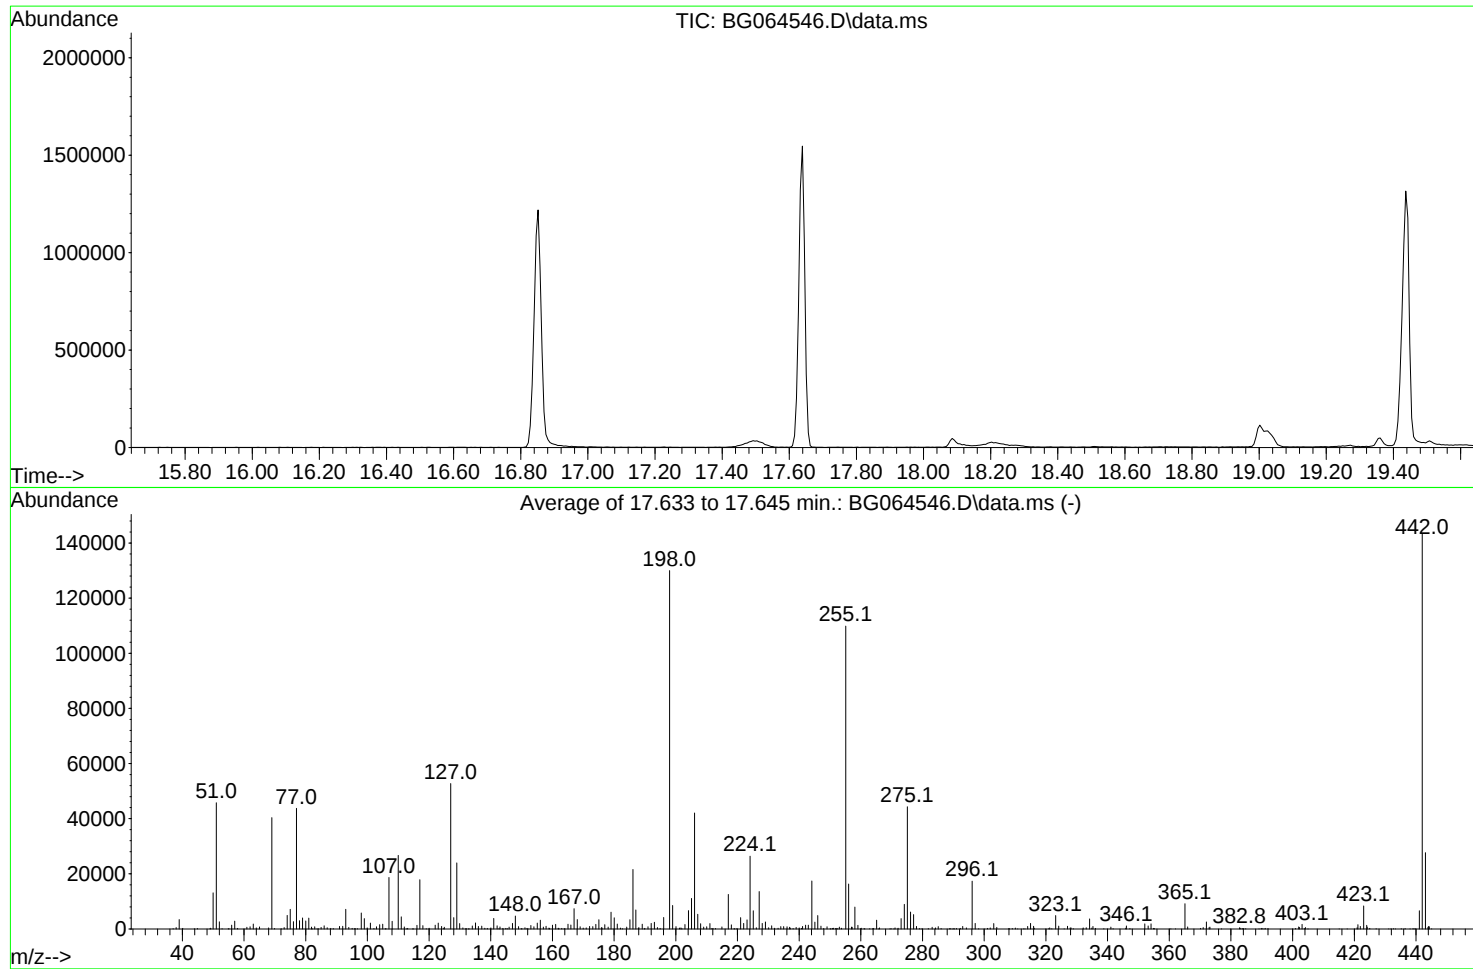




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	373	PASS
69	69	100	100	100.0	40344	PASS
70	69	0.00	2	0.3	129	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	129981	PASS
199	198	5	9	6.5	8483	PASS
365	198	1	100	7.0	9125	PASS
441	443	0.01	150	23.8	6576	PASS
442	442	100	100	100.0	143235	PASS
443	442	15	24	19.3	27637	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102025\
Data File : BG064546.D
Acq On : 20 Oct 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 20 15:49:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

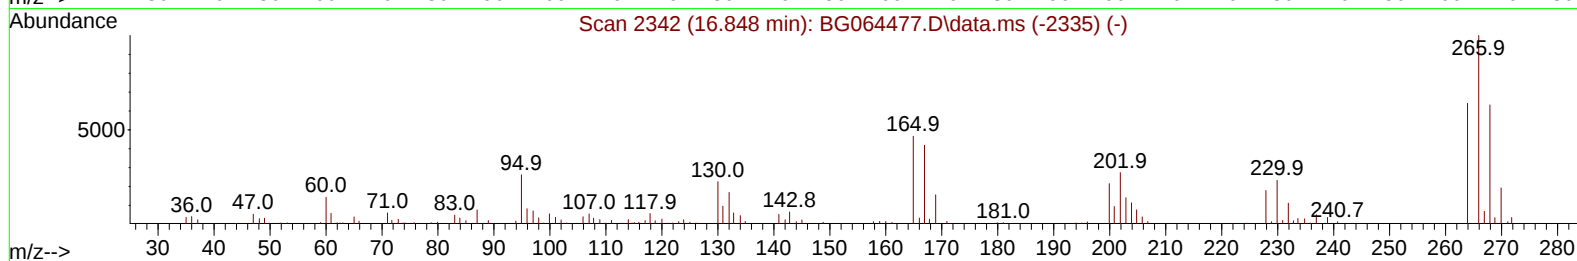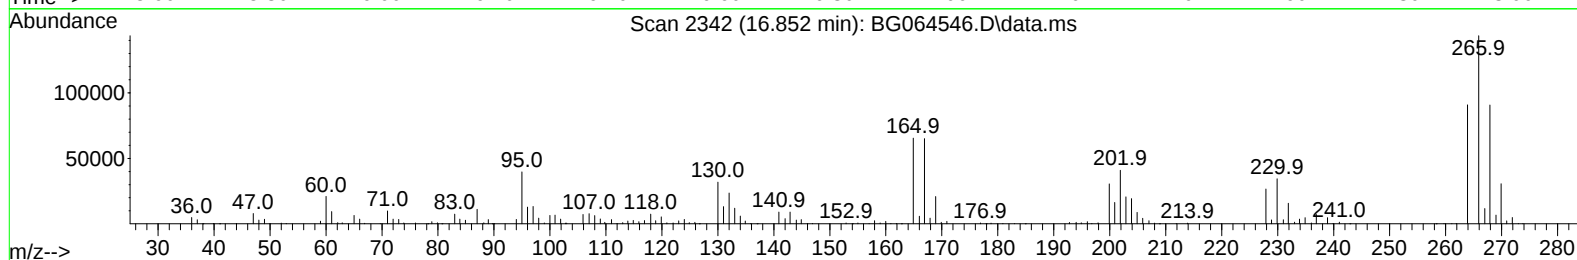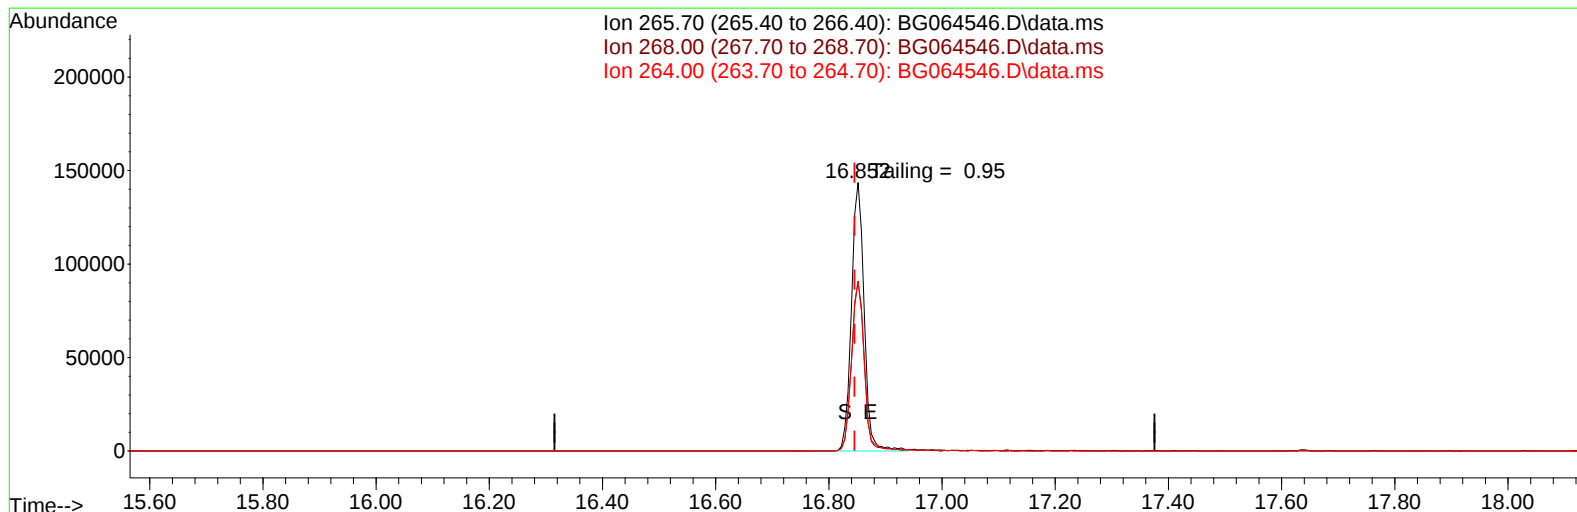

TIC: BG064546.D\data.ms

(70) Pentachlorophenol (C)

16.852min (+ 0.006) 508135.96 ng




response 224037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.21
264.00	64.00	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102025\
Data File : BG064546.D
Acq On : 20 Oct 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 20 15:49:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

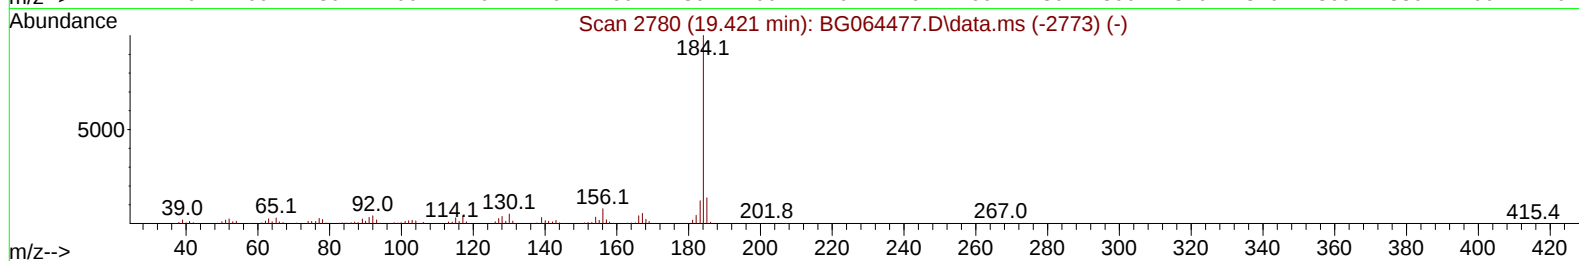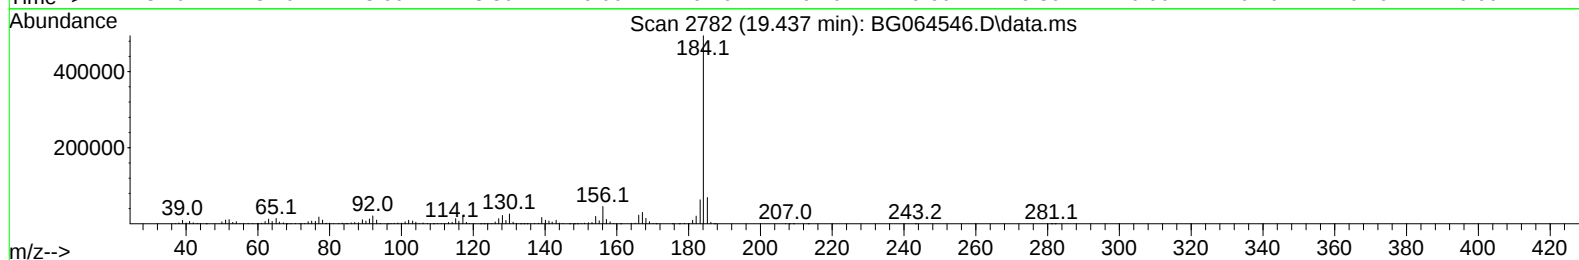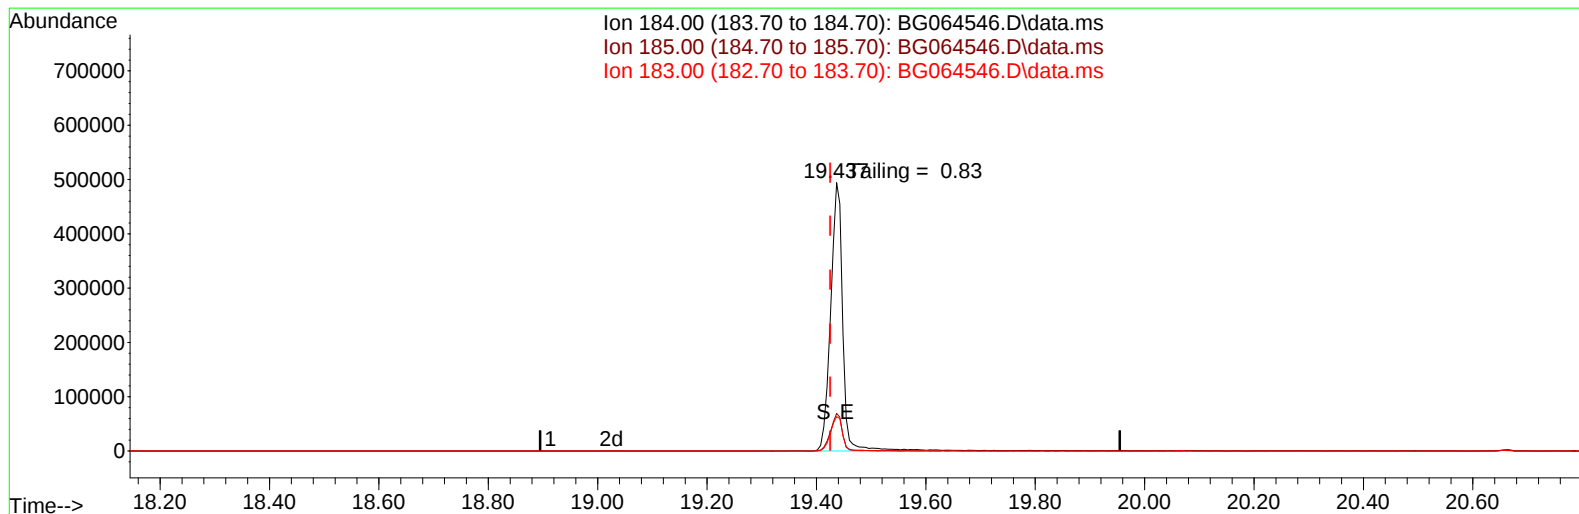

TIC: BG064546.D\data.ms

(77) Benzidine

19.437min (+ 0.012) 4548.02 ng m

response 771146

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.01
183.00	12.20	12.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2025	BNA_G	<u>BG064546.D</u>
Compound Name	Response	Retention Time
DDT	515751	20.665
DDD	4166	20.224
DDE	306	18.996
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4472	520223	0.86

Instrument :
BNA_G
ClientSampleId :
DFTPP