
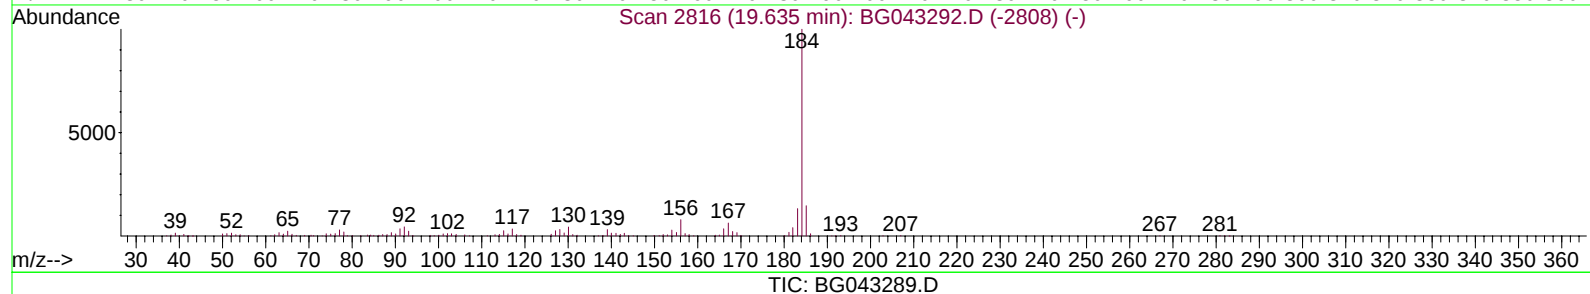
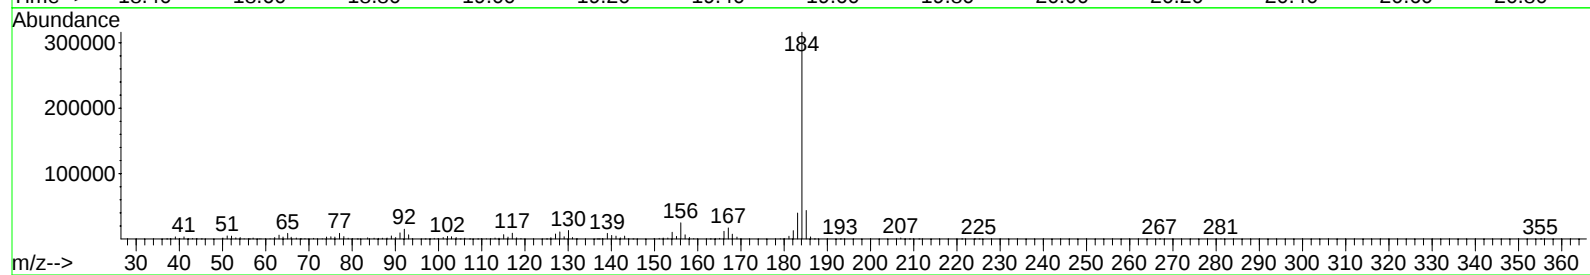


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102119\
Data File : BG043289.D
Acq On : 21 Oct 2019 9:05
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 18:24:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

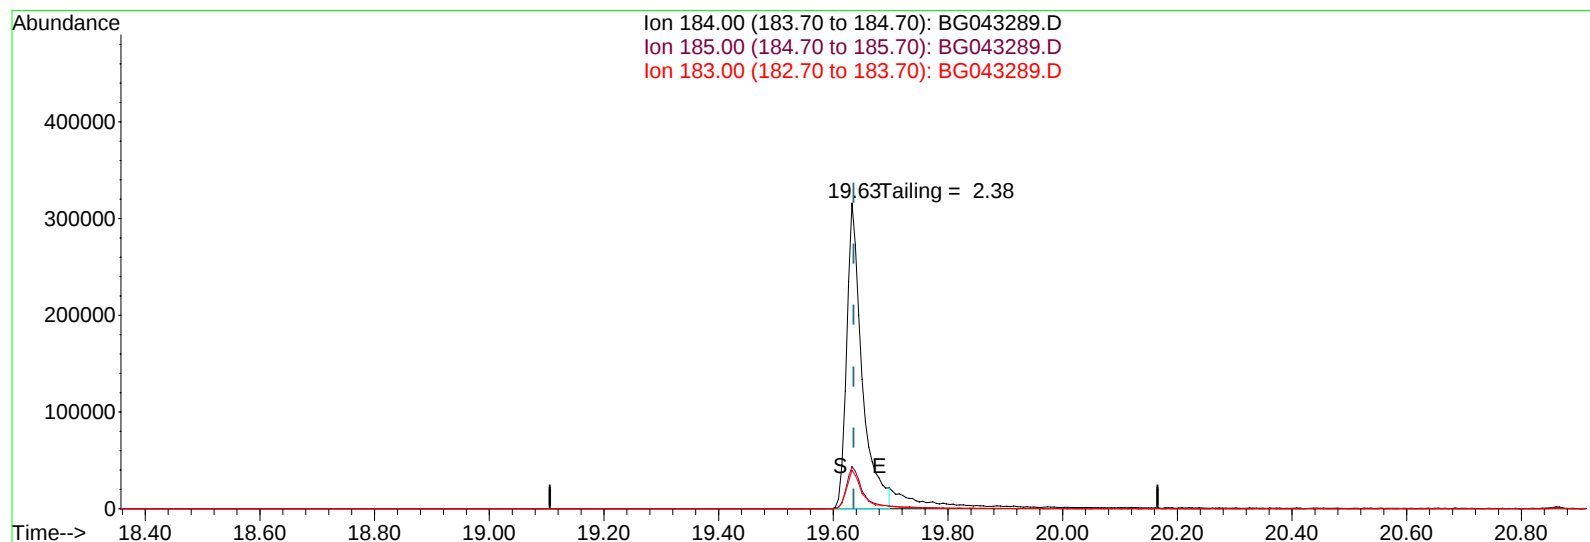

(77) Benzidine

19.632min (-0.003) 0.00ng

response 662573




Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.84
183.00	13.30	12.60
0.00	0.00	0.00

```

Data Path   : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102119\
Data File   : BG043289.D
Acq On      : 21 Oct 2019    9:05
Operator    : JU
Sample      : DFTPP
Misc        :
ALS Vial    : 1      Sample Multiplier: 1

```

Quant Time: Oct 21 18:24:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

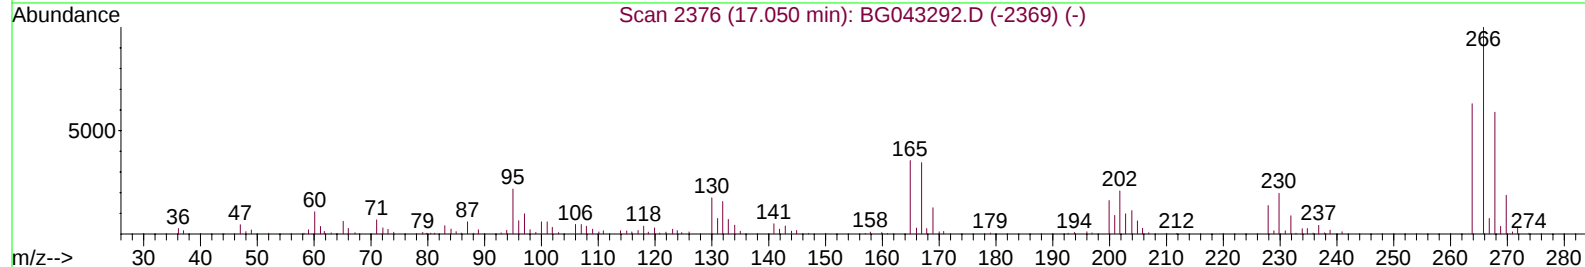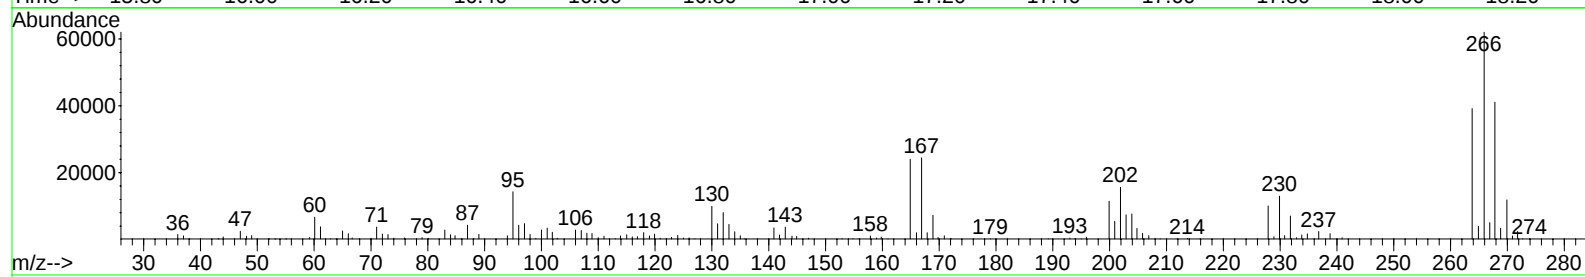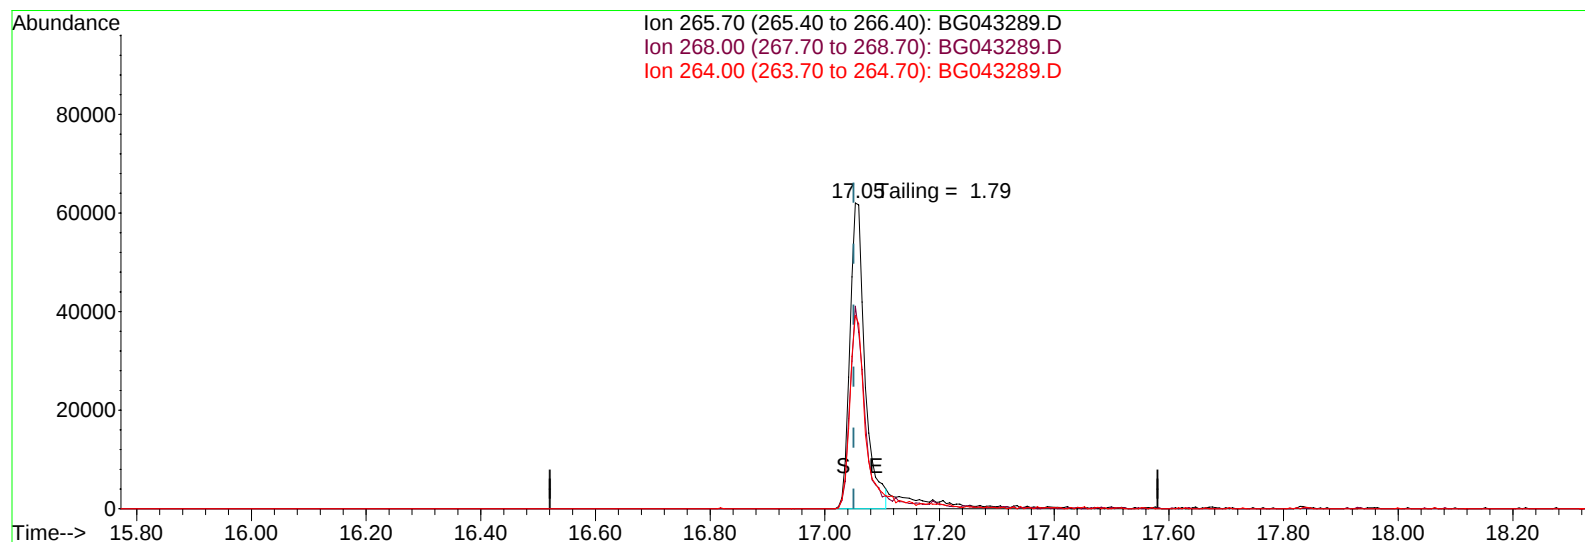

TIC: BG043289.D

(70) Pentachlorophenol (C)

17.053min (+0.003) 24175.16ng

```
response 123032
```

Ion	Exp%	Act%
265.70	100	100
268.00	58.90	66.24
264.00	63.00	63.15
0.00	0.00	0.00