


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102119\
 Data File : BG043289.D
 Acq On : 21 Oct 2019 9:05
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 21 16:37:43 2019

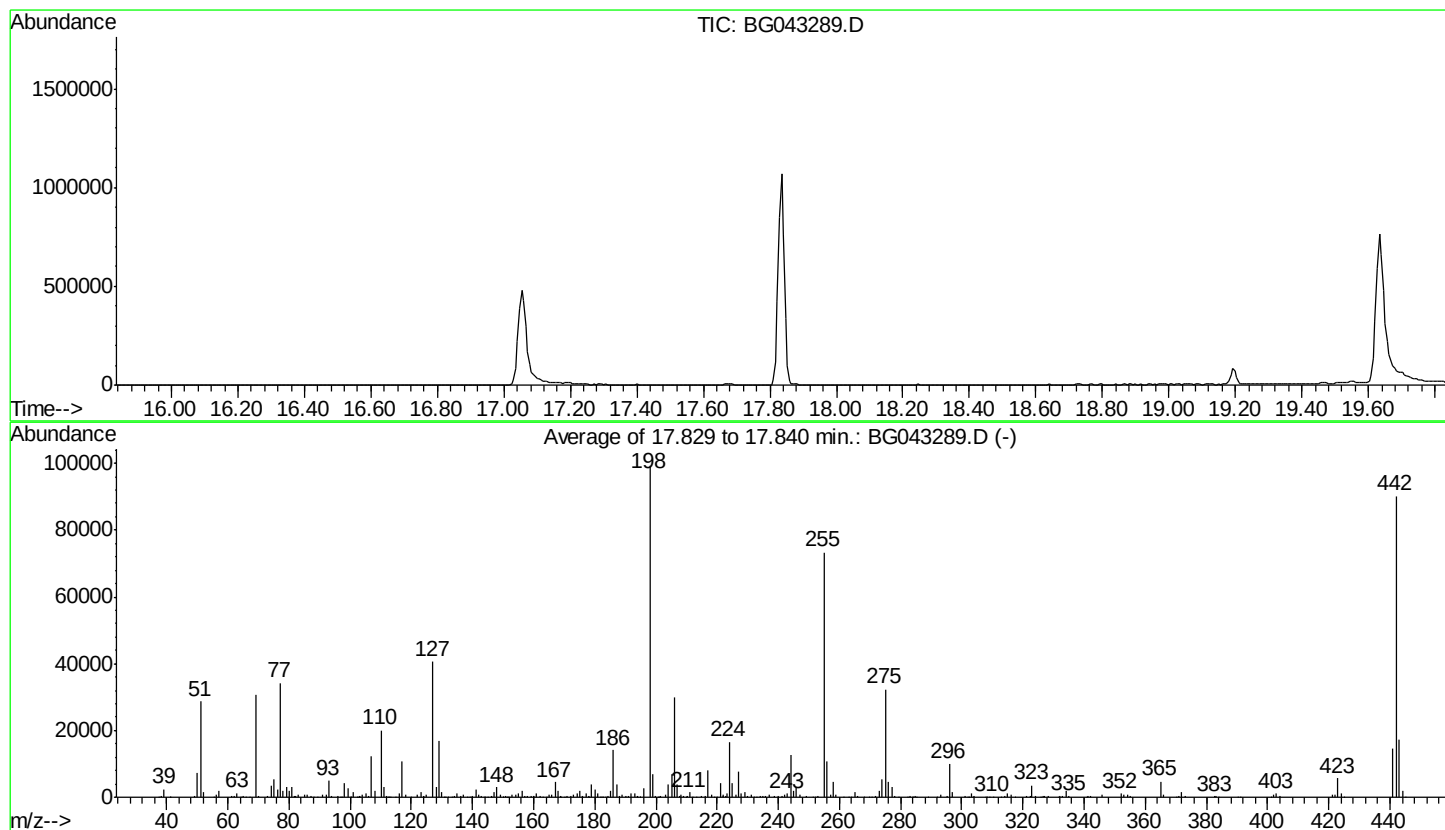

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	28634	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.7	30528	PASS
70	69	0.00	2	0.7	207	PASS
127	198	10	80	40.9	40600	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99312	PASS
199	198	5	9	6.8	6724	PASS
275	198	10	60	32.5	32272	PASS
365	198	1	100	4.7	4637	PASS
441	198	0.01	100	14.8	14740	PASS
442	198	50	100	90.8	90194	PASS
443	442	15	24	19.0	17121	PASS