
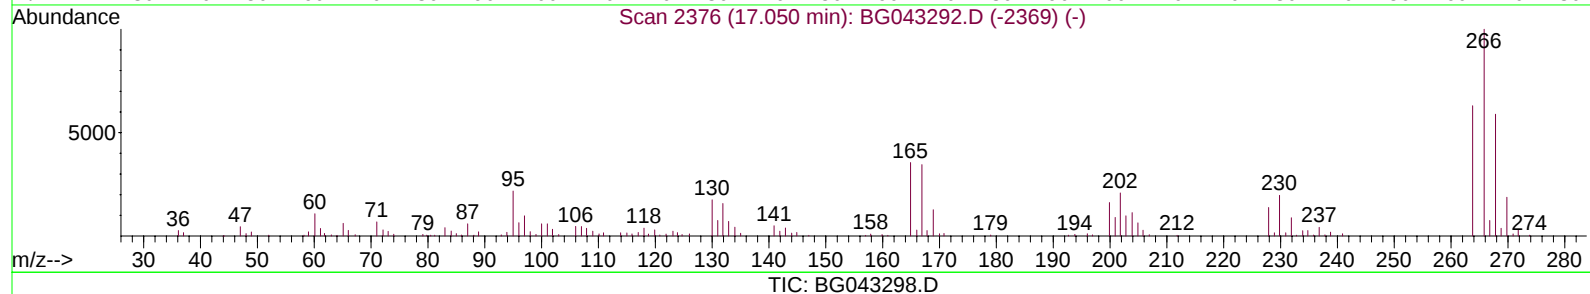
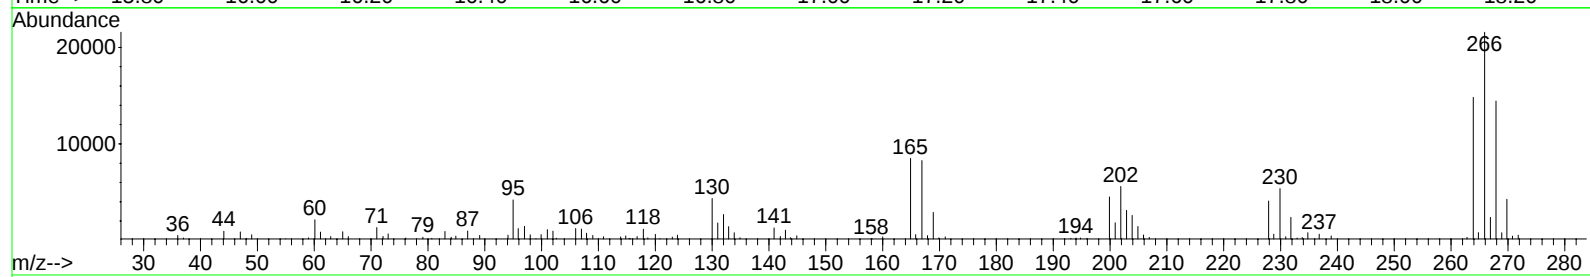


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102219\
Data File : BG043298.D
Acq On : 22 Oct 2019 9:14
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 18:50:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

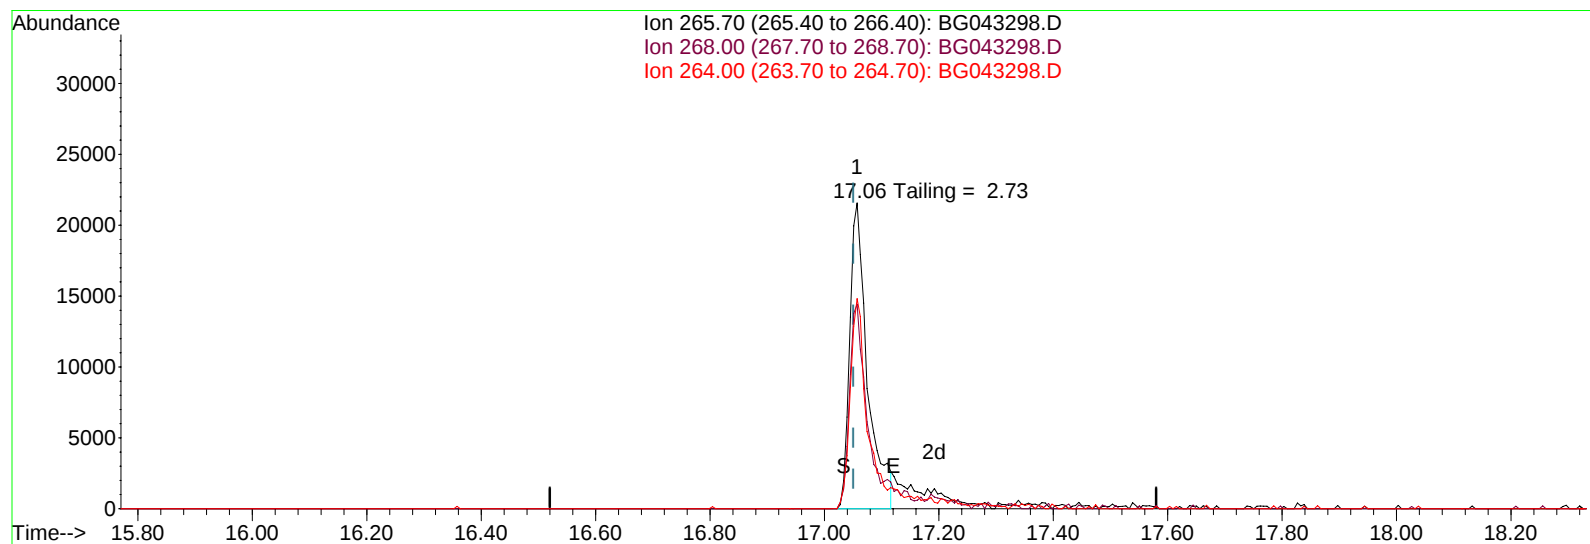

(70) Pentachlorophenol (C)




17.057min (+0.007) 24608.06ng

response 52138

Ion	Exp%	Act%
265.70	100	100
268.00	58.90	66.95
264.00	63.00	68.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102219\
 Data File : BG043298.D
 Acq On : 22 Oct 2019 9:14
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 18:50:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 21 16:37:43 2019
 Response via : Initial Calibration

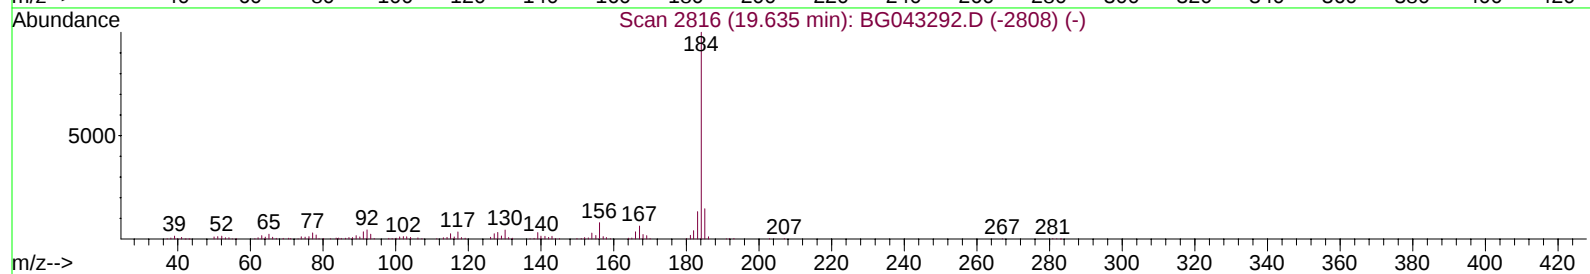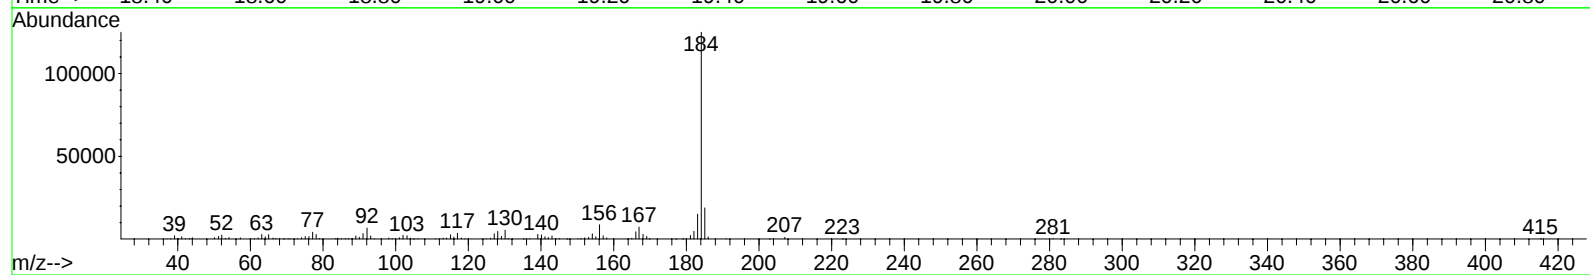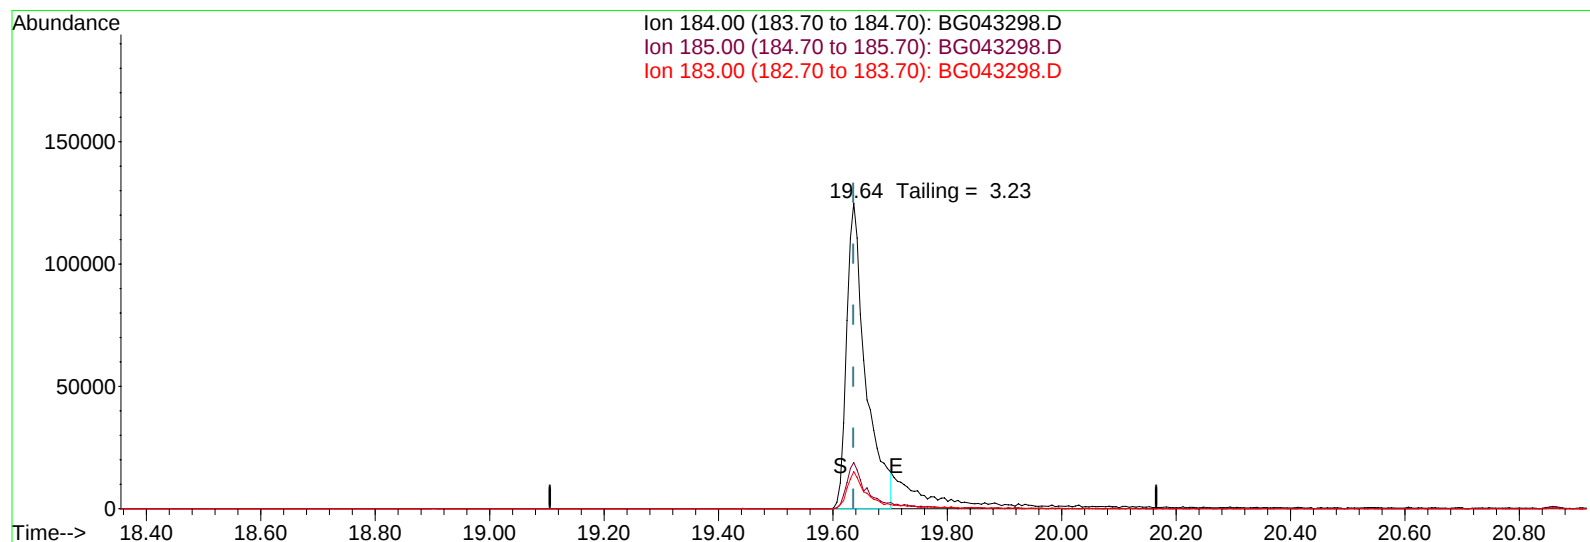

TIC: BG043298.D

(77) Benzidine

19.636min (+0.001) 0.00ng

response 338622

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.12
183.00	13.30	12.14
0.00	0.00	0.00