


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102219\
Data File : BG043298.D
Acq On : 22 Oct 2019 9:14
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 21 16:37:43 2019

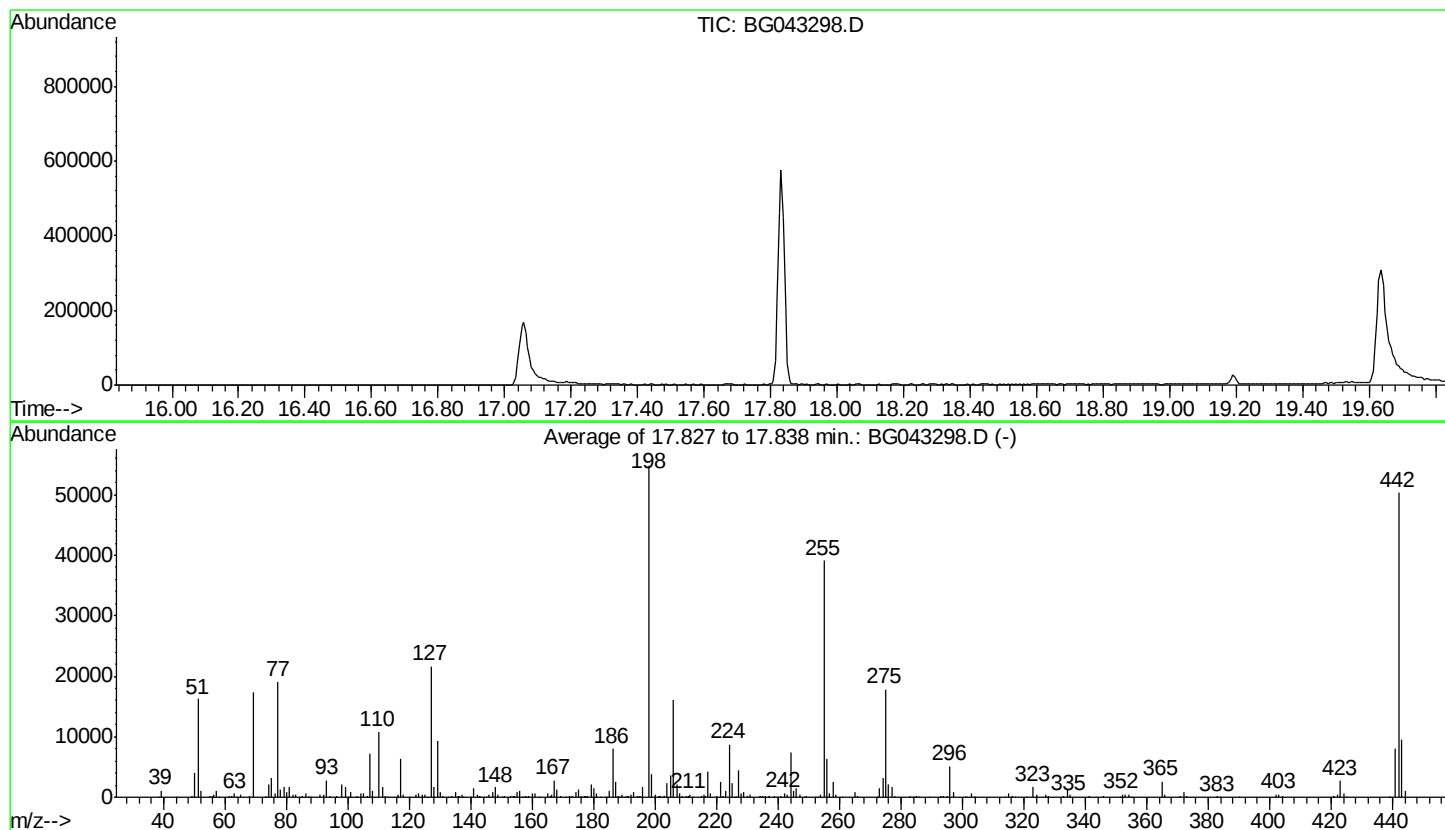

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	16292	PASS
68	69	0.00	2	1.2	205	PASS
69	198	0.00	100	31.8	17443	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.4	21610	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54816	PASS
199	198	5	9	6.8	3733	PASS
275	198	10	60	32.5	17805	PASS
365	198	1	100	4.8	2646	PASS
441	198	0.01	100	14.6	8028	PASS
442	198	50	100	91.8	50309	PASS
443	442	15	24	18.7	9426	PASS