

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102220\
 Data File : BG047053.D
 Acq On : 23 Oct 2020 5:50
 Operator : CG/JU
 Sample : L4451-02
 Misc : GCMS CONFIRMATION
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE0

Quant Time: Oct 23 07:54:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 23 04:22:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	64703	20.00	ng/ul	0.00
18) Naphthalene-d8	10.87	136	234916	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.69	164	155677	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	314981	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	326295	20.00	ng/ul	0.00
86) Perylene-d12	24.94	264	356188	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul	
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
79) Pyrene-d10	0.00	212	0	0.00	ng/ul	
90) Benzo(a)pyrene-d12	0.00	264	0	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
70) Phenanthrene	17.48	178	37863	2.143	ng/ul	96
77) Fluoranthene	19.48	202	41225	1.939	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102220\
Data File : BG047053.D
Acq On : 23 Oct 2020 5:50
Operator : CG/JU
Sample : L4451-02
Misc : GCMS CONFIRMATION
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE0

Quant Time: Oct 23 07:54:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 23 04:22:04 2020
Response via : Initial Calibration

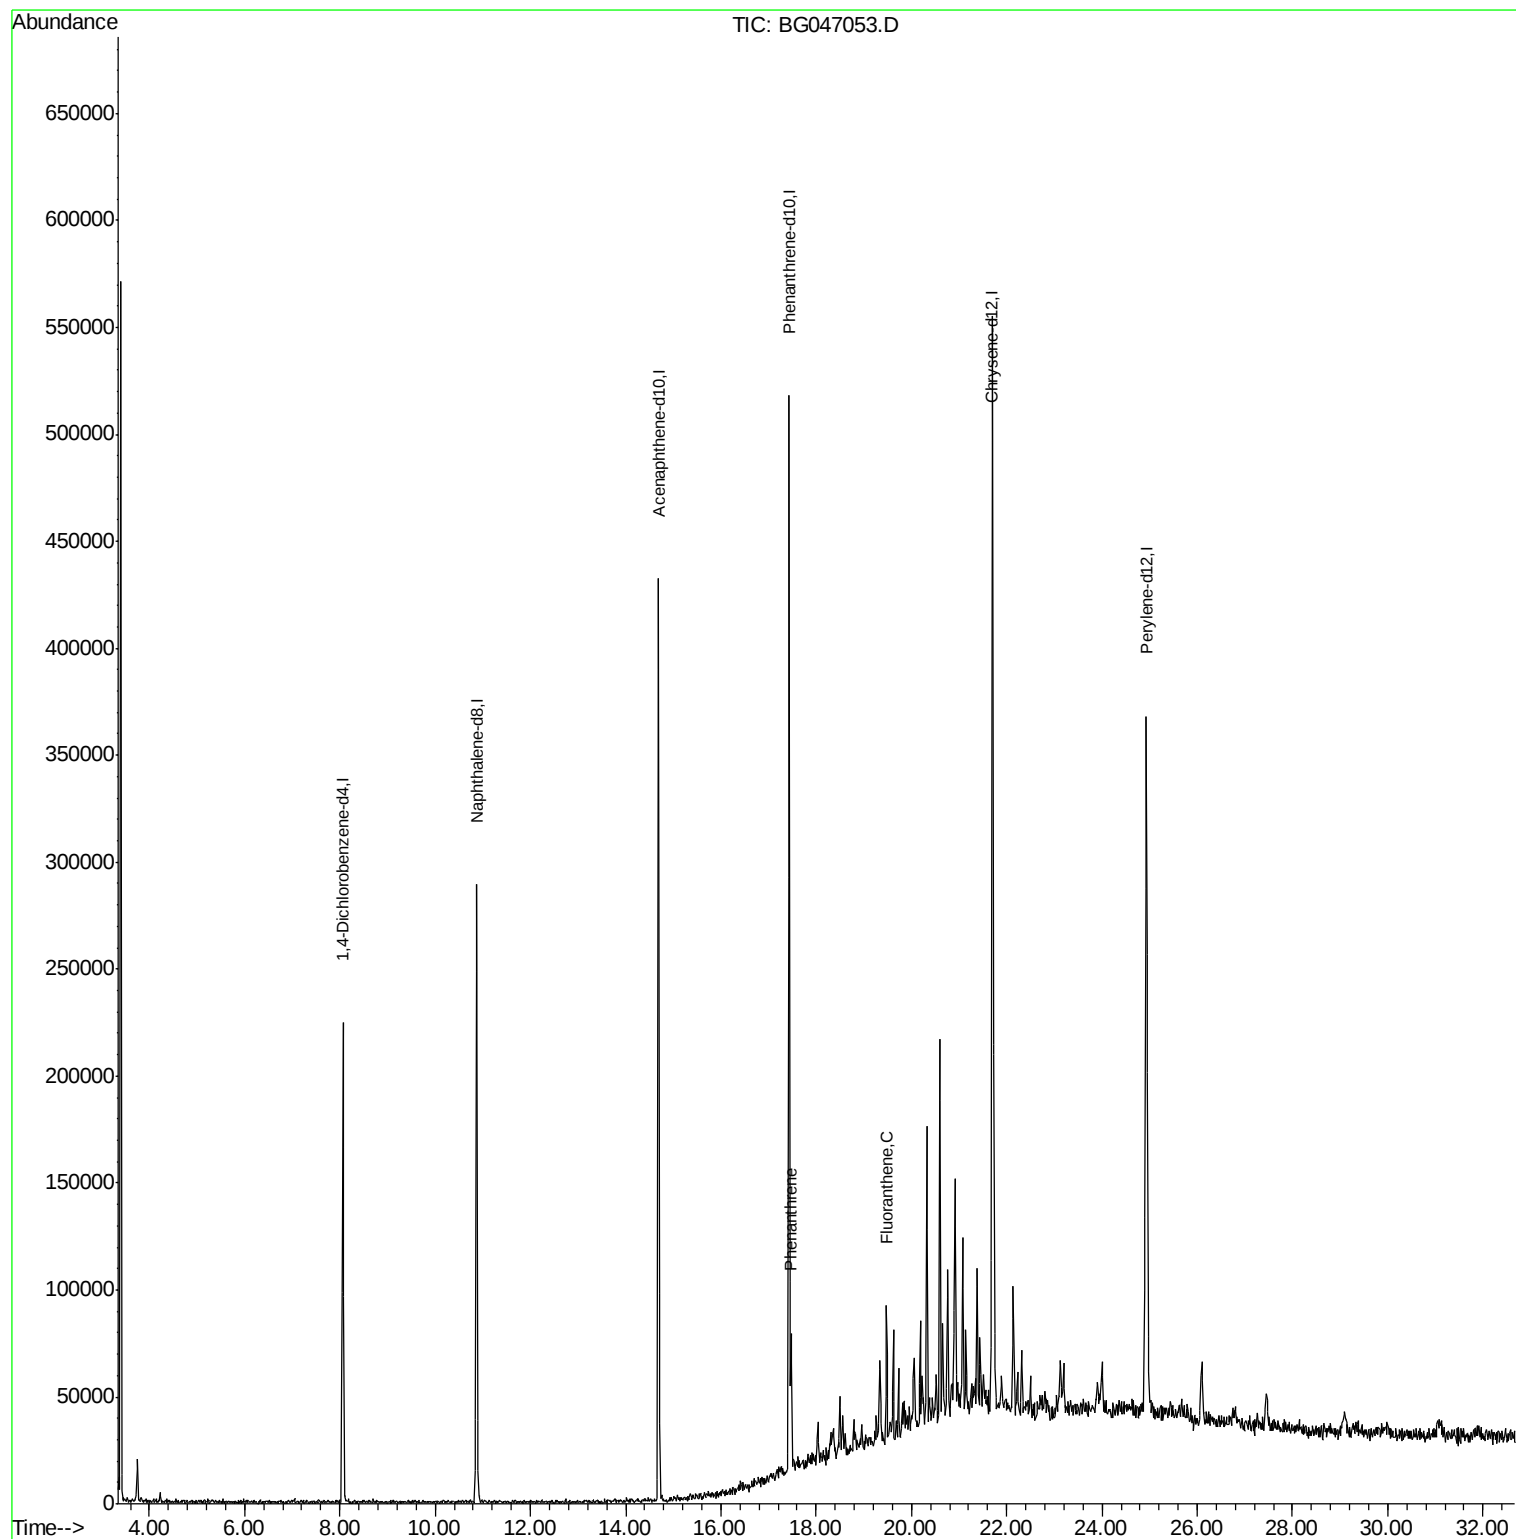


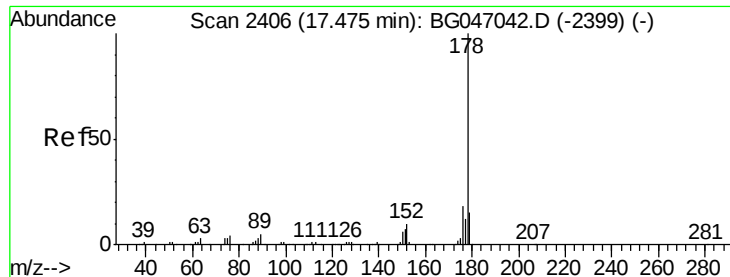




#70
Phenanthrene
Concen: 2.143 ng/ul
RT: 17.48 min Scan# 2406
Delta R.T. -0.00 min
Lab File: BG047053.D
Acq: 23 Oct 2020 5:50

Instrument :
BNA_G
ClientSampleId :
C0AE0

Tot Ion:178 Resp: 37863
Ion Ratio Lower Upper
178 100
179 15.8 13.0 19.4
176 16.2 15.5 23.3

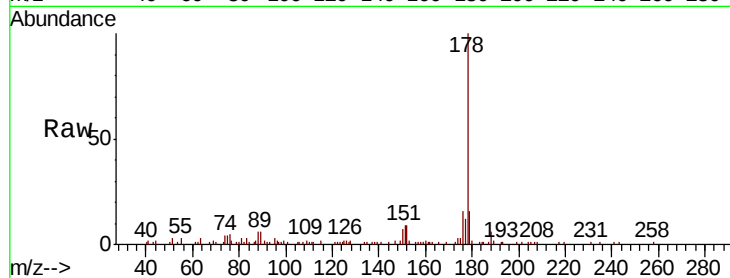


Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

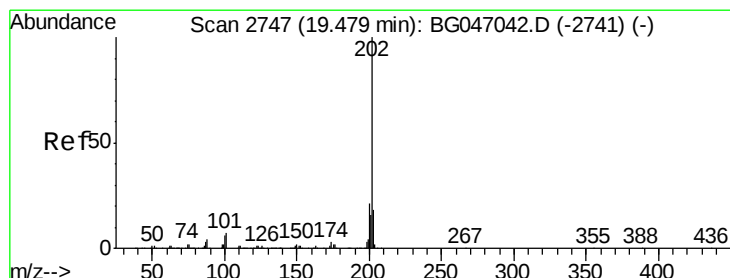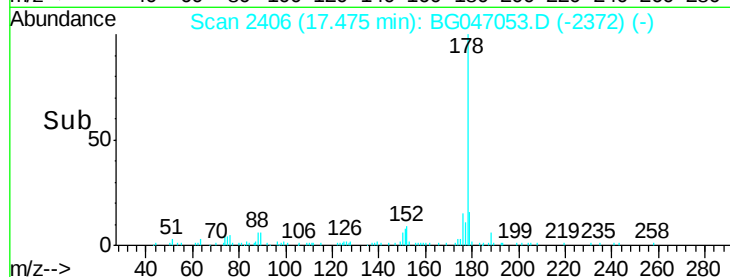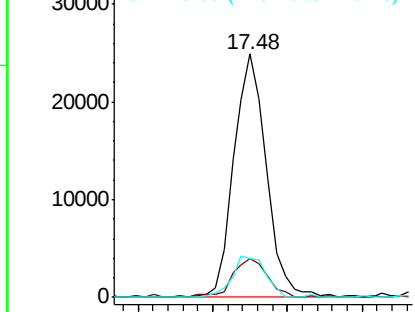

#77
Fluoranthene
Concen: 1.939 ng/ul
RT: 19.48 min Scan# 2748
Delta R.T. -0.00 min
Lab File: BG047053.D
Acq: 23 Oct 2020 5:50

Tgt Ion:202 Resp: 41225
Ion Ratio Lower Upper
202 100
101 5.6 4.9 7.3
100 3.9 4.2 6.4#

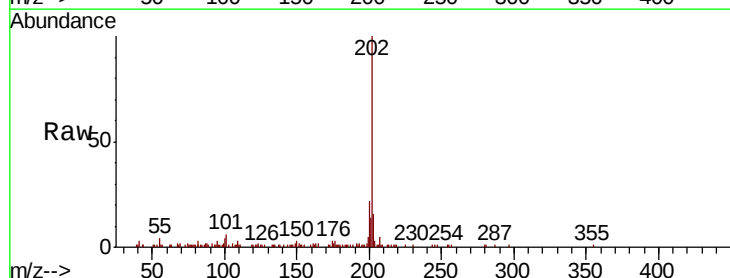

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

