
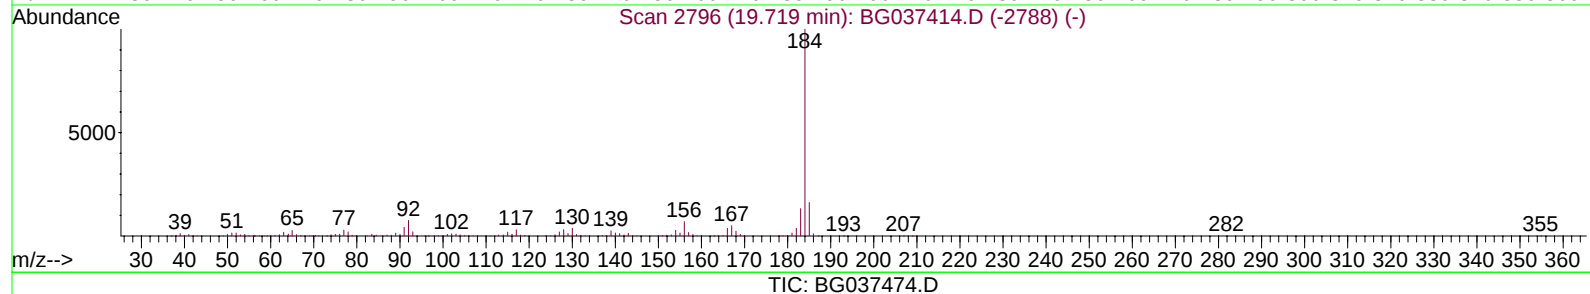
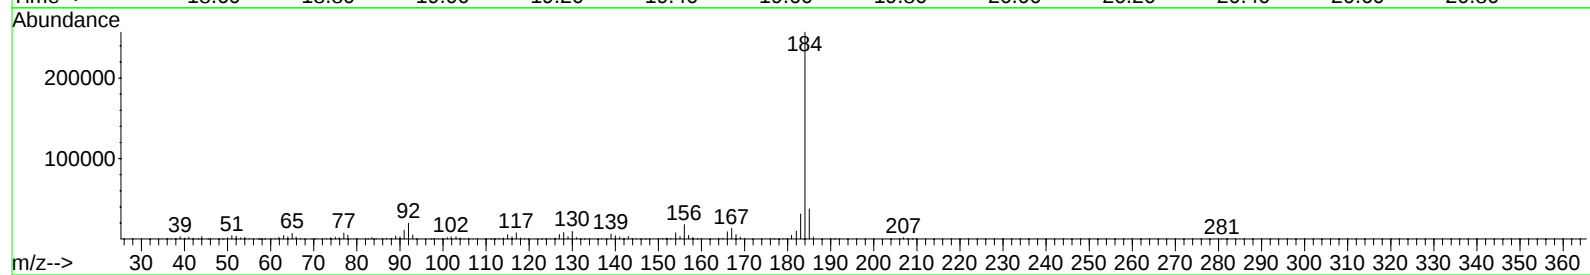


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102318\  
Data File : BG037474.D  
Acq On : 23 Oct 2018 12:57  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 09:55:45 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 18 14:06:42 2018  
Response via : Initial Calibration

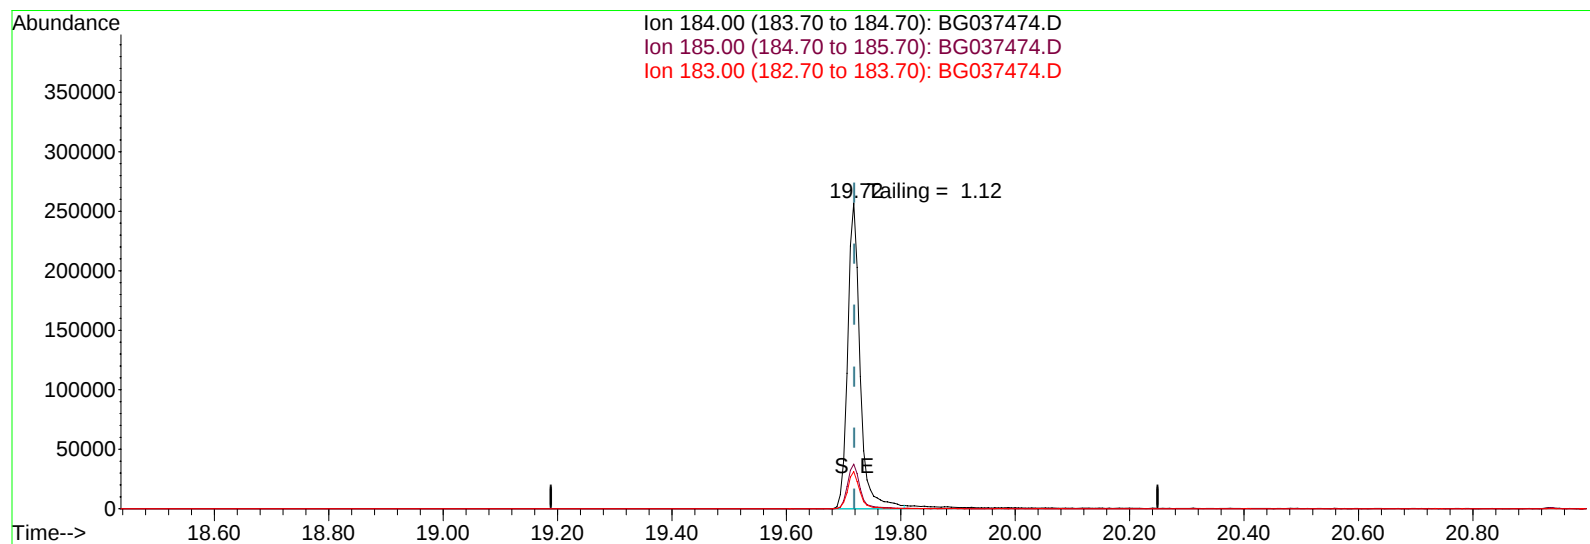

(77) Benzidine




19.718min (-0.001) 191788.62ng

response 397800

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.62 |
| 183.00 | 12.70 | 12.15 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102318\  
Data File : BG037474.D  
Acq On : 23 Oct 2018 12:57  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 09:55:45 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 18 14:06:42 2018  
Response via : Initial Calibration

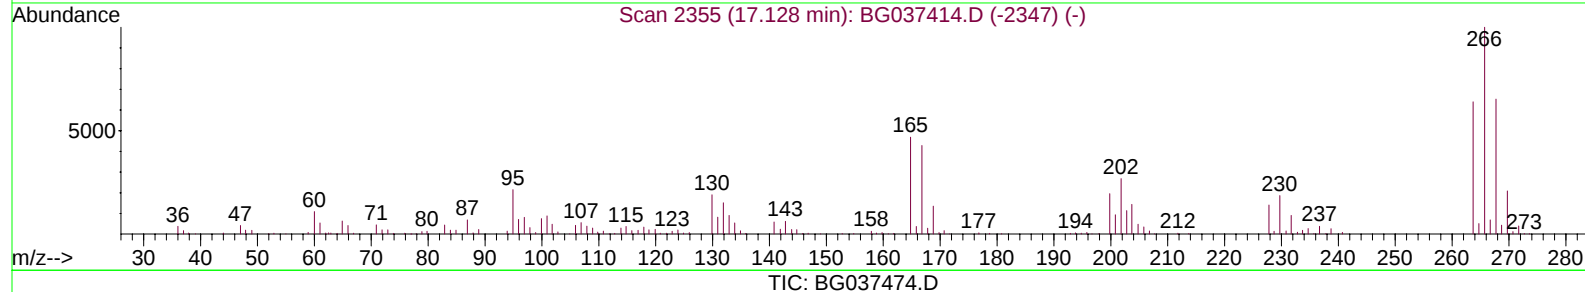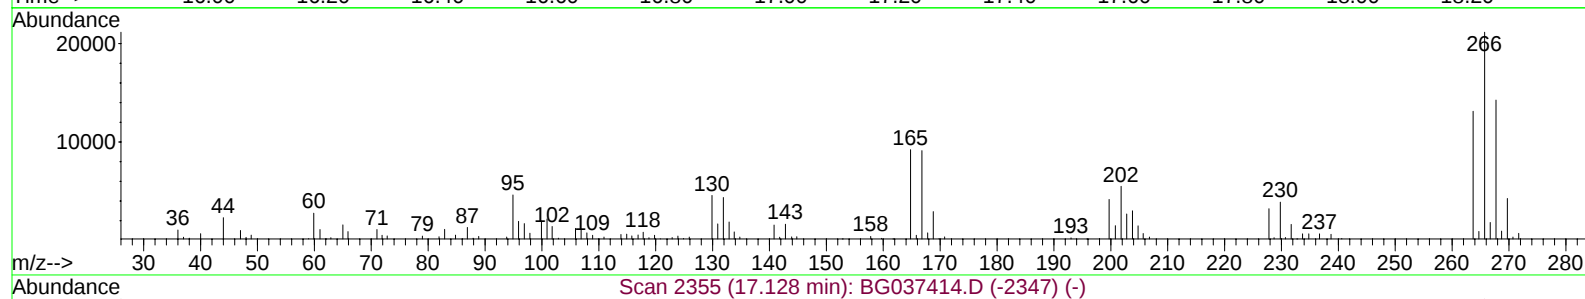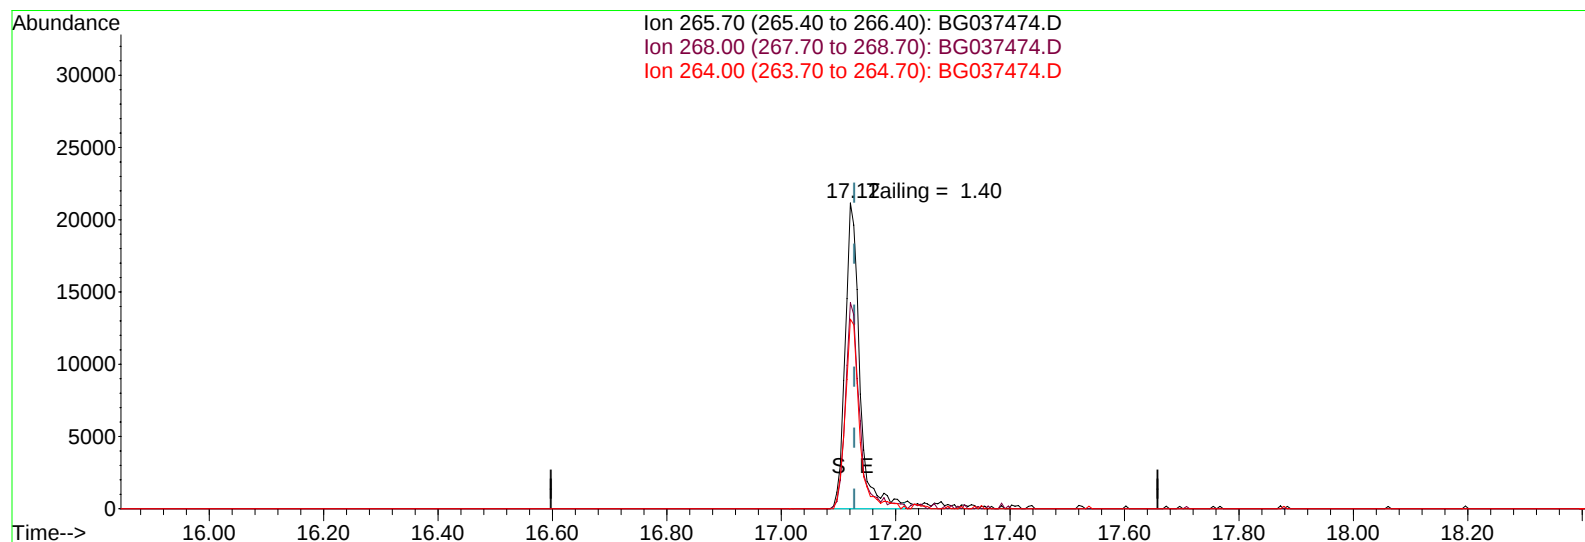

(70) Pentachlorophenol (C)

17.121min (-0.007) 85933.14ng

response 36032

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 68.80 | 71.91 |
| 264.00 | 73.60 | 66.37 |
| 0.00   | 0.00  | 0.00  |