

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102318\
 Data File : BG037490.D
 Acq On : 24 Oct 2018 00:04
 Operator : JU/SJ
 Sample : J5624-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PA-SW-02

Quant Time: Oct 24 05:41:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	58566	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	268023	20.00	ng	0.00
39) Acenaphthene-d10	14.74	164	183371	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	432430	20.00	ng	0.00
76) Chrysene-d12	21.77	240	392538	20.00	ng	0.00
87) Perylene-d12	25.10	264	400301	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	179725	51.31	ng	0.00
7) Phenol-d6	7.25	99	197427	37.27	ng	0.00
23) Nitrobenzene-d5	9.28	82	345970	72.31	ng	0.00
42) 2,4,6-Tribromophenol	16.23	330	212748	106.37	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	833105	68.51	ng	0.00
79) Terphenyl-d14	20.09	244	1283006	69.84	ng	0.00
Target Compounds						
10) Phenol	7.27	94	20513	3.670	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102318\
Data File : BG037490.D
Acq On : 24 Oct 2018 00:04
Operator : JU/SJ
Sample : J5624-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PA-SW-02

Quant Time: Oct 24 05:41:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

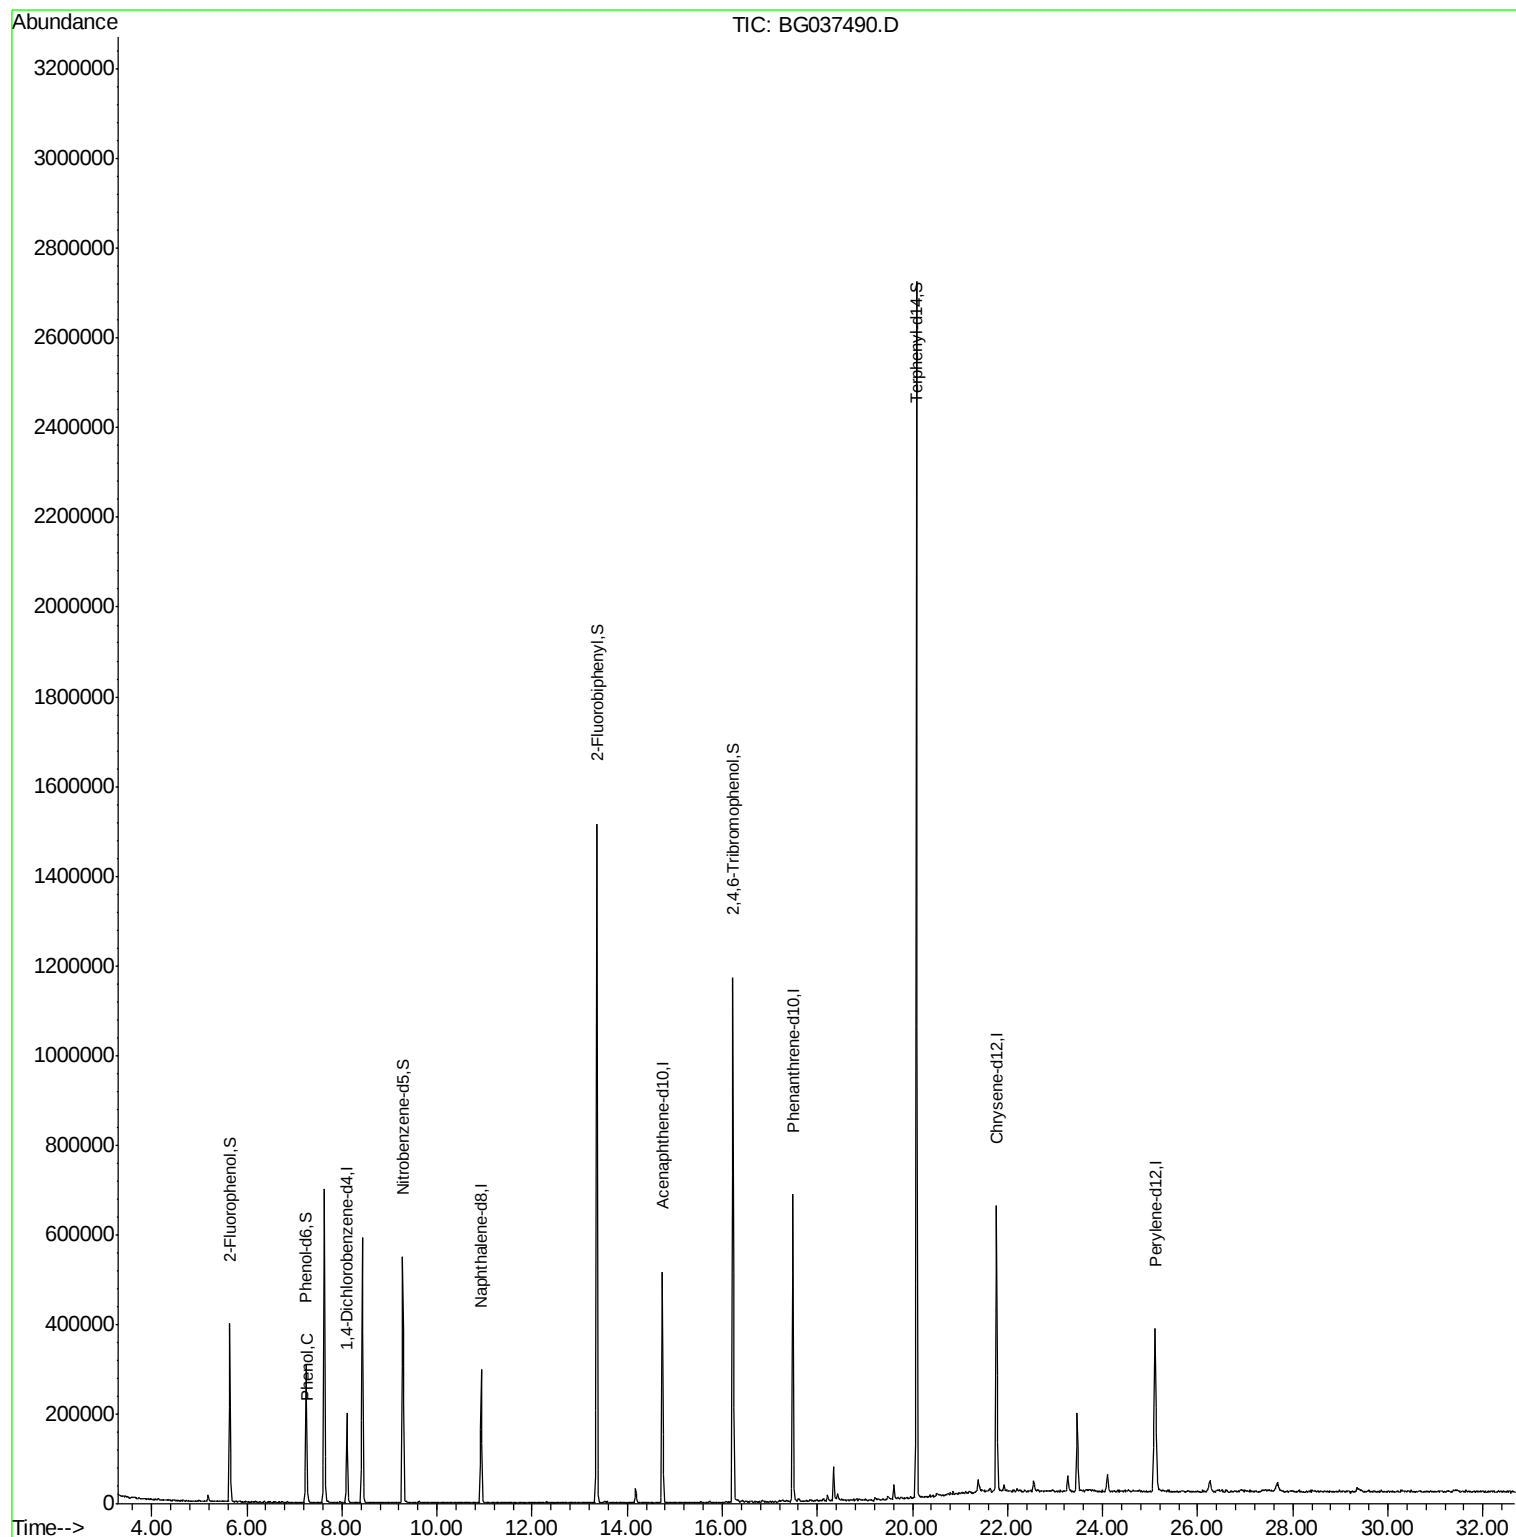




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.11 min Scan# 820
Delta R.T. -0.00 min
Lab File: BG037490.D
Acq: 24 Oct 2018 00:04

Instrument :
BNA_G
ClientSampleId :
PA-SW-02

Tot Ion:152 Resp: 58566
Ion Ratio Lower Upper
152 100
150 157.2 126.0 189.0
115 57.9 45.5 68.3

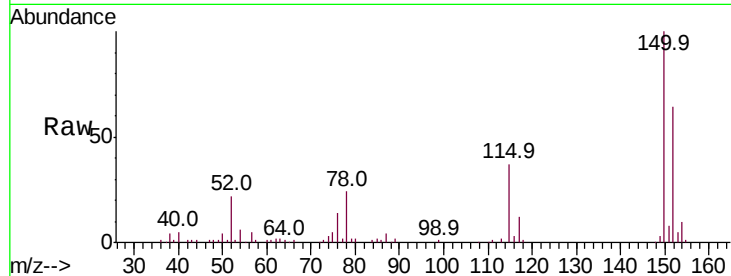


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

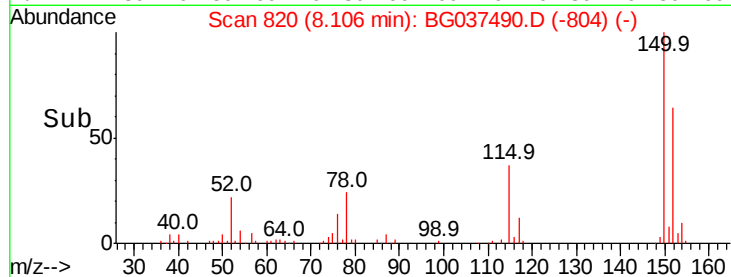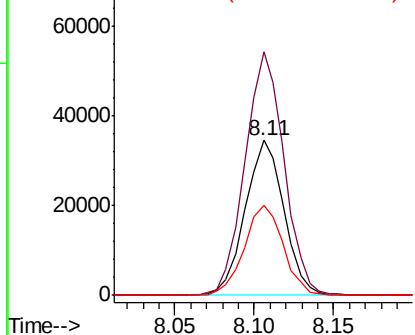



#5

2-Fluorophenol
Concen: 51.305 ng
RT: 5.64 min Scan# 401
Delta R.T. -0.00 min
Lab File: BG037490.D
Acq: 24 Oct 2018 00:04

Tgt Ion:112 Resp: 179725
Ion Ratio Lower Upper
112 100
64 65.6 53.1 79.7
63 34.5 27.3 40.9

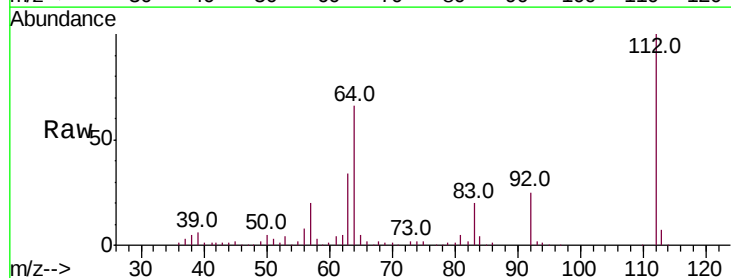

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

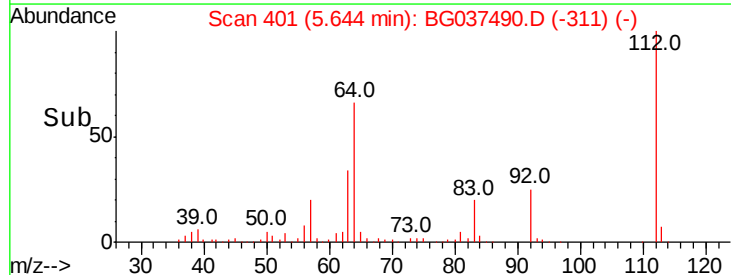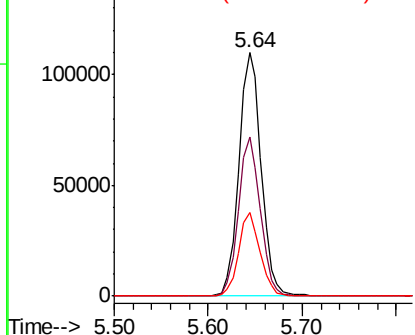



#7

Phenol-d6

Concen: 37.271 ng

RT: 7.25 min Scan# 674

Delta R.T. -0.00 min

Lab File: BG037490.D

Acq: 24 Oct 2018 00:04

Instrument :

BNA_G

ClientSampled :

PA-SW-02


Tot Ion: 99 Resp: 197427

Ion Ratio Lower Upper




99 100

42 17.4 15.0 22.4

71 28.2 25.5 38.3

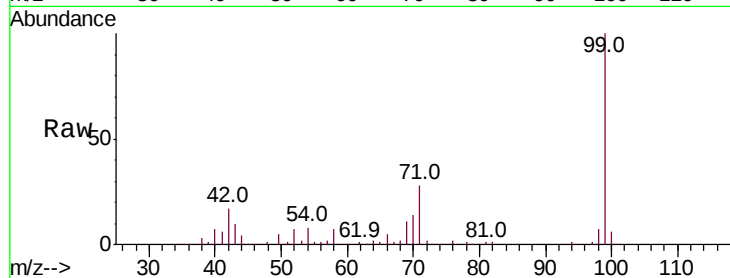

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

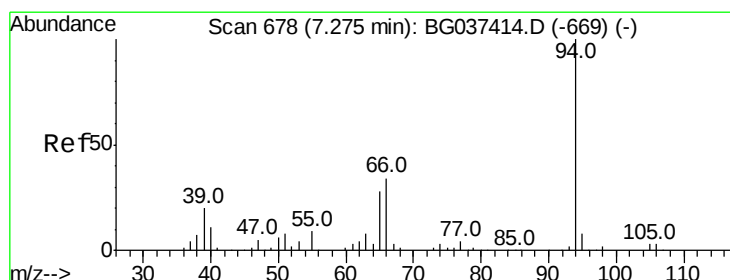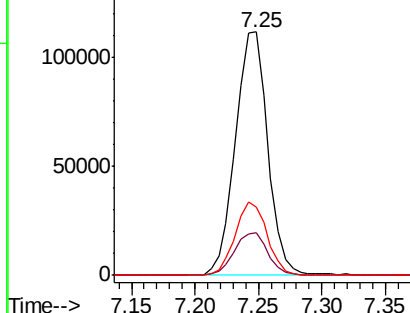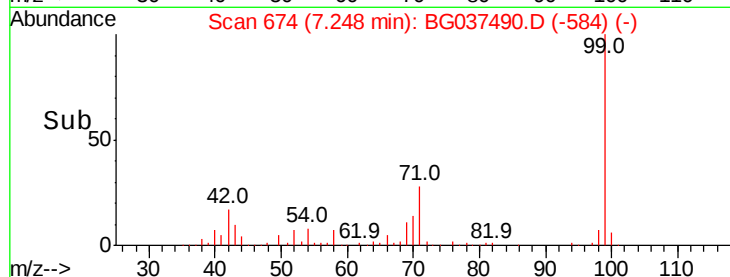

#10

Phenol

Concen: 3.670 ng

RT: 7.27 min Scan# 678

Delta R.T. -0.00 min

Lab File: BG037490.D

Acq: 24 Oct 2018 00:04


Tgt Ion: 94 Resp: 20513

Ion Ratio Lower Upper



94 100


65 28.2 9.7 49.7

66 36.0 15.9 55.9

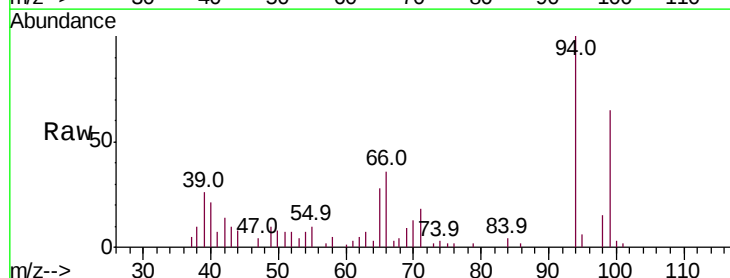

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

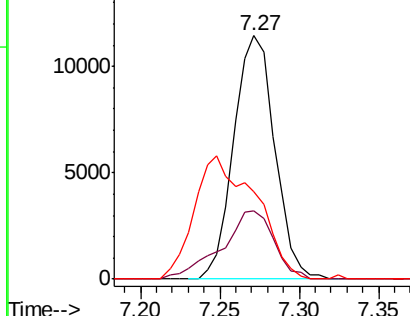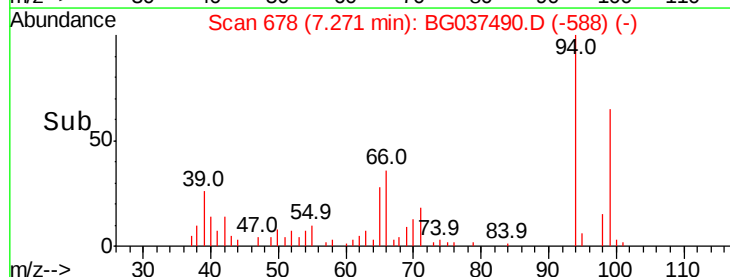


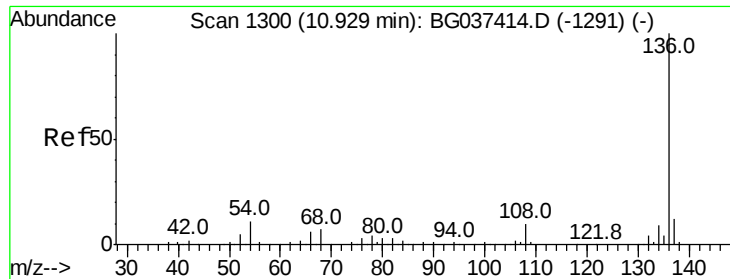




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.93 min Scan# 1300
Delta R.T. -0.00 min
Lab File: BG037490.D
Acq: 24 Oct 2018 00:04

Instrument :
BNA_G
ClientSampleId :
PA-SW-02

Tot Ion:	136	Resp:	268023
Ion	Ratio	Lower	Upper
136	100		
137	10.7	9.6	14.4
54	10.2	7.9	11.9
68	6.2	4.8	7.2

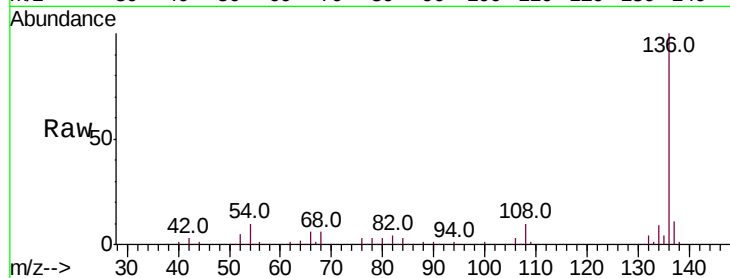


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

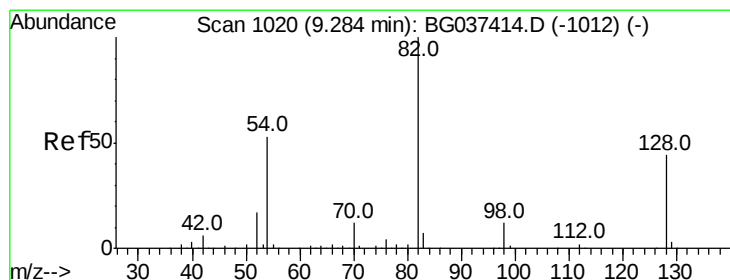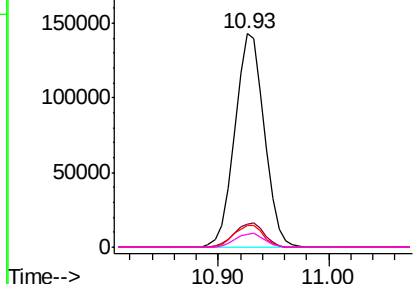
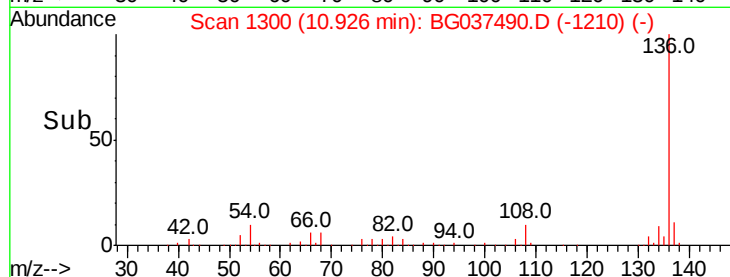


#23
Nitrobenzene-d5
Concen: 72.311 ng
RT: 9.28 min Scan# 1020
Delta R.T. -0.00 min
Lab File: BG037490.D
Acq: 24 Oct 2018 00:04

Tgt Ion:	82	Resp:	345970
Ion	Ratio	Lower	Upper
82	100		
128	44.2	34.6	51.8
54	54.2	45.3	67.9

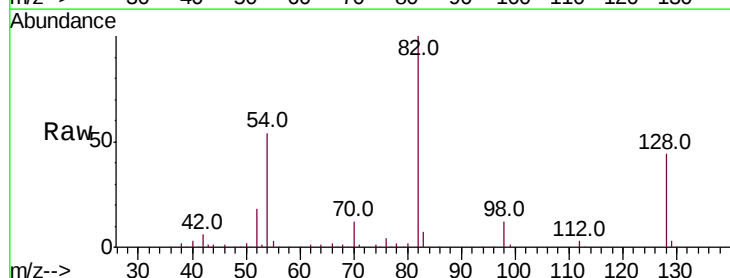

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

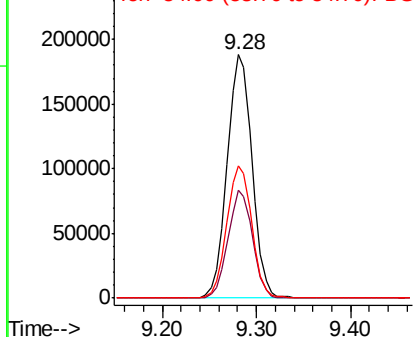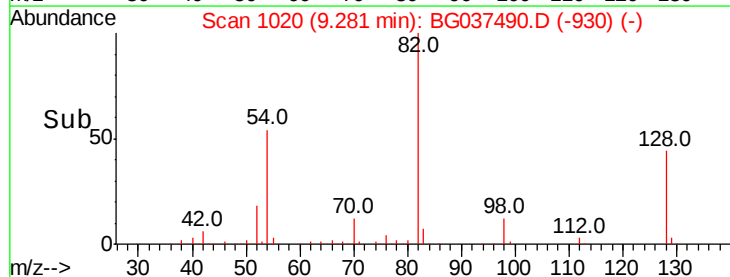



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.74 min Scan# 1949

Delta R.T. -0.00 min

Lab File: BG037490.D

Acq: 24 Oct 2018 00:04

Instrument :

BNA_G

ClientSampleId :

PA-SW-02


Tot Ion:164 Resp: 183371

Ion Ratio Lower Upper

164 100

162 103.5 81.3 121.9




160 46.7 36.3 54.5

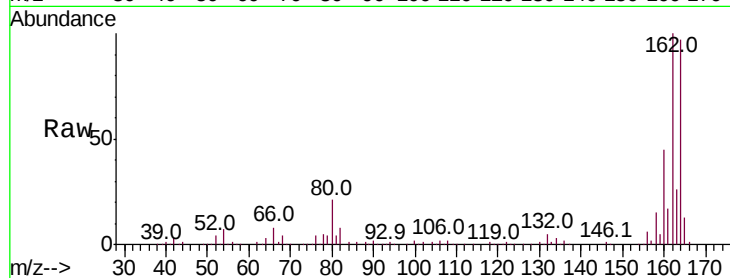

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

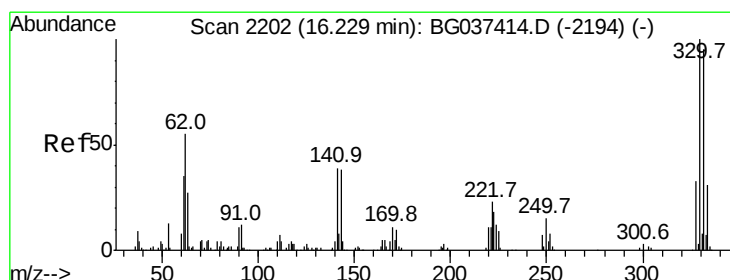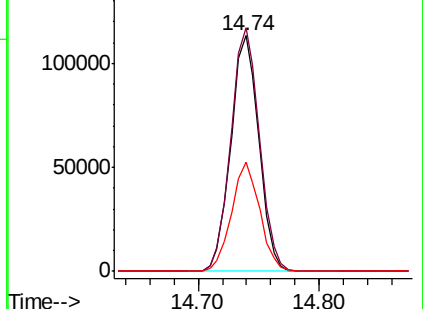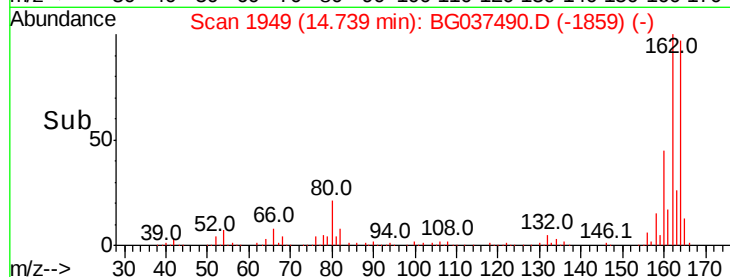

#42

2,4,6-Tribromophenol

Concen: 106.374 ng

RT: 16.23 min Scan# 2202

Delta R.T. -0.00 min

Lab File: BG037490.D

Acq: 24 Oct 2018 00:04


Tgt Ion:330 Resp: 212748

Ion Ratio Lower Upper

330 100

332 95.2 78.4 117.6



141 41.2 32.2 48.2

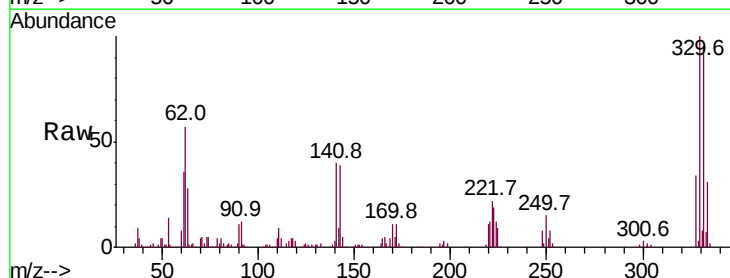

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



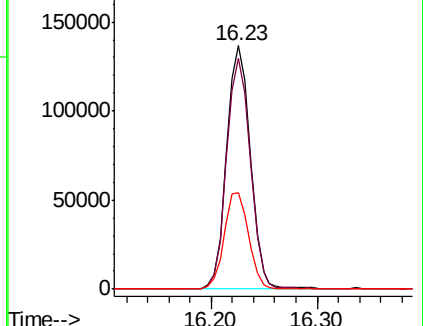
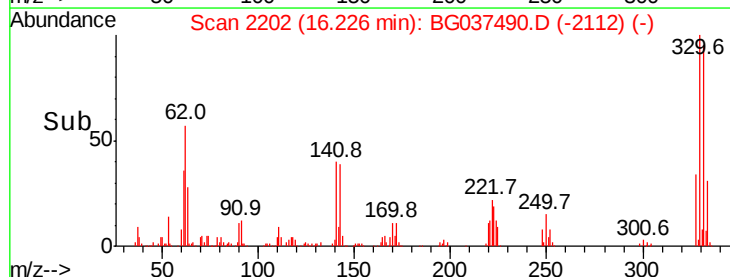




#45
 2-Fluorobiphenyl
 Concen: 68.510 ng
 RT: 13.36 min Scan# 1715
 Delta R.T. -0.00 min
 Lab File: BG037490.D
 Acq: 24 Oct 2018 00:04




Instrument :
 BNA_G
 ClientSampleId :
 PA-SW-02


Tot Ion	Ratio	Lower	Upper
172	100		
171	38.0	31.0	46.4
170	25.0	20.2	30.2

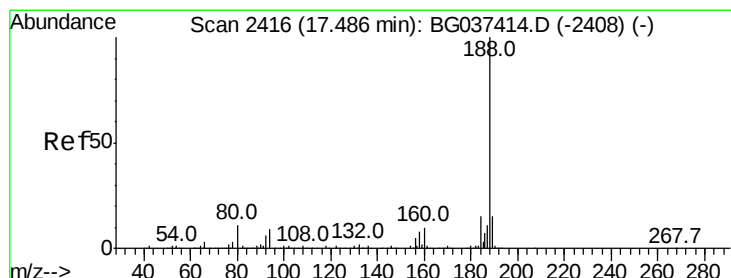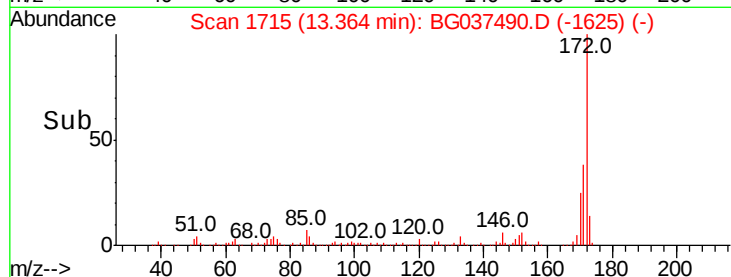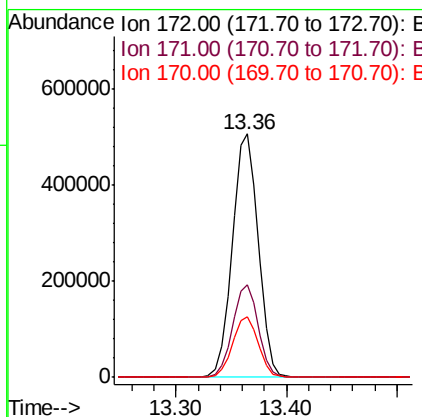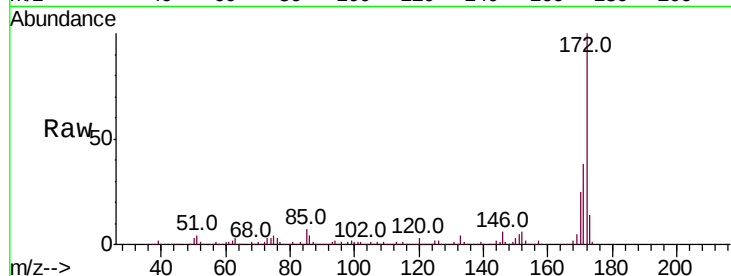

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.48 min Scan# 2416
 Delta R.T. -0.00 min
 Lab File: BG037490.D
 Acq: 24 Oct 2018 00:04

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.2	7.2	10.8
80	10.3	7.7	11.5


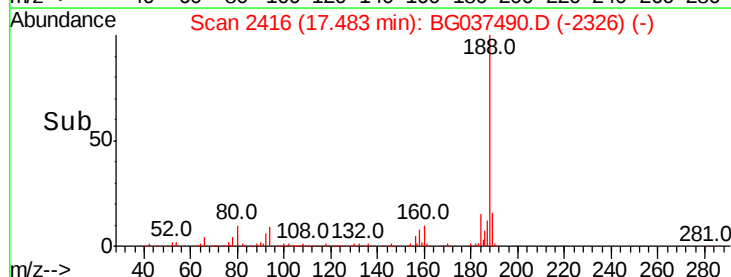
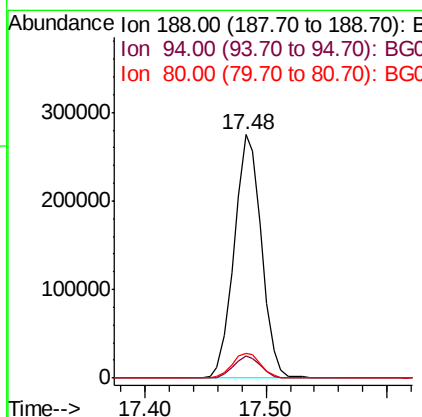
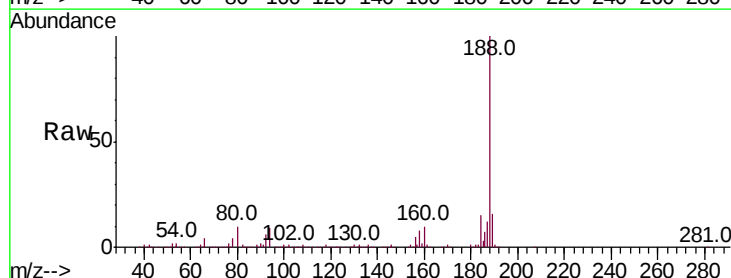


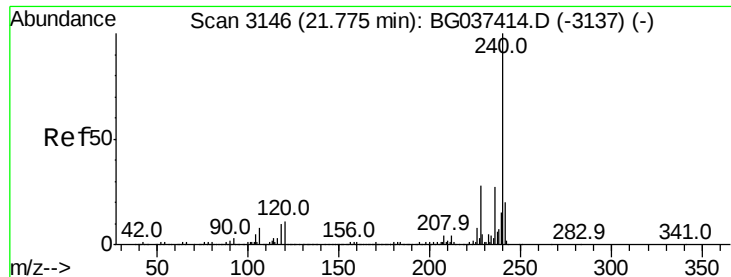

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.77 min Scan# 3146
 Delta R.T. -0.00 min
 Lab File: BG037490.D
 Acq: 24 Oct 2018 00:04




Instrument :
 BNA_G
 ClientSampleId :
 PA-SW-02


Tot Ion	Ratio	Lower	Upper
240	100		
120	10.0	8.1	12.1
236	26.0	21.4	32.0

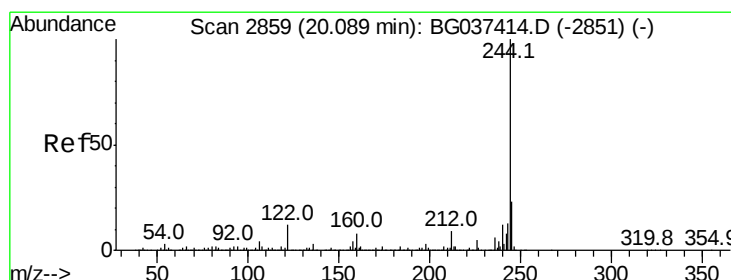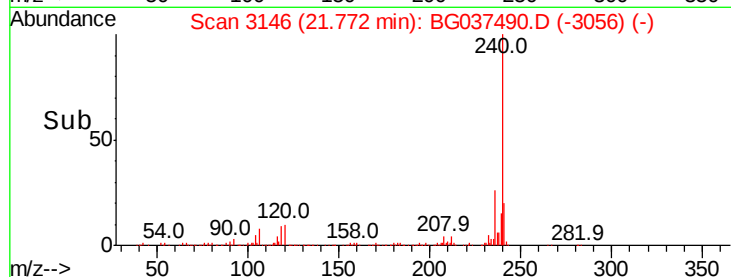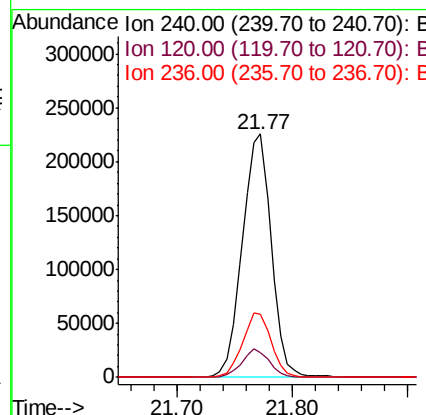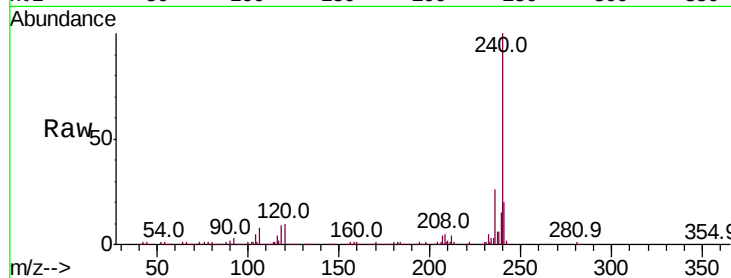

#79
 Terphenyl-d14
 Concen: 69.840 ng
 RT: 20.09 min Scan# 2859
 Delta R.T. -0.00 min
 Lab File: BG037490.D
 Acq: 24 Oct 2018 00:04

Tgt Ion	Ratio	Lower	Upper
244	100		
212	8.7	6.5	9.7
122	11.7	9.0	13.4

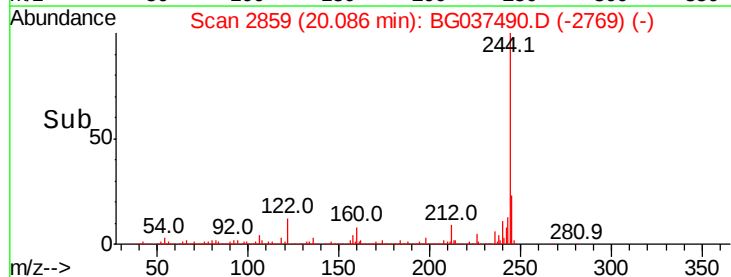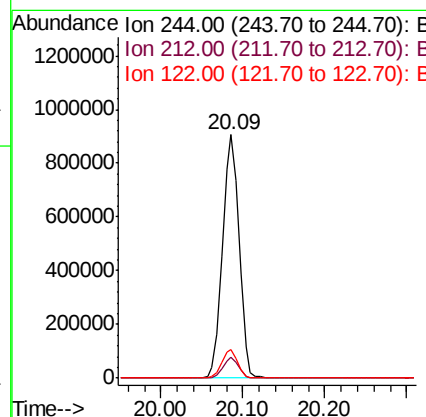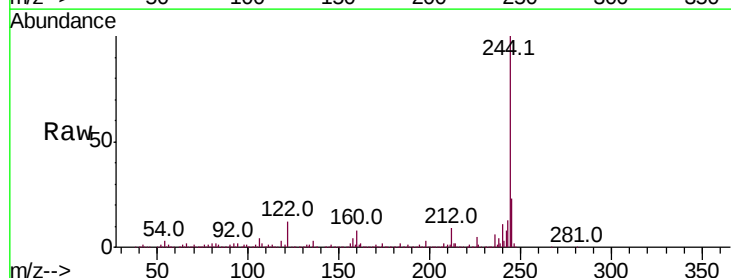

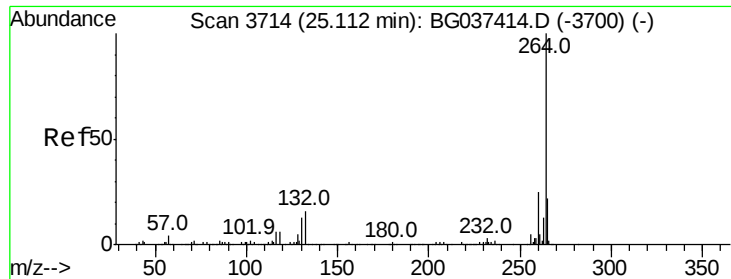

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.10 min Scan# 3713
Delta R.T. -0.01 min
Lab File: BG037490.D
Acq: 24 Oct 2018 00:04

Instrument :
BNA_G
ClientSampleId :
PA-SW-02

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.7	18.2	27.4
265	21.2	17.9	26.9

