

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102318\
 Data File : BG037509.D
 Acq On : 24 Oct 2018 13:32
 Operator : JU/SJ
 Sample : J5623-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 101918-TIPC-E-D-M

Quant Time: Oct 24 14:38:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	57593	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	262281	20.00	ng	0.00
39) Acenaphthene-d10	14.74	164	178651	20.00	ng	0.00
64) Phenanthrene-d10	17.49	188	427749	20.00	ng	0.00
76) Chrysene-d12	21.77	240	391414	20.00	ng	0.00
87) Perylene-d12	25.10	264	394693	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	153692	44.61	ng	0.00
7) Phenol-d6	7.25	99	133035	25.54	ng	0.00
23) Nitrobenzene-d5	9.28	82	457333	97.68	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	195783	100.48	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	1134513	95.76	ng	0.00
79) Terphenyl-d14	20.08	244	1483138	80.97	ng	0.00
Target Compounds						
10) Phenol	7.27	94	25549	4.649	ng	92
50) Dimethylphthalate	14.18	163	42272	3.059	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102318\
Data File : BG037509.D
Acq On : 24 Oct 2018 13:32
Operator : JU/SJ
Sample : J5623-07
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
101918-TIPC-E-D-M

Quant Time: Oct 24 14:38:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

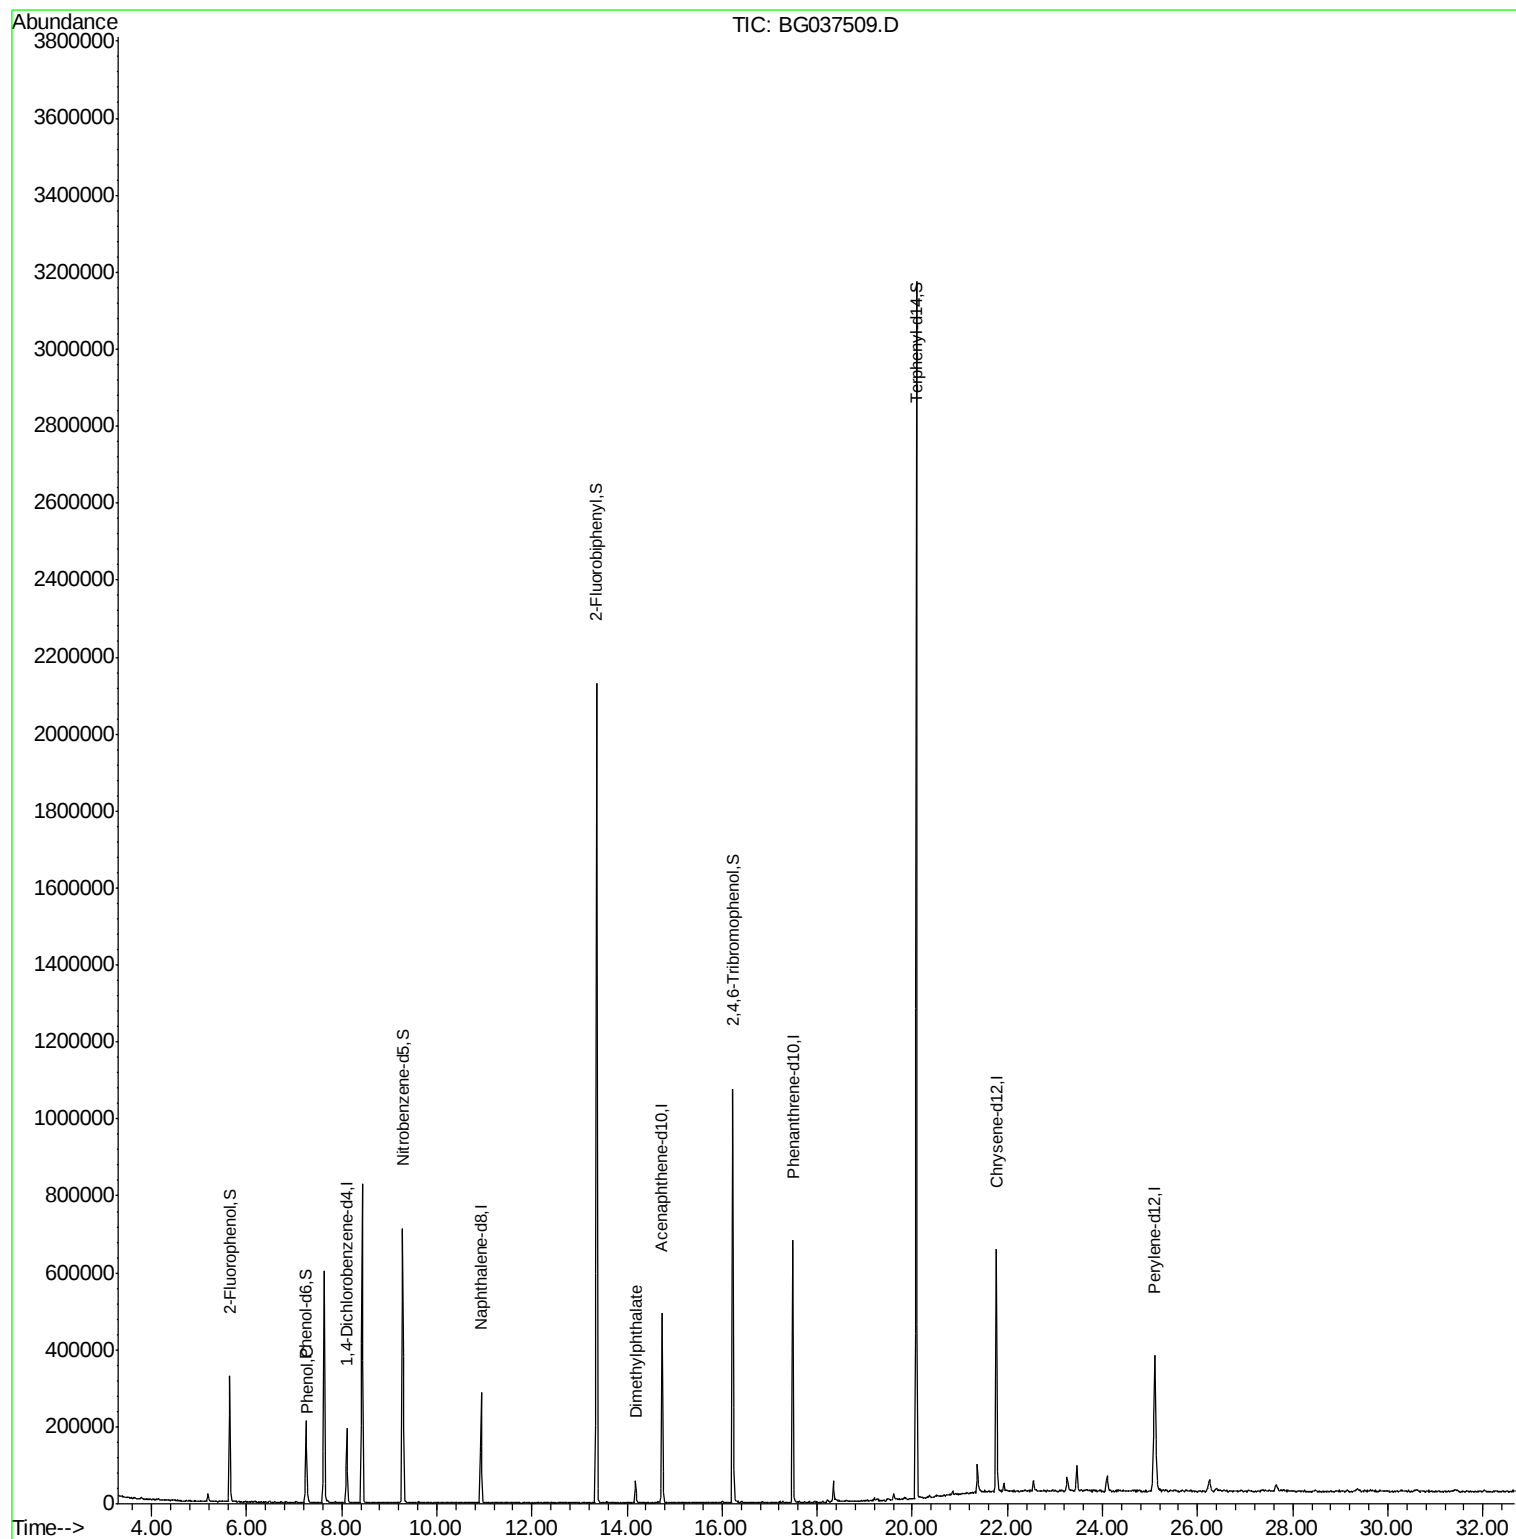




#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.10 min Scan# 819
 Delta R.T. -0.01 min
 Lab File: BG037509.D
 Acq: 24 Oct 2018 13:32

Instrument :
 BNA_G
 ClientSampleId :
 101918-TIPC-E-D-M

Tot Ion:152 Resp: 57593
 Ion Ratio Lower Upper
 152 100
 150 161.5 126.0 189.0
 115 56.6 45.5 68.3

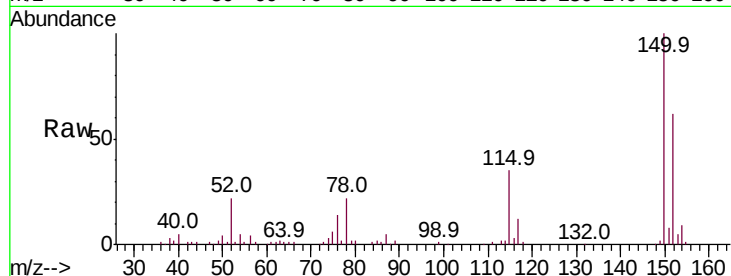


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

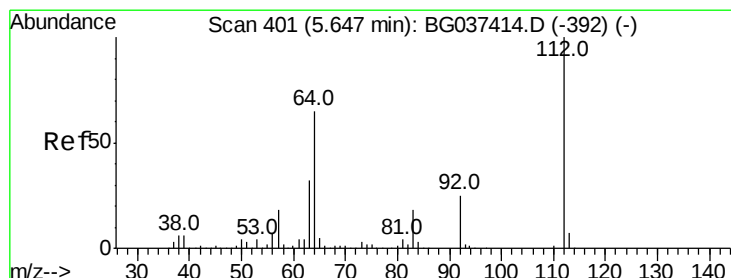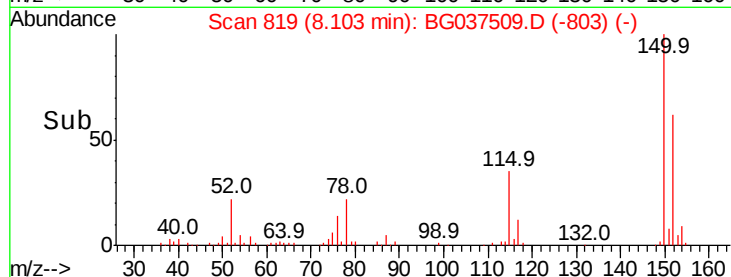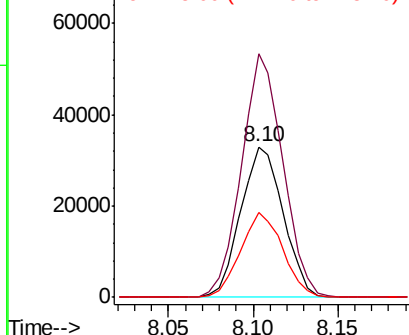



#5

2-Fluorophenol
 Concen: 44.615 ng
 RT: 5.65 min Scan# 401
 Delta R.T. 0.00 min
 Lab File: BG037509.D
 Acq: 24 Oct 2018 13:32

Tgt Ion:112 Resp: 153692
 Ion Ratio Lower Upper
 112 100
 64 60.8 53.1 79.7
 63 31.4 27.3 40.9

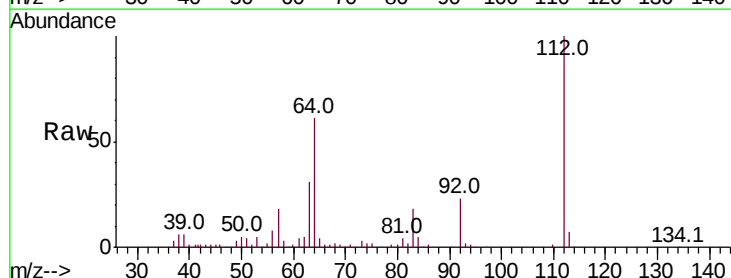

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

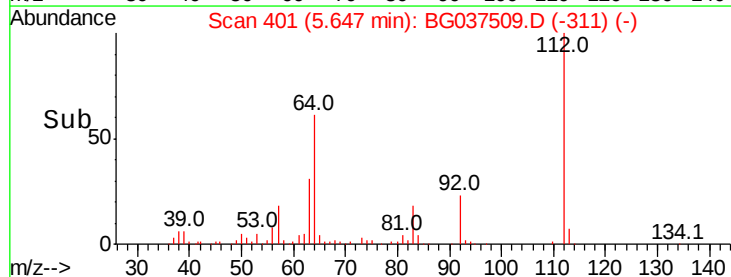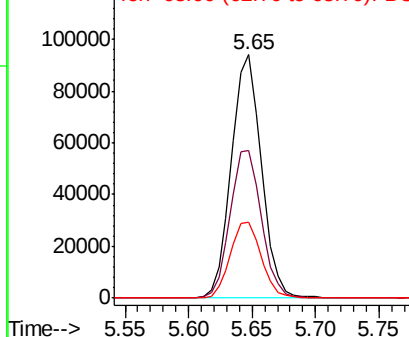



#7

Phenol-d6

Concen: 25.539 ng

RT: 7.25 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037509.D

Acq: 24 Oct 2018 13:32

Instrument :

BNA_G

ClientSampleId :

101918-TIPC-E-D-M


Tot Ion: 99 Resp: 133035

Ion Ratio Lower Upper




99 100

42 16.7 15.0 22.4

71 26.9 25.5 38.3

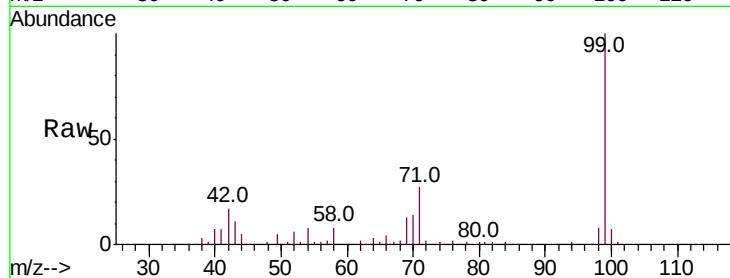

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

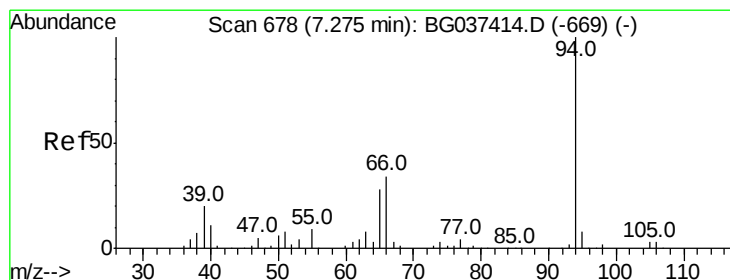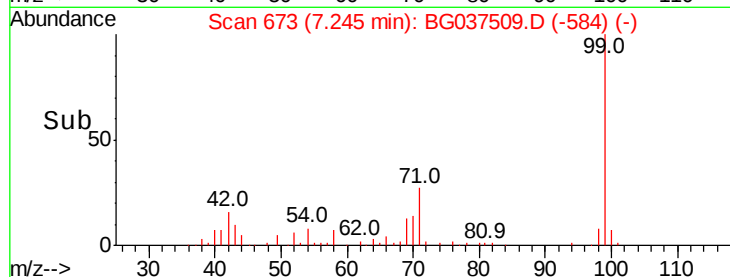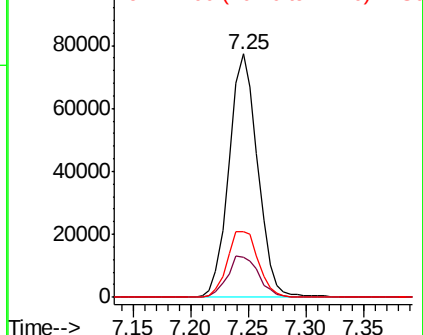

#10

Phenol

Concen: 4.649 ng

RT: 7.27 min Scan# 678

Delta R.T. 0.00 min

Lab File: BG037509.D

Acq: 24 Oct 2018 13:32


Tgt Ion: 94 Resp: 25549

Ion Ratio Lower Upper



94 100

65 25.8 9.7 49.7

66 31.3 15.9 55.9

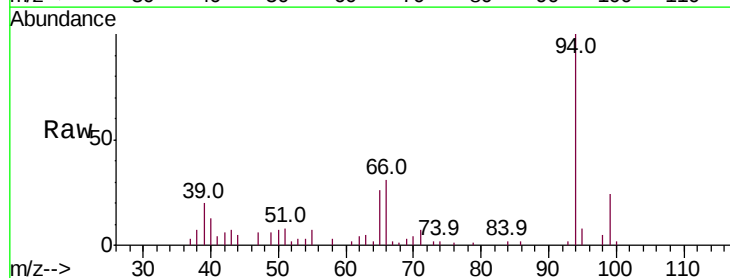

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

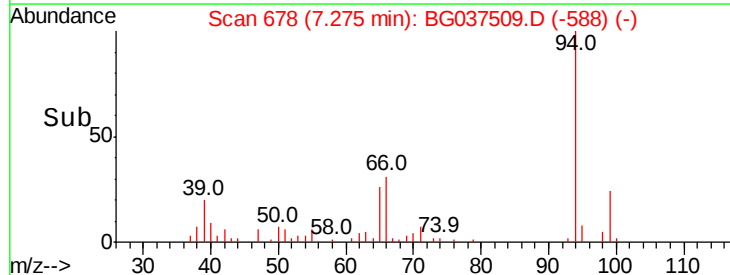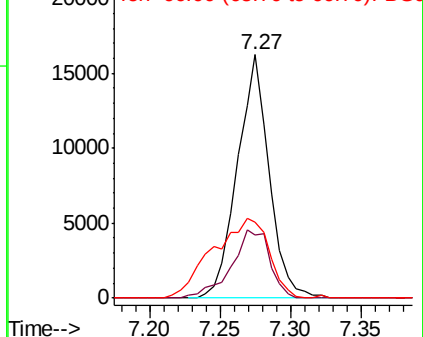







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.92 min Scan# 1299
Delta R.T. -0.01 min
Lab File: BG037509.D
Acq: 24 Oct 2018 13:32

Instrument :
BNA_G
ClientSampleId :
101918-TIPC-E-D-M

Tot Ion:	136	Resp:	262281
Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.6	14.4
54	9.7	7.9	11.9
68	6.3	4.8	7.2

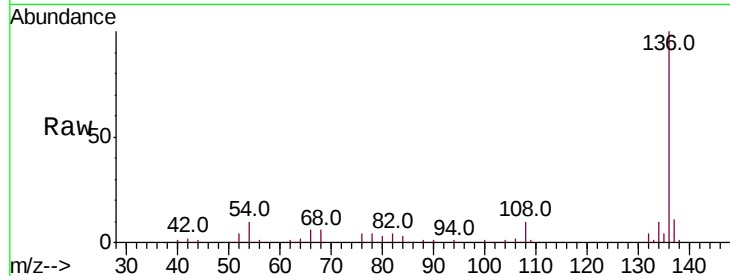


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BG
Ion 68.00 (67.70 to 68.70): BG

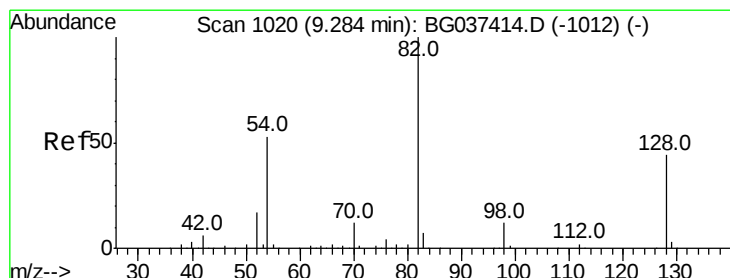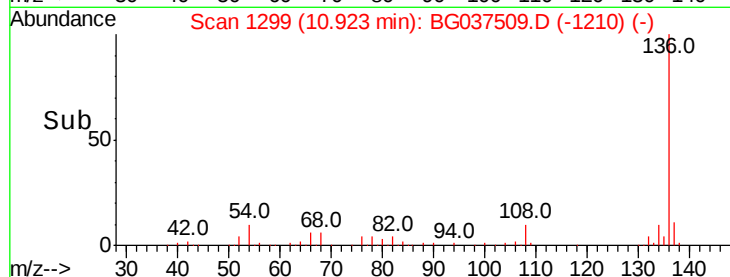
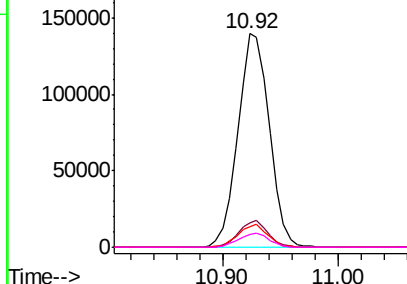



#23
Nitrobenzene-d5
Concen: 97.679 ng
RT: 9.28 min Scan# 1020
Delta R.T. 0.00 min
Lab File: BG037509.D
Acq: 24 Oct 2018 13:32

Tgt Ion:	82	Resp:	457333
Ion	Ratio	Lower	Upper
82	100		
128	44.9	34.6	51.8
54	54.9	45.3	67.9

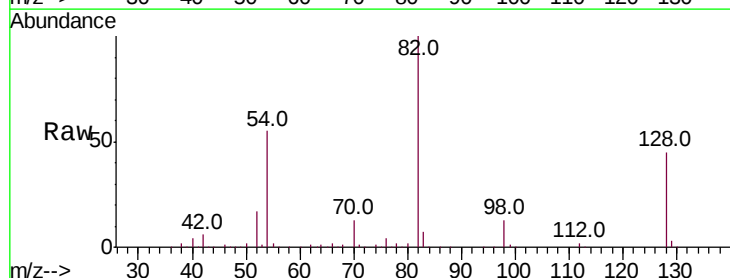

Abundance Ion 82.00 (81.70 to 82.70): BG
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BG

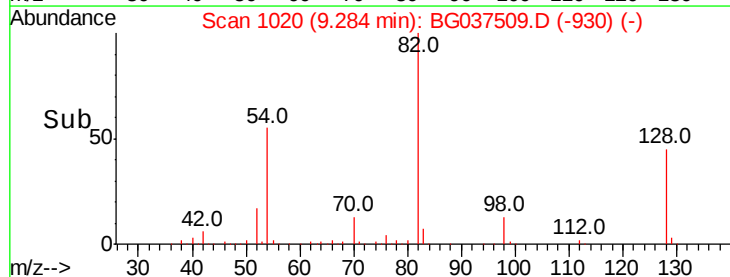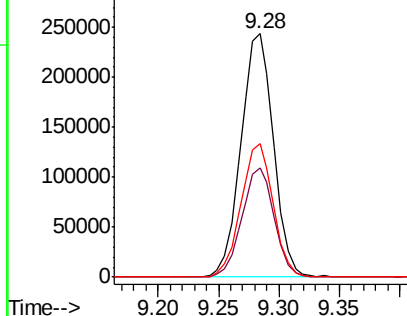

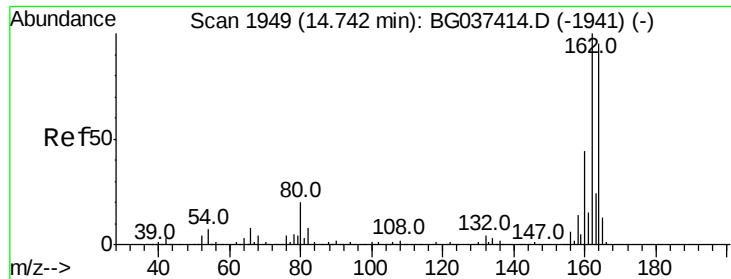

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.74 min Scan# 1948

Delta R.T. -0.01 min

Lab File: BG037509.D

Acq: 24 Oct 2018 13:32

Instrument :

BNA_G

ClientSampleId :

101918-TIPC-E-D-M


Tot Ion:164 Resp: 178651

Ion Ratio Lower Upper

164 100

162 105.5 81.3 121.9




160 46.6 36.3 54.5

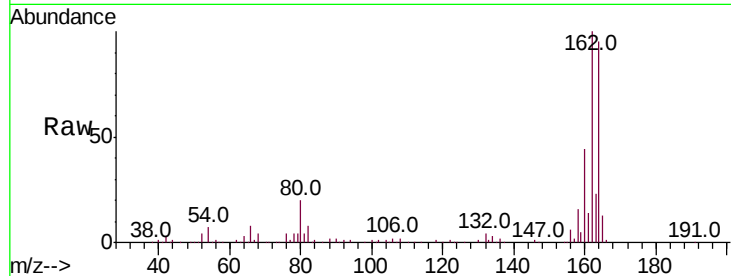

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

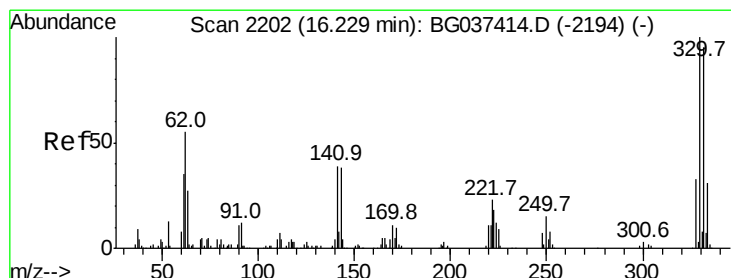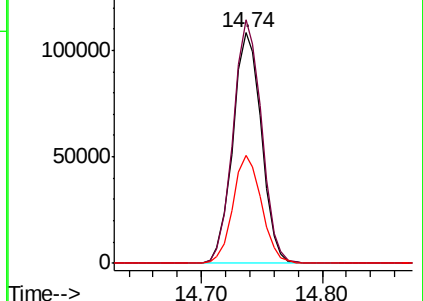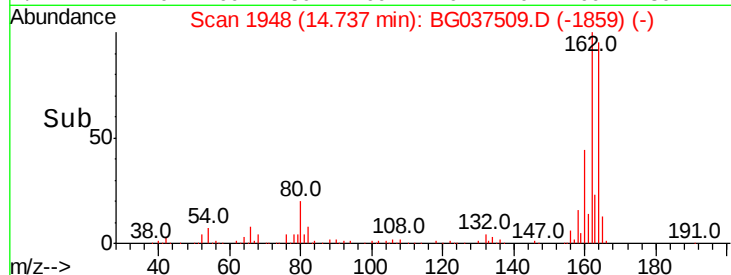

#42

2,4,6-Tribromophenol

Concen: 100.477 ng

RT: 16.22 min Scan# 2201

Delta R.T. -0.01 min

Lab File: BG037509.D

Acq: 24 Oct 2018 13:32


Tgt Ion:330 Resp: 195783

Ion Ratio Lower Upper

330 100

332 94.1 78.4 117.6



141 39.5 32.2 48.2

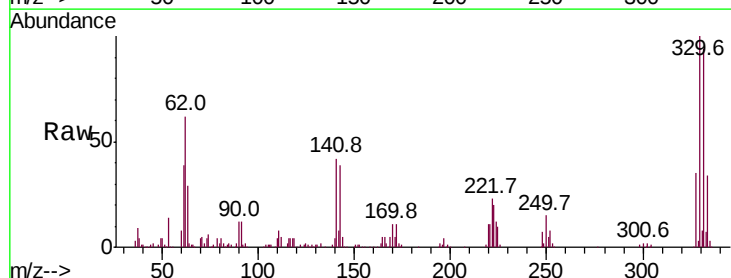

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



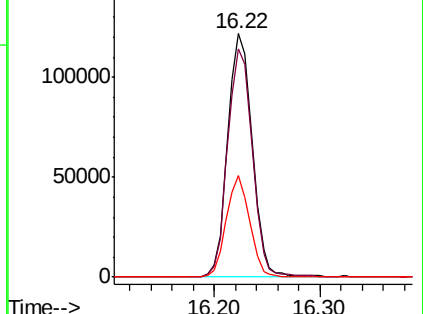
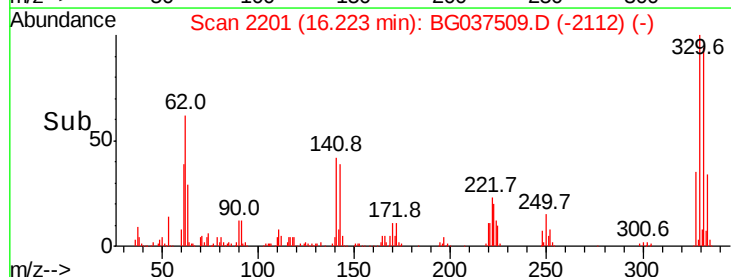




#45
2-Fluorobiphenyl
Concen: 95.761 ng
RT: 13.36 min Scan# 1714
Delta R.T. -0.01 min
Lab File: BG037509.D
Acq: 24 Oct 2018 13:32




Instrument :
BNA_G
ClientSampleId :
101918-TIPC-E-D-M


Tot Ion:172 Resp: 1134513
Ion Ratio Lower Upper
172 100
171 38.5 31.0 46.4
170 25.6 20.2 30.2

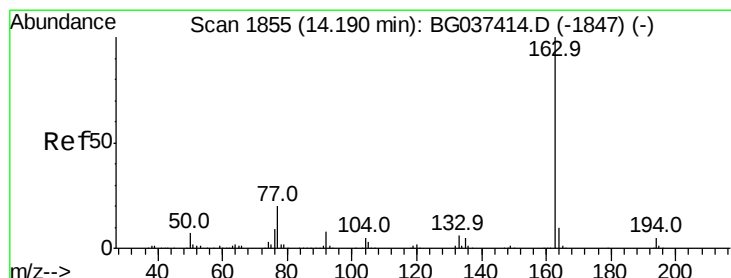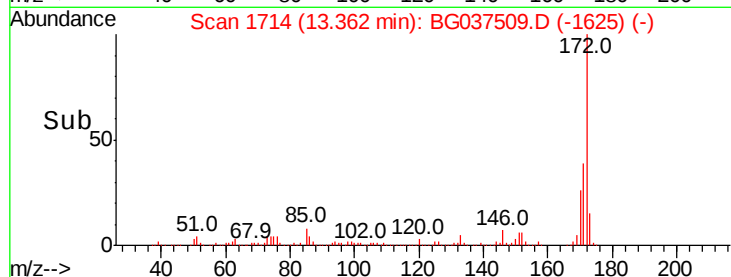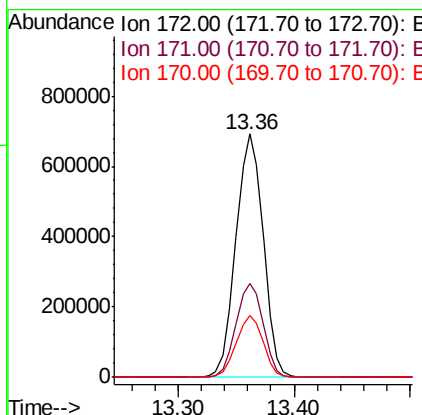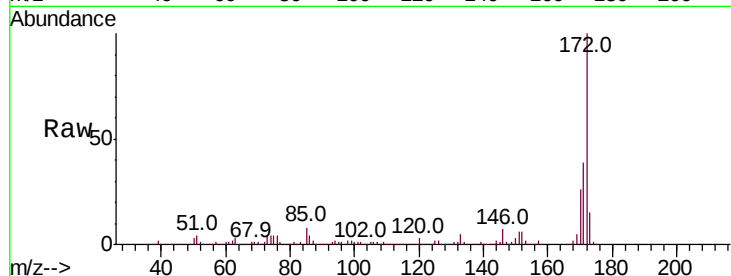

#50
Dimethylphthalate
Concen: 3.059 ng
RT: 14.18 min Scan# 1854
Delta R.T. -0.01 min
Lab File: BG037509.D
Acq: 24 Oct 2018 13:32

Tgt Ion:163 Resp: 42272
Ion Ratio Lower Upper
163 100
194 4.0 3.5 5.3
164 11.7 8.5 12.7

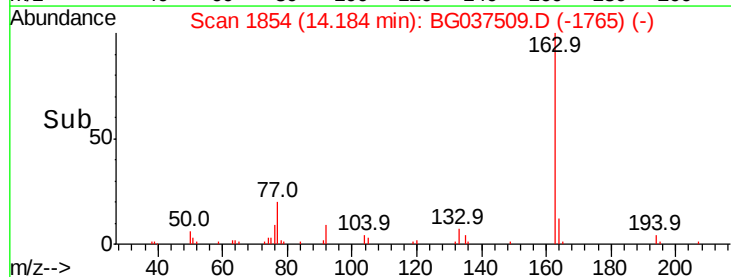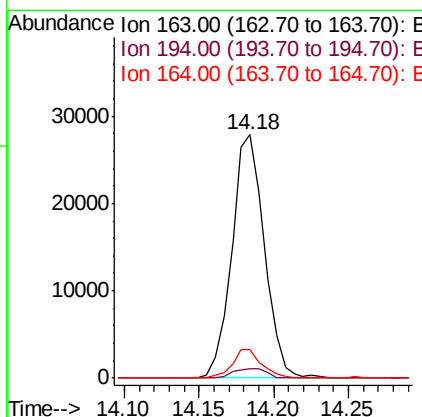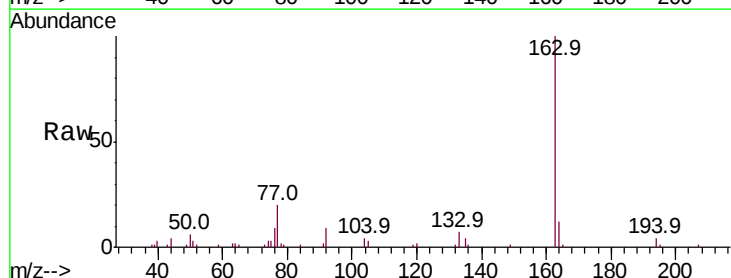

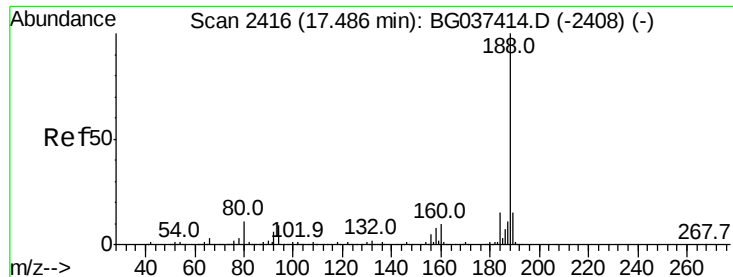

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.49 min Scan# 2416

Delta R.T. 0.00 min

Lab File: BG037509.D

Acq: 24 Oct 2018 13:32

Instrument :

BNA_G

ClientSampleId :

101918-TIPC-E-D-M


Tot Ion:188 Resp: 427749

Ion Ratio Lower Upper

188 100

94 8.9 7.2 10.8




80 9.9 7.7 11.5

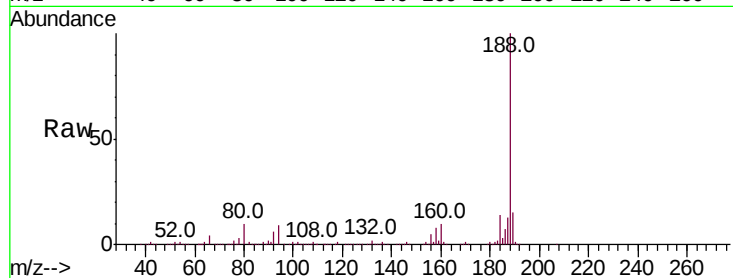

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

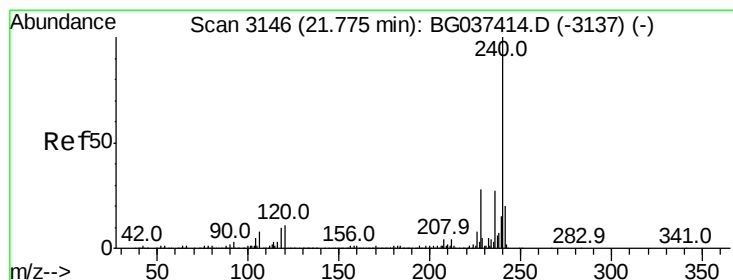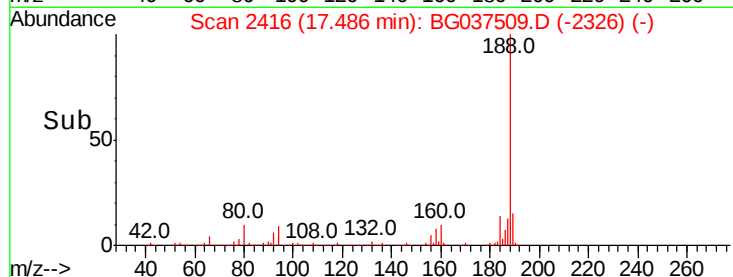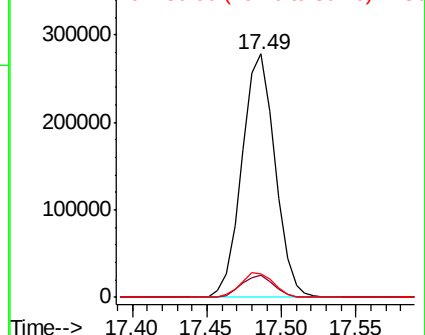

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.77 min Scan# 3145

Delta R.T. -0.01 min

Lab File: BG037509.D

Acq: 24 Oct 2018 13:32


Tgt Ion:240 Resp: 391414

Ion Ratio Lower Upper

240 100

120 10.5 8.1 12.1



236 26.7 21.4 32.0

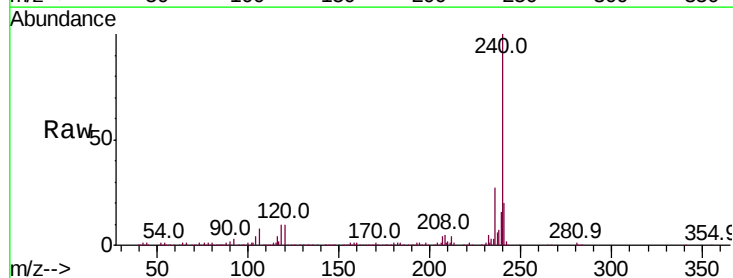


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

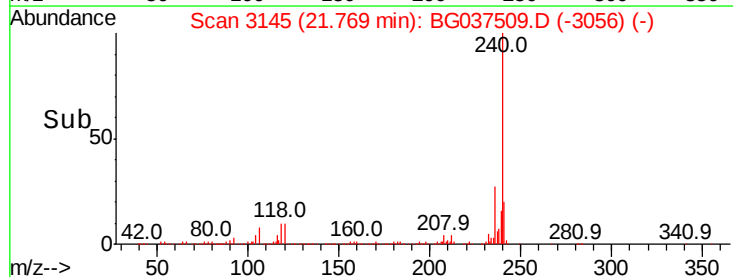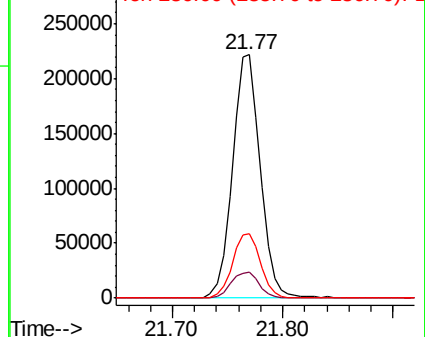

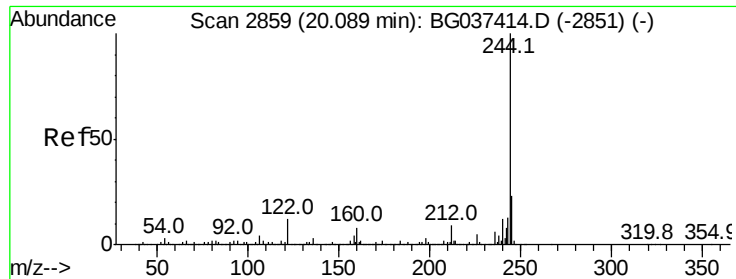

#79

Terphenyl-d14

Concen: 80.966 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BG037509.D

Acq: 24 Oct 2018 13:32

Instrument :

BNA_G

ClientSampleId :

101918-TIPC-E-D-M


Tot Ion:244 Resp: 1483138

Ion Ratio Lower Upper

244 100

212 8.9 6.5 9.7




122 12.5 9.0 13.4

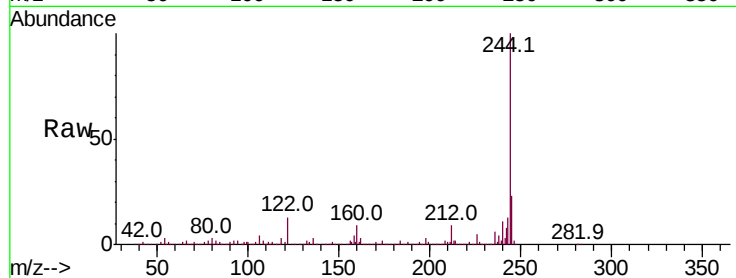

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

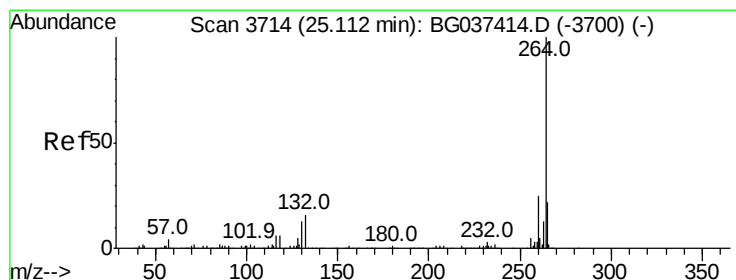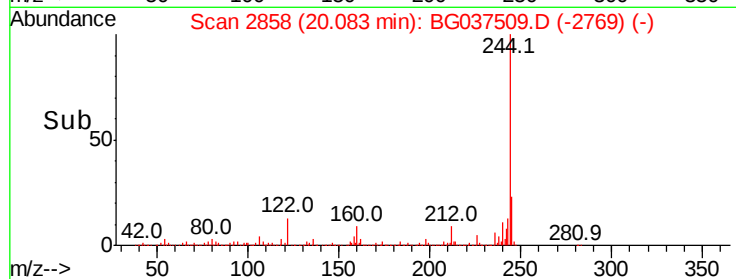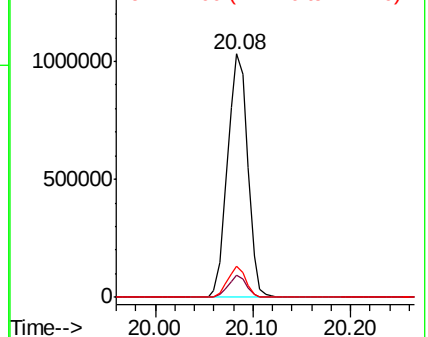

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.10 min Scan# 3712

Delta R.T. -0.01 min

Lab File: BG037509.D

Acq: 24 Oct 2018 13:32


Tgt Ion:264 Resp: 394693

Ion Ratio Lower Upper

264 100

260 24.9 18.2 27.4

265 22.2 17.9 26.9

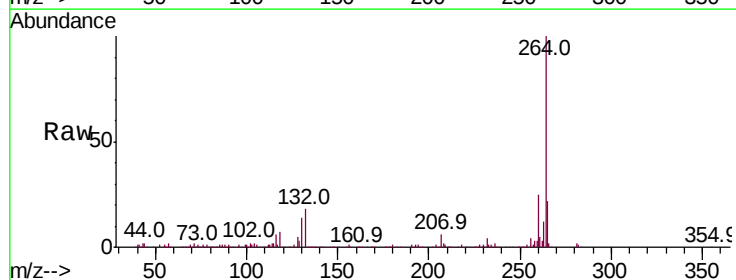

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

