


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102318\
 Data File : BG037474.D
 Acq On : 23 Oct 2018 12:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

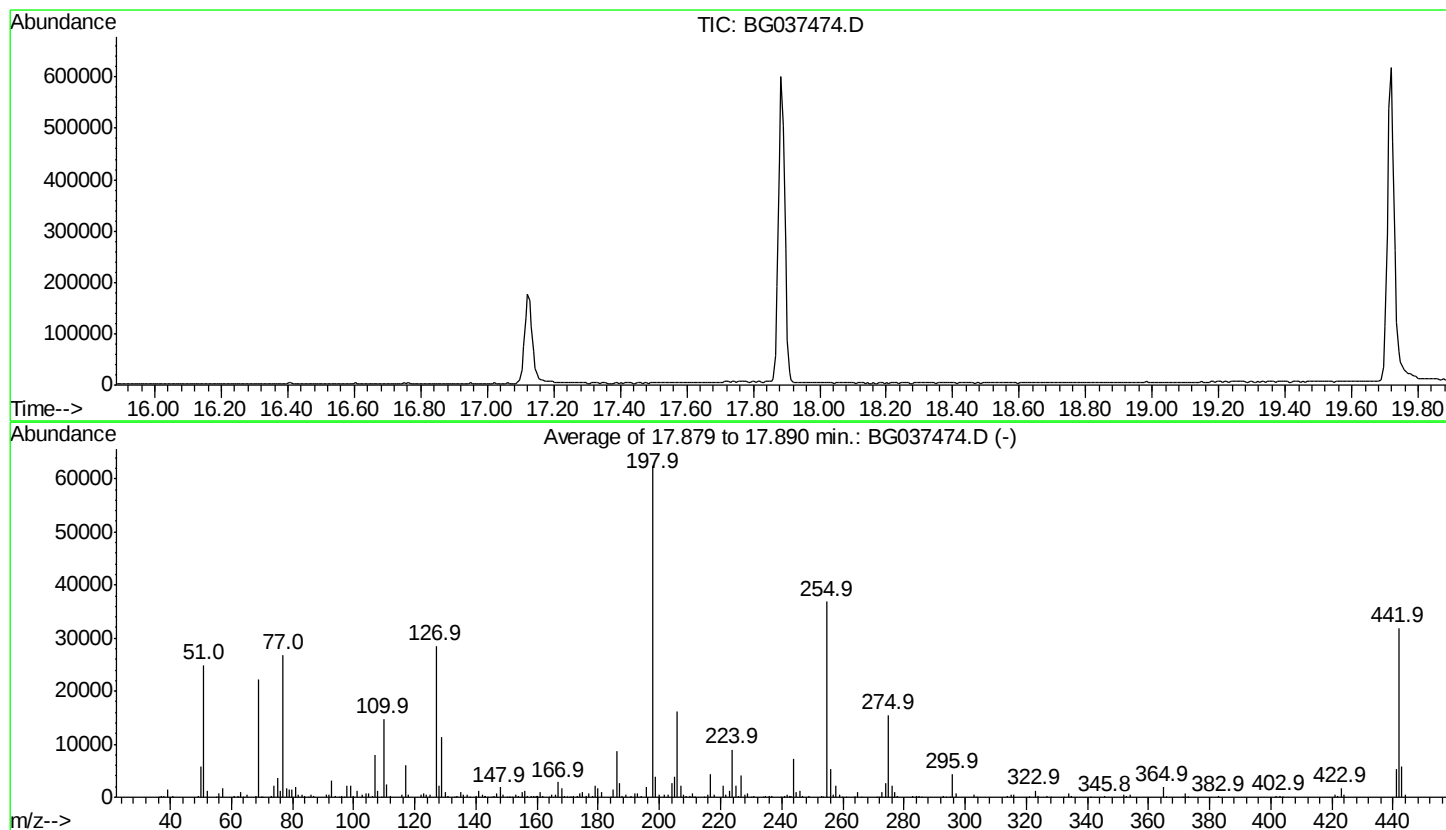

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	24944	PASS
68	69	0.00	2	1.3	289	PASS
69	198	0.00	100	35.6	22248	PASS
70	69	0.00	2	0.4	85	PASS
127	198	10	80	45.7	28570	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62496	PASS
199	198	5	9	6.1	3796	PASS
275	198	10	60	24.8	15519	PASS
365	198	1	100	3.1	1958	PASS
441	198	0.01	100	8.4	5224	PASS
442	198	50	100	51.1	31965	PASS
443	442	15	24	17.8	5705	PASS