


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102318\
 Data File : BG037492.D
 Acq On : 24 Oct 2018 2:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

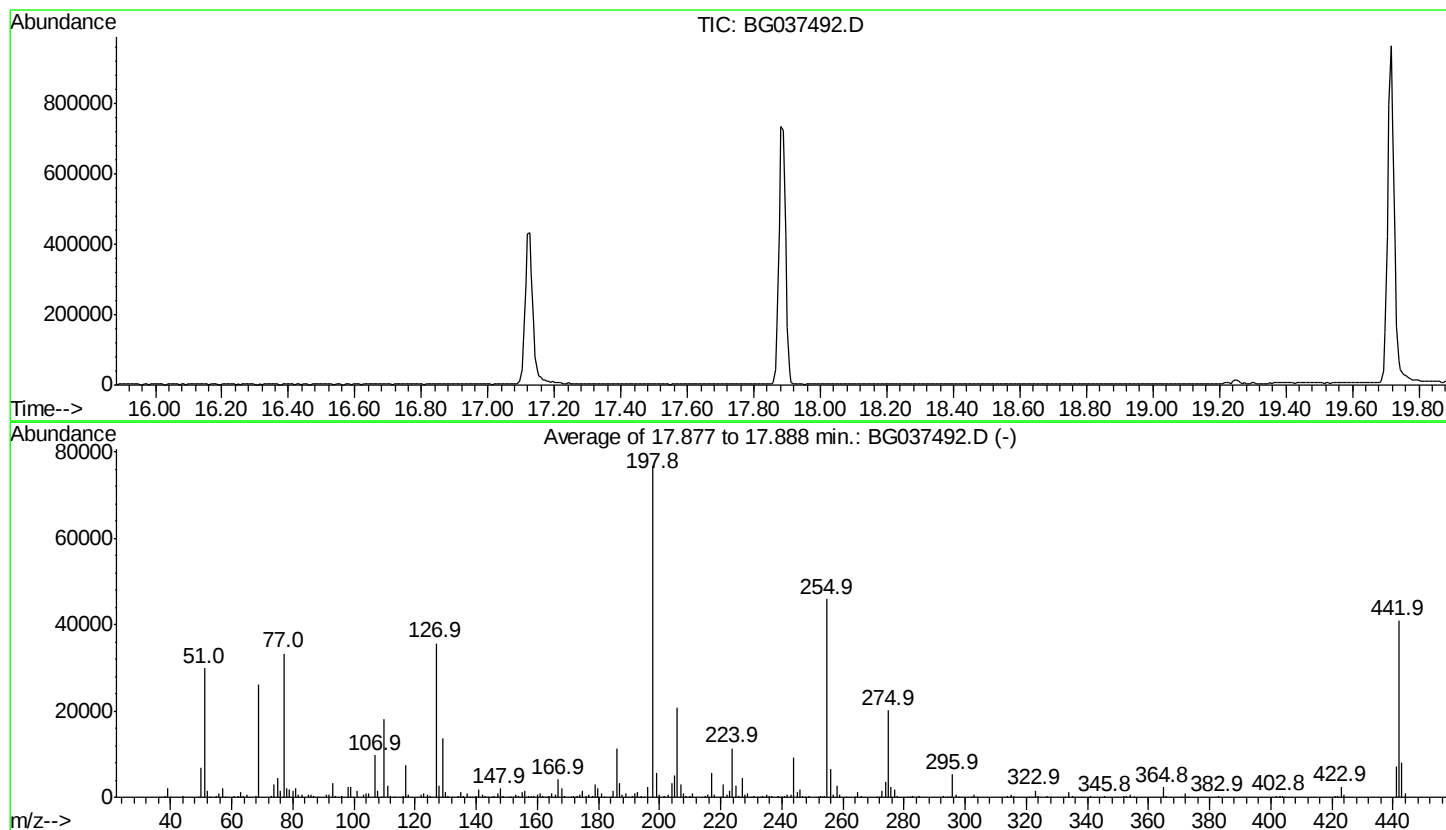

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	29829	PASS
68	69	0.00	2	1.0	255	PASS
69	198	0.00	100	34.0	26074	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.4	35629	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76768	PASS
199	198	5	9	7.4	5675	PASS
275	198	10	60	26.2	20125	PASS
365	198	1	100	2.9	2249	PASS
441	198	0.01	100	9.1	7024	PASS
442	198	50	100	53.1	40789	PASS
443	442	15	24	19.3	7892	PASS