

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102319\
 Data File : BG043310.D
 Acq On : 23 Oct 2019 16:06
 Operator : JU
 Sample : PB124203BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB124203BL

Quant Time: Oct 24 06:54:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 21 16:37:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	34994	20.00	ng	0.00
21) Naphthalene-d8	10.84	136	109685	20.00	ng	0.00
39) Acenaphthene-d10	14.65	164	90482	20.00	ng	0.00
64) Phenanthrene-d10	17.40	188	229554	20.00	ng	0.00
76) Chrysene-d12	21.67	240	308762	20.00	ng	0.00
87) Perylene-d12	24.87	264	347203	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	222888	116.71	ng	0.00
7) Phenol-d6	7.20	99	317783	115.66	ng	0.00
23) Nitrobenzene-d5	9.19	82	182489	85.77	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	210066	122.00	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	529350	80.84	ng	0.00
79) Terphenyl-d14	20.01	244	1332173	80.94	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102319\
Data File : BG043310.D
Acq On : 23 Oct 2019 16:06
Operator : JU
Sample : PB124203BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124203BL

Quant Time: Oct 24 06:54:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

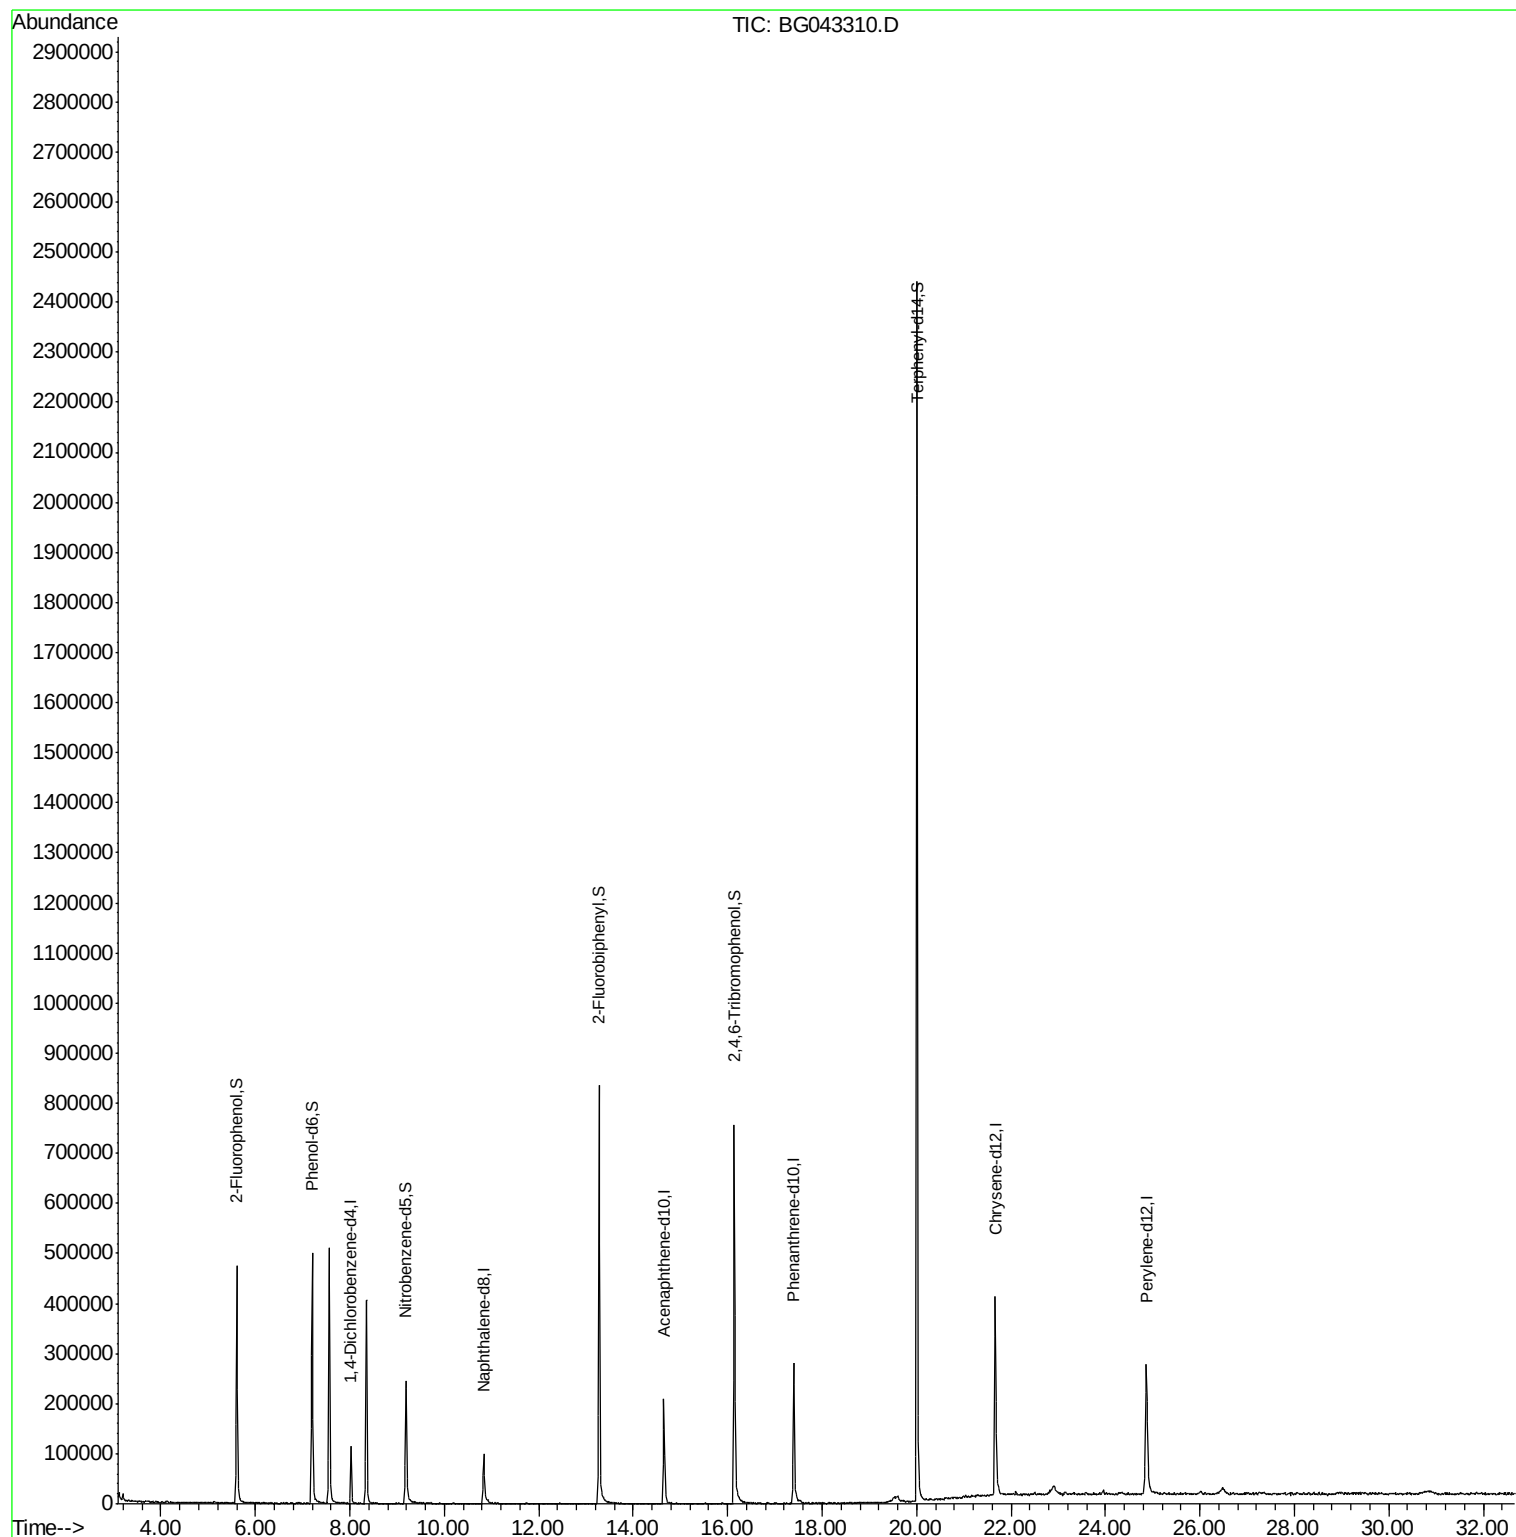




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.02 min Scan# 840
Delta R.T. -0.00 min
Lab File: BG043310.D
Acq: 23 Oct 2019 16:06

Instrument :
BNA_G
ClientSampleId :
PB124203BL

Tot Ion	152	Resp	34994
Ion	Ratio	Lower	Upper
152	100		
150	147.2	113.6	170.4
115	61.0	45.9	68.9



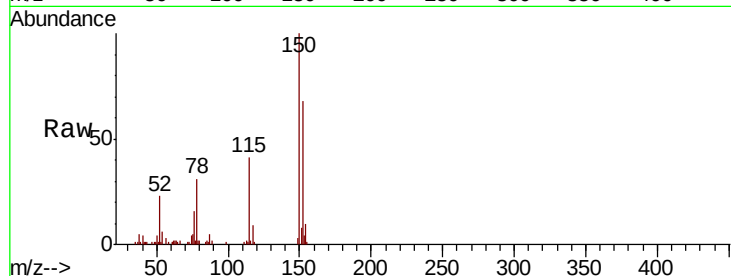


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

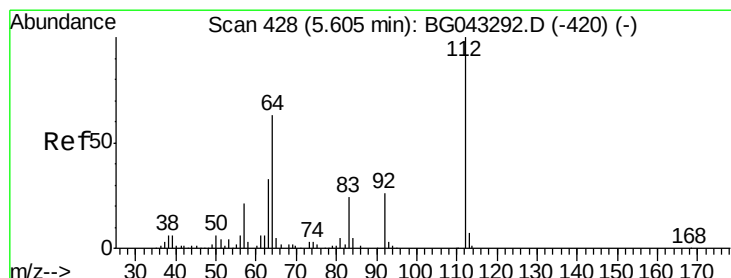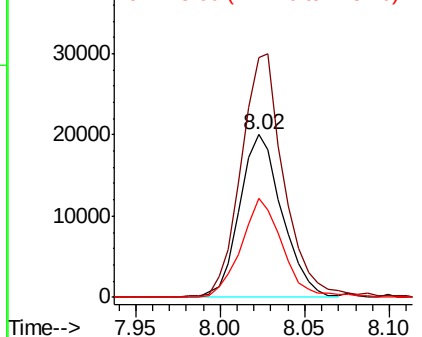

#5

2-Fluorophenol
Concen: 116.714 ng
RT: 5.61 min Scan# 429
Delta R.T. 0.00 min
Lab File: BG043310.D
Acq: 23 Oct 2019 16:06

Tgt Ion	112	Resp	222888
Ion	Ratio	Lower	Upper
112	100		
64	60.1	50.2	75.2
63	35.5	26.7	40.1


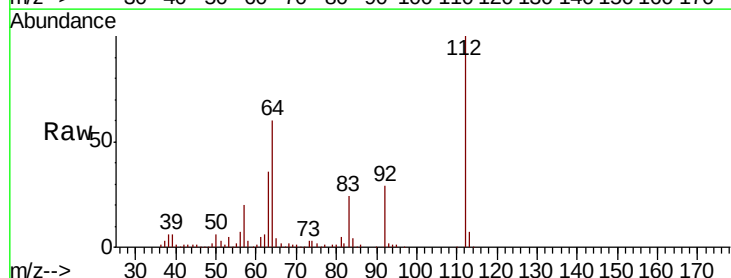



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

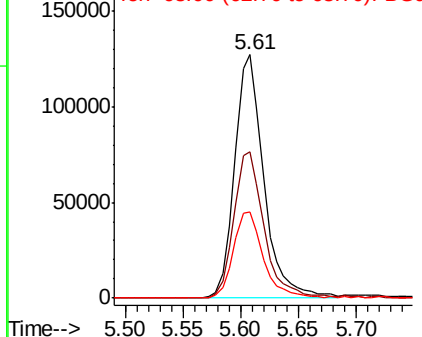



#7

Phenol-d6

Concen: 115.659 ng

RT: 7.20 min Scan# 700

Delta R.T. -0.00 min

Lab File: BG043310.D

Acq: 23 Oct 2019 16:06

Instrument :

BNA_G

ClientSampleId :

PB124203BL


Tot Ion: 99 Resp: 317783

Ion Ratio Lower Upper




99 100

42 18.4 14.9 22.3

71 41.4 32.2 48.2

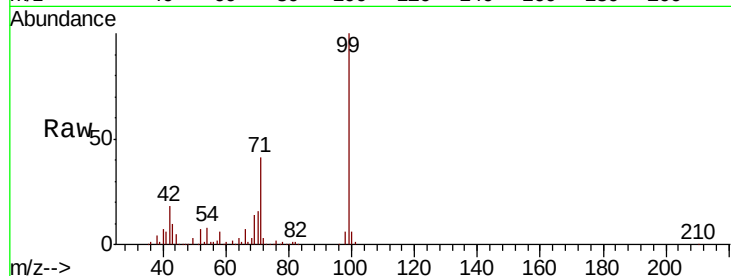

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

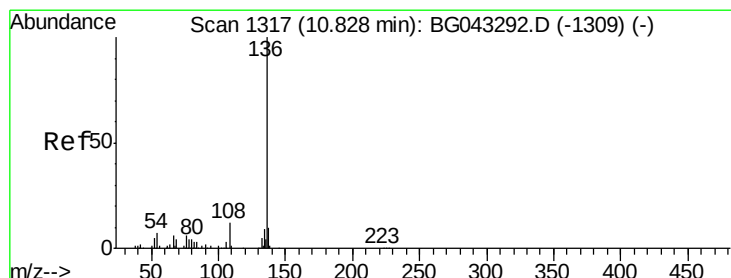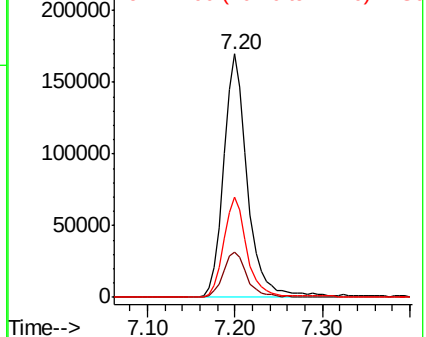

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.84 min Scan# 1319

Delta R.T. 0.01 min

Lab File: BG043310.D

Acq: 23 Oct 2019 16:06

Tgt Ion: 136 Resp: 109685


Ion Ratio Lower Upper

136 100



137 11.6 8.2 12.2


54 7.2 5.4 8.2

68 5.6 3.3 4.9#

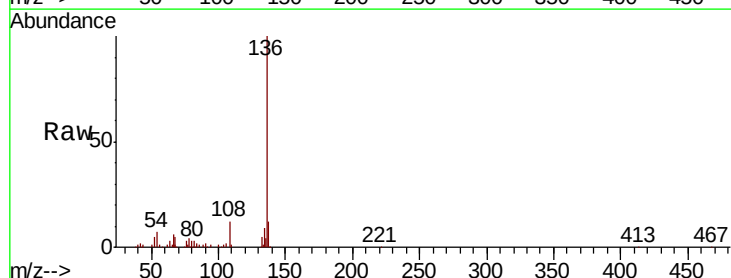

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




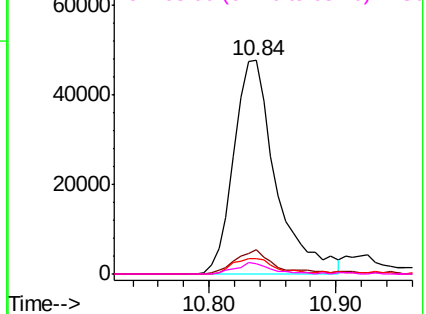




#23
Nitrobenzene-d5
Concen: 85.774 ng
RT: 9.19 min Scan# 1038
Delta R.T. -0.00 min
Lab File: BG043310.D
Acq: 23 Oct 2019 16:06




Instrument :
BNA_G
ClientSampled :
PB124203BL


Tot Ion	82	Resp	182489
Ion Ratio	100	Lower	Upper
128	40.4	35.3	52.9
54	52.3	42.3	63.5

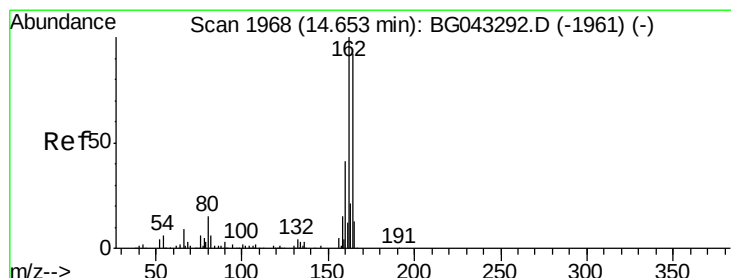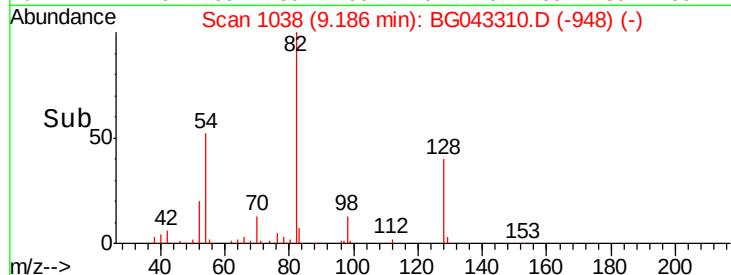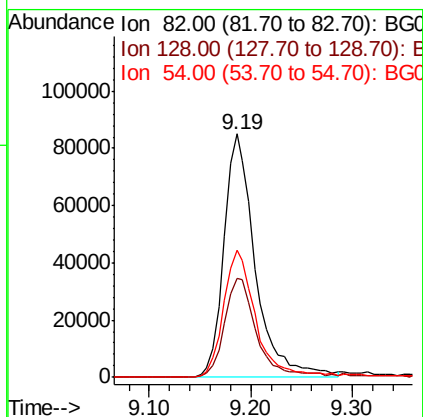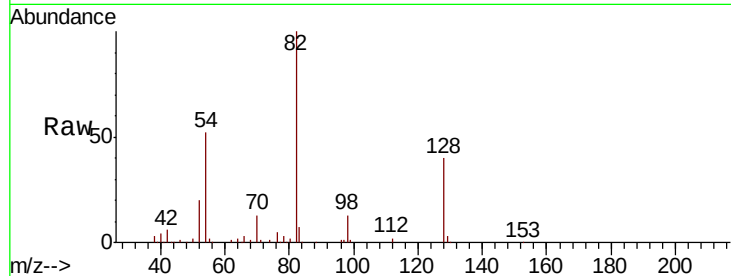

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.65 min Scan# 1968
Delta R.T. -0.00 min
Lab File: BG043310.D
Acq: 23 Oct 2019 16:06

Tgt Ion	164	Resp	90482
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
162	97.7	87.0	130.4
160	44.3	35.5	53.3

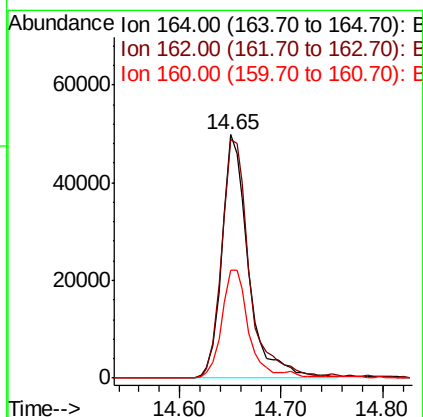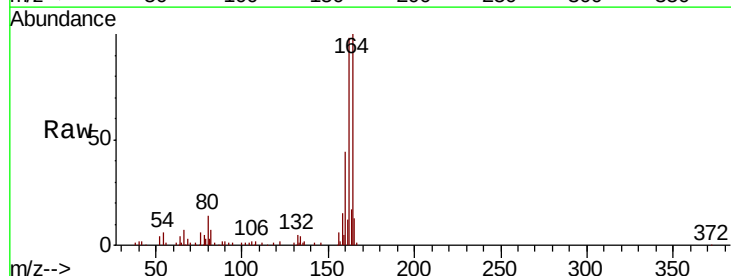







#42
 2,4,6-Tribromophenol
 Concen: 121.998 ng
 RT: 16.14 min Scan# 2222
 Delta R.T. -0.00 min
 Lab File: BG043310.D
 Acq: 23 Oct 2019 16:06

Instrument :
 BNA_G
 ClientSampleId :
 PB124203BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.1	76.4	114.6
141	26.7	21.4	32.0

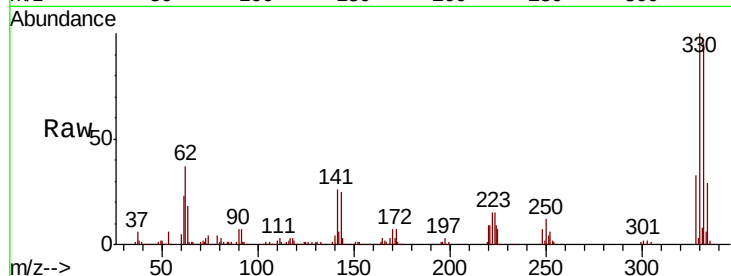


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

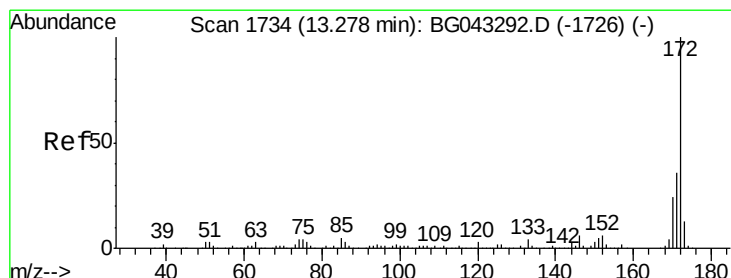
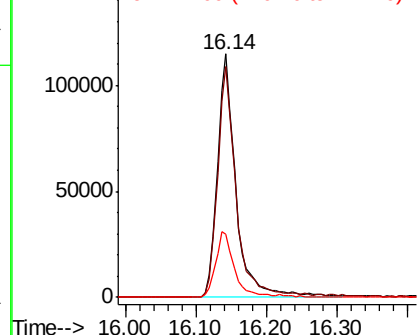



#45
 2-Fluorobiphenyl
 Concen: 80.840 ng
 RT: 13.28 min Scan# 1734
 Delta R.T. -0.00 min
 Lab File: BG043310.D
 Acq: 23 Oct 2019 16:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.1	28.5	42.7
170	22.0	18.8	28.2

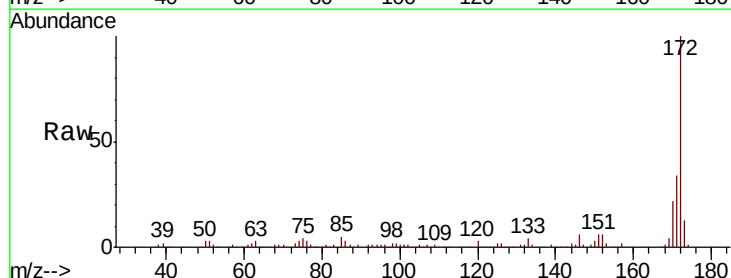

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

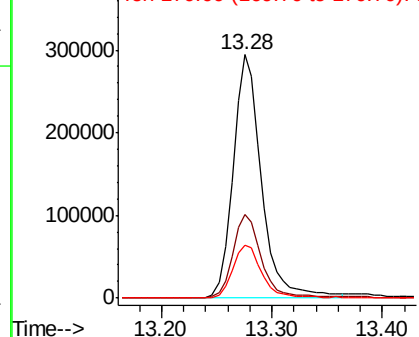

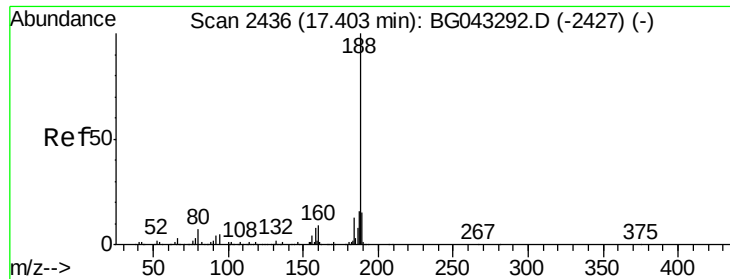

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.40 min Scan# 2436

Delta R.T. -0.00 min

Lab File: BG043310.D

Acq: 23 Oct 2019 16:06

Instrument :

BNA_G

ClientSampleId :

PB124203BL


Tot Ion:188 Resp: 229554

Ion Ratio Lower Upper

188 100

94 6.0 4.2 6.2




80 7.0 5.2 7.8

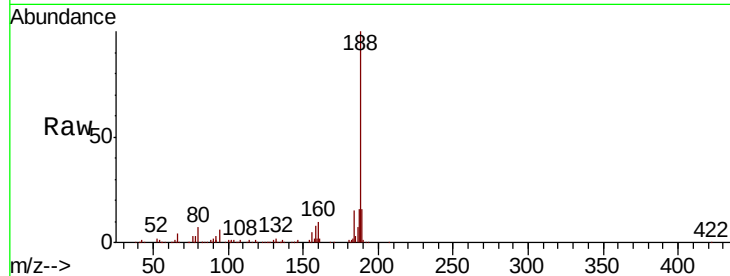

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

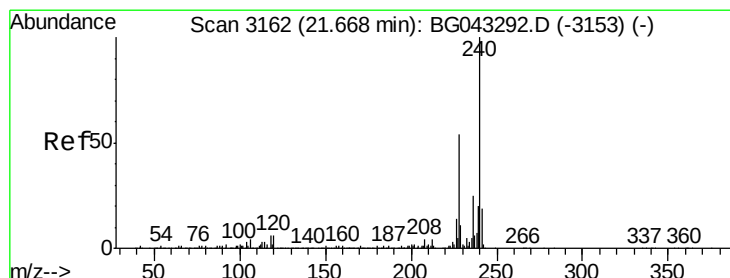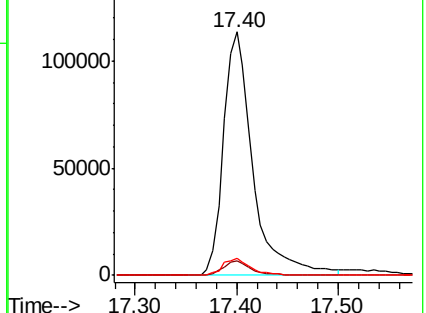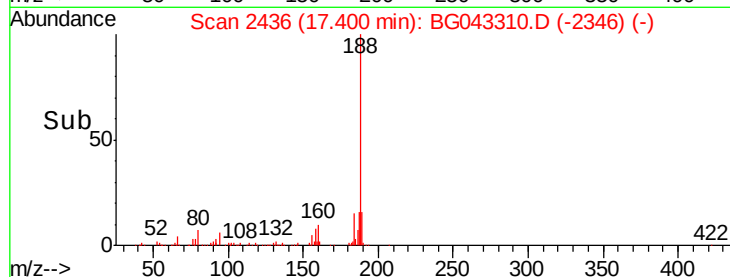

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.67 min Scan# 3162

Delta R.T. -0.00 min

Lab File: BG043310.D

Acq: 23 Oct 2019 16:06


Tgt Ion:240 Resp: 308762

Ion Ratio Lower Upper

240 100

120 5.5 4.6 7.0



236 26.4 20.2 30.4

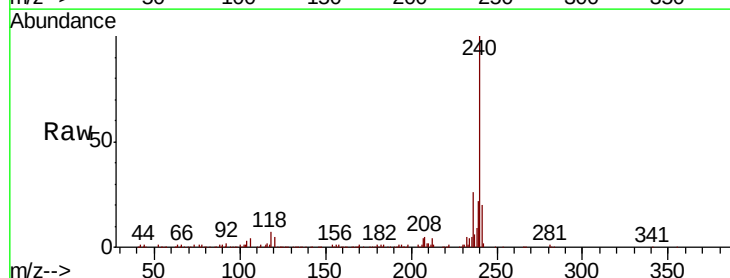


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

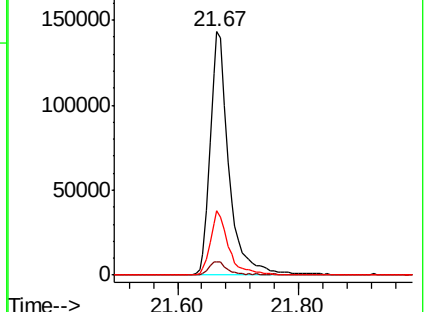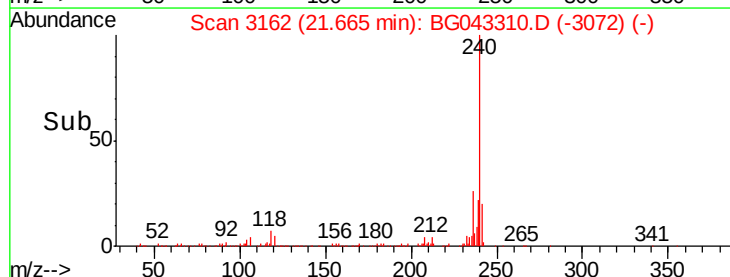



#79

Terphenyl-d14

Concen: 80.944 ng

RT: 20.01 min Scan# 2880

Delta R.T. -0.00 min

Lab File: BG043310.D

Acq: 23 Oct 2019 16:06

Instrument :

BNA_G

ClientSampleId :

PB124203BL


Tot Ion:244 Resp: 1332173

Ion Ratio Lower Upper

244 100

212 7.2 6.4 9.6




122 7.1 5.3 7.9

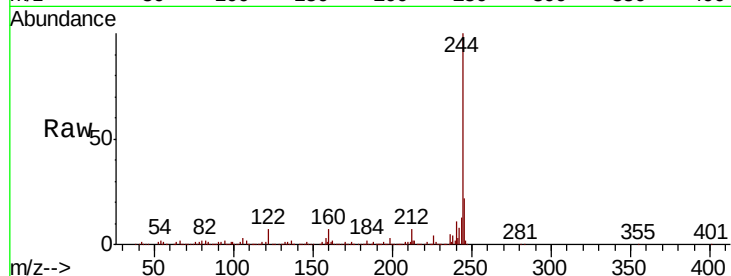

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

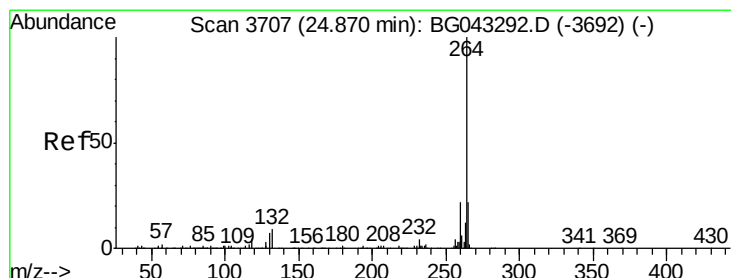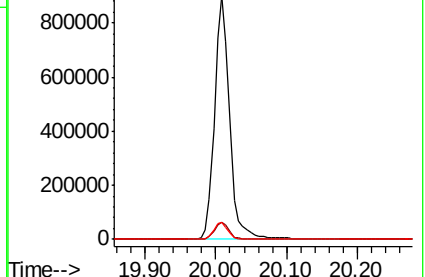

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.87 min Scan# 3708

Delta R.T. 0.00 min

Lab File: BG043310.D

Acq: 23 Oct 2019 16:06


Tgt Ion:264 Resp: 347203

Ion Ratio Lower Upper

264 100

260 22.4 17.9 26.9

265 21.1 17.4 26.2

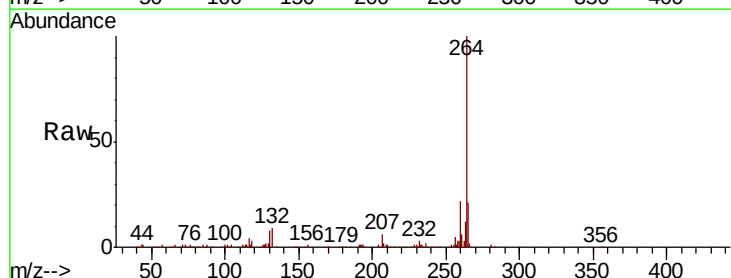

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

