
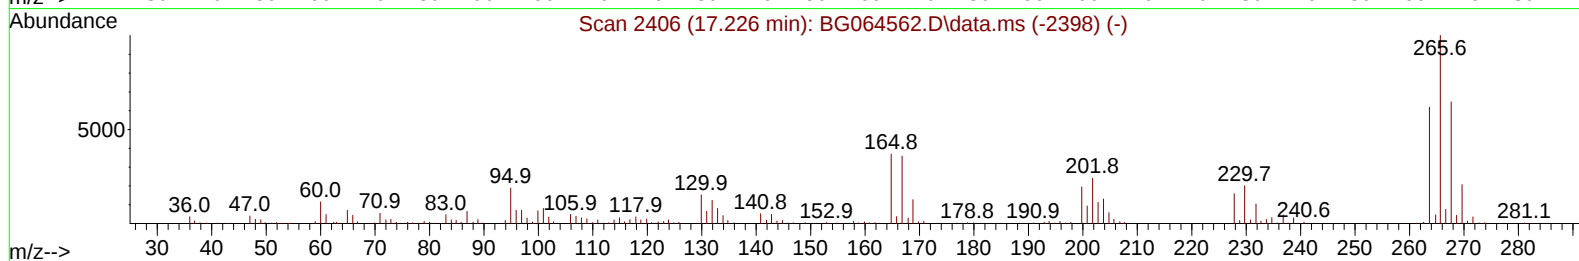
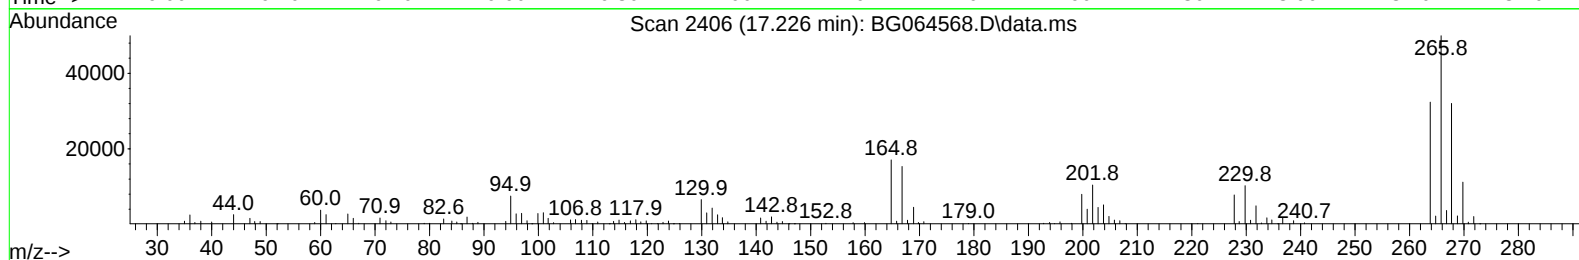


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102425\
Data File : BG064568.D
Acq On : 24 Oct 2025 8:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 12:18:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 12:16:12 2025
Response via : Initial Calibration

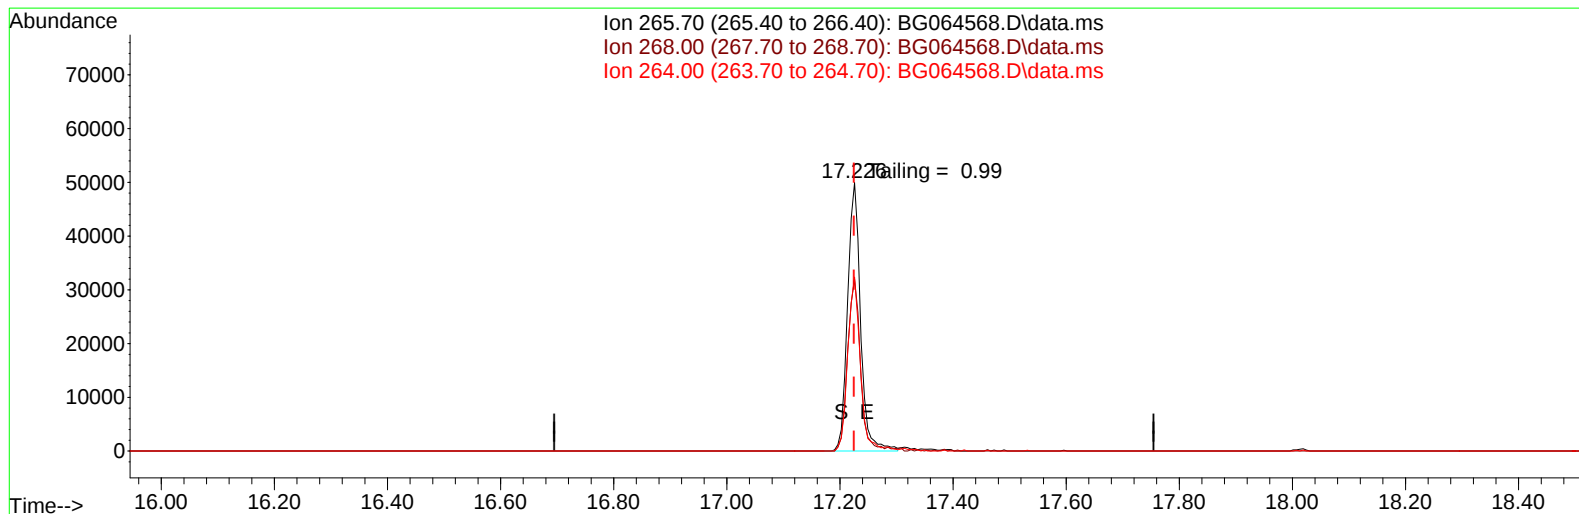

TIC: BG064568.D\data.ms

(70) Pentachlorophenol (C)




17.226min (+ 0.001) 15878.32 ng

response 79720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.10	64.11
264.00	61.90	64.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102425\
Data File : BG064568.D
Acq On : 24 Oct 2025 8:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 12:18:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 12:16:12 2025
Response via : Initial Calibration

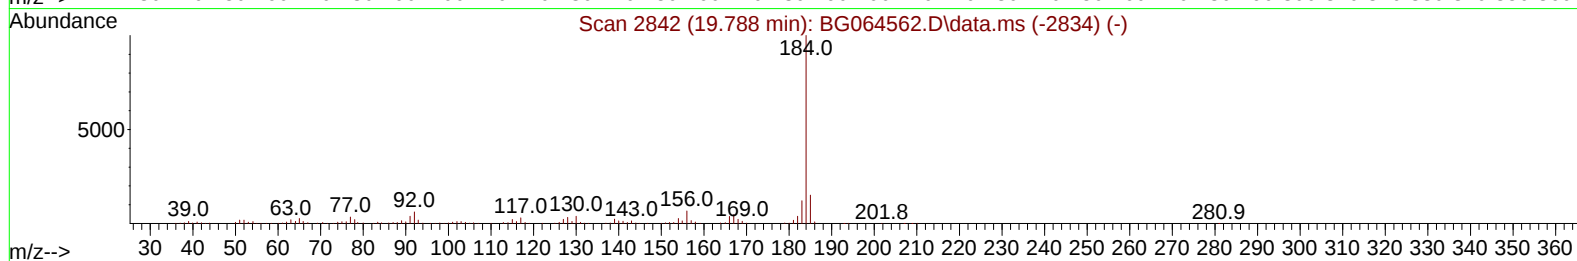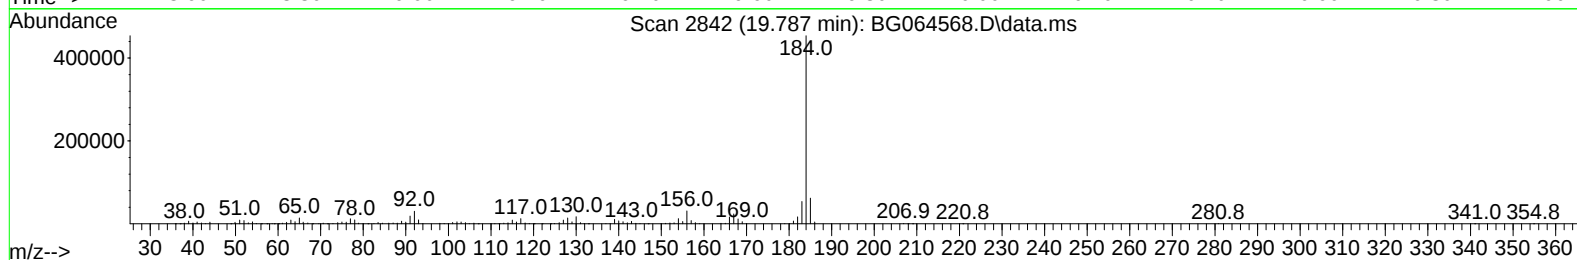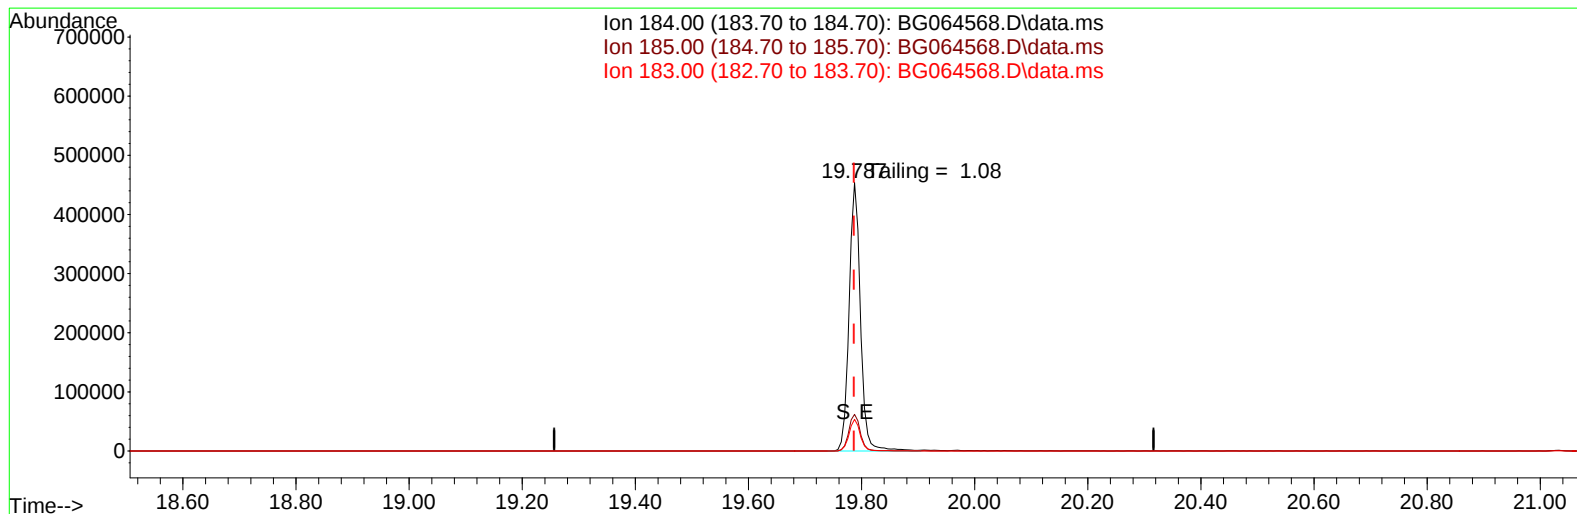

TIC: BG064568.D\data.ms

(77) Benzidine

19.787min (+ 0.001) 0.00 ng

response 632825

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.68
183.00	12.10	11.84
0.00	0.00	0.00