

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102518\
 Data File : BG037571.D
 Acq On : 26 Oct 2018 8:42
 Operator : JU/SJ
 Sample : J5655-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 S37-0002

Quant Time: Oct 26 13:38:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	57782	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	258903	20.00	ng	0.00
39) Acenaphthene-d10	14.73	164	172905	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	413427	20.00	ng	0.00
76) Chrysene-d12	21.77	240	374037	20.00	ng	0.00
87) Perylene-d12	25.10	264	380590	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	192839	55.80	ng	0.00
7) Phenol-d6	7.24	99	177957	34.05	ng	0.00
23) Nitrobenzene-d5	9.28	82	372222	80.54	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	232437	123.25	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	903435	78.79	ng	0.00
79) Terphenyl-d14	20.08	244	1245733	71.17	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.18	163	129650	9.693	ng	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102518\
Data File : BG037571.D
Acq On : 26 Oct 2018 8:42
Operator : JU/SJ
Sample : J5655-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S37-0002

Quant Time: Oct 26 13:38:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

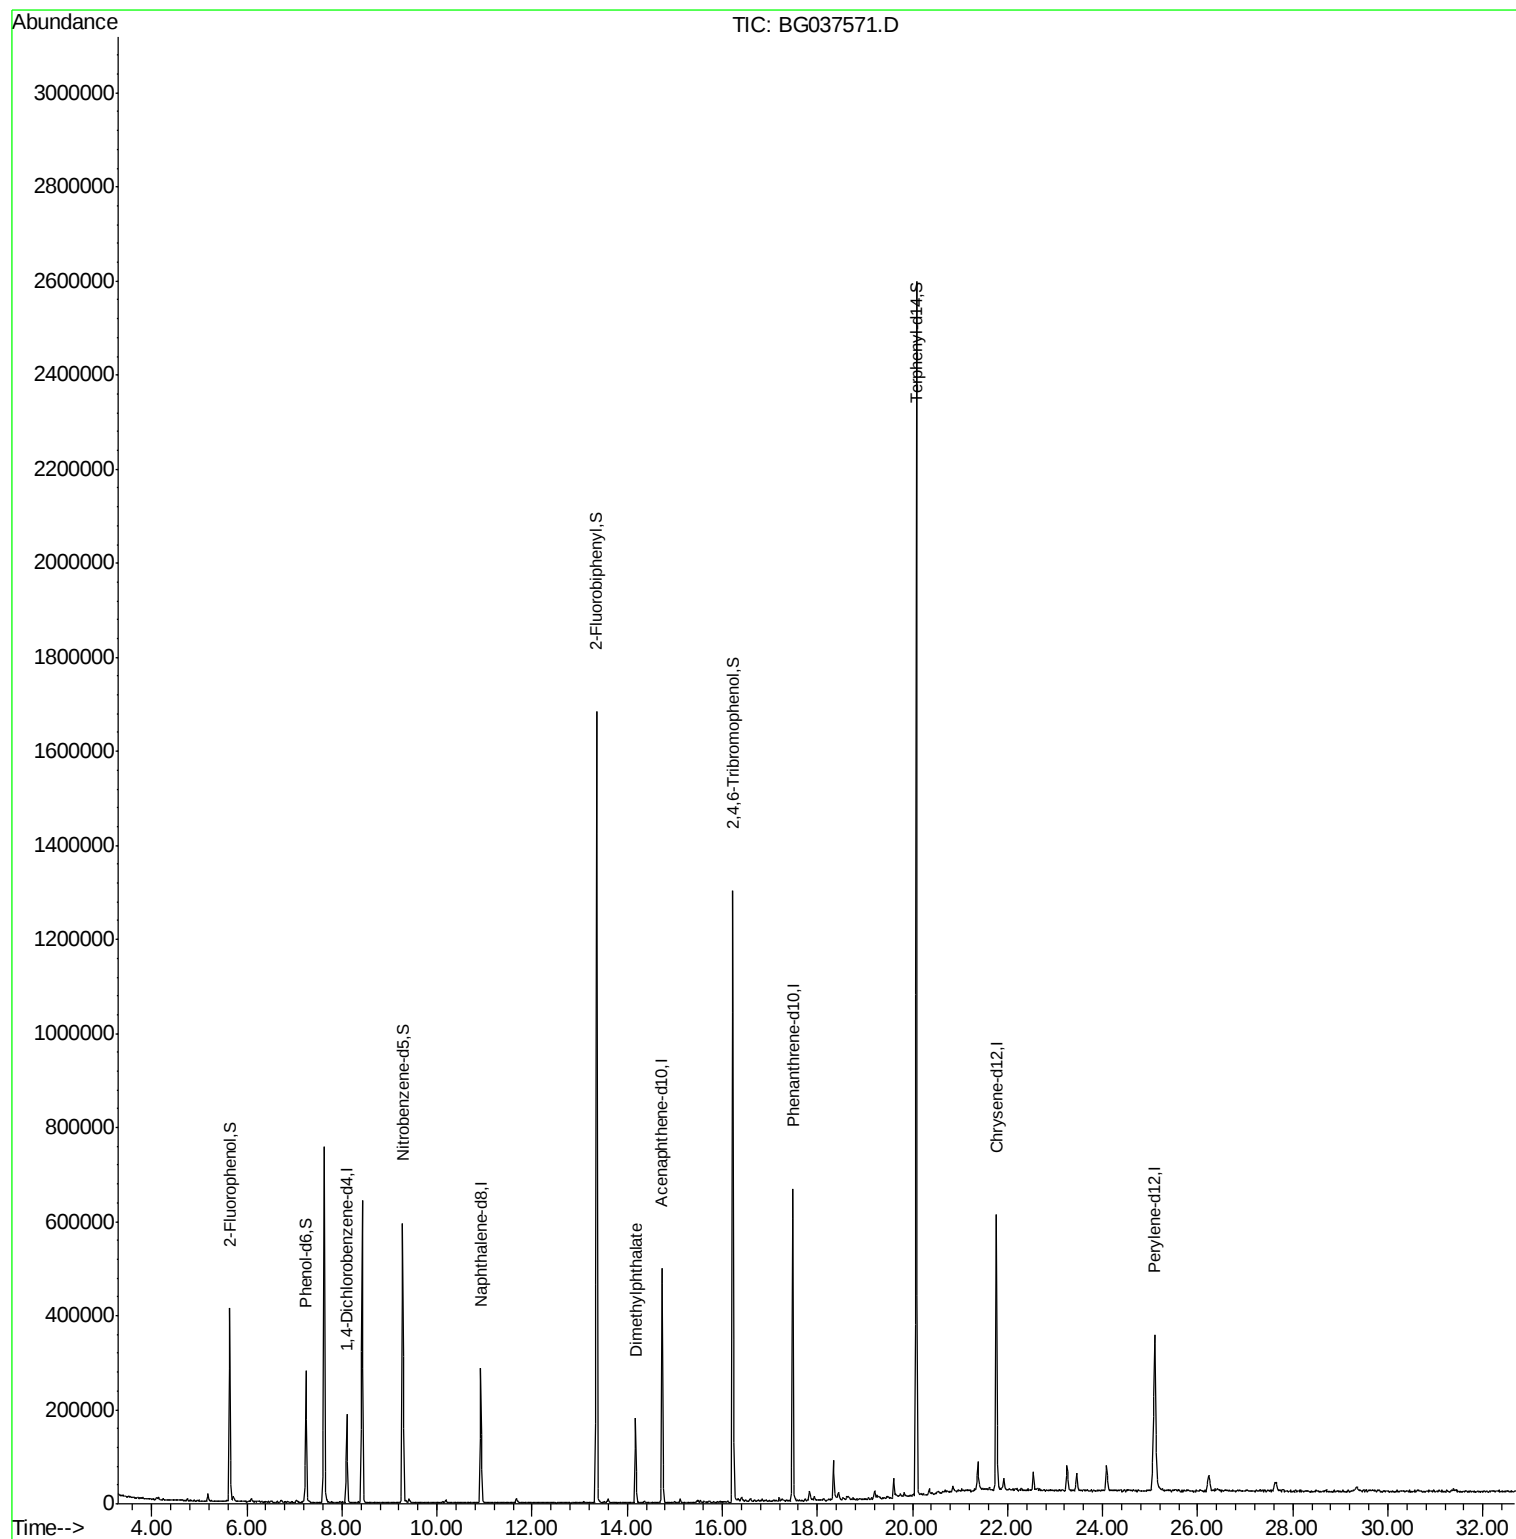




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 819
Delta R.T. -0.01 min
Lab File: BG037571.D
Acq: 26 Oct 2018 8:42

Instrument :
BNA_G
ClientSampleId :
S37-0002

Tot Ion:152 Resp: 57782
Ion Ratio Lower Upper
152 100
150 153.3 126.0 189.0
115 54.3 45.5 68.3

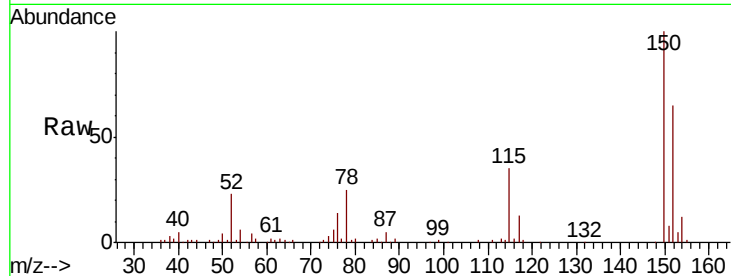


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

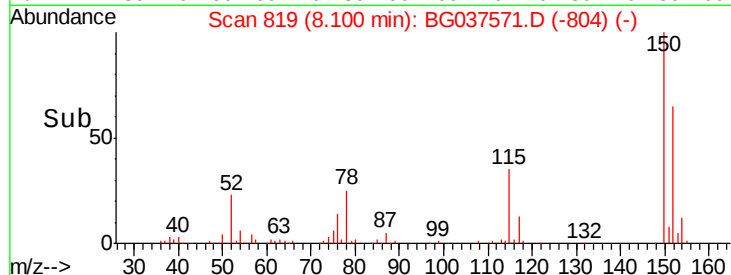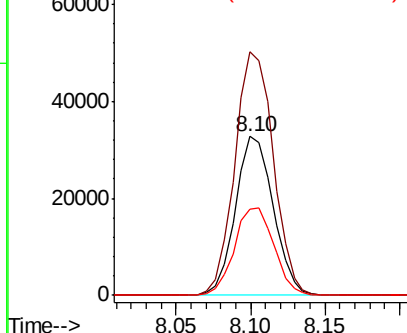



#5

2-Fluorophenol
Concen: 55.796 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG037571.D
Acq: 26 Oct 2018 8:42

Tgt Ion:112 Resp: 192839
Ion Ratio Lower Upper
112 100
64 64.2 53.1 79.7
63 32.7 27.3 40.9

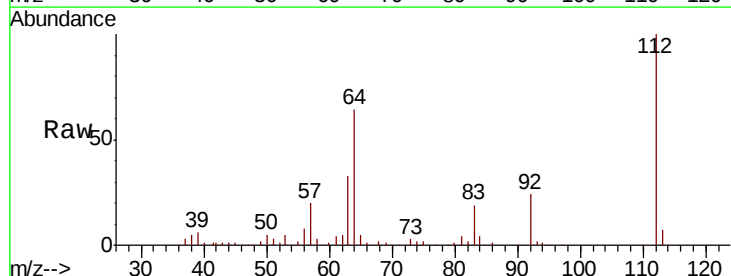

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

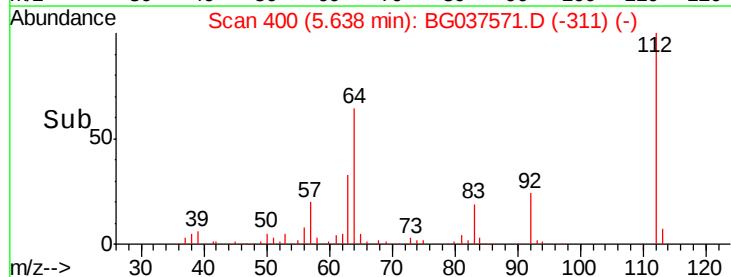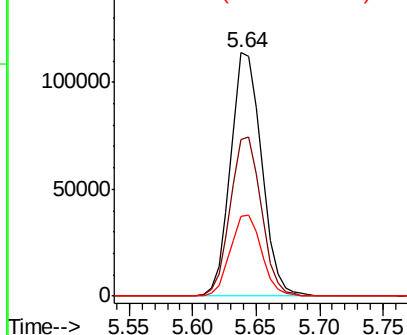



#7

Phenol-d6

Concen: 34.051 ng

RT: 7.24 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037571.D

Acq: 26 Oct 2018 8:42

Instrument :

BNA_G

ClientSampled :

S37-0002


Tot Ion: 99 Resp: 177957

Ion Ratio Lower Upper




99 100

42 17.1 15.0 22.4

71 29.5 25.5 38.3

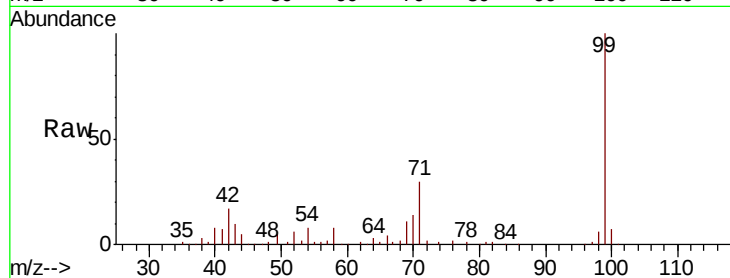

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

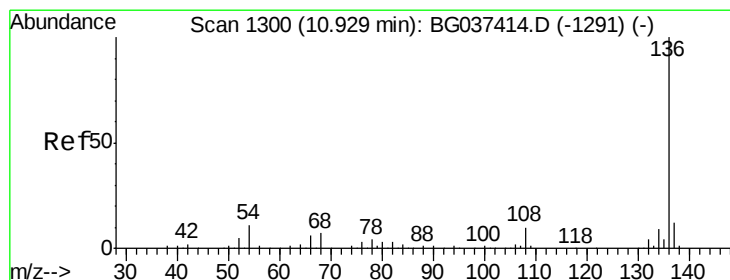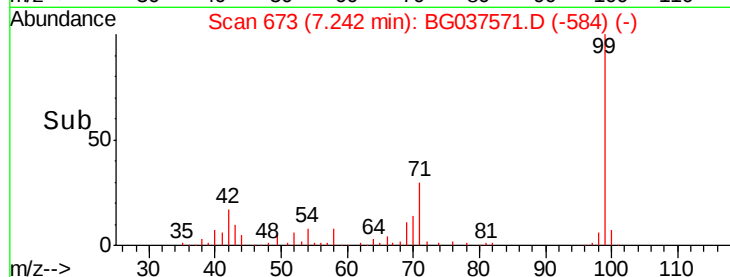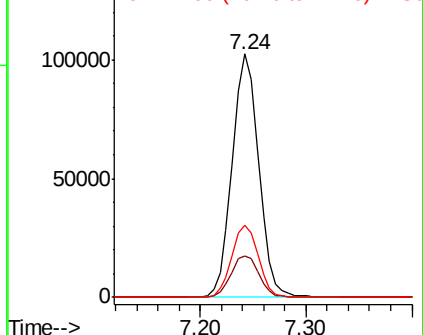

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.92 min Scan# 1299

Delta R.T. -0.01 min

Lab File: BG037571.D

Acq: 26 Oct 2018 8:42

Tgt Ion: 136 Resp: 258903


Ion Ratio Lower Upper

136 100



137 11.7 9.6 14.4


54 10.4 7.9 11.9

68 7.4 4.8 7.2#

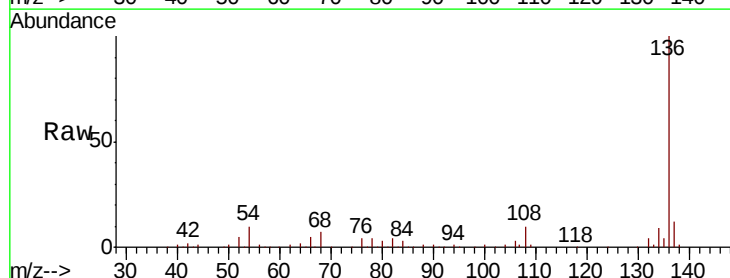

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

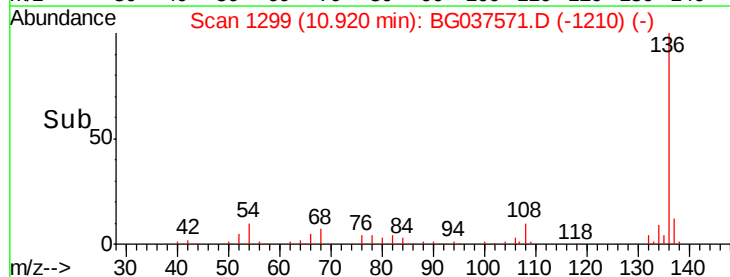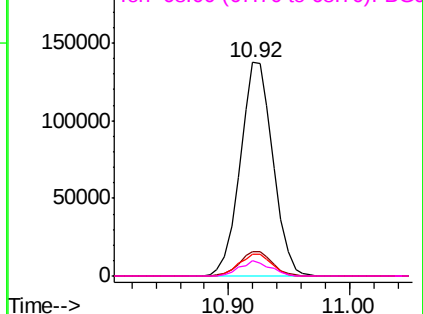


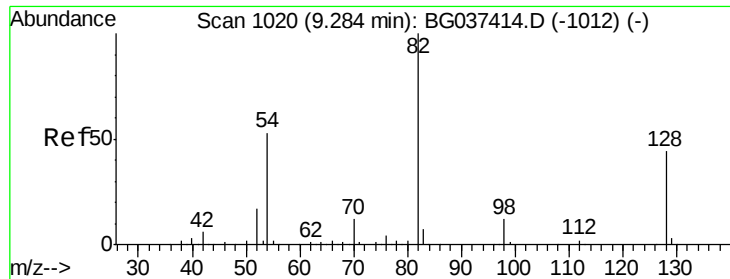




#23
Nitrobenzene-d5
Concen: 80.538 ng
RT: 9.28 min Scan# 1020
Delta R.T. -0.00 min
Lab File: BG037571.D
Acq: 26 Oct 2018 8:42

Instrument :
BNA_G
ClientSampled :
S37-0002

Tot Ion: 82 Resp: 372222
Ion Ratio Lower Upper
82 100
128 47.4 34.6 51.8
54 56.0 45.3 67.9

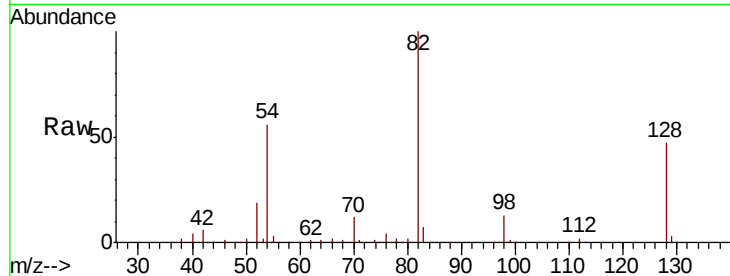


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

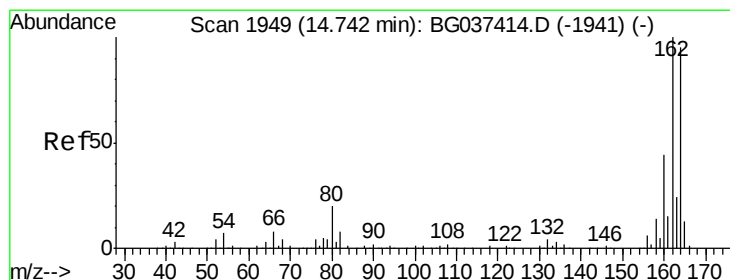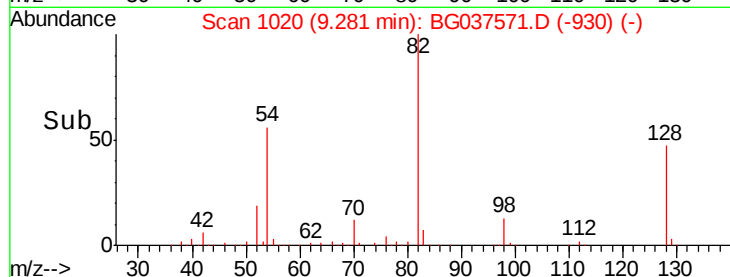
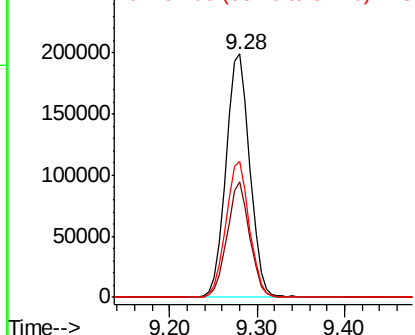



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.73 min Scan# 1948
Delta R.T. -0.01 min
Lab File: BG037571.D
Acq: 26 Oct 2018 8:42

Tgt Ion:164 Resp: 172905
Ion Ratio Lower Upper
164 100
162 103.5 81.3 121.9
160 47.9 36.3 54.5

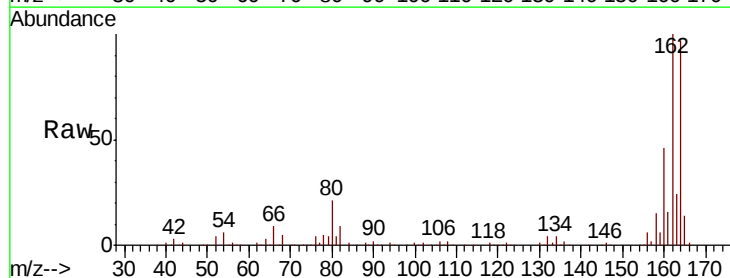

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

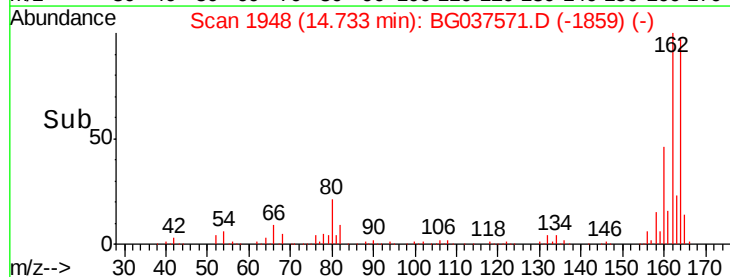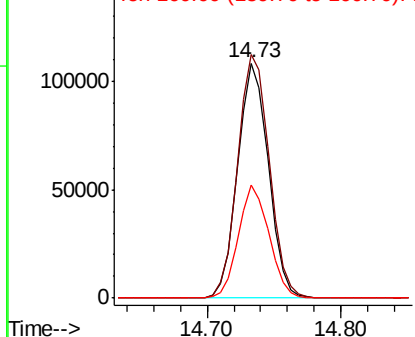

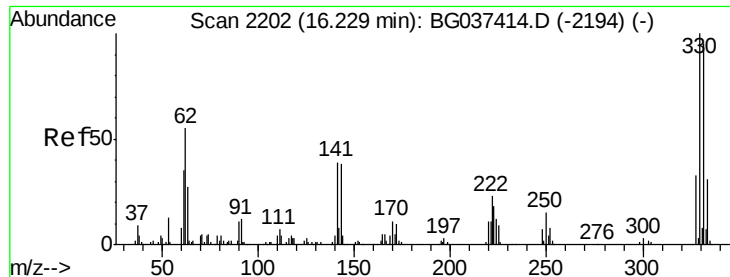

#42

2,4,6-Tribromophenol

Concen: 123.253 ng

RT: 16.22 min Scan# 2201

Delta R.T. -0.01 min

Lab File: BG037571.D

Acq: 26 Oct 2018 8:42

Instrument :

BNA_G

ClientSampleId :

S37-0002


Tot Ion:330 Resp: 232437

Ion Ratio Lower Upper

330 100

332 97.4 78.4 117.6

141 41.0 32.2 48.2



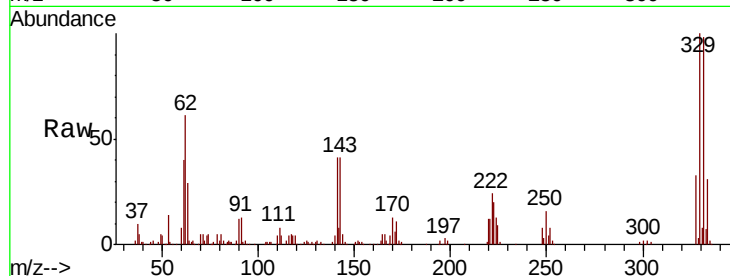


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

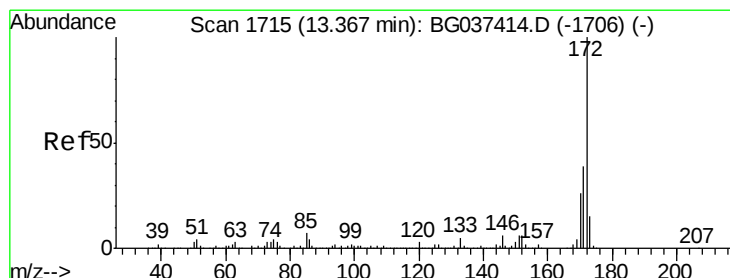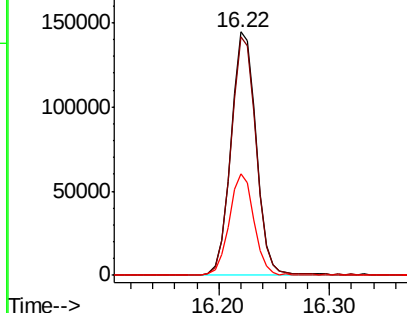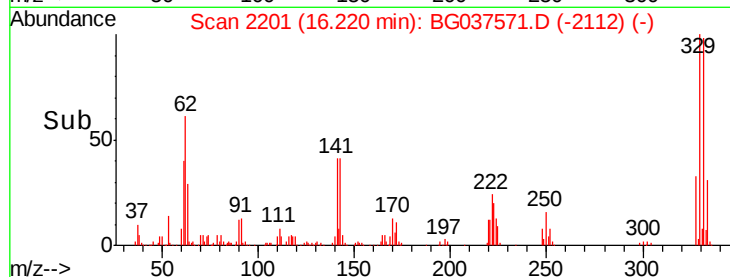

#45

2-Fluorobiphenyl

Concen: 78.791 ng

RT: 13.36 min Scan# 1714

Delta R.T. -0.01 min

Lab File: BG037571.D

Acq: 26 Oct 2018 8:42


Tgt Ion:172 Resp: 903435

Ion Ratio Lower Upper

172 100

171 37.4 31.0 46.4

170 24.8 20.2 30.2


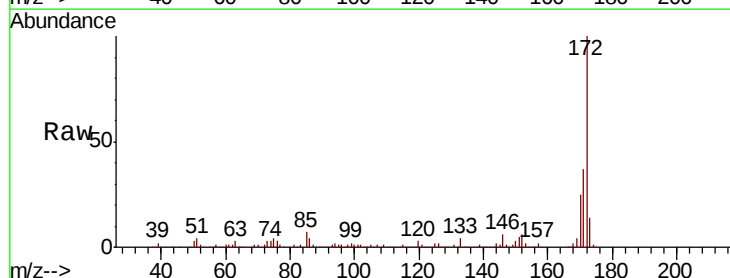



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

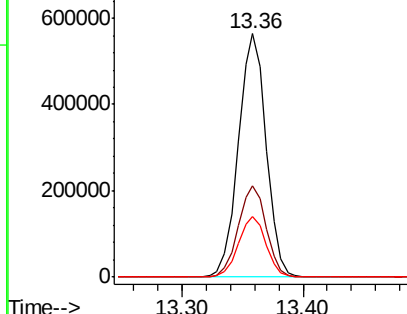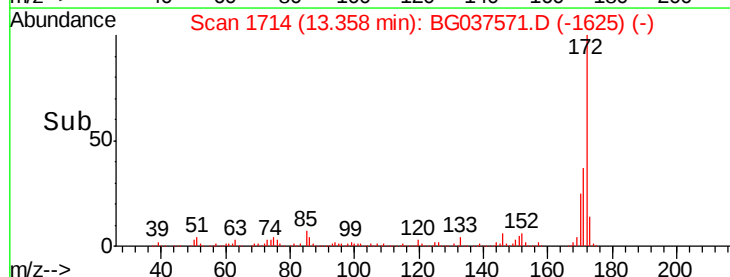

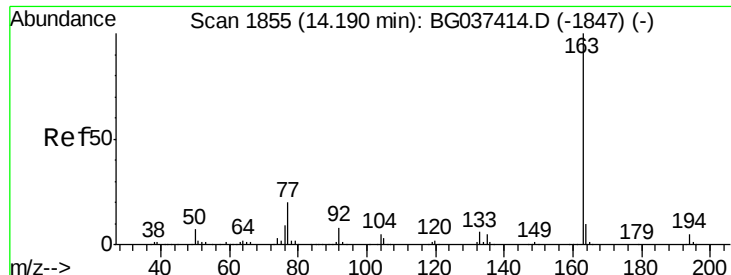

#50

Dimethylphthalate

Concen: 9.693 ng

RT: 14.18 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BG037571.D

Acq: 26 Oct 2018 8:42

Instrument :

BNA_G

ClientSampled :

S37-0002


Tot Ion:163 Resp: 129650

Ion Ratio Lower Upper

163 100

194 5.0 3.5 5.3




164 9.3 8.5 12.7

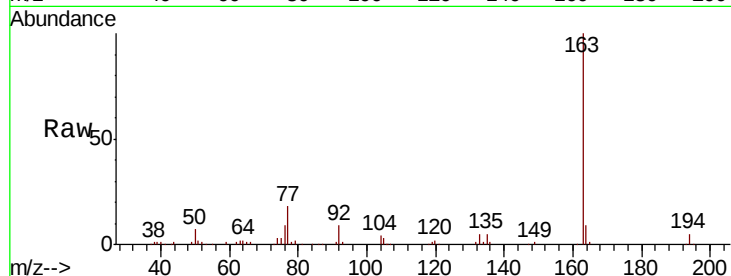

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

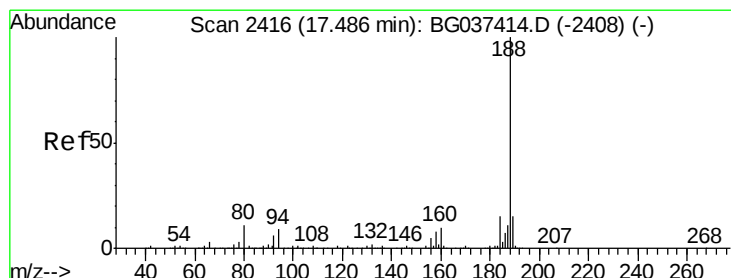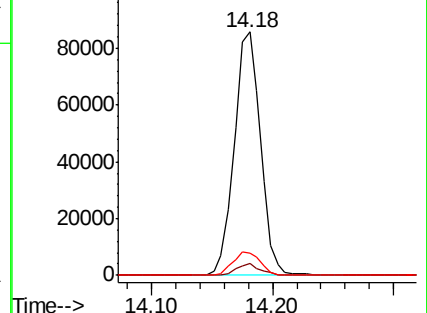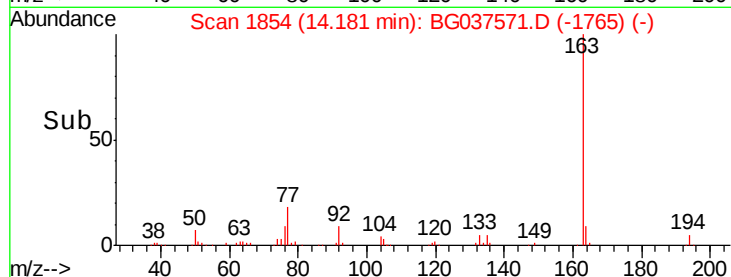

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.48 min Scan# 2416

Delta R.T. -0.00 min

Lab File: BG037571.D

Acq: 26 Oct 2018 8:42


Tgt Ion:188 Resp: 413427

Ion Ratio Lower Upper

188 100

94 9.4 7.2 10.8



80 10.3 7.7 11.5

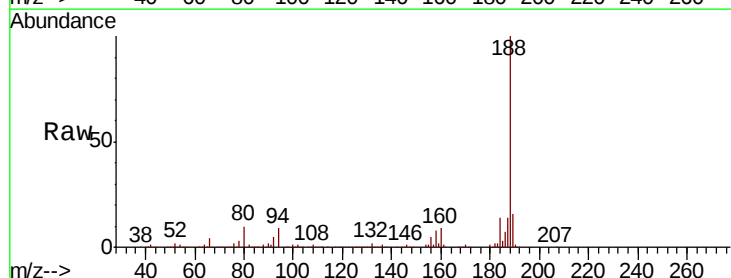


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



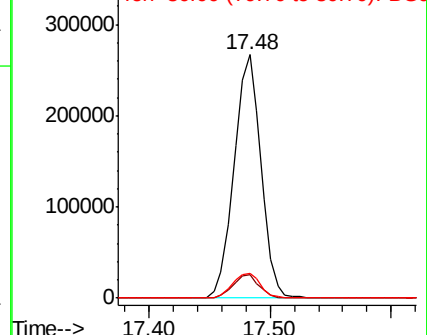
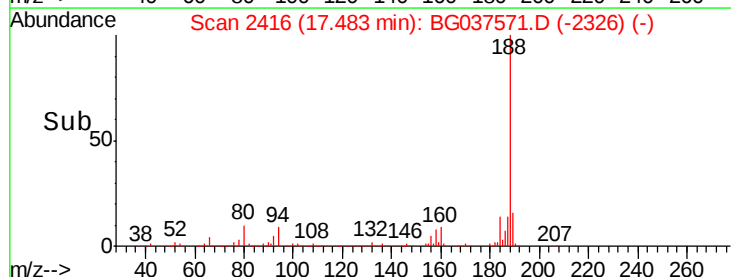


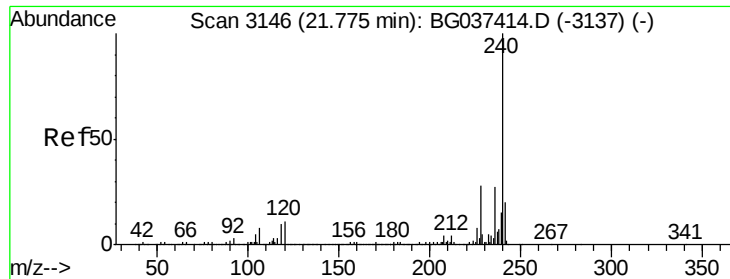

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.77 min Scan# 3145
 Delta R.T. -0.01 min
 Lab File: BG037571.D
 Acq: 26 Oct 2018 8:42




Instrument :
 BNA_G
 ClientSampled :
 S37-0002


Tot Ion	Ratio	Lower	Upper
240	100		
120	10.4	8.1	12.1
236	25.7	21.4	32.0

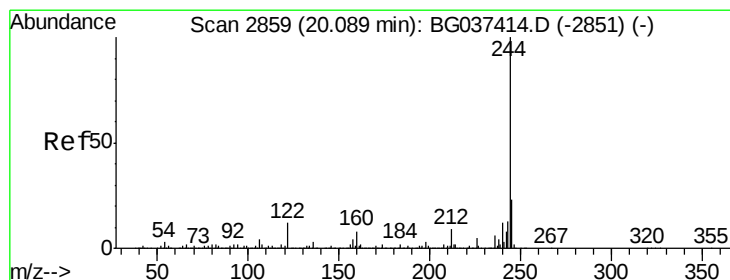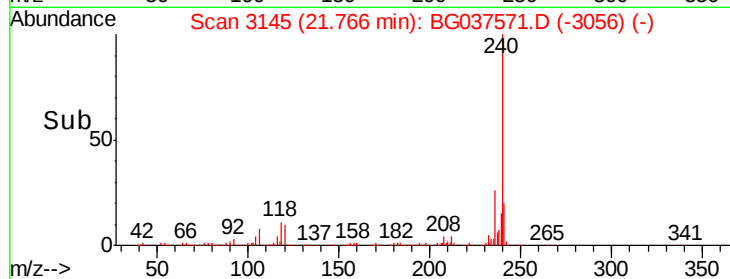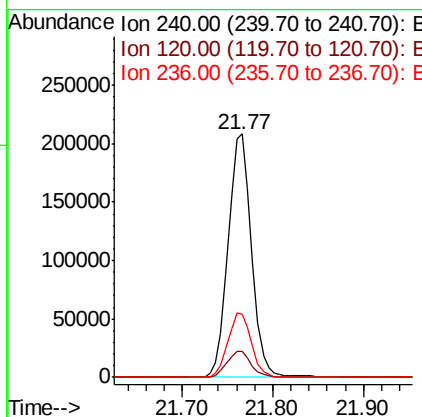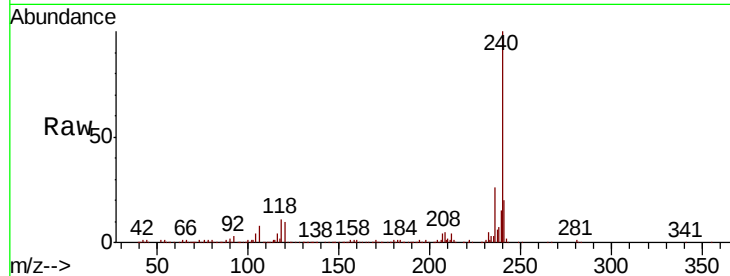

#79
 Terphenyl-d14
 Concen: 71.165 ng
 RT: 20.08 min Scan# 2858
 Delta R.T. -0.01 min
 Lab File: BG037571.D
 Acq: 26 Oct 2018 8:42

Tgt Ion	Ratio	Lower	Upper
244	100		
212	8.3	6.5	9.7
122	11.3	9.0	13.4

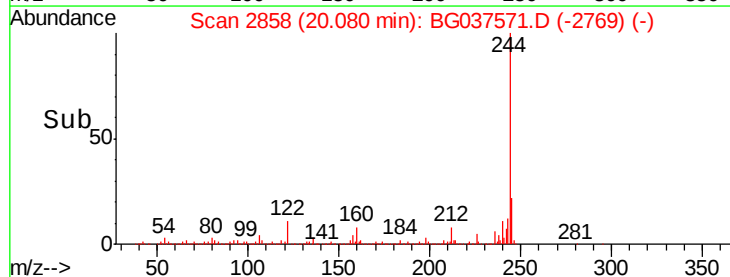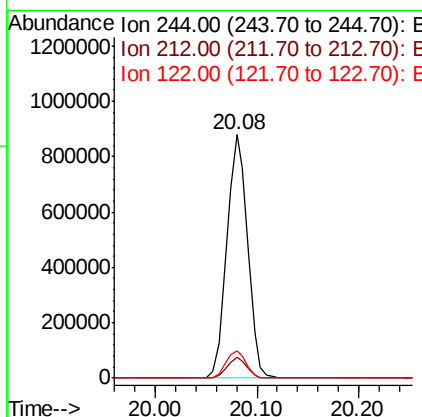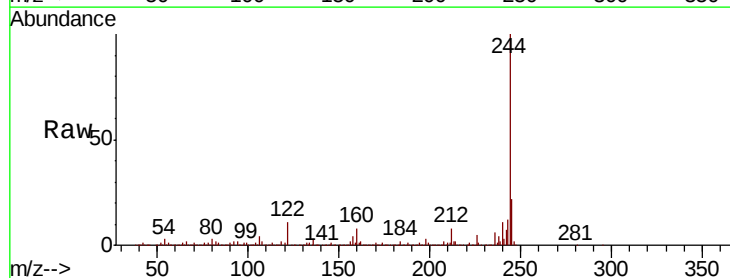

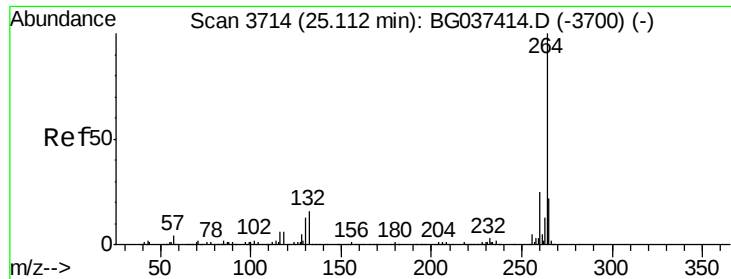

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 25.10 min Scan# 3712
 Delta R.T. -0.01 min
 Lab File: BG037571.D
 Acq: 26 Oct 2018 8:42

Instrument :
 BNA_G
 ClientSampleId :
 S37-0002

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.4	18.2	27.4
265	21.5	17.9	26.9

