

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102518\
 Data File : BG037575.D
 Acq On : 26 Oct 2018 11:18
 Operator : JU/SJ
 Sample : J5655-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 S37-0007

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.641	393	400	411	rBV	345531	566140	15.47%	3.459%
2	7.239	665	672	683	rVB	213860	379413	10.36%	2.318%
3	7.627	729	738	747	rBV	667007	1170540	31.98%	7.152%
4	8.103	811	819	830	rBV	173058	306086	8.36%	1.870%
5	8.426	866	874	886	rVB	589342	1061923	29.01%	6.488%
6	9.278	1010	1019	1028	rBV	541904	981081	26.80%	5.994%
7	10.923	1291	1299	1307	rBV	260472	474436	12.96%	2.899%
8	13.356	1706	1713	1721	rBV	1511604	2416055	66.00%	14.762%
9	14.737	1940	1948	1955	rBV2	448750	733985	20.05%	4.484%
10	16.223	2194	2201	2222	rBV	1096079	1788610	48.86%	10.928%
11	17.480	2408	2415	2425	rBV	604268	940134	25.68%	5.744%
12	20.083	2851	2858	2868	rBV	2580898	3660535	100.00%	22.365%
13	21.764	3137	3144	3154	rBV	556586	980123	26.78%	5.988%
14	25.095	3700	3711	3731	rBV2	278789	908140	24.81%	5.549%


Sum of corrected areas: 16367201

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102518\
Data File : BG037575.D
Acq On : 26 Oct 2018 11:18
Operator : JU/SJ
Sample : J5655-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S37-0007

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

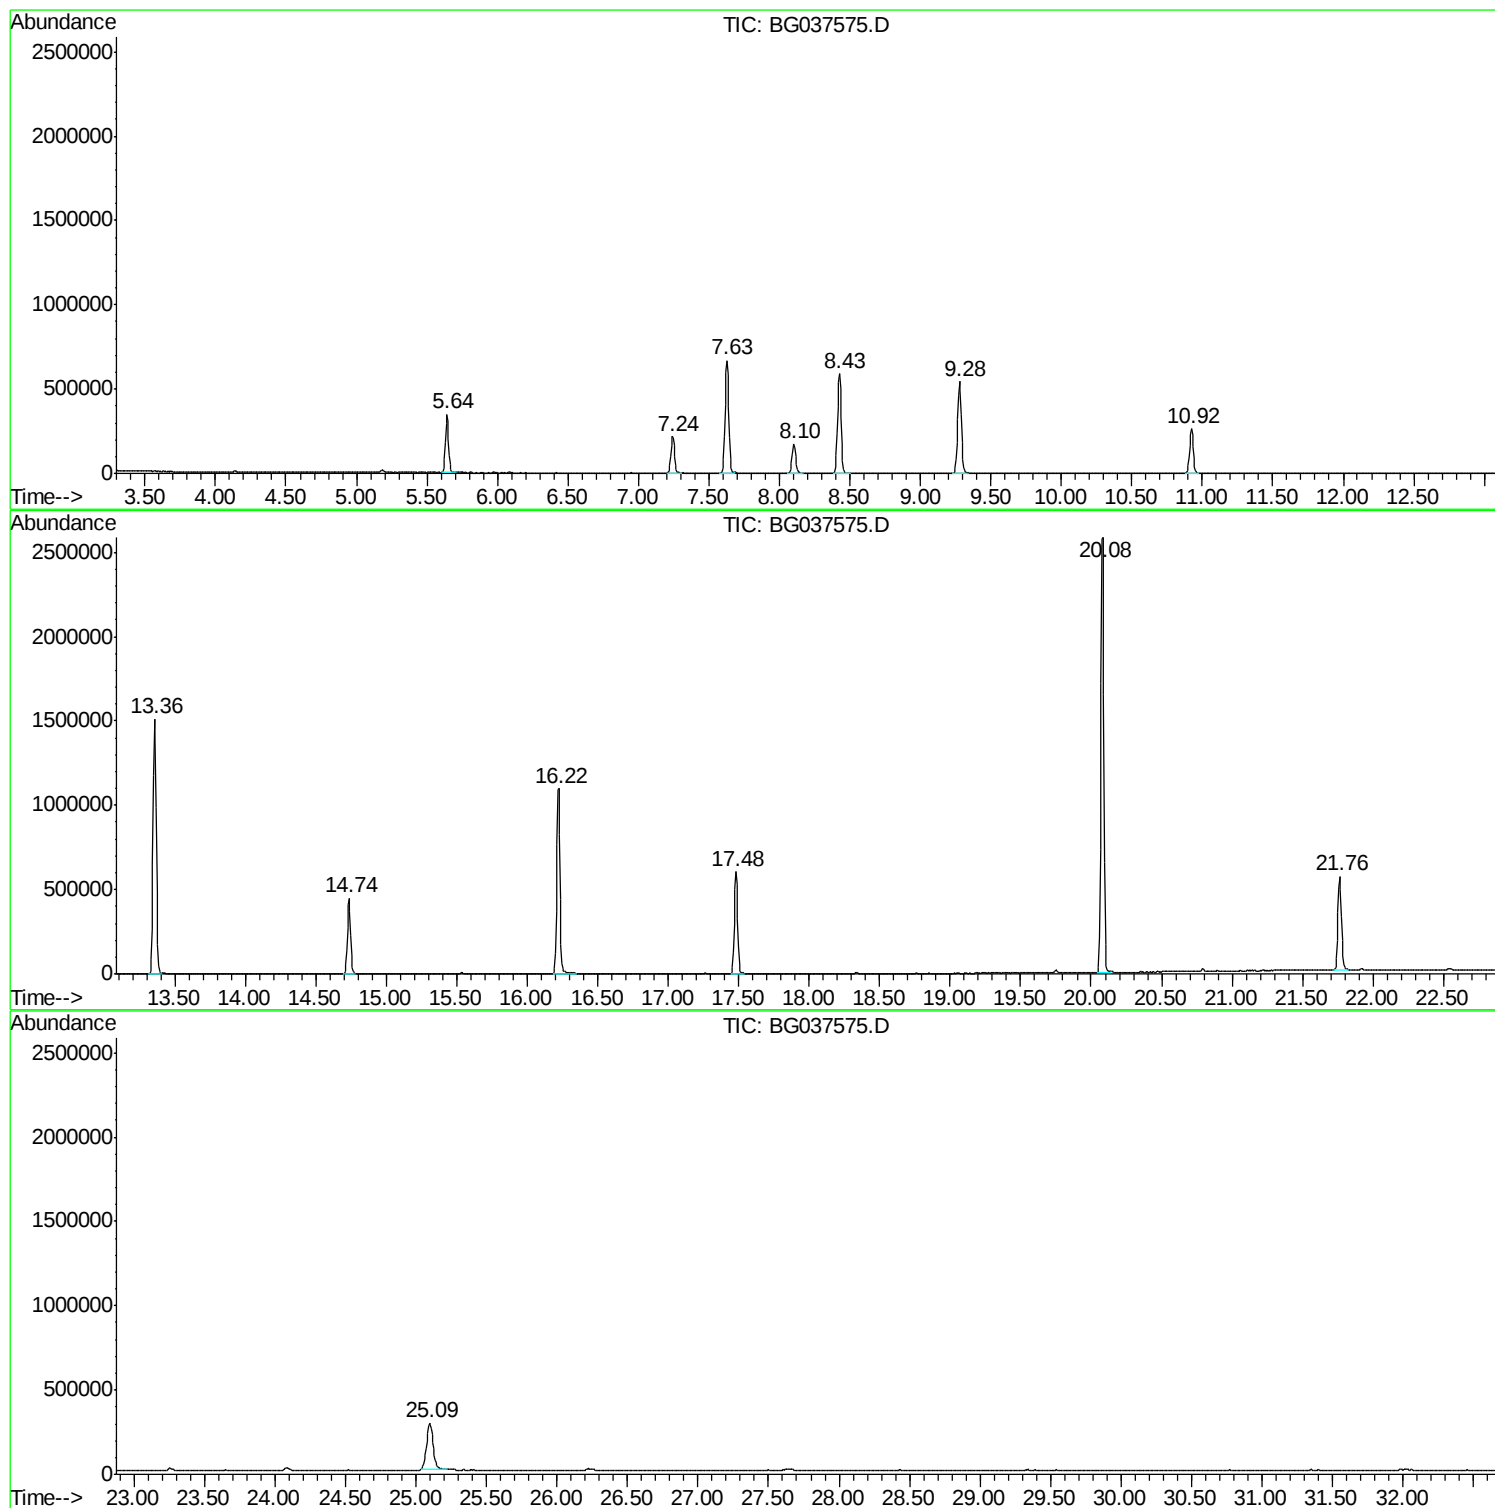

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102518\
Data File : BG037575.D
Acq On : 26 Oct 2018 11:18
Operator : JU/SJ
Sample : J5655-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S37-0007










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.63	76.48 ng	1170540	1,4-Dichlorobenzene-d4	8.10

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

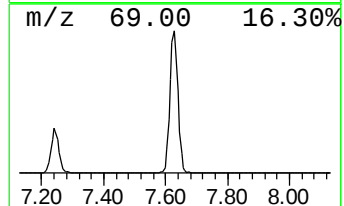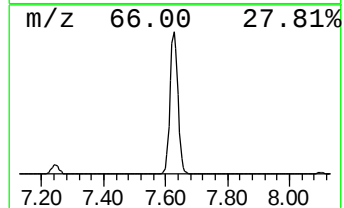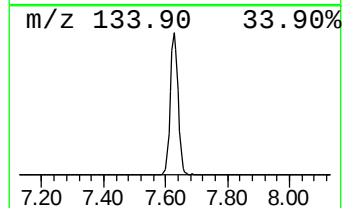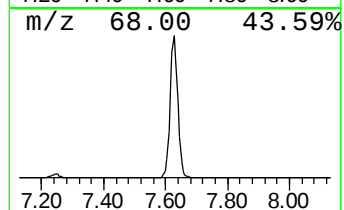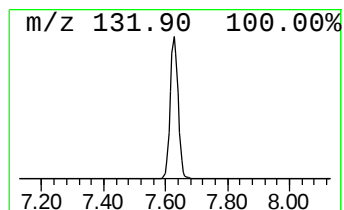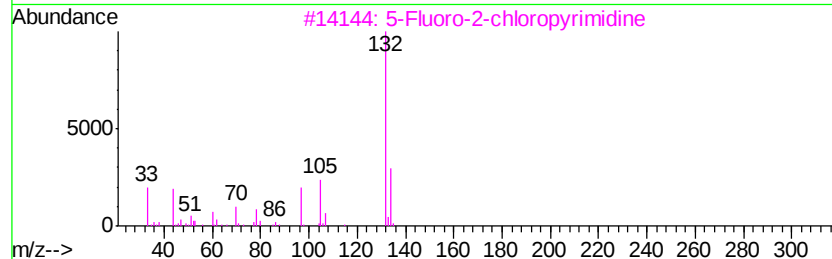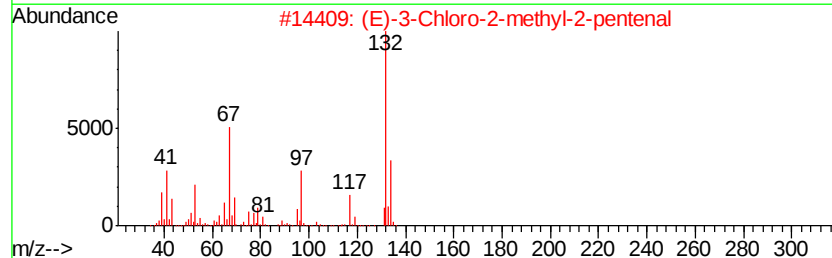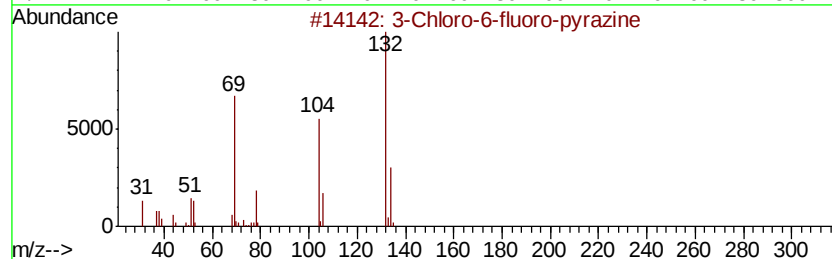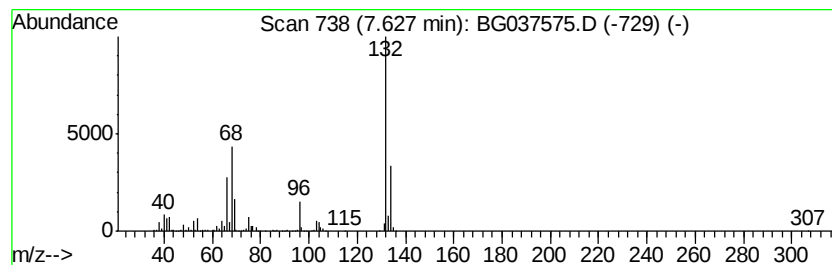

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102518\
Data File : BG037575.D
Acq On : 26 Oct 2018 11:18
Operator : JU/SJ
Sample : J5655-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S37-0007

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.63	7.63	76.5	ng	1170540	1	8.10	306086	20.0