


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102518\
 Data File : BG037561.D
 Acq On : 26 Oct 2018 2:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

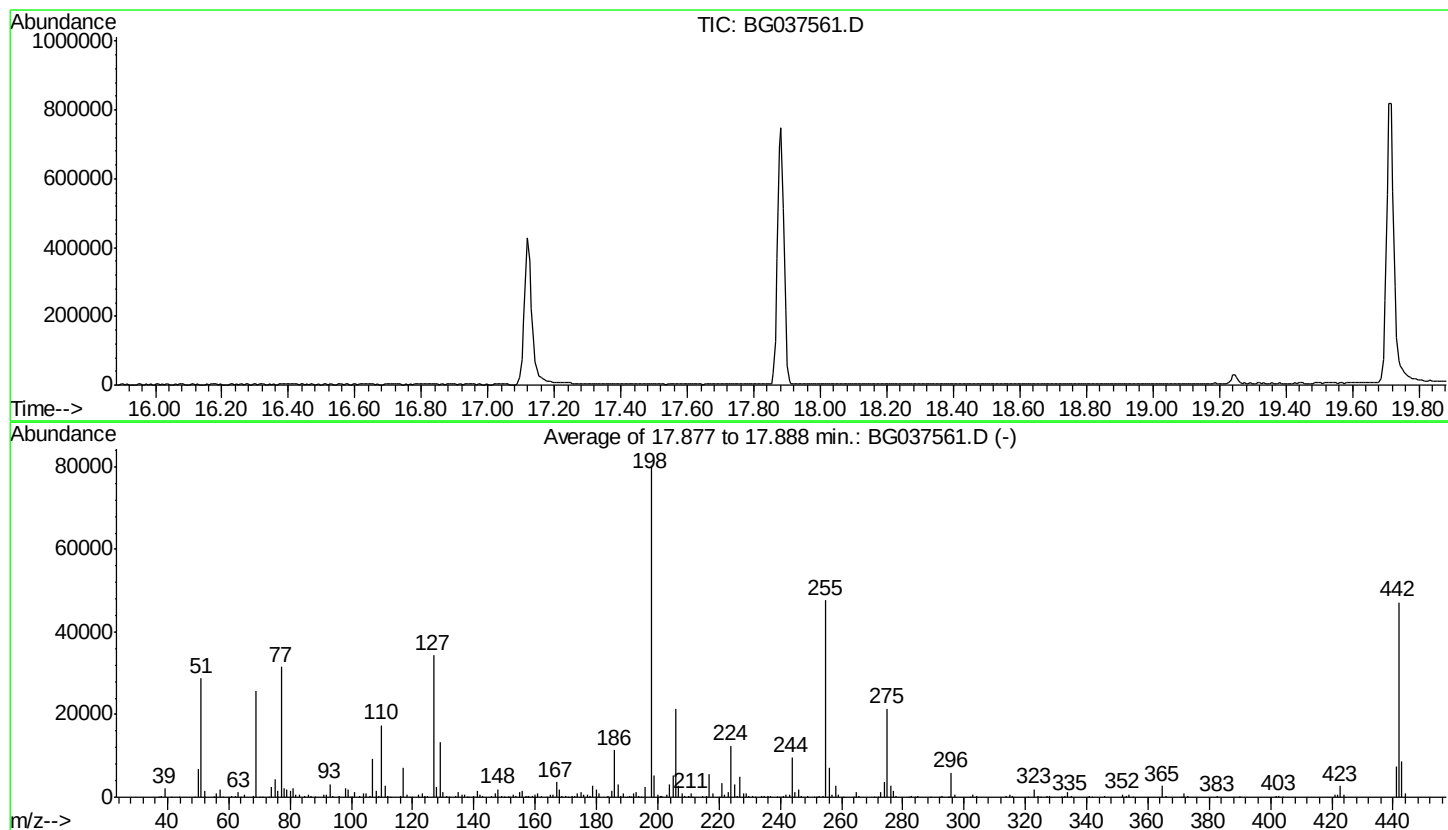

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	28813	PASS
68	69	0.00	2	0.9	234	PASS
69	198	0.00	100	32.2	25872	PASS
70	69	0.00	2	0.3	70	PASS
127	198	10	80	42.8	34352	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80277	PASS
199	198	5	9	6.7	5375	PASS
275	198	10	60	26.8	21509	PASS
365	198	1	100	3.5	2779	PASS
441	198	0.01	100	9.4	7559	PASS
442	198	50	100	58.8	47192	PASS
443	442	15	24	18.6	8787	PASS