
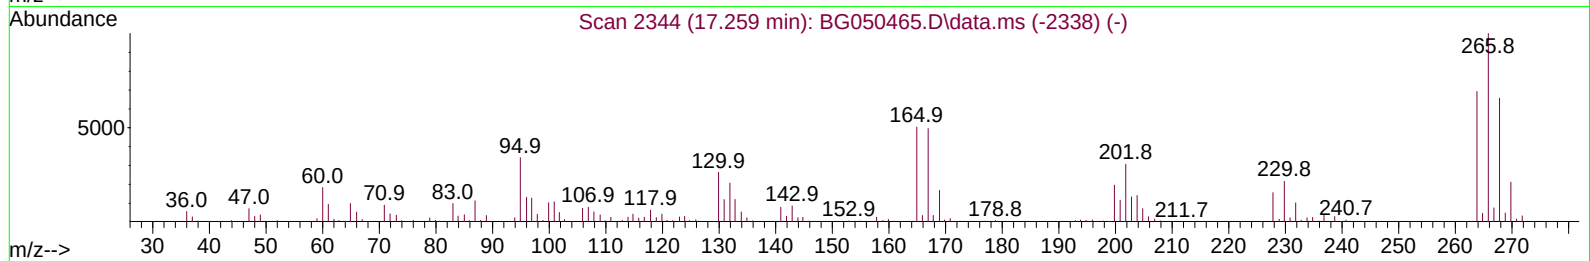
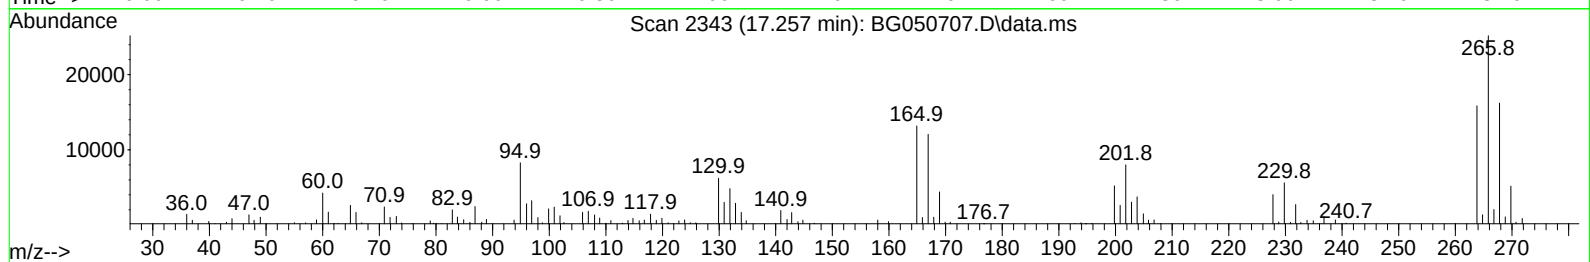


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102521\
Data File : BG050707.D
Acq On : 25 Oct 2021 11:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 12:33:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

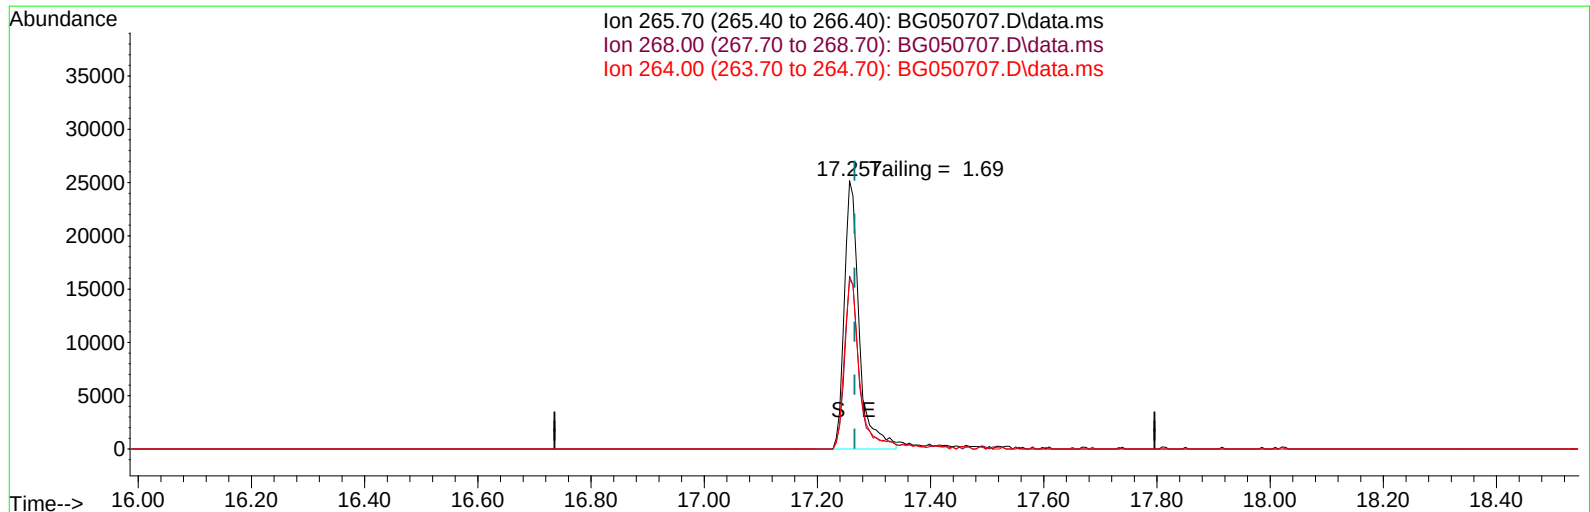

TIC: BG050707.D\data.ms

(70) Pentachlorophenol (C)




17.257min (-0.009) 26333.83 ng

response 47578

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.42
264.00	61.30	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102521\
Data File : BG050707.D
Acq On : 25 Oct 2021 11:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 12:33:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

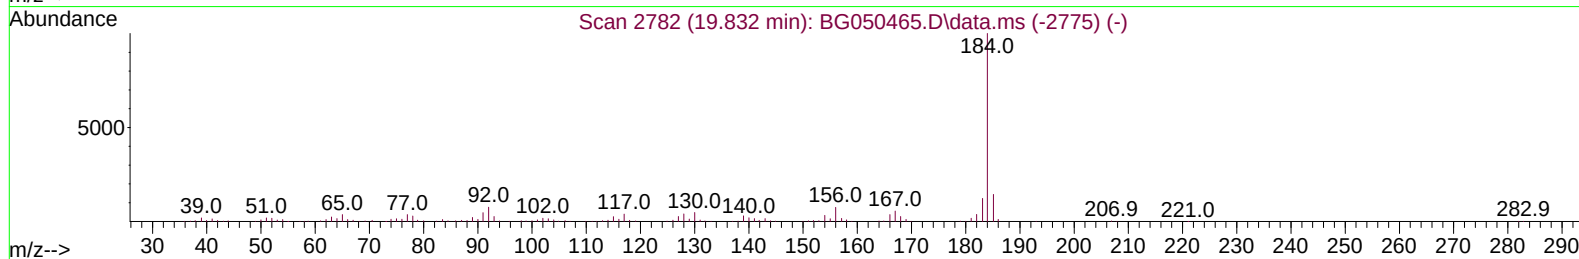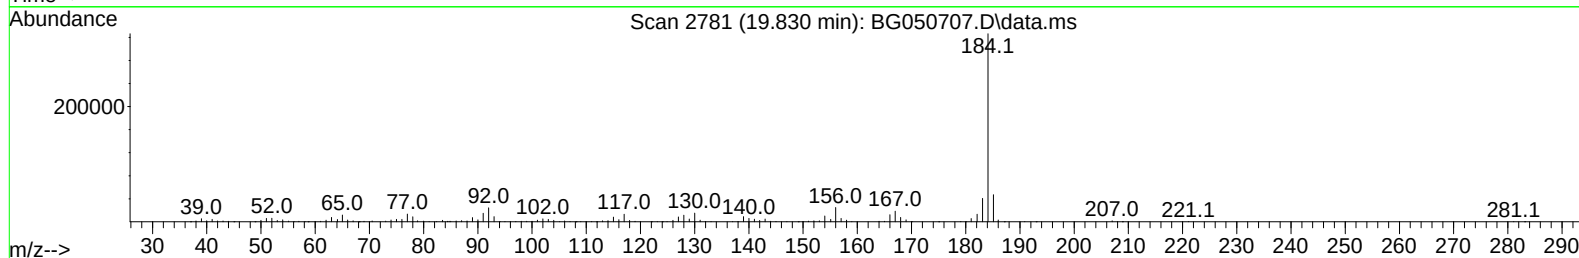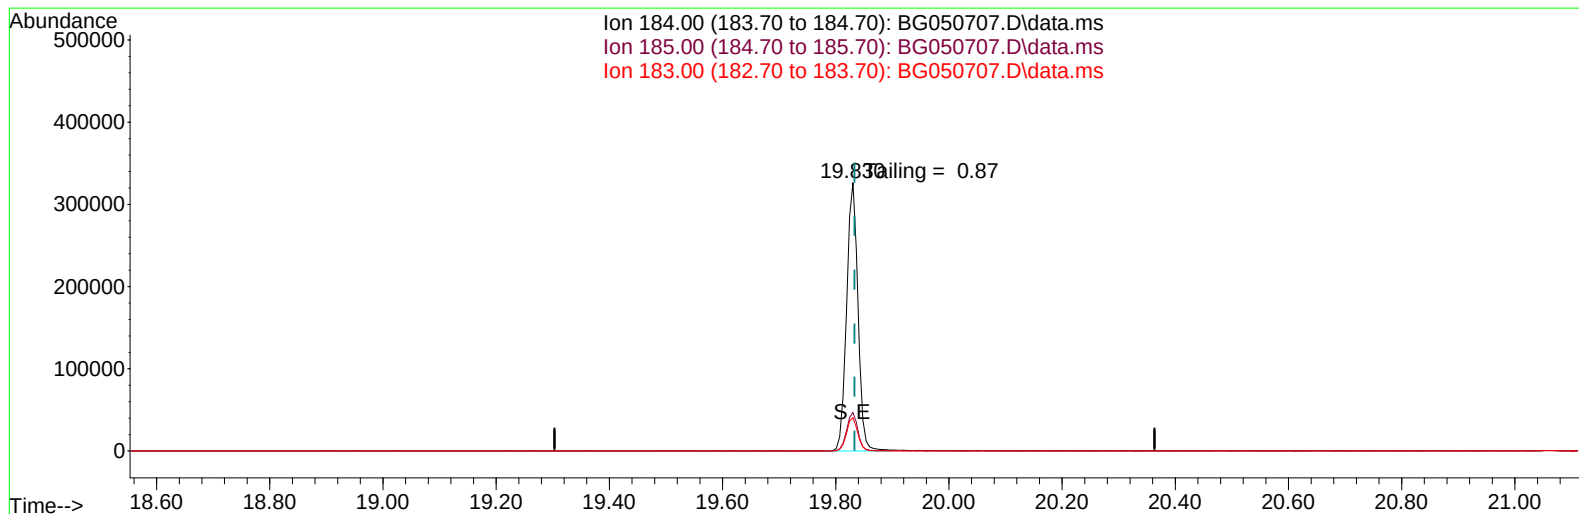

TIC: BG050707.D\data.ms

(77) Benzidine**19.830min (-0.003) 190958.90 ng****response 458001**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.39
183.00	11.70	12.50
0.00	0.00	0.00