


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102521\
 Data File : BG050707.D
 Acq On : 25 Oct 2021 11:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

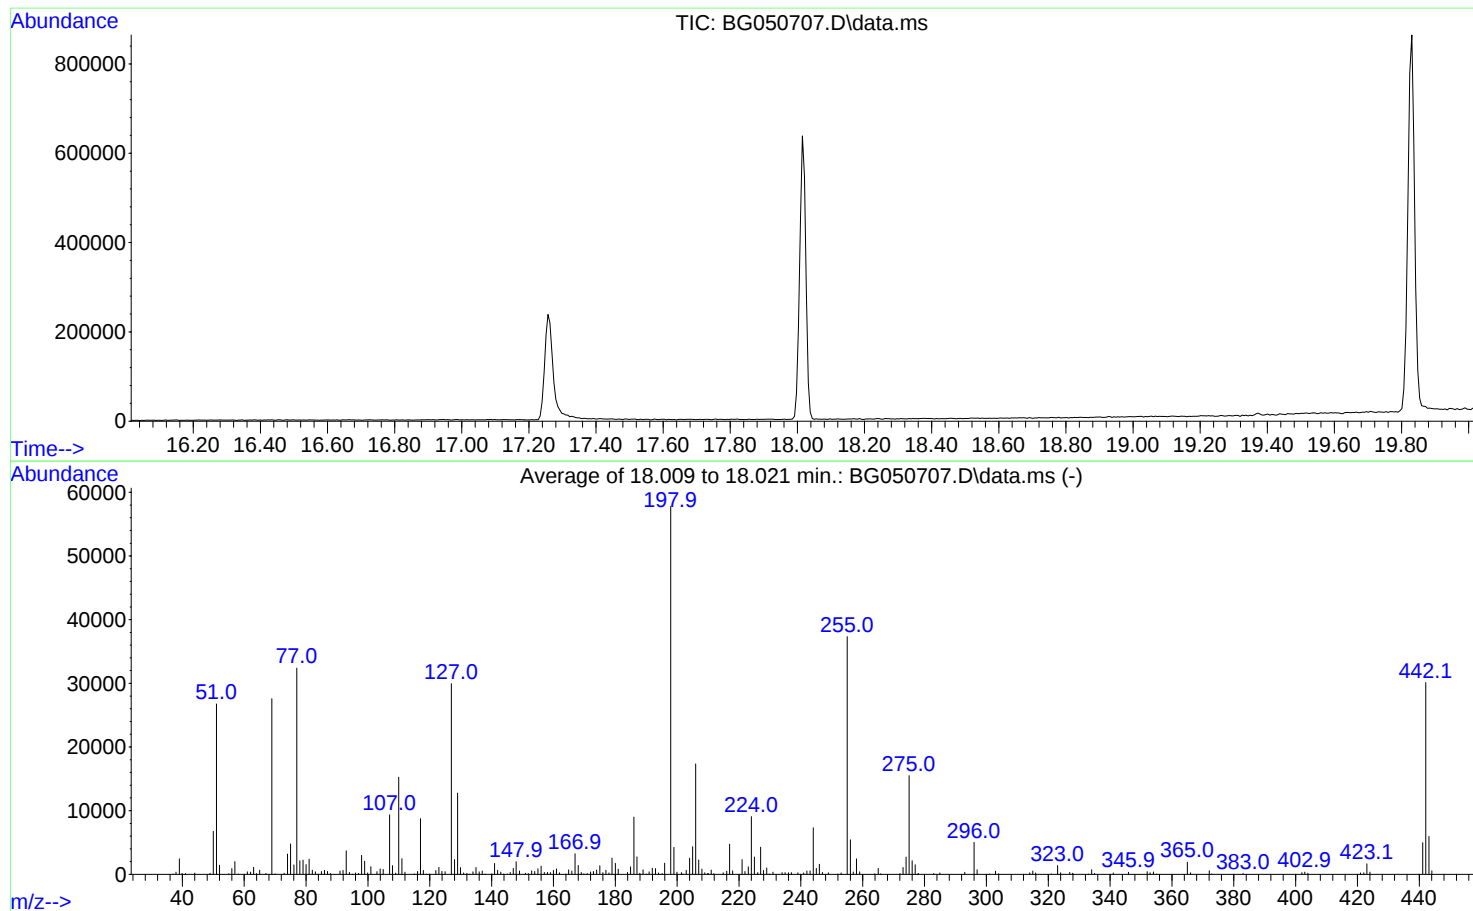




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	26757	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.8	27597	PASS
70	69	0.00	2	0.2	66	PASS
127	198	10	80	51.8	29944	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57768	PASS
199	198	5	9	7.4	4257	PASS
275	198	10	60	26.8	15507	PASS
365	198	1	100	3.3	1918	PASS
441	198	0.01	100	8.6	4980	PASS
442	442	50	100	100.0	30128	PASS
443	442	15	24	19.8	5953	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102521\
Data File : BG050707.D
Acq On : 25 Oct 2021 11:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 25 12:33:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

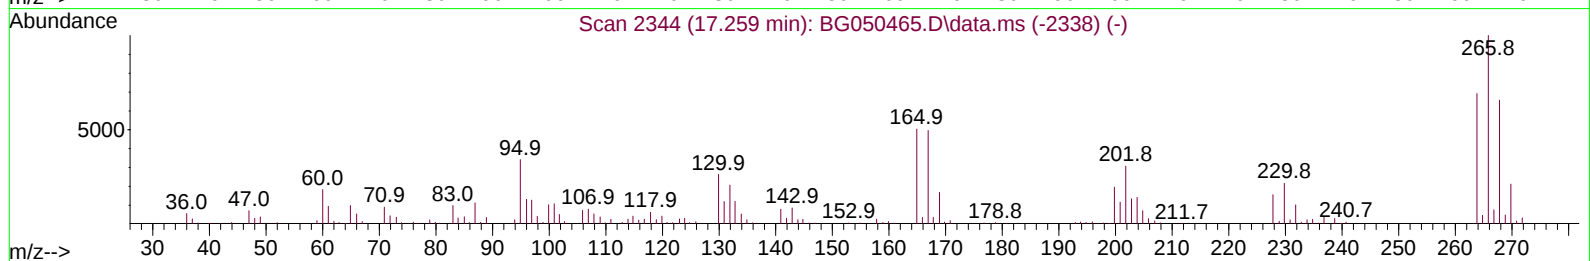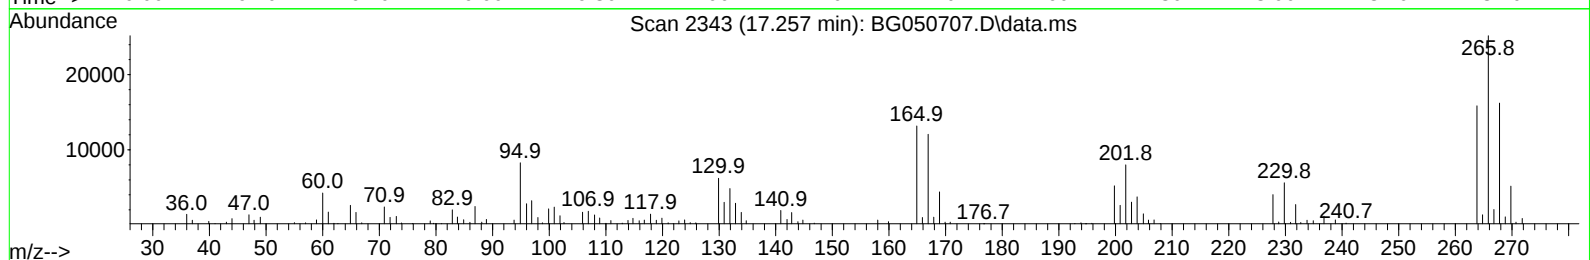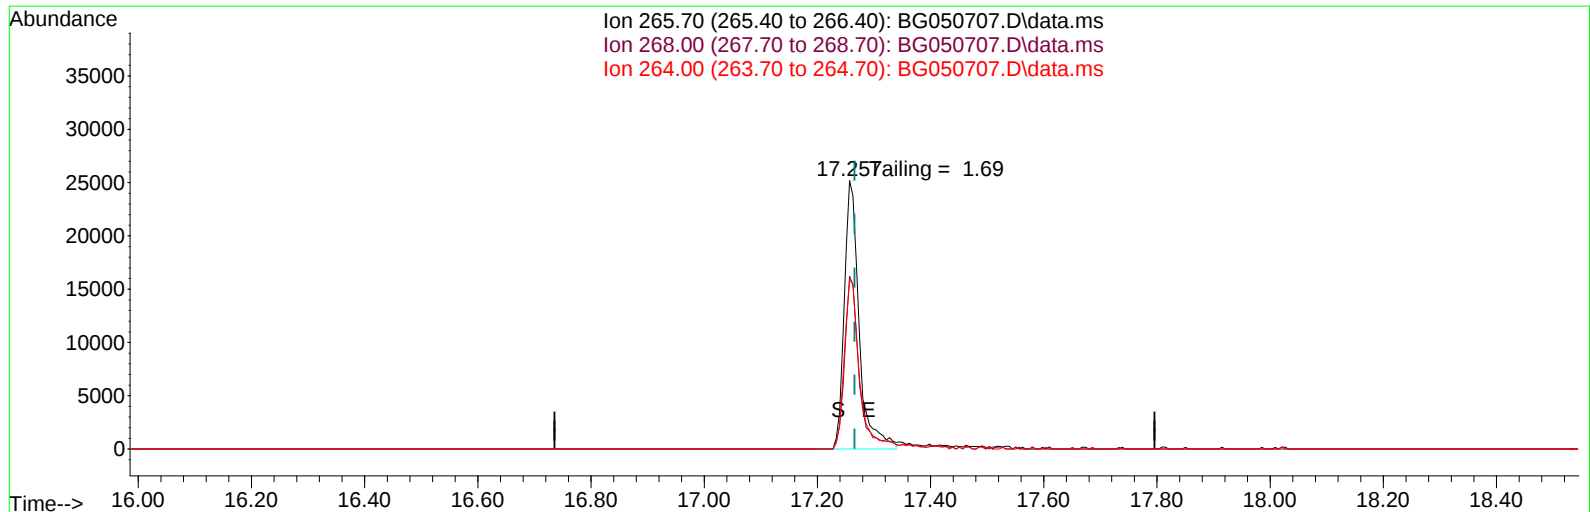

TIC: BG050707.D\data.ms

(70) Pentachlorophenol (C)




17.257min (-0.009) 26333.83 ng

response 47578

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.42
264.00	61.30	62.94
0.00	0.00	0.00

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 25 12:33:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

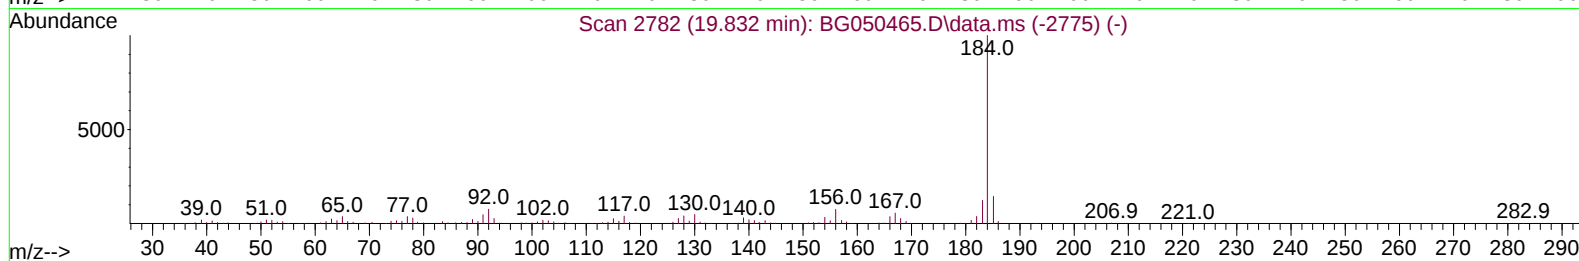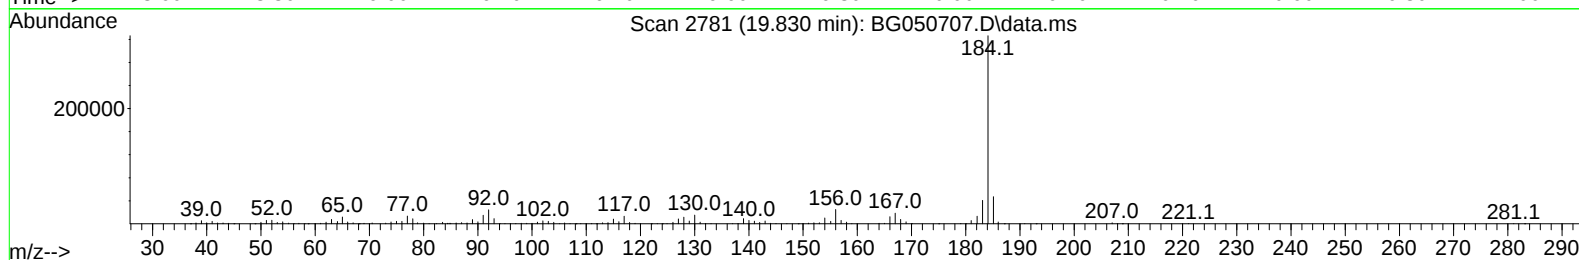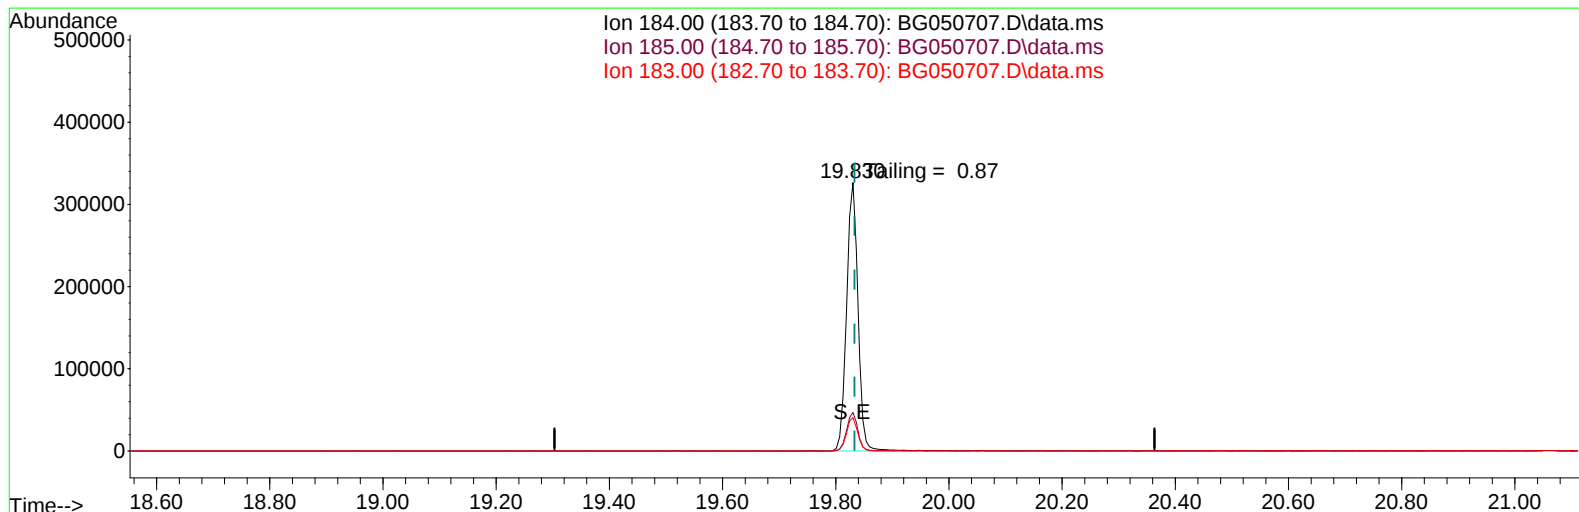

TIC: BG050707.D\data.ms

(77) Benzidine

19.830min (-0.003) 190958.90 ng

response **458001**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	13.40	14.39
--------	-------	-------

183.00	11.70	12.50
--------	-------	-------

0.00 0.00 0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/25/2021	BNA_G	BG050707.D
Compound Name	Response	Retention Time
DDT	182116	21.06
DDD	1095	20.61
DDE	0	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1095	183211	0.60

Instrument :
BNA_G
ClientSampleId :
DFTPP