

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102618\
 Data File : BG037598.D
 Acq On : 27 Oct 2018 2:20
 Operator : JU/SJ
 Sample : J5676-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB-1018-S-TCLP-GRID40

Quant Time: Oct 27 03:42:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	55788	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	241238	20.00	ng	0.00
39) Acenaphthene-d10	14.73	164	161762	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	407220	20.00	ng	0.00
76) Chrysene-d12	21.77	240	378449	20.00	ng	0.00
87) Perylene-d12	25.10	264	351066	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	387446	116.11	ng	0.00
7) Phenol-d6	7.24	99	505457	100.17	ng	0.00
23) Nitrobenzene-d5	9.28	82	365421	84.86	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	214758	121.72	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	854251	79.63	ng	0.00
79) Terphenyl-d14	20.08	244	1428976	80.68	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.28	70	44403	12.779	ng	# 71
51) 2,6-Dinitrotoluene	14.73	165	20585	7.436	ng	# 25
57) 2,4-Dinitrotoluene	14.73	165	20585	5.665	ng	# 25
65) 4,6-Dinitro-2-methylphenol	16.23	198	603	8.740	ng	69
67) 4-Bromophenyl-phenylether	16.22	248	15939	3.564	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102618\
Data File : BG037598.D
Acq On : 27 Oct 2018 2:20
Operator : JU/SJ
Sample : J5676-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB-1018-S-TCLP-GRID40

Quant Time: Oct 27 03:42:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

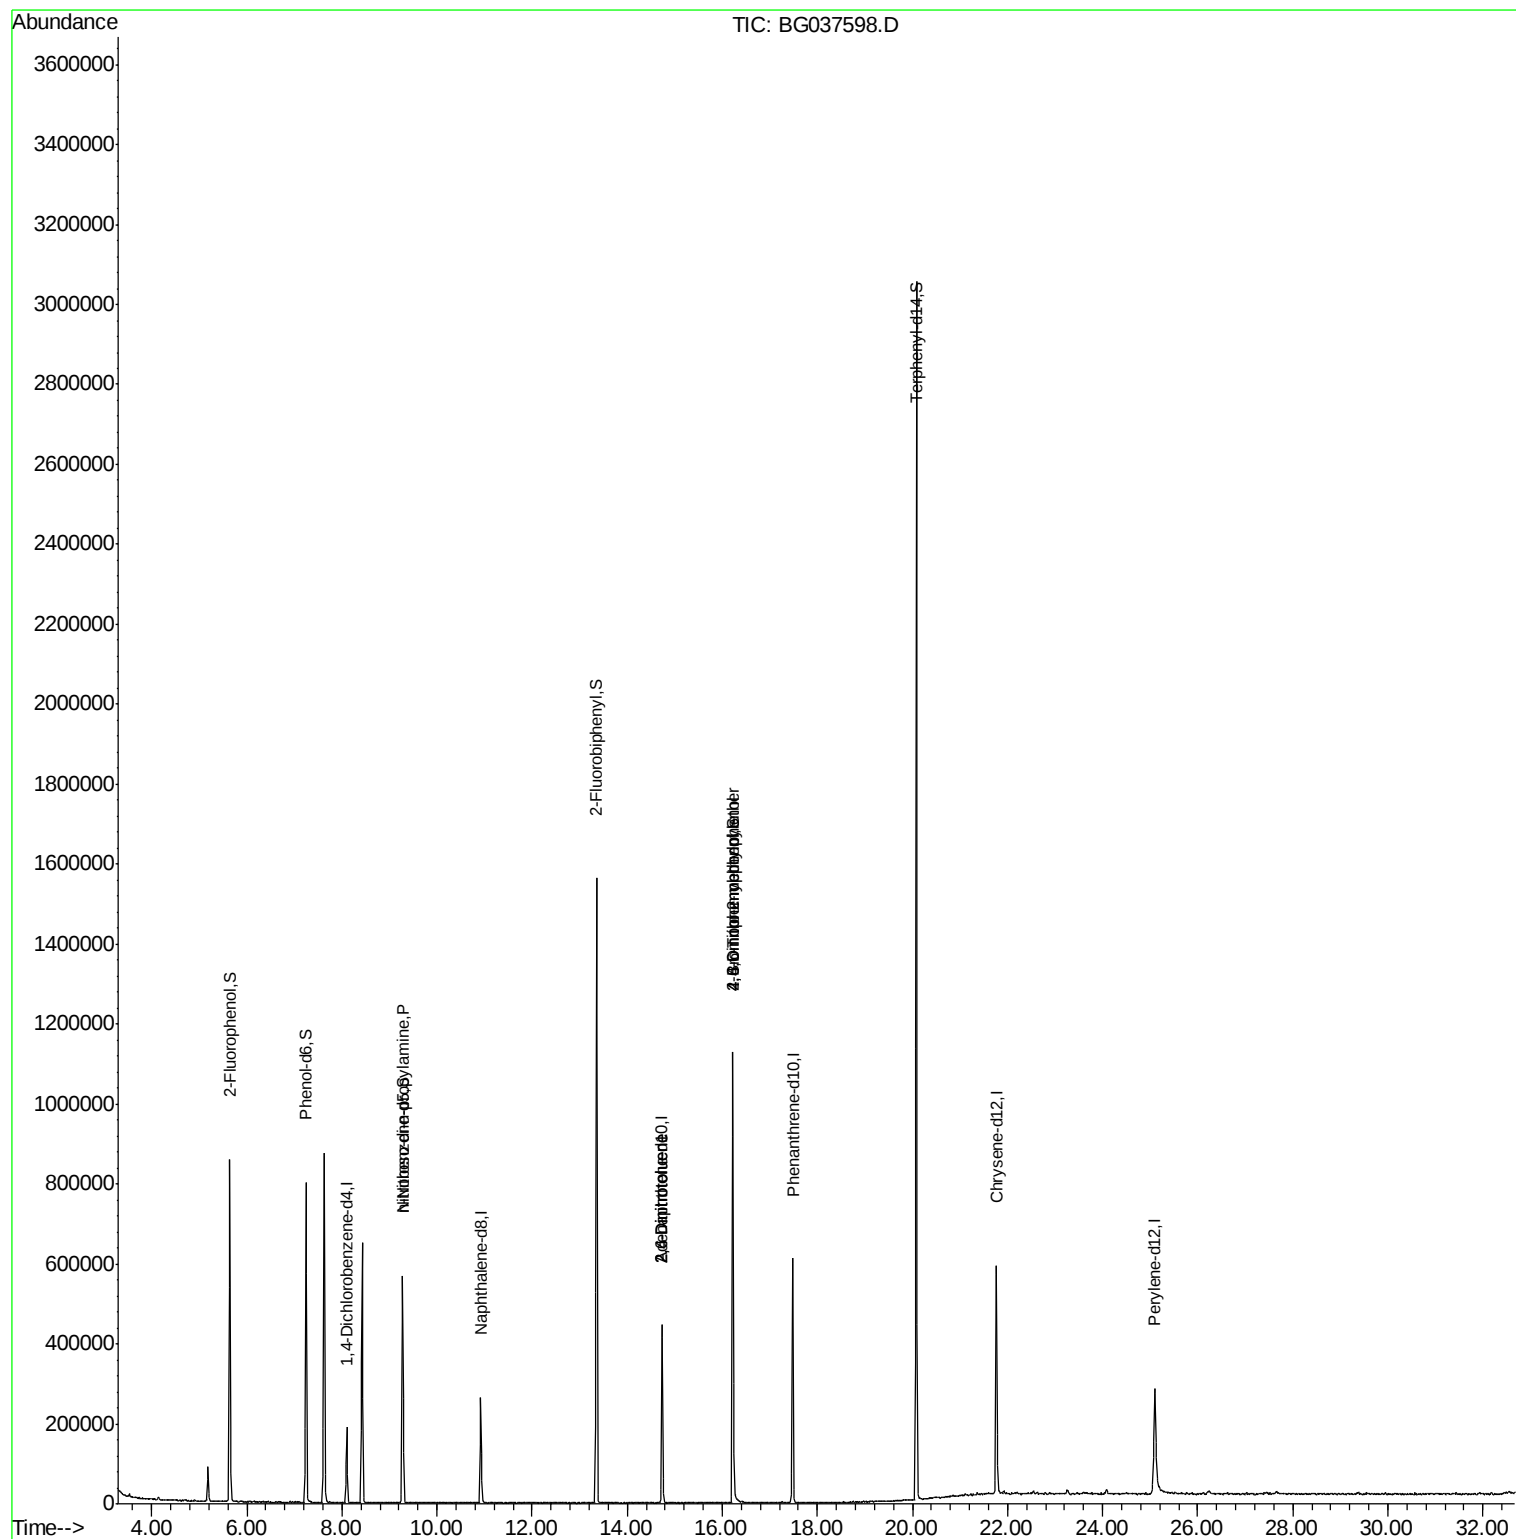

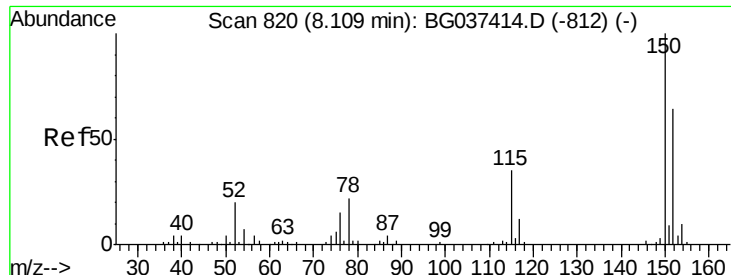

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.10 min Scan# 819

Delta R.T. -0.01 min

Lab File: BG037598.D

Acq: 27 Oct 2018 2:20

Instrument :

BNA_G

ClientSampleId :

CB-1018-S-TCLP-GRID40


Tot Ion:152 Resp: 55788

Ion Ratio Lower Upper

152 100

150 160.1 126.0 189.0

115 59.3 45.5 68.3






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

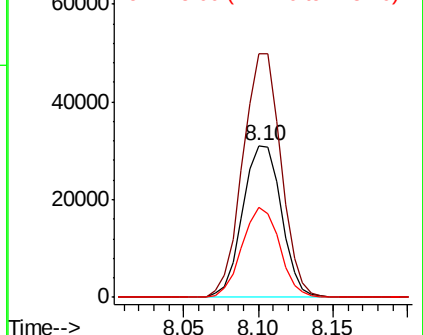

#5

2-Fluorophenol

Concen: 116.110 ng

RT: 5.64 min Scan# 401

Delta R.T. -0.00 min

Lab File: BG037598.D

Acq: 27 Oct 2018 2:20


Tgt Ion:112 Resp: 387446

Ion Ratio Lower Upper

112 100

64 65.8 53.1 79.7

63 32.7 27.3 40.9






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

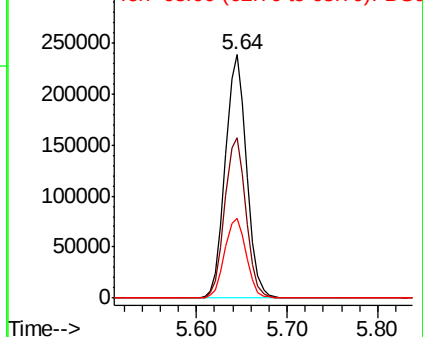

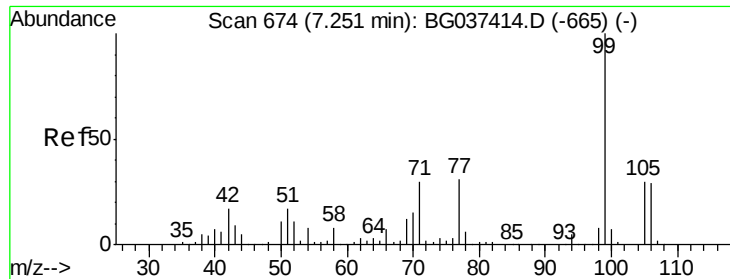

#7

Phenol-d6

Concen: 100.174 ng

RT: 7.24 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037598.D

Acq: 27 Oct 2018 2:20

Instrument :

BNA_G

ClientSampleId :

CB-1018-S-TCLP-GRID40


Tot Ion: 99 Resp: 505457

Ion Ratio Lower Upper

99 100

42 17.6 15.0 22.4

71 30.1 25.5 38.3



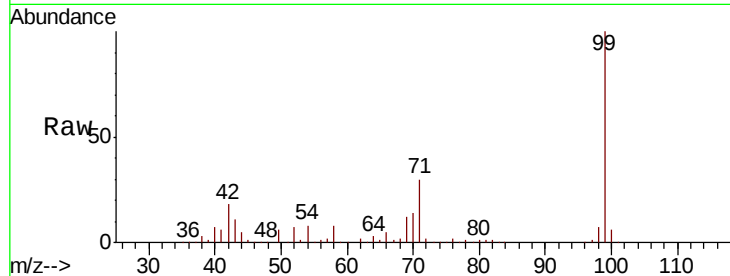


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

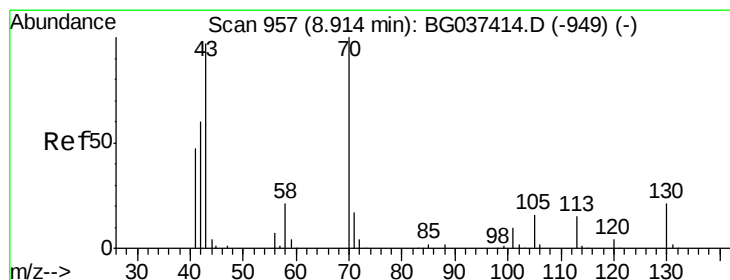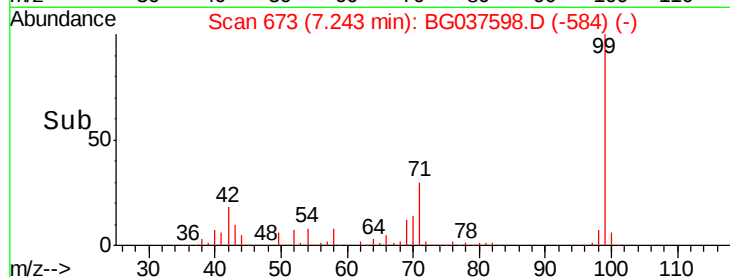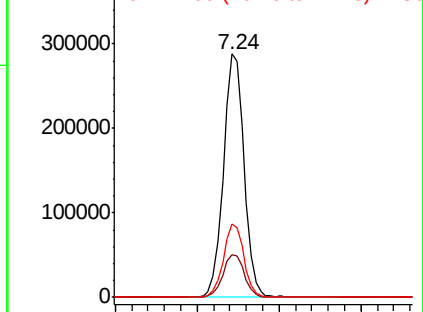

#19

n-Nitroso-di-n-propylamine

Concen: 12.779 ng

RT: 9.28 min Scan# 1019

Delta R.T. 0.36 min

Lab File: BG037598.D

Acq: 27 Oct 2018 2:20

Tgt Ion: 70 Resp: 44403


Ion Ratio Lower Upper

70 100

42 47.7 53.9 80.9#

101 0.0 8.2 12.2#

130 2.7 18.2 27.4#

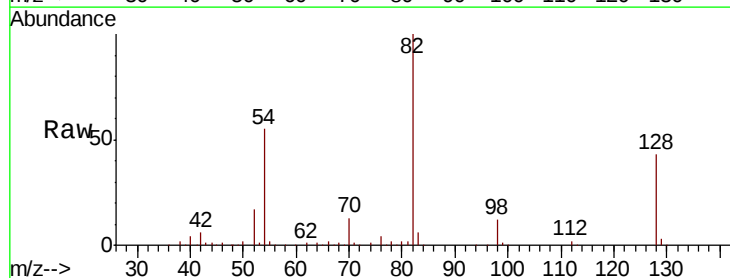



Abundance


Ion 70.00 (69.70 to 70.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 101.00 (100.70 to 101.70): BGC

Ion 130.00 (129.70 to 130.70): BGC



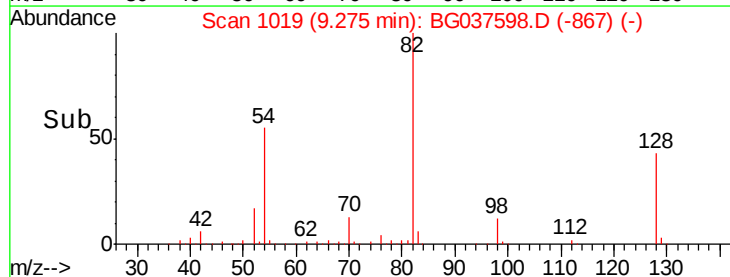
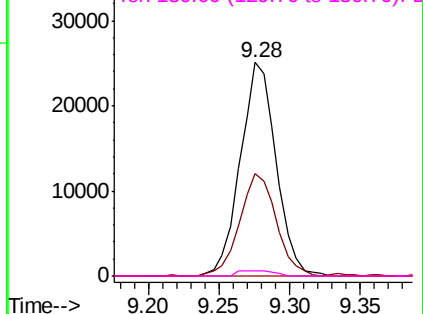


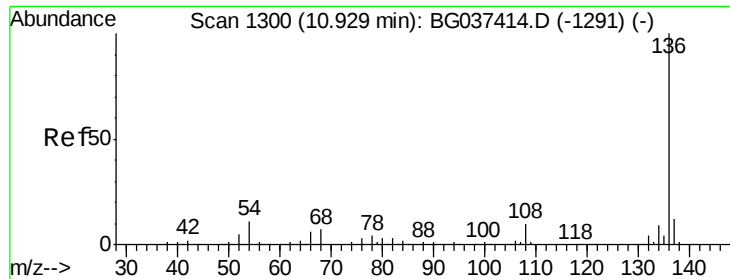

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.92 min Scan# 1299
Delta R.T. -0.01 min
Lab File: BG037598.D
Acq: 27 Oct 2018 2:20




Instrument :
BNA_G
ClientSampleId :
CB-1018-S-TCLP-GRID40


Tot Ion:136	Resp:	241238
Ion Ratio	Lower	Upper
136	100	
137	12.3	9.6 14.4
54	10.7	7.9 11.9
68	7.3	4.8 7.2#

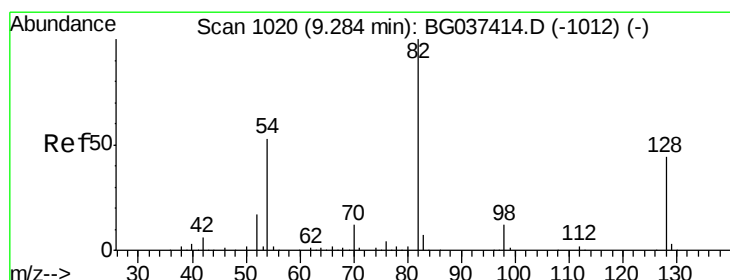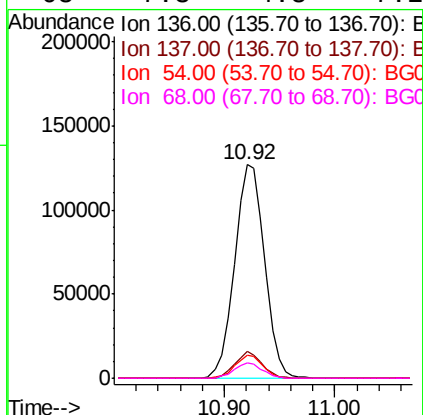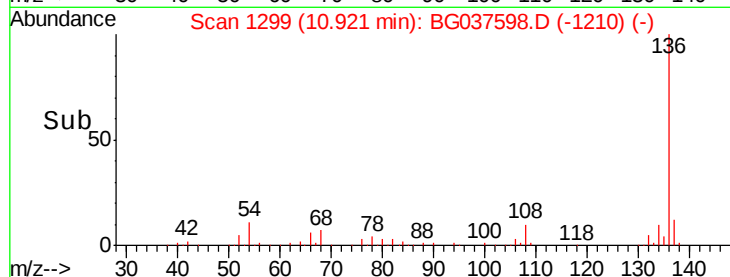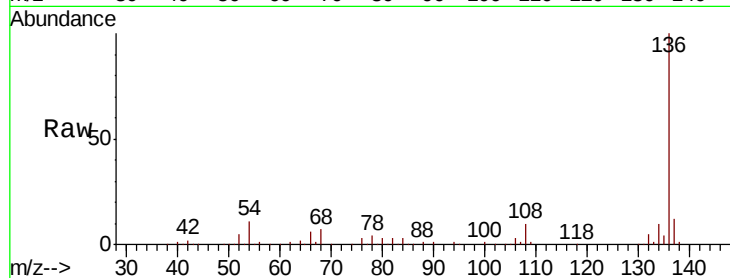

#23
Nitrobenzene-d5
Concen: 84.856 ng
RT: 9.28 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BG037598.D
Acq: 27 Oct 2018 2:20

Tgt Ion: 82	Resp:	365421
Ion Ratio	Lower	Upper
82	100	
128	43.3	34.6 51.8
54	55.4	45.3 67.9

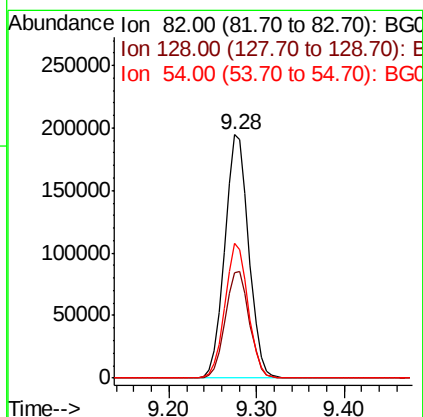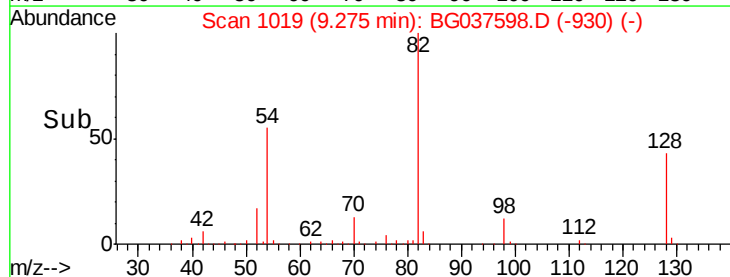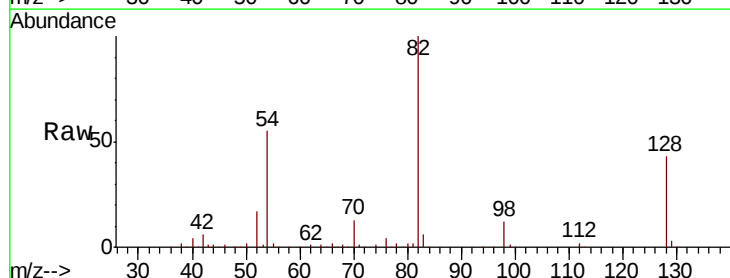


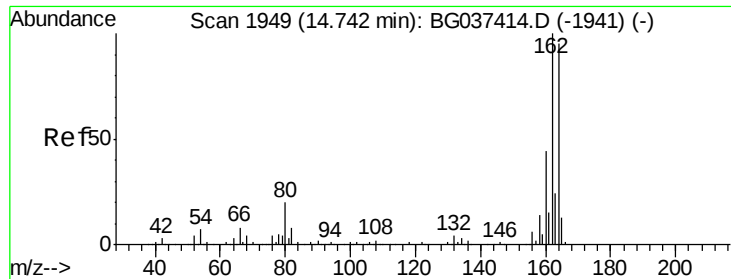




#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.73 min Scan# 1948
 Delta R.T. -0.01 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20

Instrument :
 BNA_G
 ClientSampleId :
 CB-1018-S-TCLP-GRID40

Tot Ion:164 Resp: 161762
 Ion Ratio Lower Upper
 164 100
 162 107.9 81.3 121.9
 160 47.1 36.3 54.5




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

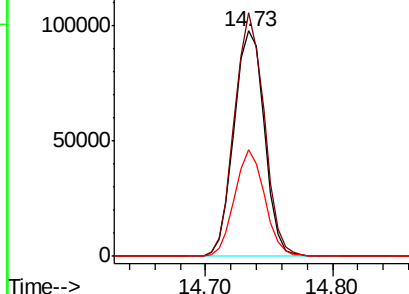




#42
 2,4,6-Tribromophenol
 Concen: 121.723 ng
 RT: 16.22 min Scan# 2201
 Delta R.T. -0.01 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20

Tgt Ion:330 Resp: 214758
 Ion Ratio Lower Upper
 330 100
 332 97.7 78.4 117.6
 141 39.4 32.2 48.2



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



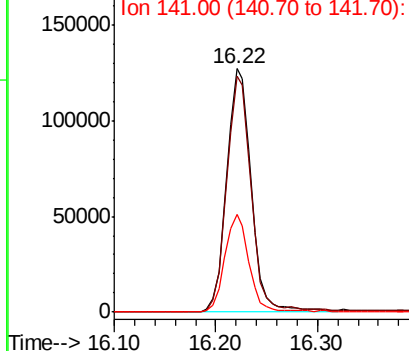





#45
 2-Fluorobiphenyl
 Concen: 79.633 ng
 RT: 13.36 min Scan# 1714
 Delta R.T. -0.01 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20




Instrument :
 BNA_G
 ClientSampleId :
 CB-1018-S-TCLP-GRID40


Tot Ion	Ratio	Lower	Upper
172	100		
171	37.4	31.0	46.4
170	25.0	20.2	30.2

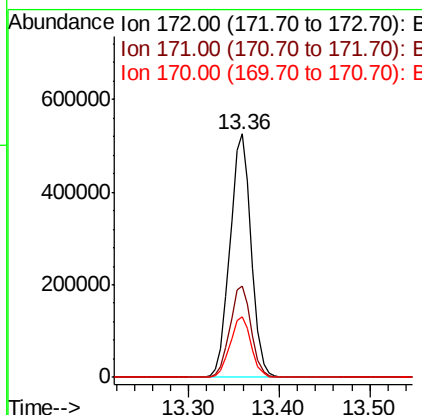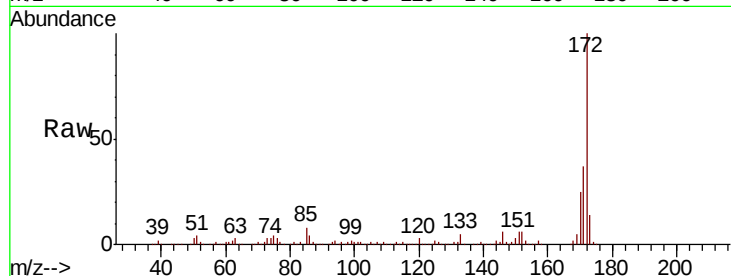

#51
 2,6-Dinitrotoluene
 Concen: 7.436 ng
 RT: 14.73 min Scan# 1948
 Delta R.T. 0.41 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	43.4	65.2#
89	1.3	45.8	68.6#

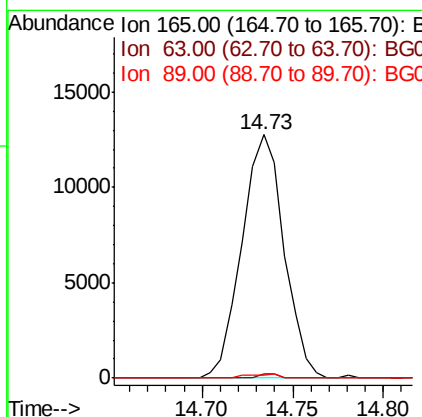


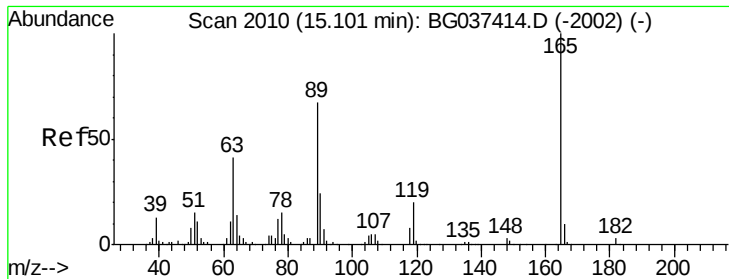

#57
 2,4-Dinitrotoluene
 Concen: 5.665 ng
 RT: 14.73 min Scan# 1948
 Delta R.T. -0.37 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20

Instrument :
 BNA_G
 ClientSampleId :
 CB-1018-S-TCLP-GRID40

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.5	33.4	50.0#
89	1.3	57.2	85.8#
182	0.0	2.6	4.0#



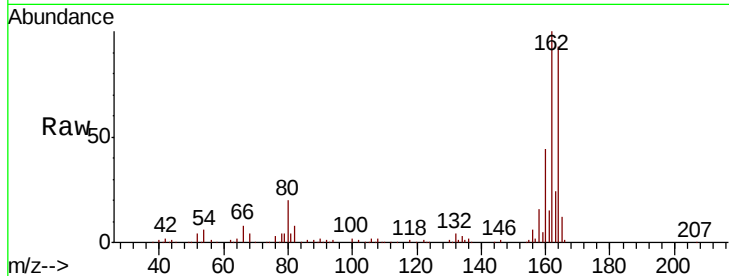


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

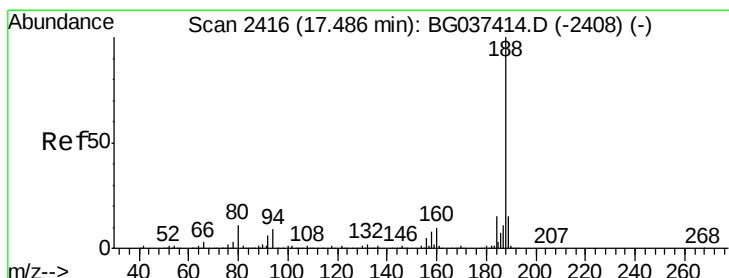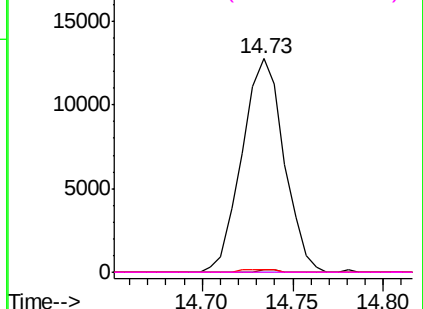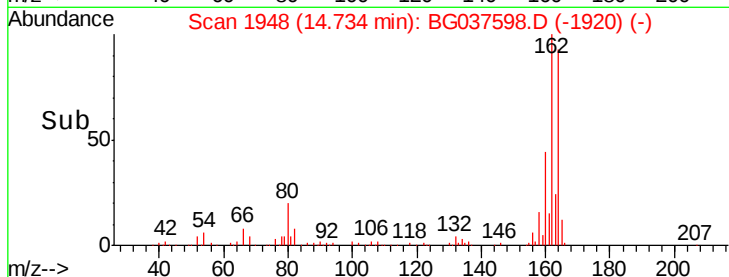

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.48 min Scan# 2416
 Delta R.T. -0.00 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20



Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.4	7.2	10.8
80	10.3	7.7	11.5

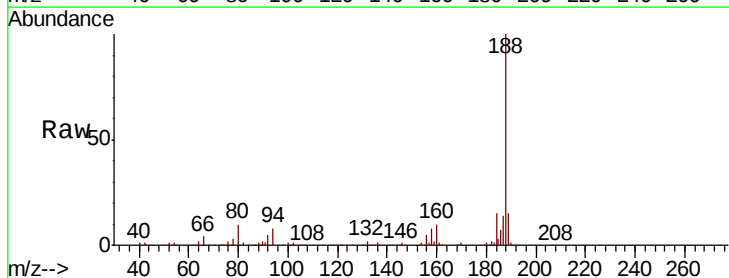


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

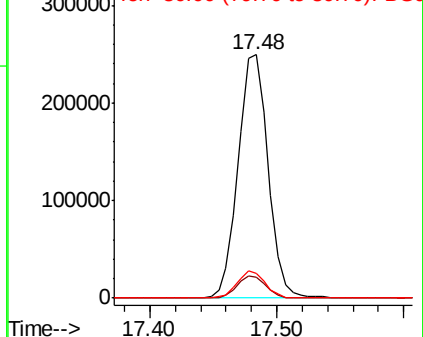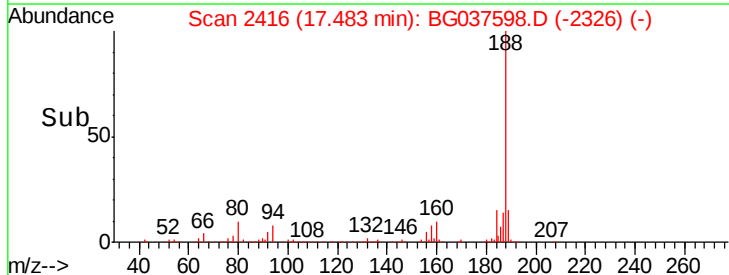


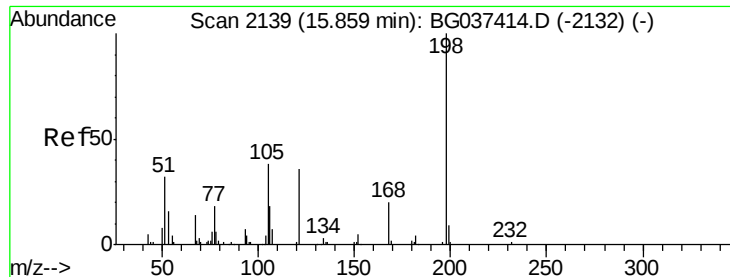




#65
 4,6-Dinitro-2-methylphenol
 Concen: 8.740 ng
 RT: 16.23 min Scan# 2202
 Delta R.T. 0.37 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20

Instrument :
 BNA_G
 ClientSampleId :
 CB-1018-S-TCLP-GRID40

Tot Ion:198 Resp: 603
 Ion Ratio Lower Upper
 198 100
 51 23.9 22.7 62.7
 105 20.0 19.7 59.7

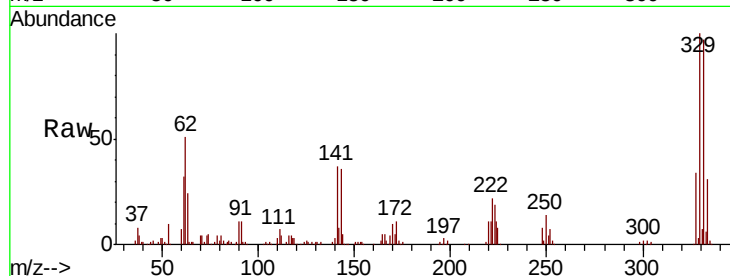


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BG
 Ion 105.00 (104.70 to 105.70): E

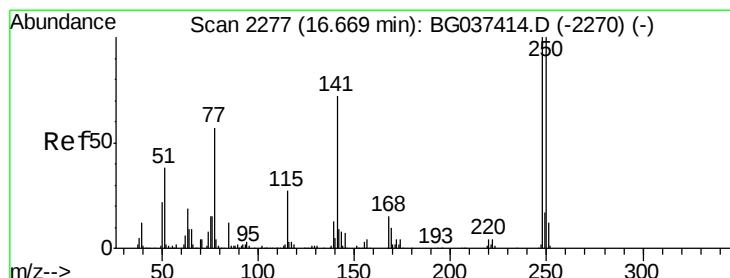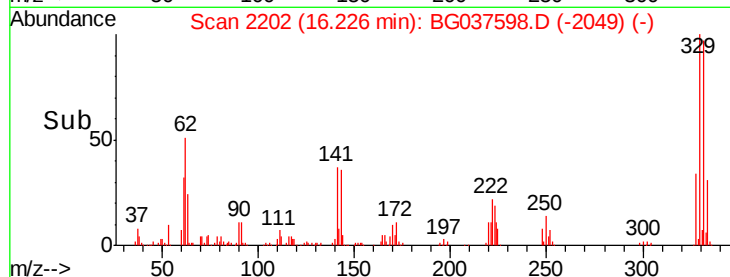
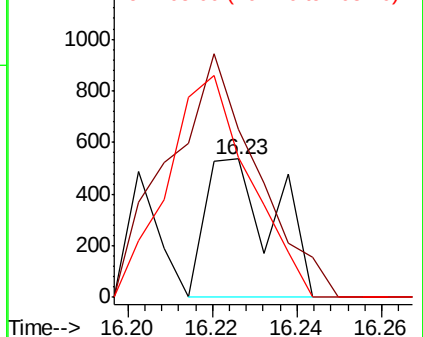



#67
 4-Bromophenyl-phenylether
 Concen: 3.564 ng
 RT: 16.22 min Scan# 2201
 Delta R.T. -0.45 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20

Tgt Ion:248 Resp: 15939
 Ion Ratio Lower Upper
 248 100
 250 177.8 77.0 115.6#
 141 369.5 55.5 83.3#

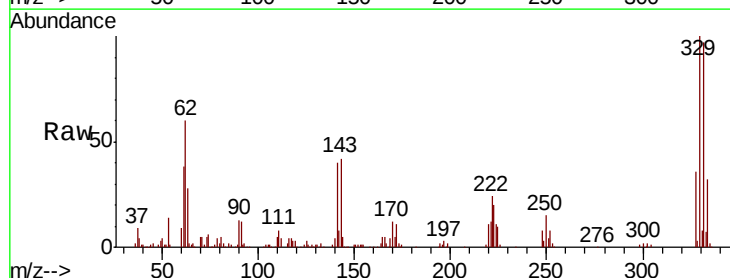

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E



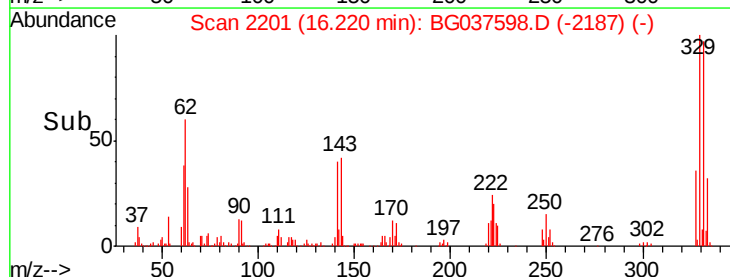
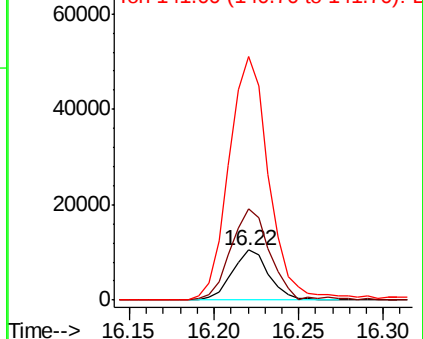




#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.77 min Scan# 3145
 Delta R.T. -0.01 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20




Instrument :
 BNA_G
 ClientSampleId :
 CB-1018-S-TCLP-GRID40


Tot Ion:240 Resp: 378449
 Ion Ratio Lower Upper
 240 100
 120 11.3 8.1 12.1
 236 26.7 21.4 32.0

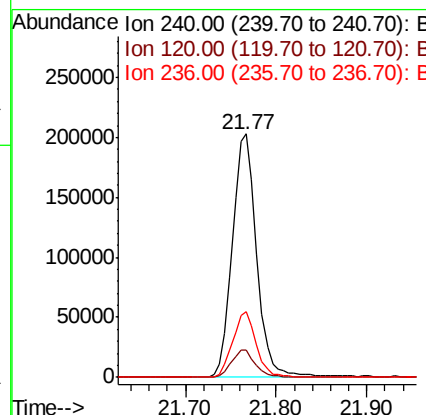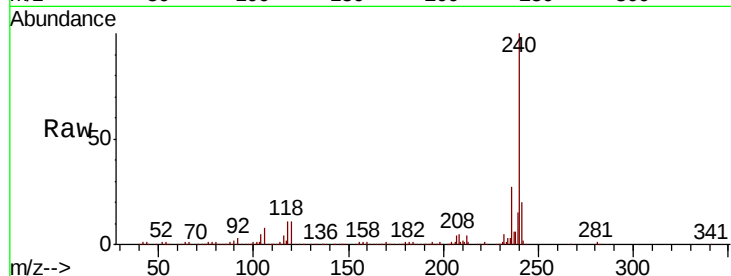

#79
 Terphenyl-d14
 Concen: 80.682 ng
 RT: 20.08 min Scan# 2858
 Delta R.T. -0.01 min
 Lab File: BG037598.D
 Acq: 27 Oct 2018 2:20

Tgt Ion:244 Resp: 1428976
 Ion Ratio Lower Upper
 244 100
 212 8.7 6.5 9.7
 122 12.1 9.0 13.4

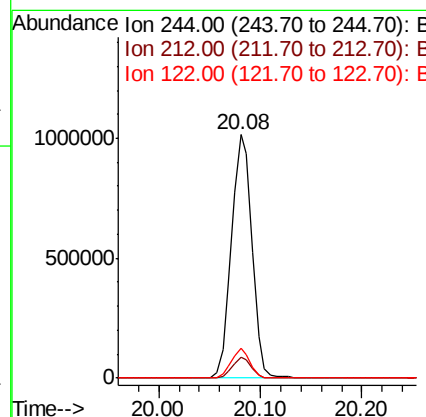

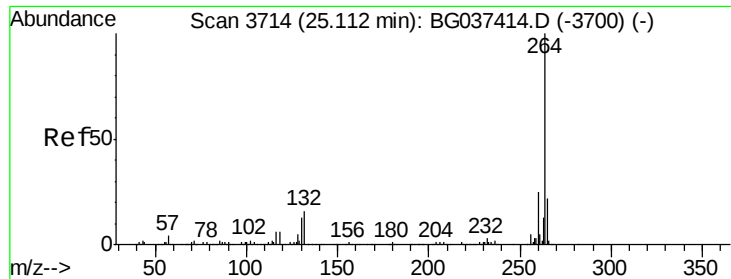

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.10 min Scan# 3712
Delta R.T. -0.01 min
Lab File: BG037598.D
Acq: 27 Oct 2018 2:20

Instrument :
BNA_G
ClientSampleId :
CB-1018-S-TCLP-GRID40

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.5	18.2	27.4
265	21.9	17.9	26.9

