

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102618\
 Data File : BG037610.D
 Acq On : 27 Oct 2018 10:10
 Operator : JU/SJ
 Sample : J5662-16
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 29 04:11:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	58909	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	254630	20.00	ng	0.00
39) Acenaphthene-d10	14.73	164	176660	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	431854	20.00	ng	0.00
76) Chrysene-d12	21.77	240	392728	20.00	ng	0.00
87) Perylene-d12	25.10	264	380023	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	145122	41.19	ng	0.00
7) Phenol-d6	7.24	99	129233	24.26	ng	0.00
23) Nitrobenzene-d5	9.28	82	443516	97.57	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	174410	90.52	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	1063061	90.74	ng	0.00
79) Terphenyl-d14	20.09	244	1636573	89.04	ng	0.00
Target Compounds						
10) Phenol	7.27	94	28126	5.003	ng	93
19) n-Nitroso-di-n-propylamine	9.28	70	56718	15.459	ng	# 68
51) 2,6-Dinitrotoluene	14.73	165	23193	7.671	ng	# 24
57) 2,4-Dinitrotoluene	14.73	165	23193	5.844	ng	# 24
65) 4,6-Dinitro-2-methylphenol	16.22	198	505	8.691	ng	86
67) 4-Bromophenyl-phenylether	16.23	248	12408	2.616	ng	# 1
77) Benzidine	20.08	184	28304	2.120	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102618\
Data File : BG037610.D
Acq On : 27 Oct 2018 10:10
Operator : JU/SJ
Sample : J5662-16
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 29 04:11:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

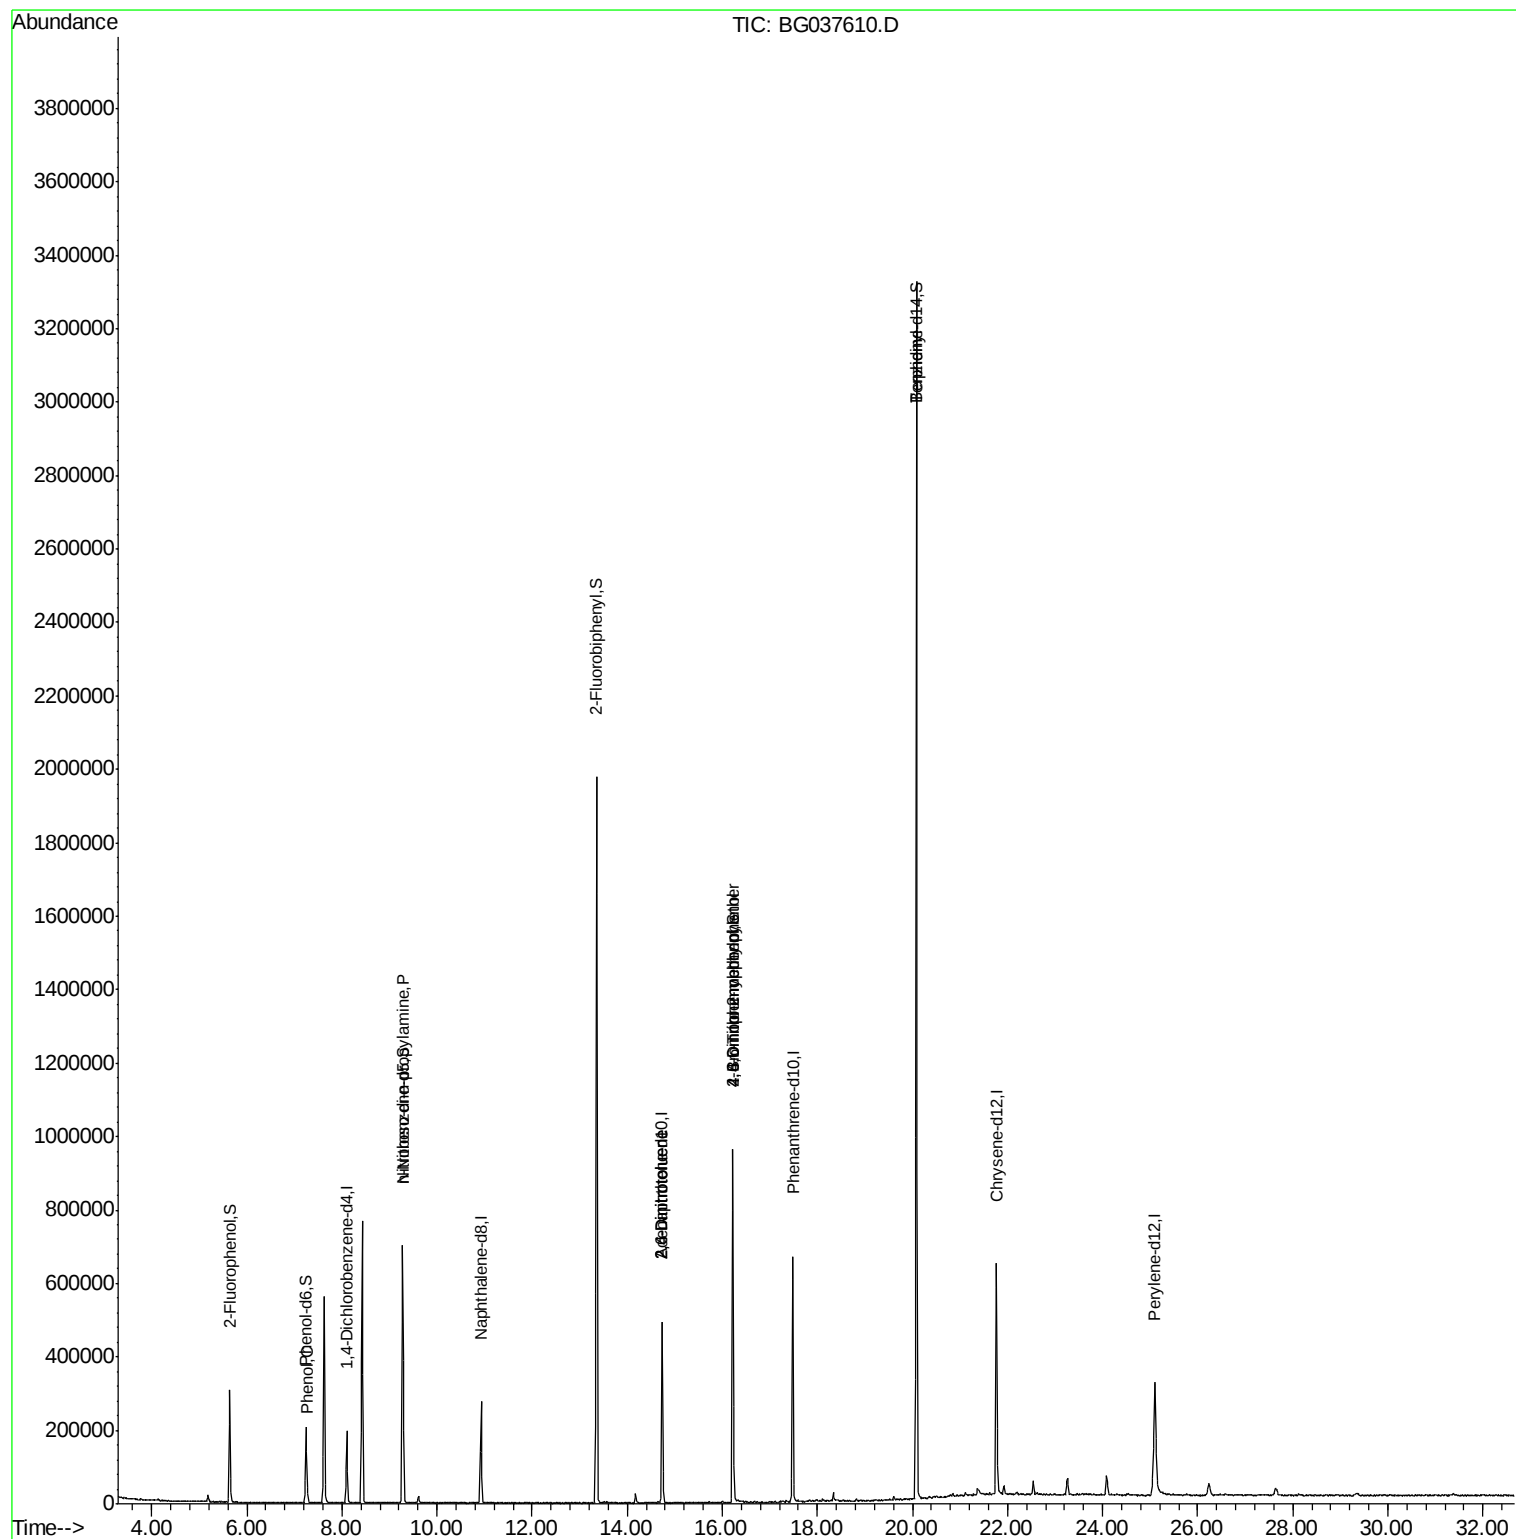

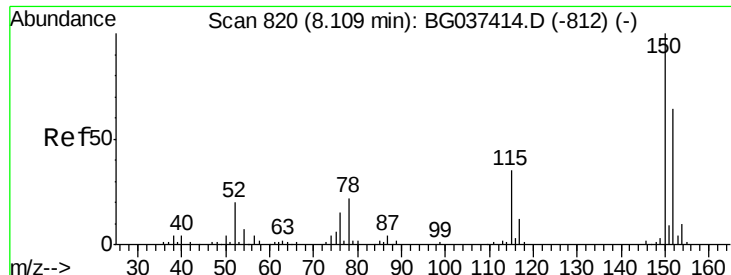


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 819
Delta R.T. -0.01 min
Lab File: BG037610.D
Acq: 27 Oct 2018 10:10

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	152.9	126.0	189.0
115	56.9	45.5	68.3

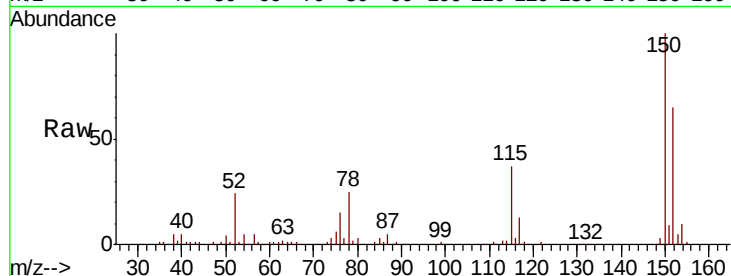


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

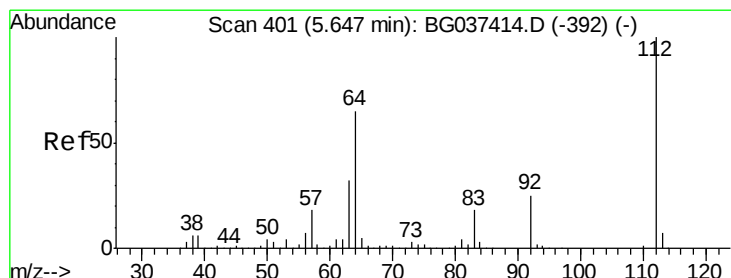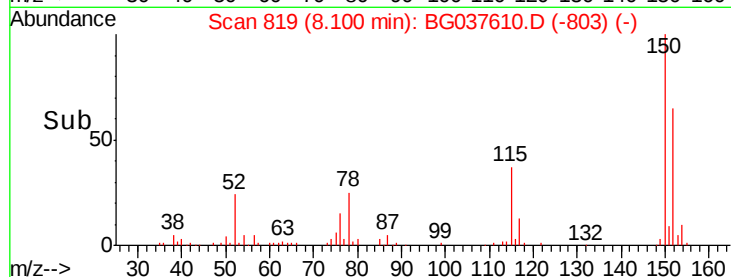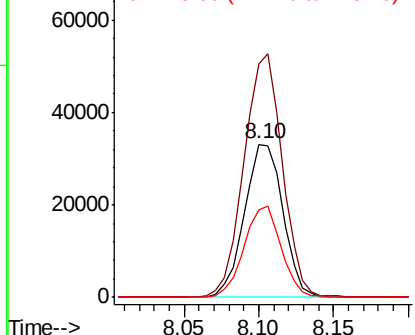



#5

2-Fluorophenol
Concen: 41.186 ng
RT: 5.64 min Scan# 401
Delta R.T. -0.00 min
Lab File: BG037610.D
Acq: 27 Oct 2018 10:10

Tgt Ion	Ratio	Lower	Upper
112	100		
64	65.4	53.1	79.7
63	32.8	27.3	40.9

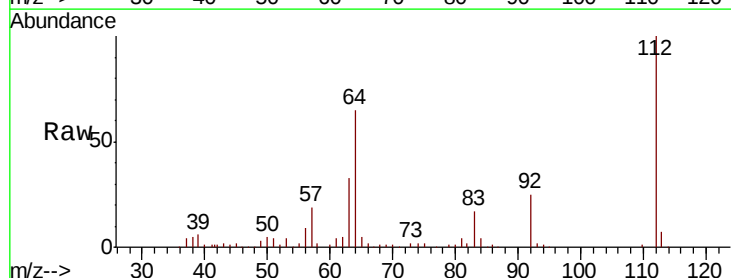

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

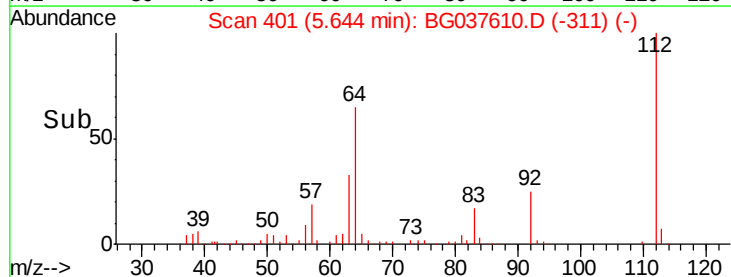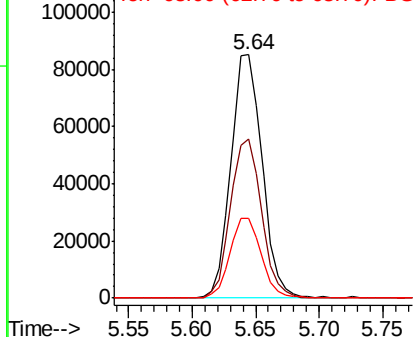



#7

Phenol-d6

Concen: 24.255 ng

RT: 7.24 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037610.D

Acq: 27 Oct 2018 10:10

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 129233

Ion Ratio Lower Upper




99 100

42 18.0 15.0 22.4

71 30.1 25.5 38.3

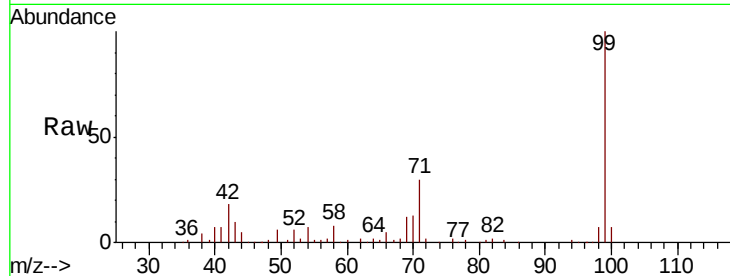

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

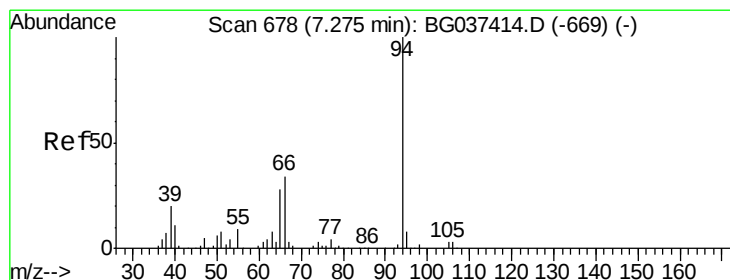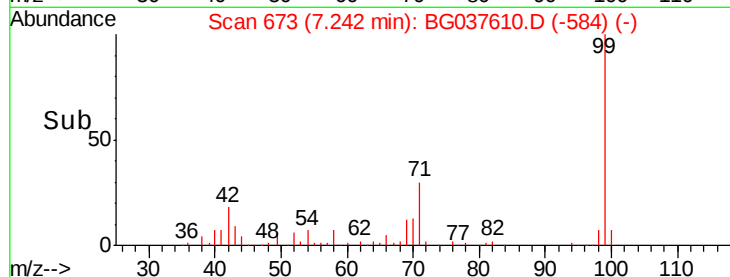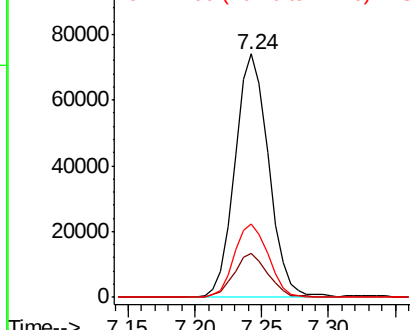

#10

Phenol

Concen: 5.003 ng

RT: 7.27 min Scan# 678

Delta R.T. -0.00 min

Lab File: BG037610.D

Acq: 27 Oct 2018 10:10


Tgt Ion: 94 Resp: 28126

Ion Ratio Lower Upper



94 100

65 30.8 9.7 49.7

66 42.0 15.9 55.9

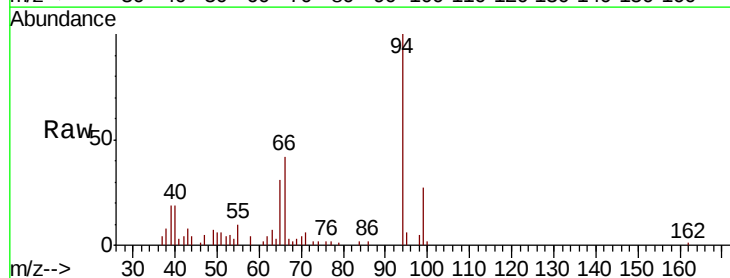

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC


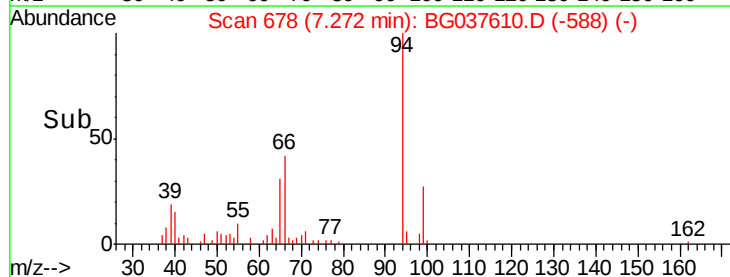
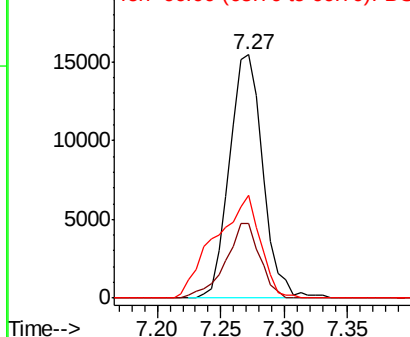




#19
n-Nitroso-di-n-propylamine
Concen: 15.459 ng
RT: 9.28 min Scan# 1020
Delta R.T. 0.37 min
Lab File: BG037610.D
Acq: 27 Oct 2018 10:10




Instrument :
BNA_G
ClientSampleId :

Tot Ion: 70 Resp: 56718
Ion Ratio Lower Upper
70 100
42 44.5 53.9 80.9#
101 0.0 8.2 12.2#
130 1.5 18.2 27.4#

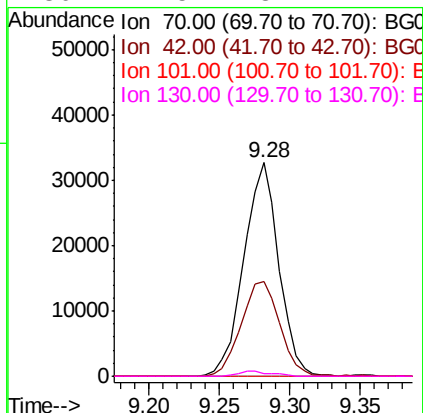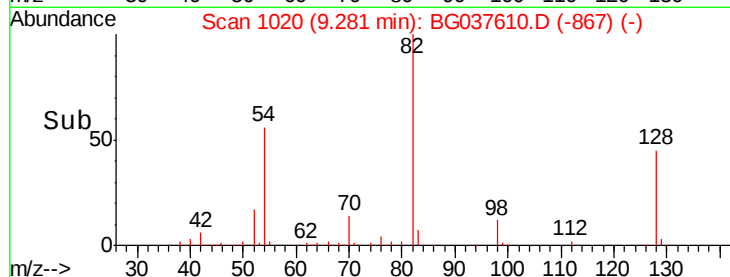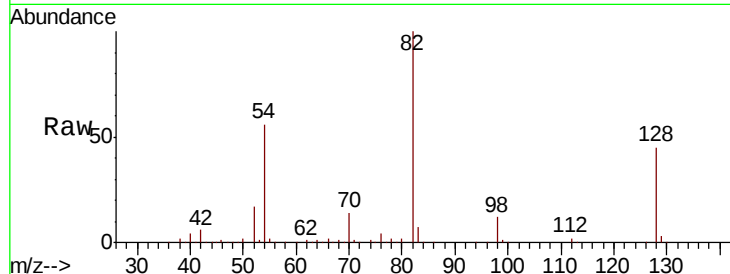

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.93 min Scan# 1300
Delta R.T. -0.00 min
Lab File: BG037610.D
Acq: 27 Oct 2018 10:10

Tgt Ion: 136 Resp: 254630
Ion Ratio Lower Upper
136 100
137 11.7 9.6 14.4
54 9.9 7.9 11.9
68 6.4 4.8 7.2


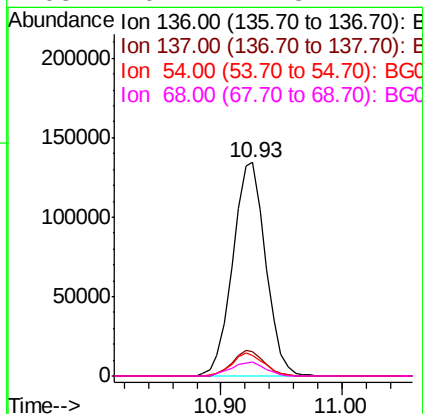
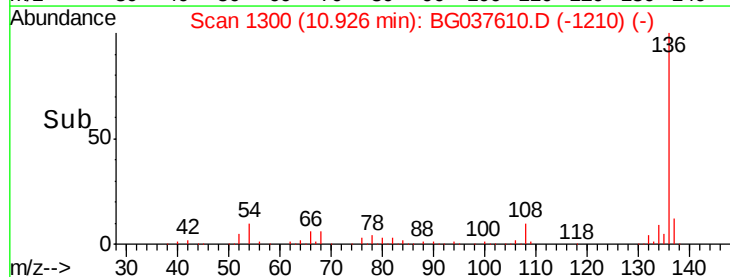
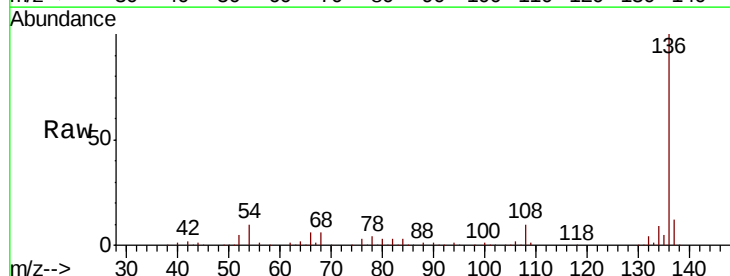




#23
 Nitrobenzene-d5
 Concen: 97.574 ng
 RT: 9.28 min Scan# 1020
 Delta R.T. -0.00 min
 Lab File: BG037610.D
 Acq: 27 Oct 2018 10:10




Instrument :
 BNA_G
 ClientSampleID :


Tot Ion	82	Resp	443516
Ion Ratio	Lower	Upper	
82	100		
128	45.5	34.6	51.8
54	56.1	45.3	67.9

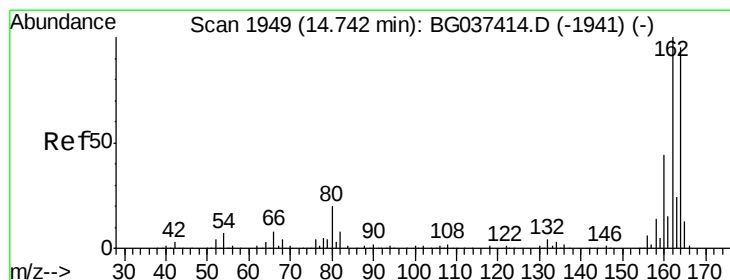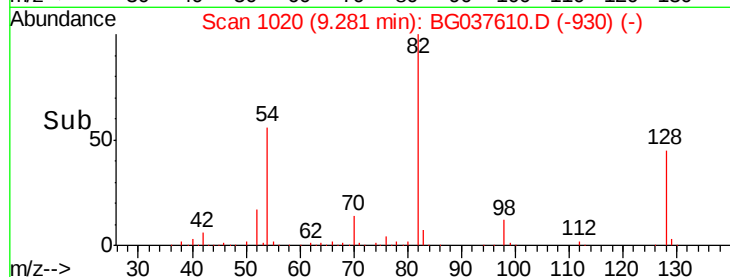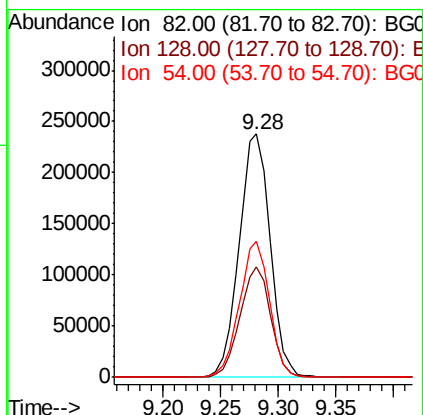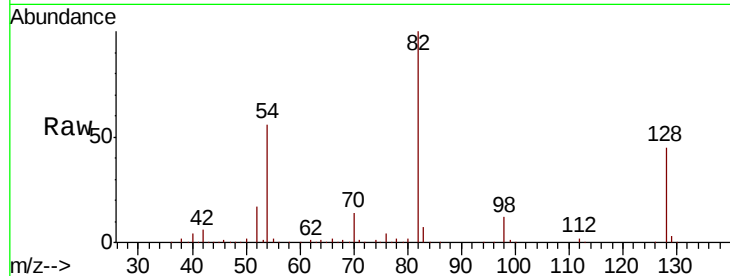

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.73 min Scan# 1948
 Delta R.T. -0.01 min
 Lab File: BG037610.D
 Acq: 27 Oct 2018 10:10

Tgt Ion	164	Resp	176660
Ion Ratio	Lower	Upper	
164	100		
162	104.4	81.3	121.9
160	46.0	36.3	54.5

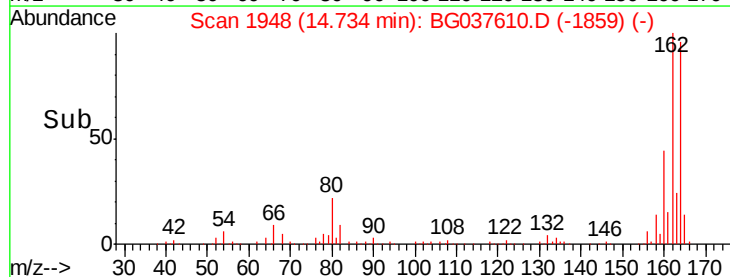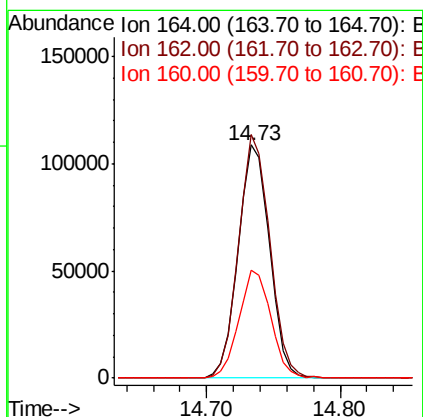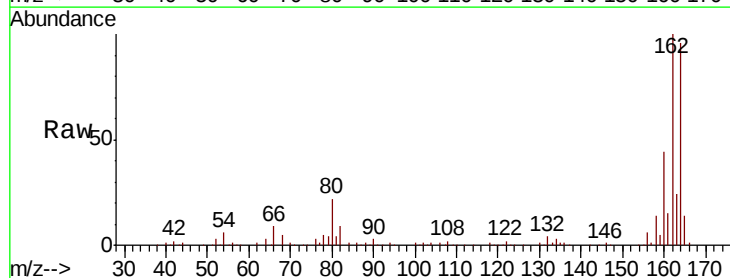


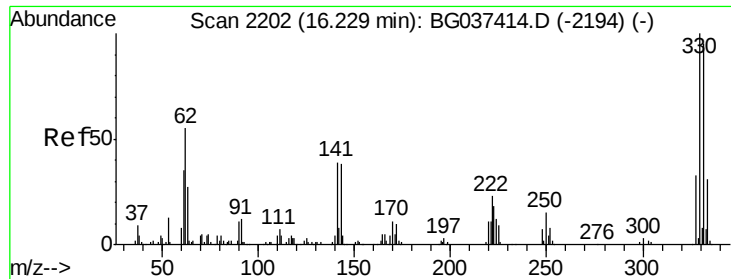

#42
 2,4,6-Tribromophenol
 Concen: 90.517 ng
 RT: 16.22 min Scan# 2201
 Delta R.T. -0.01 min
 Lab File: BG037610.D
 Acq: 27 Oct 2018 10:10

Instrument :
 BNA_G
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.1	78.4	117.6
141	40.9	32.2	48.2



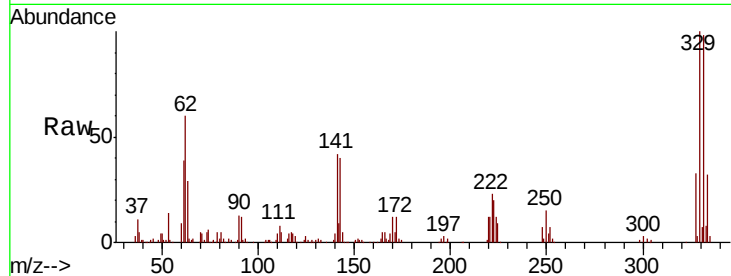


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

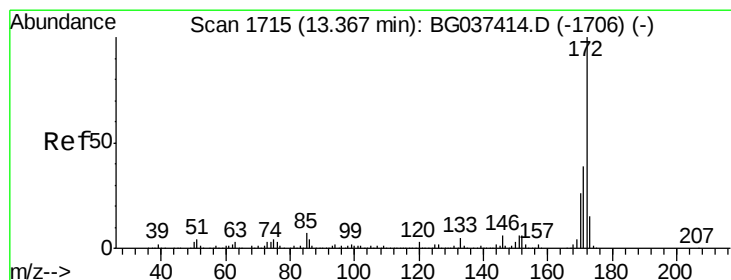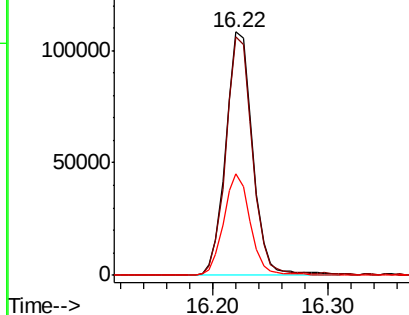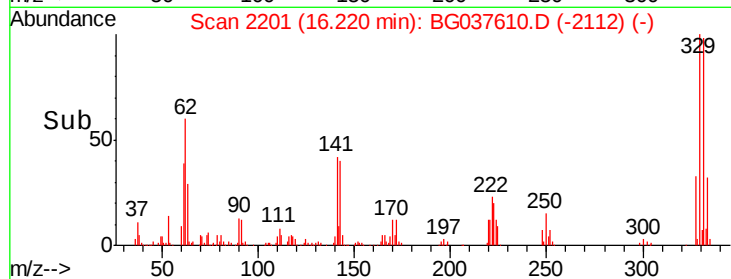

#45
 2-Fluorobiphenyl
 Concen: 90.741 ng
 RT: 13.36 min Scan# 1714
 Delta R.T. -0.01 min
 Lab File: BG037610.D
 Acq: 27 Oct 2018 10:10

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.4	31.0	46.4
170	25.5	20.2	30.2


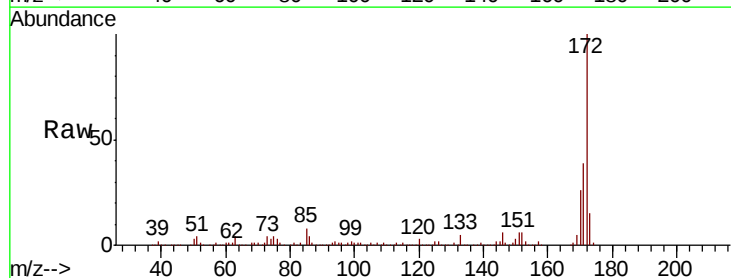



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

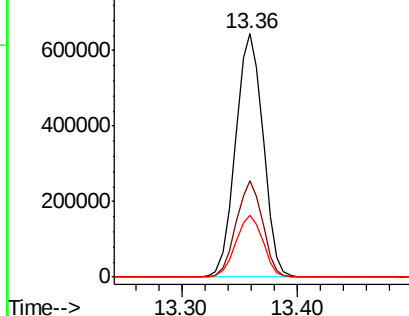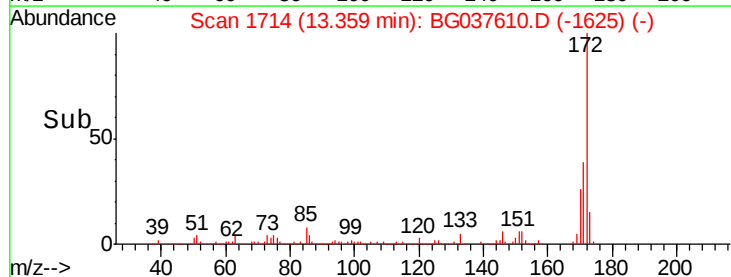

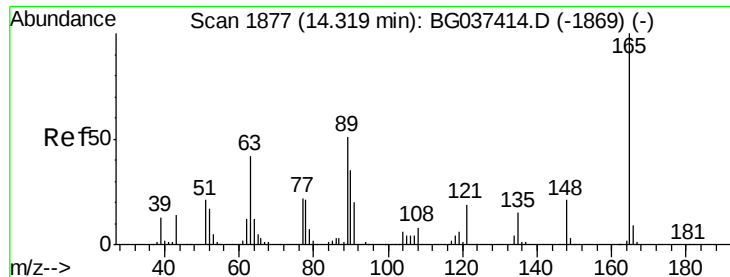

#51

2,6-Dinitrotoluene

Concen: 7.671 ng

RT: 14.73 min Scan# 1948

Delta R.T. 0.41 min

Lab File: BG037610.D

Acq: 27 Oct 2018 10:10

Instrument :

BNA_G

ClientSampleId :


Tot Ion:165 Resp: 23193

Ion Ratio Lower Upper

165 100

63 0.0 43.4 65.2#




89 1.4 45.8 68.6#

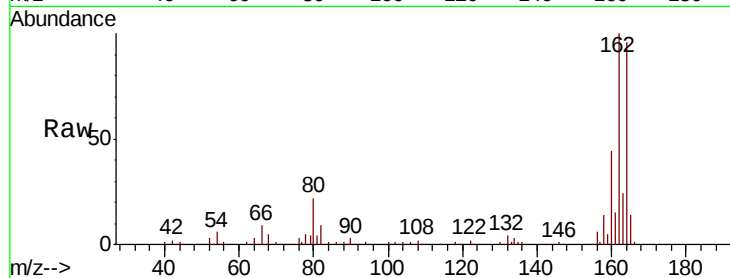

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

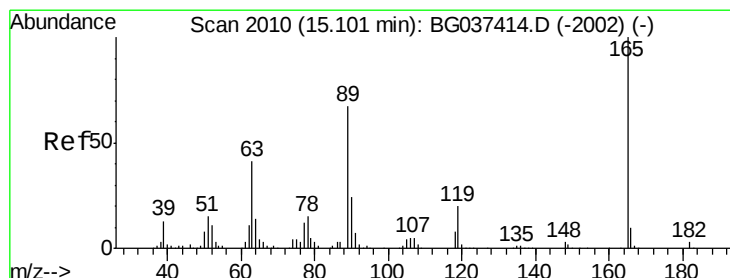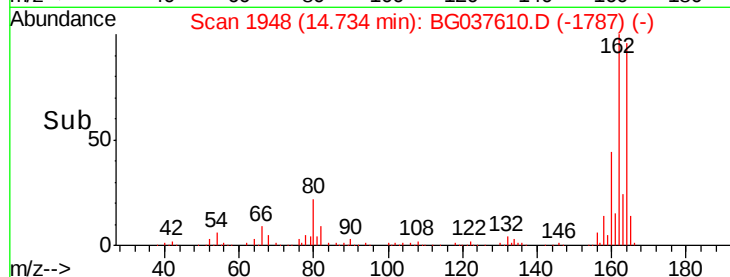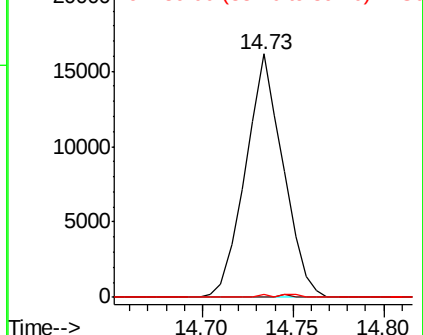

#57

2,4-Dinitrotoluene

Concen: 5.844 ng

RT: 14.73 min Scan# 1948

Delta R.T. -0.37 min

Lab File: BG037610.D

Acq: 27 Oct 2018 10:10

Tgt Ion:165 Resp: 23193


Ion Ratio Lower Upper

165 100

63 0.0 33.4 50.0#

89 1.4 57.2 85.8#

182 0.0 2.6 4.0#


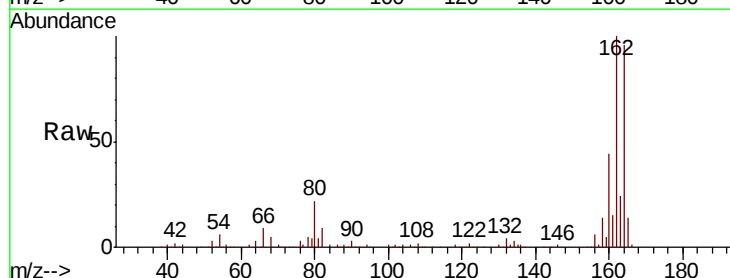



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

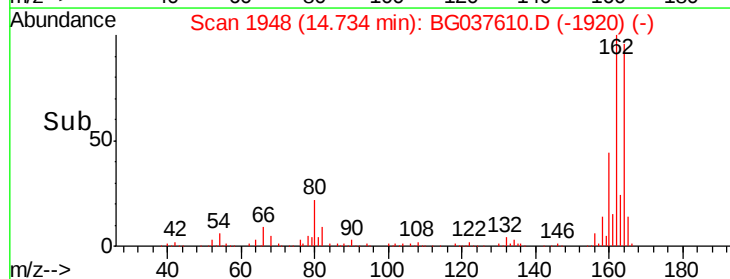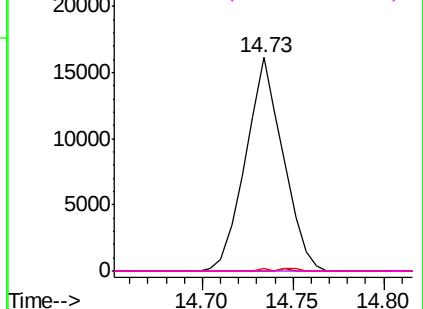

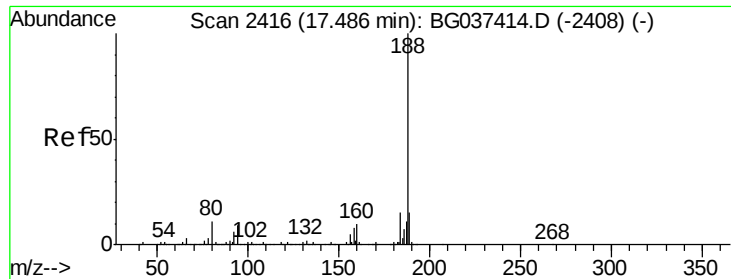

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.48 min Scan# 2416

Delta R.T. -0.00 min

Lab File: BG037610.D

Acq: 27 Oct 2018 10:10

Instrument :

BNA_G

ClientSampleId :


Tot Ion:188 Resp: 431854

Ion Ratio Lower Upper

188 100

94 9.1 7.2 10.8




80 10.6 7.7 11.5

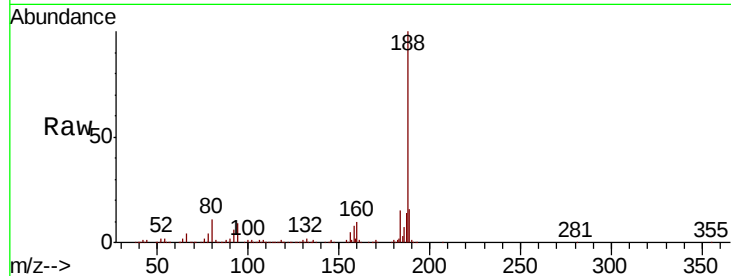

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

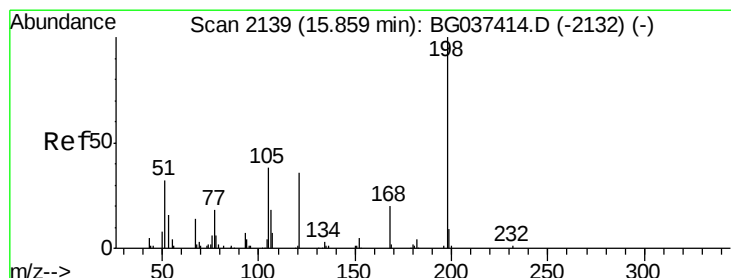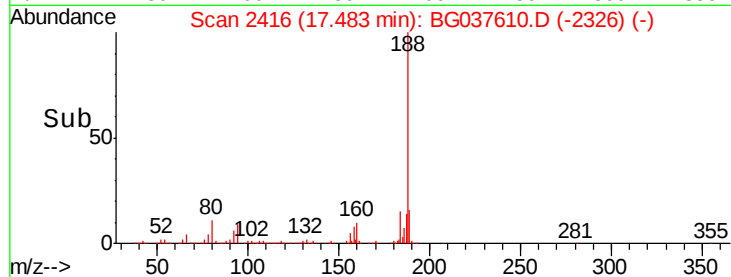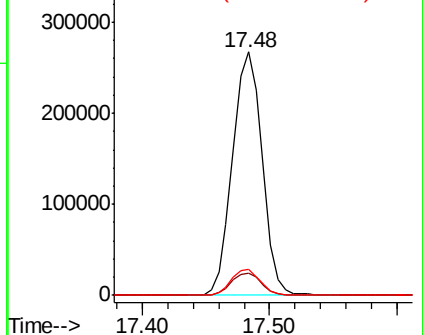

#65

4,6-Dinitro-2-methylphenol

Concen: 8.691 ng

RT: 16.22 min Scan# 2201

Delta R.T. 0.36 min

Lab File: BG037610.D

Acq: 27 Oct 2018 10:10


Tgt Ion:198 Resp: 505

Ion Ratio Lower Upper

198 100

51 29.9 22.7 62.7



105 34.5 19.7 59.7

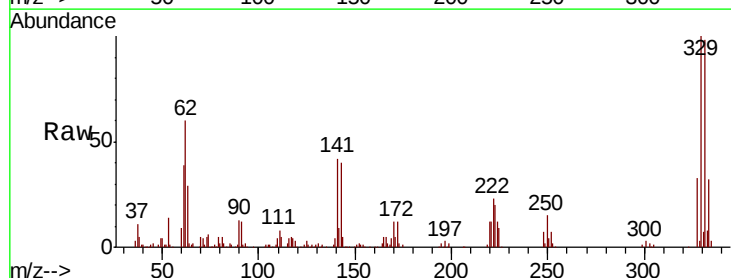

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BG

Ion 105.00 (104.70 to 105.70): E

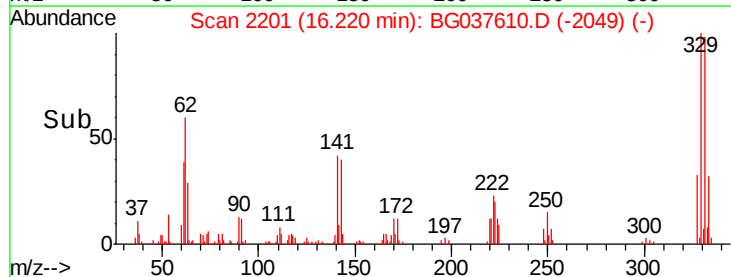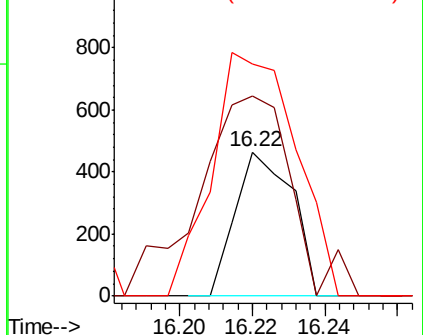







#67
4-Bromophenyl-phenylether
Concen: 2.616 ng
RT: 16.23 min Scan# 2202
Delta R.T. -0.44 min
Lab File: BG037610.D
Acq: 27 Oct 2018 10:10

Instrument :
BNA_G
ClientSampleId :

Tot Ion:248 Resp: 12408
Ion Ratio Lower Upper
248 100
250 187.4 77.0 115.6#
141 378.2 55.5 83.3#

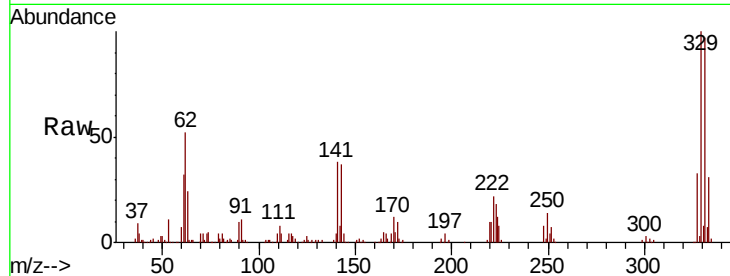


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

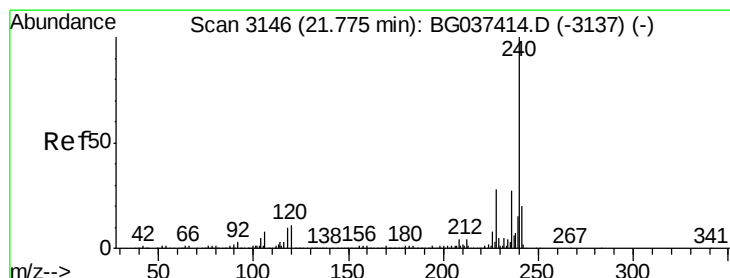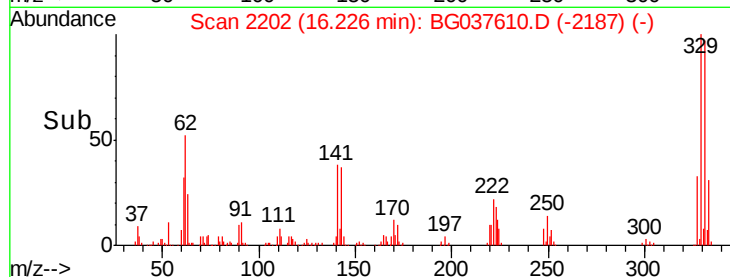
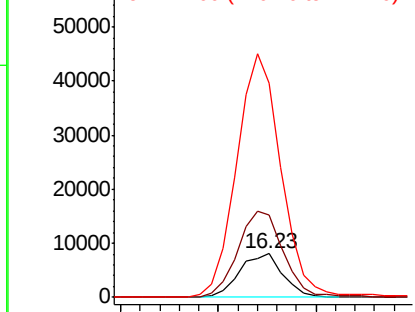



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.77 min Scan# 3145
Delta R.T. -0.01 min
Lab File: BG037610.D
Acq: 27 Oct 2018 10:10

Tgt Ion:240 Resp: 392728
Ion Ratio Lower Upper
240 100
120 11.1 8.1 12.1
236 26.5 21.4 32.0

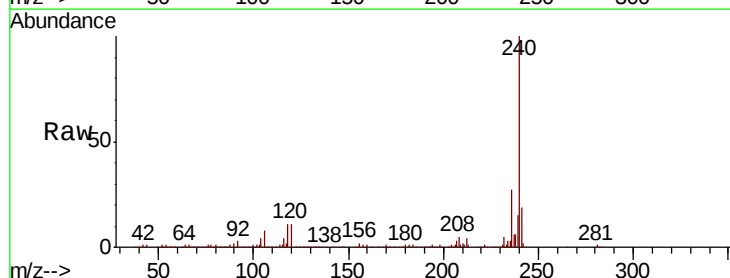

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



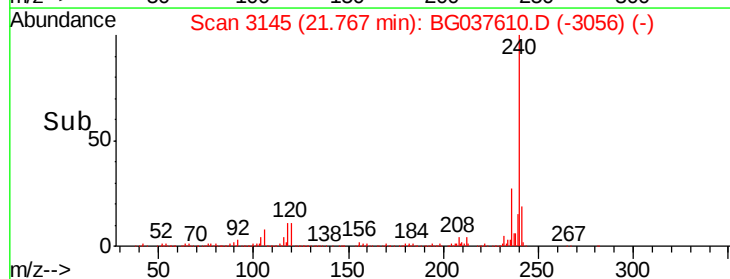
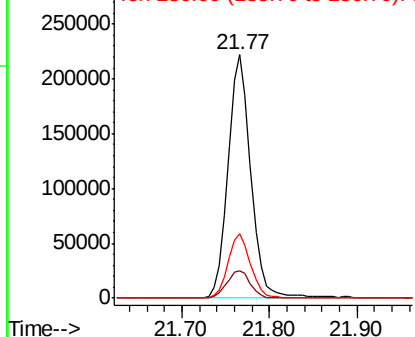


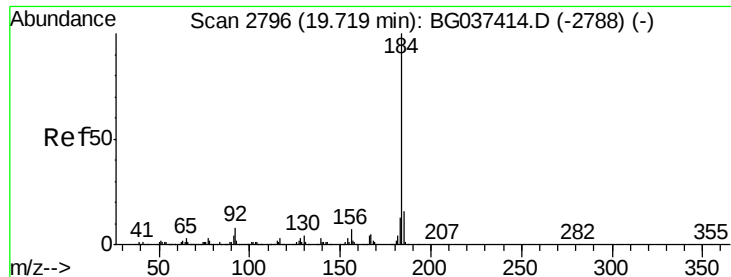

#77
Benzidine
Concen: 2.120 ng
RT: 20.08 min Scan# 2858
Delta R.T. 0.36 min
Lab File: BG037610.D
Acq: 27 Oct 2018 10:10




Instrument :
BNA_G
ClientSampled :


Tot Ion:184 Resp: 28304
Ion Ratio Lower Upper
184 100
185 14.4 12.6 18.8
183 10.4 10.2 15.2

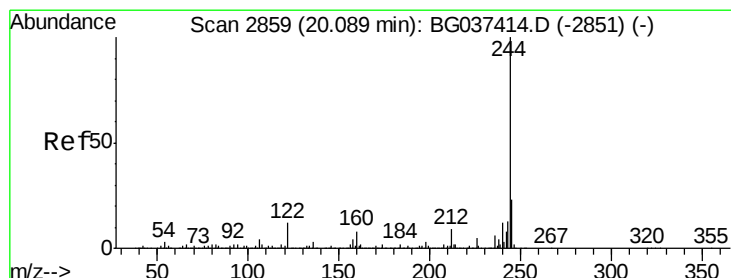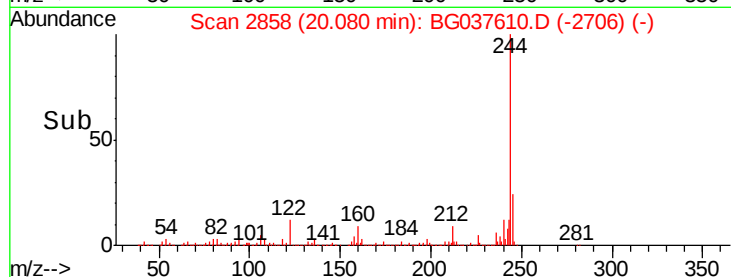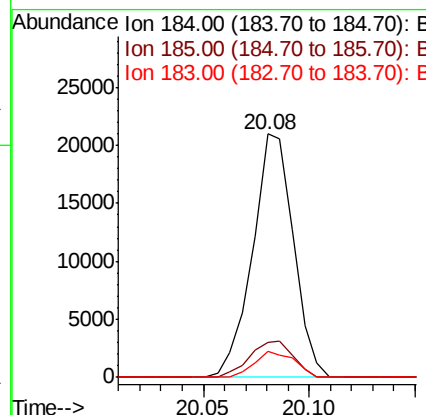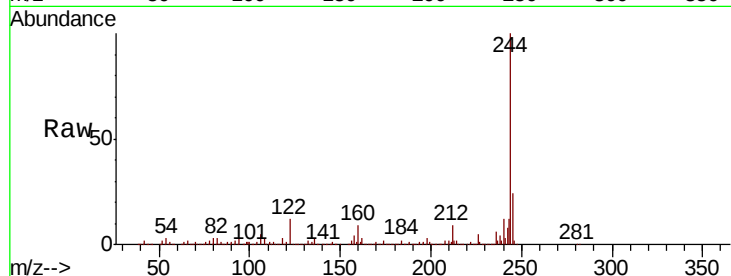

#79
Terphenyl-d14
Concen: 89.043 ng
RT: 20.09 min Scan# 2859
Delta R.T. -0.00 min
Lab File: BG037610.D
Acq: 27 Oct 2018 10:10

Tgt Ion:244 Resp: 1636573
Ion Ratio Lower Upper
244 100
212 8.8 6.5 9.7
122 11.7 9.0 13.4

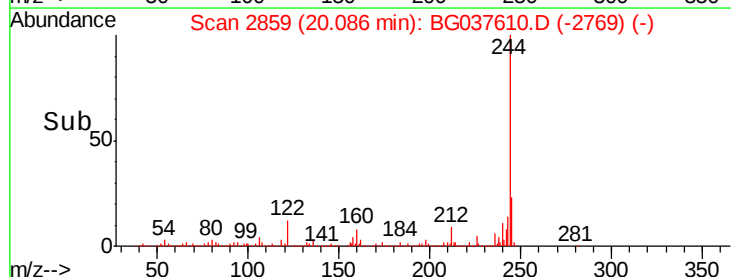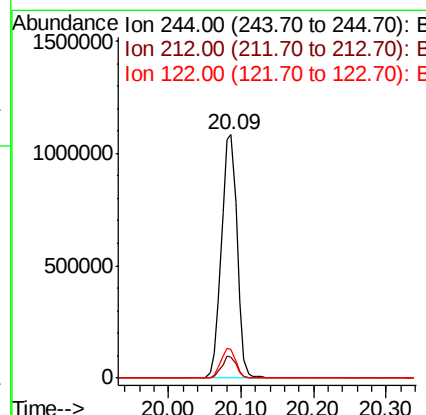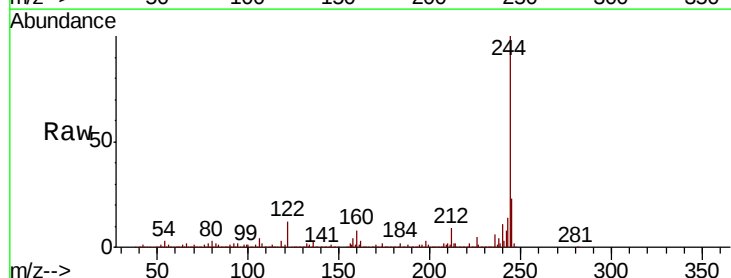

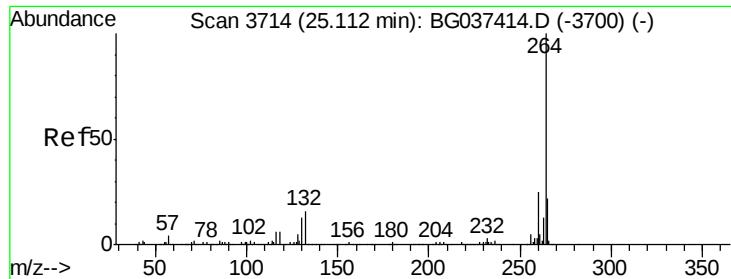

#87
Pervlone-d12
Concen: 20.000 ng
RT: 25.10 min Scan# 3712
Delta R.T. -0.01 min
Lab File: BG037610.D
Acq: 27 Oct 2018 10:10

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.3	18.2	27.4
265	21.6	17.9	26.9

