
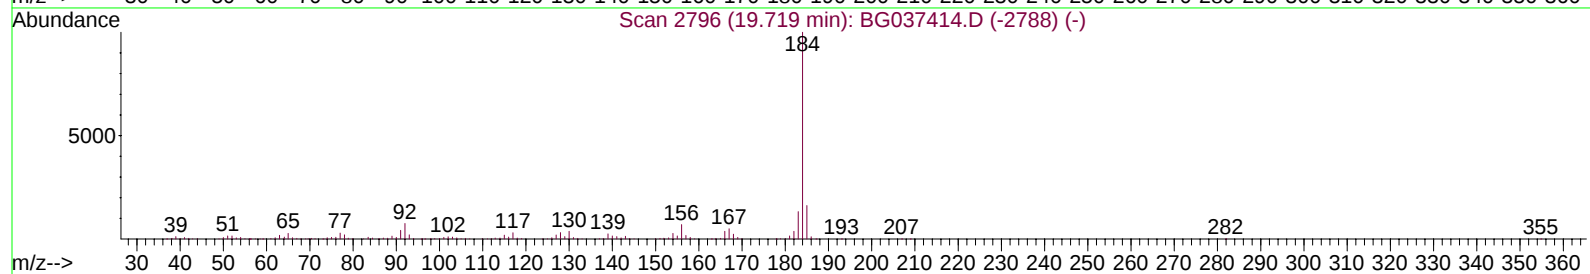
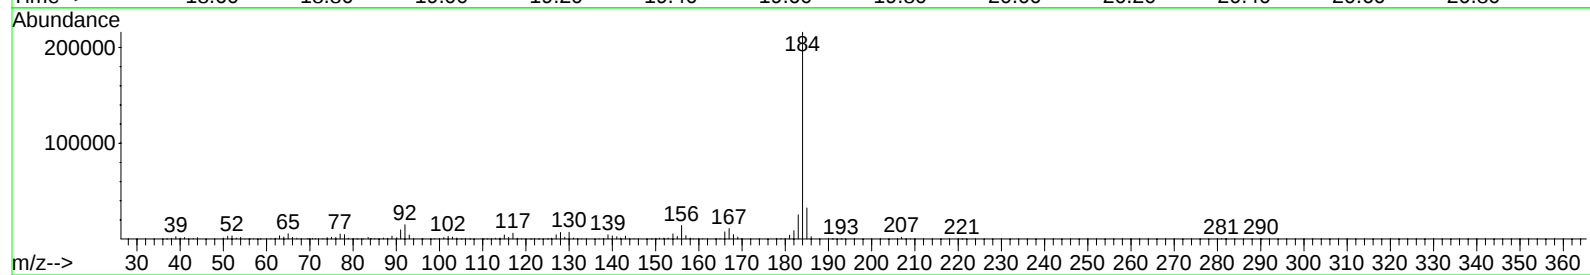


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102618\
 Data File : BG037596.D
 Acq On : 27 Oct 2018 1:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 05:19:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration

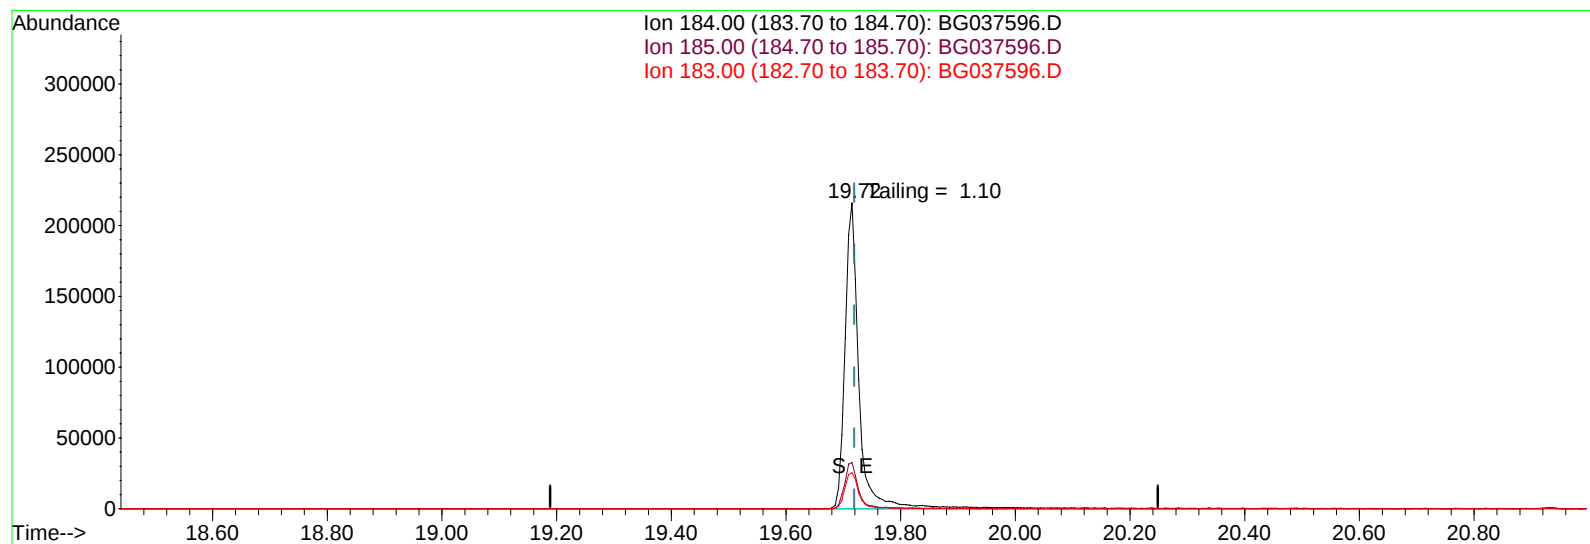

TIC: BG037596.D

(77) Benzidine




19.715min (-0.004) 59169.27ng

response 354096

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.10
183.00	12.70	11.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102618\
Data File : BG037596.D
Acq On : 27 Oct 2018 1:01
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 05:19:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

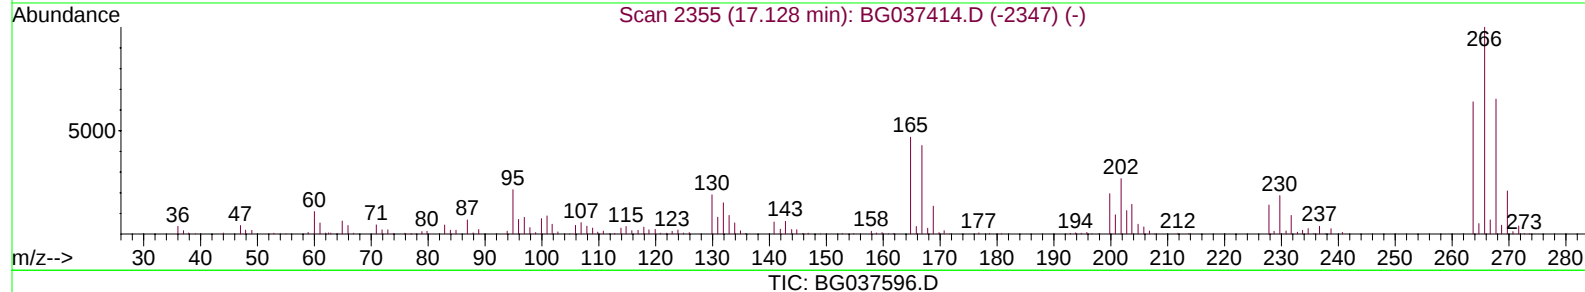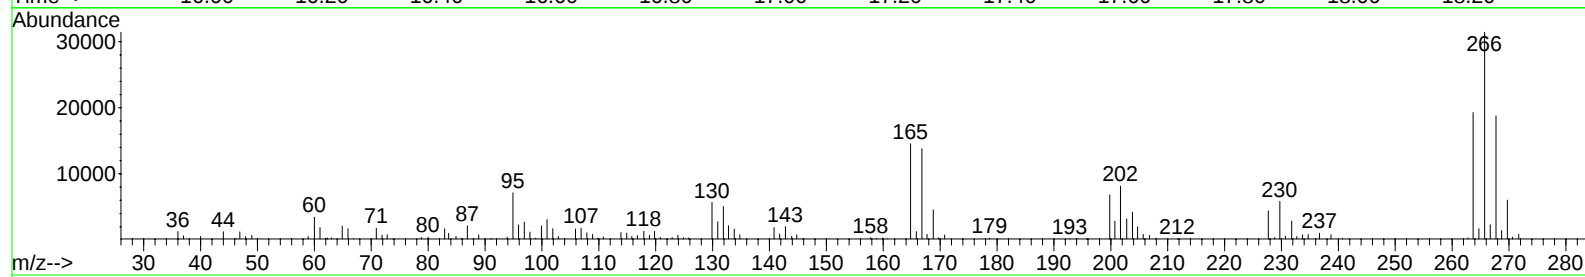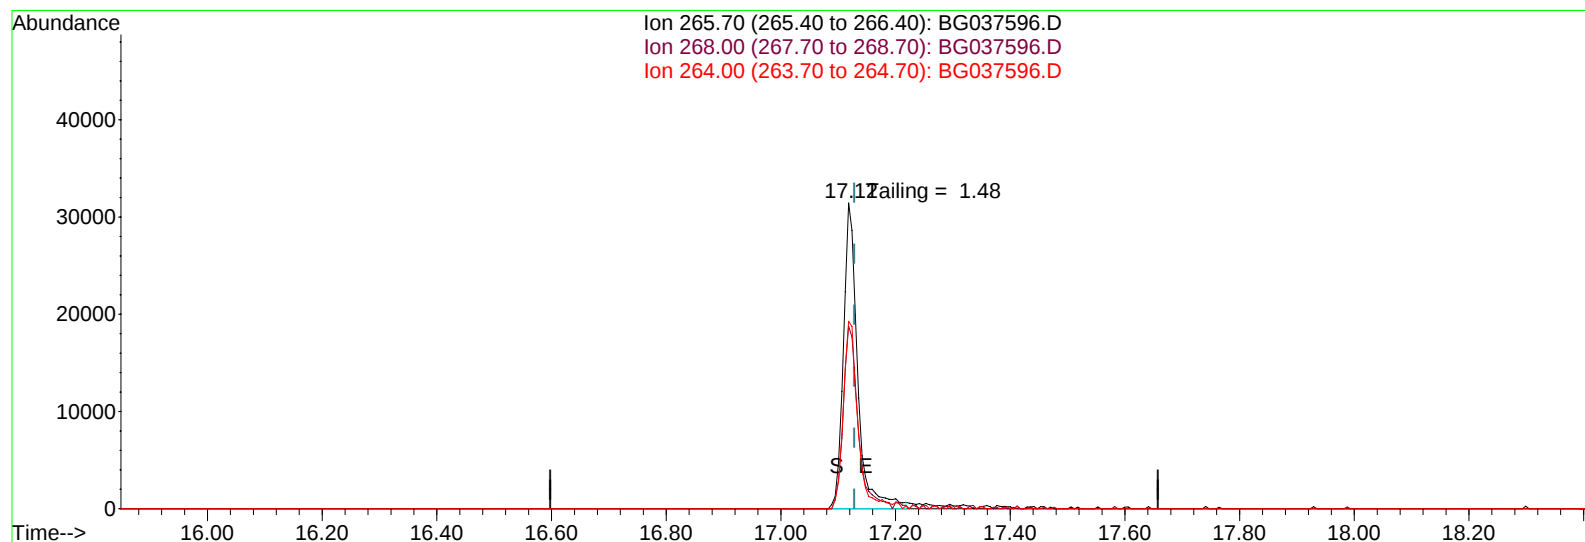

(70) Pentachlorophenol (C)

17.118min (-0.010) 41336.59ng

response 55149

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	64.28
264.00	73.60	66.70
0.00	0.00	0.00