

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102618\
 Data File : BG037601.D
 Acq On : 27 Oct 2018 4:17
 Operator : JU/SJ
 Sample : J5661-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 VB44949

Quant Time: Oct 27 07:00:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	58424	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	257337	20.00	ng	0.00
39) Acenaphthene-d10	14.73	164	172297	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	422252	20.00	ng	0.00
76) Chrysene-d12	21.77	240	385311	20.00	ng	0.00
87) Perylene-d12	25.10	264	358525	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	389986	111.60	ng	0.00
7) Phenol-d6	7.24	99	497400	94.13	ng	0.00
23) Nitrobenzene-d5	9.28	82	371905	80.96	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	209557	111.51	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	885136	77.47	ng	0.00
79) Terphenyl-d14	20.08	244	1377302	76.38	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102618\
Data File : BG037601.D
Acq On : 27 Oct 2018 4:17
Operator : JU/SJ
Sample : J5661-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
VB44949

Quant Time: Oct 27 07:00:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

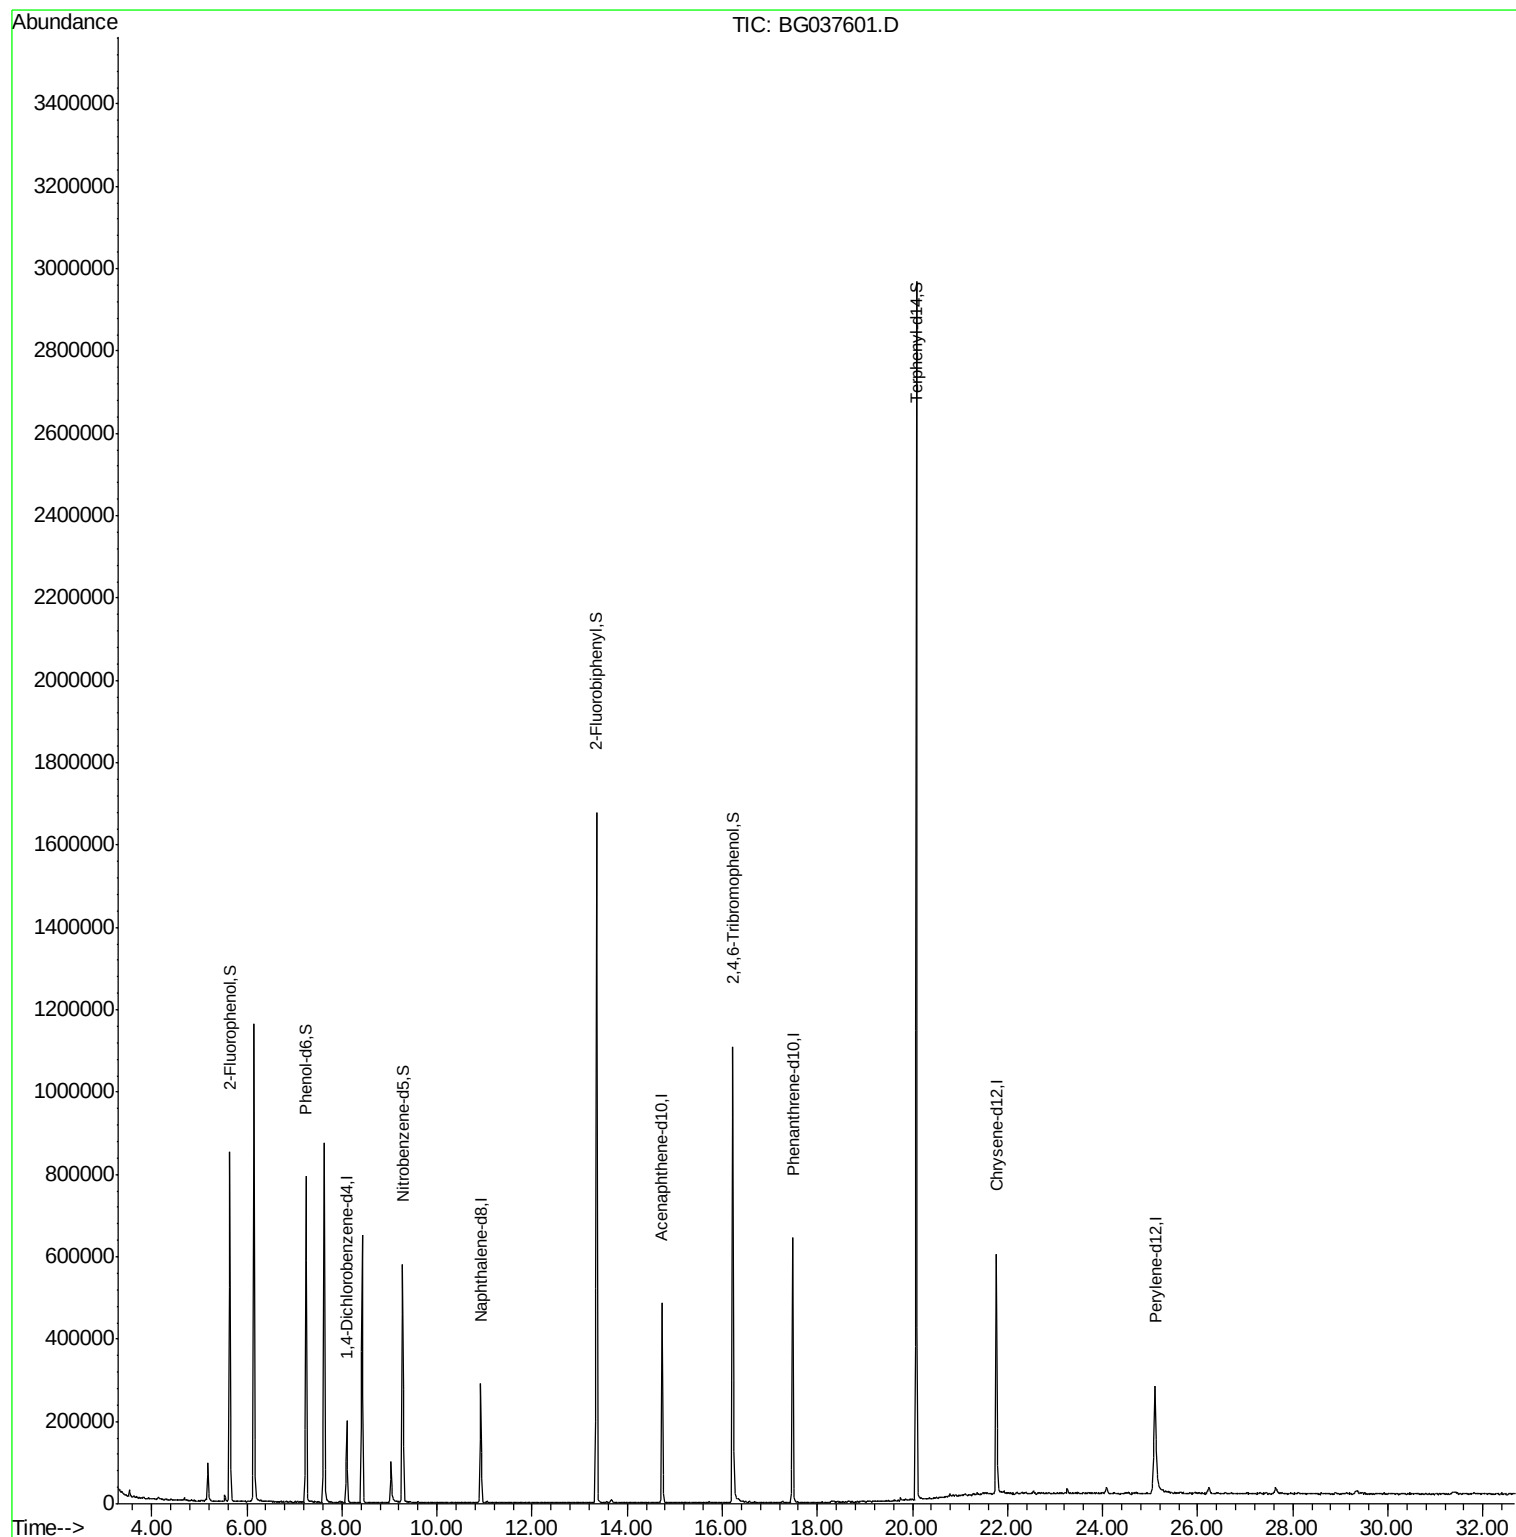

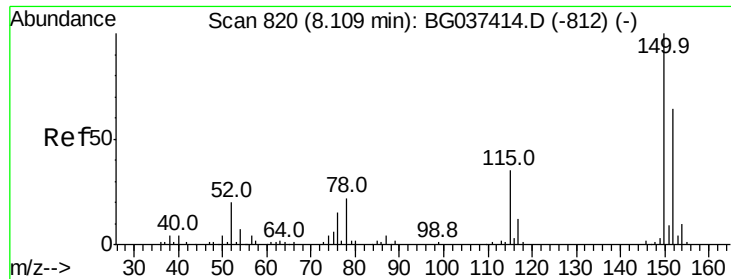


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 819
Delta R.T. -0.01 min
Lab File: BG037601.D
Acq: 27 Oct 2018 4:17

Instrument :
BNA_G
ClientSampleId :
VB44949

Tot Ion:152 Resp: 58424
Ion Ratio Lower Upper
152 100
150 154.1 126.0 189.0
115 57.1 45.5 68.3

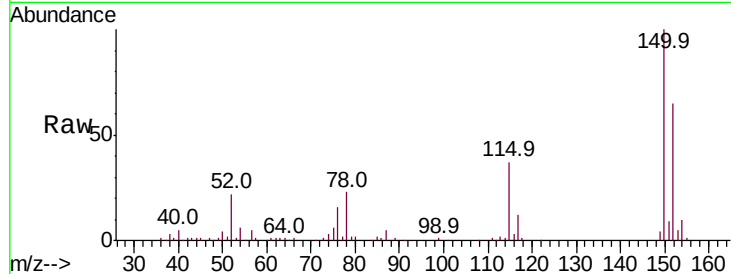


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

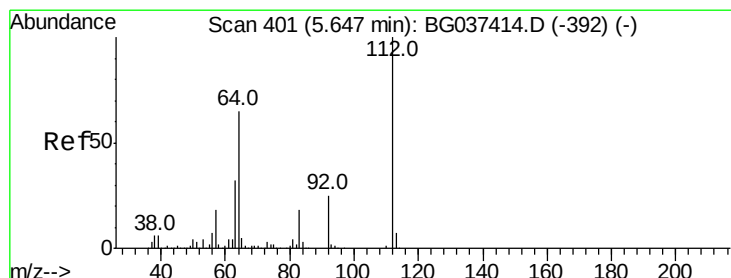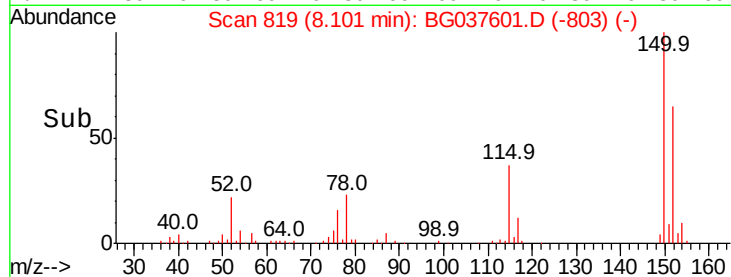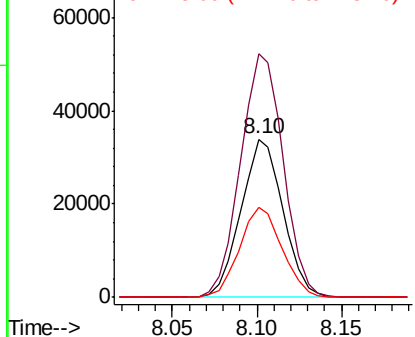



#5


2-Fluorophenol
Concen: 111.598 ng
RT: 5.64 min Scan# 401
Delta R.T. -0.00 min
Lab File: BG037601.D
Acq: 27 Oct 2018 4:17

Tgt Ion:112 Resp: 389986
Ion Ratio Lower Upper
112 100
64 65.3 53.1 79.7
63 33.6 27.3 40.9

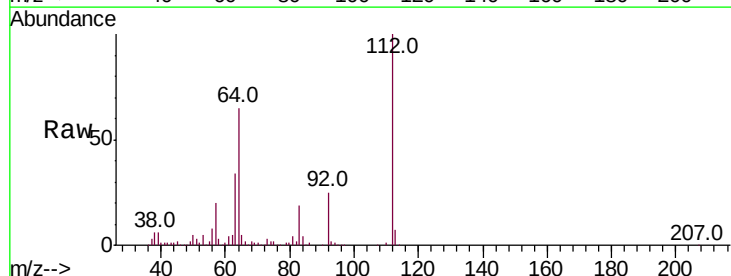

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

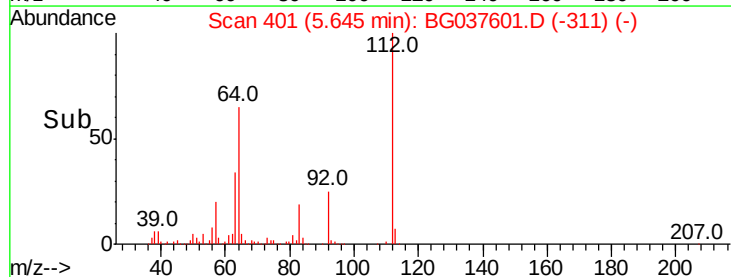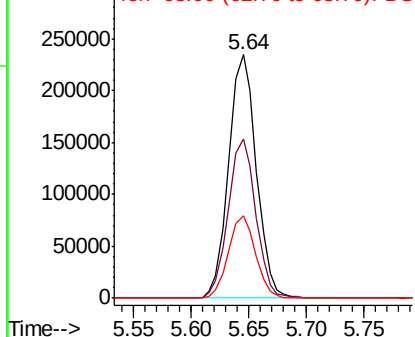

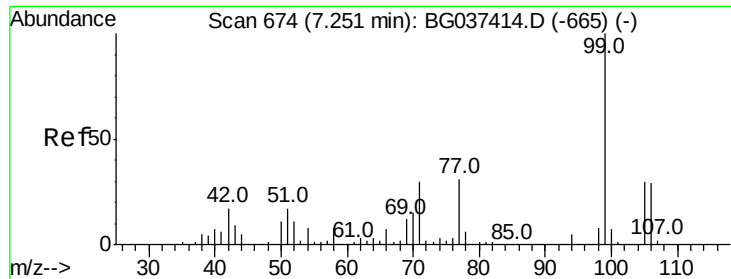

#7

Phenol-d6

Concen: 94.129 ng

RT: 7.24 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037601.D

Acq: 27 Oct 2018 4:17

Instrument :

BNA_G

ClientSampleId :

VB44949


Tot Ion: 99 Resp: 497400

Ion Ratio Lower Upper




99 100

42 18.6 15.0 22.4

71 31.0 25.5 38.3

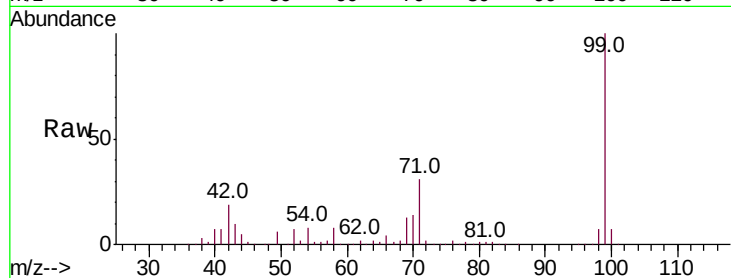

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

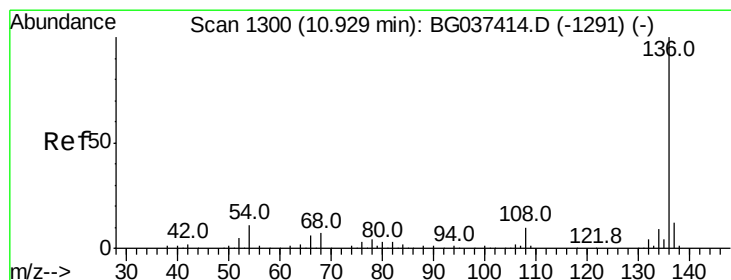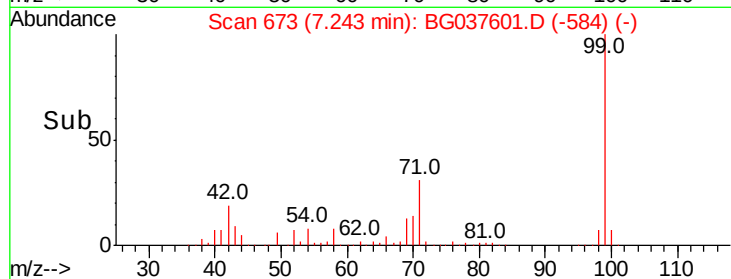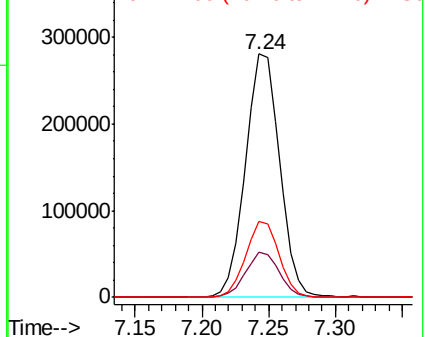

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.92 min Scan# 1299

Delta R.T. -0.01 min

Lab File: BG037601.D

Acq: 27 Oct 2018 4:17

Tgt Ion: 136 Resp: 257337


Ion Ratio Lower Upper

136 100



137 11.1 9.6 14.4


54 10.3 7.9 11.9

68 7.1 4.8 7.2

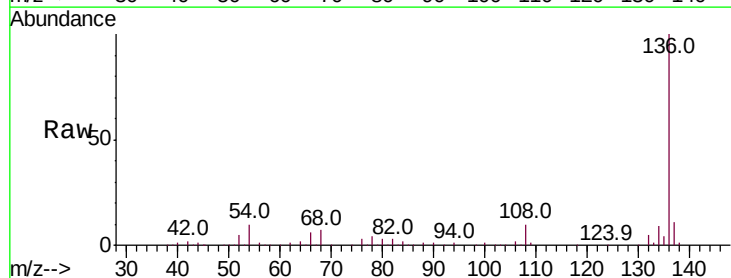

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



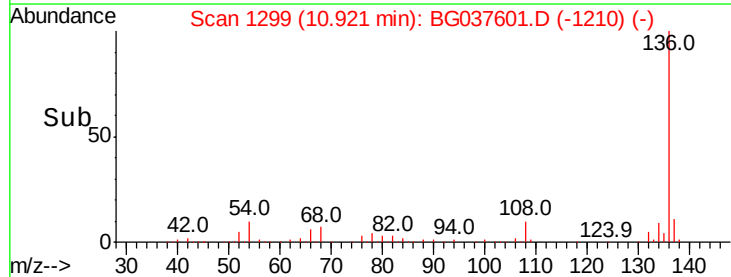
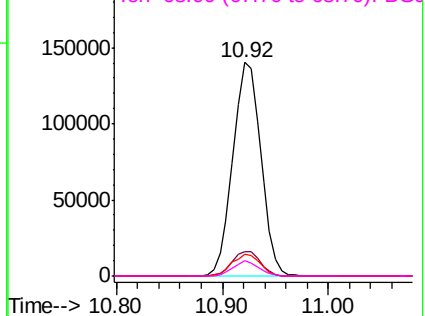


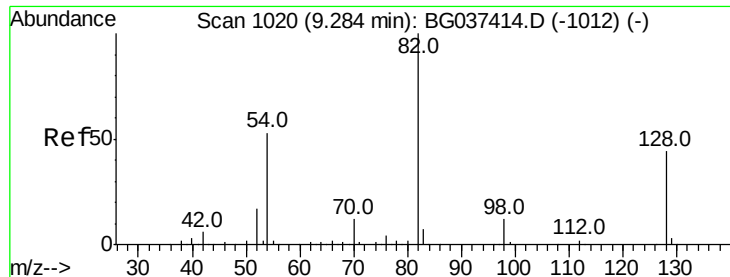

#23
Nitrobenzene-d5
Concen: 80.959 ng
RT: 9.28 min Scan# 1020
Delta R.T. -0.00 min
Lab File: BG037601.D
Acq: 27 Oct 2018 4:17




Instrument :
BNA_G
ClientSampled :
VB44949


Tot Ion	Ratio	Lower	Upper
82	100		
128	44.2	34.6	51.8
54	53.2	45.3	67.9

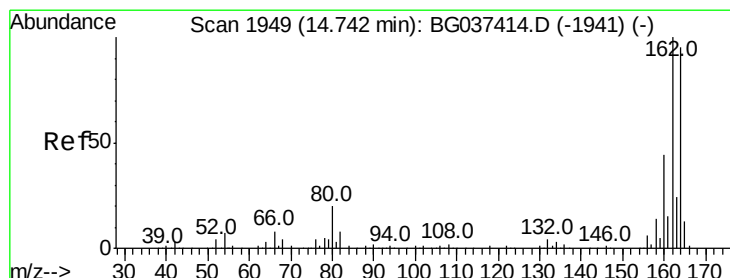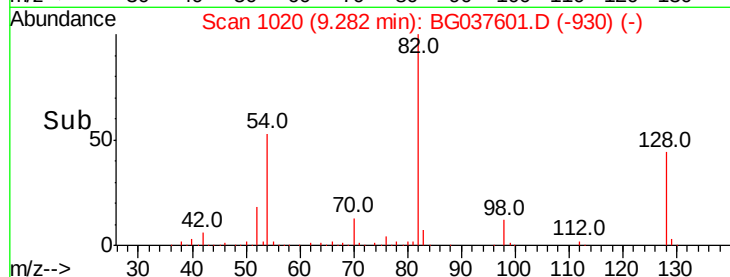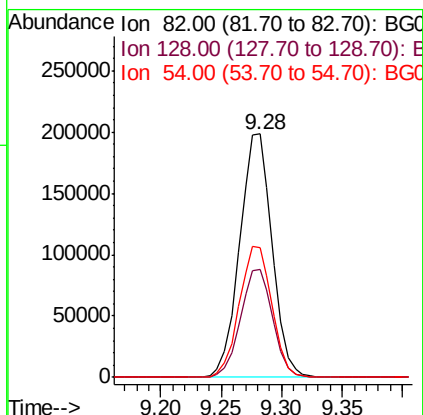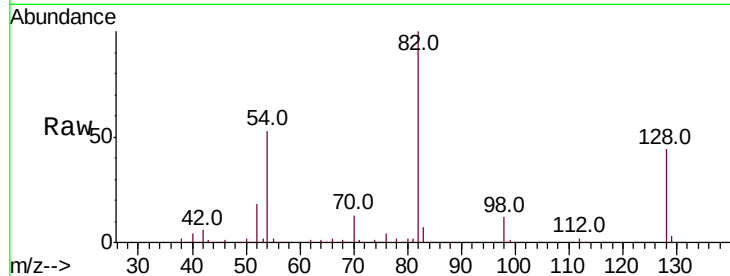

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.73 min Scan# 1948
Delta R.T. -0.01 min
Lab File: BG037601.D
Acq: 27 Oct 2018 4:17

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.4	81.3	121.9
160	45.8	36.3	54.5

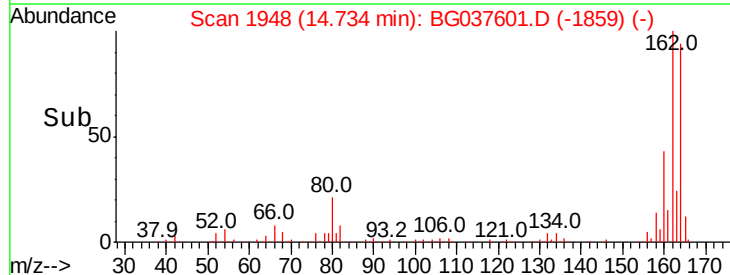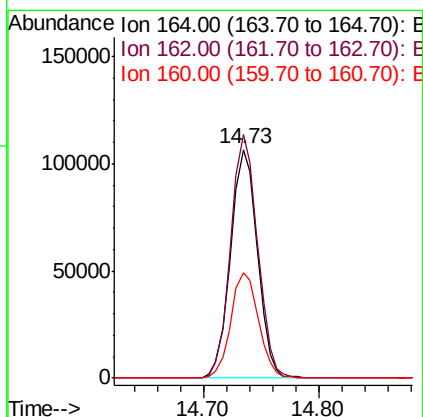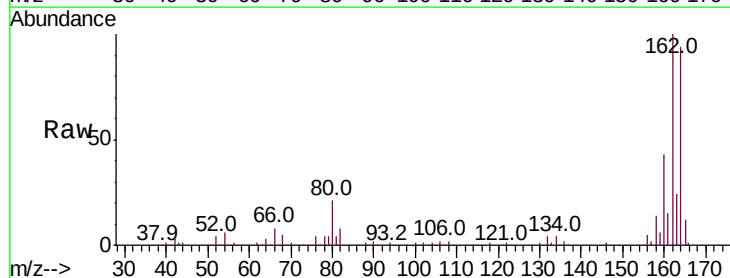

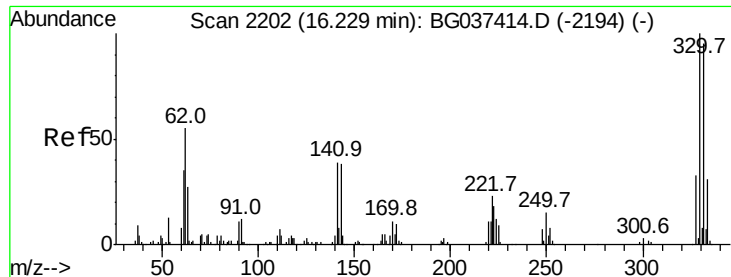

#42

2,4,6-Tribromophenol

Concen: 111.512 ng

RT: 16.22 min Scan# 2201

Delta R.T. -0.01 min

Lab File: BG037601.D

Acq: 27 Oct 2018 4:17

Instrument :

BNA_G

ClientSampleId :

VB44949


Tot Ion:330 Resp: 209557

Ion Ratio Lower Upper

330 100

332 96.3 78.4 117.6




141 40.0 32.2 48.2

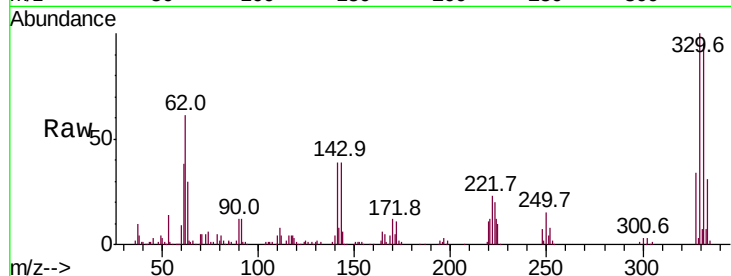

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

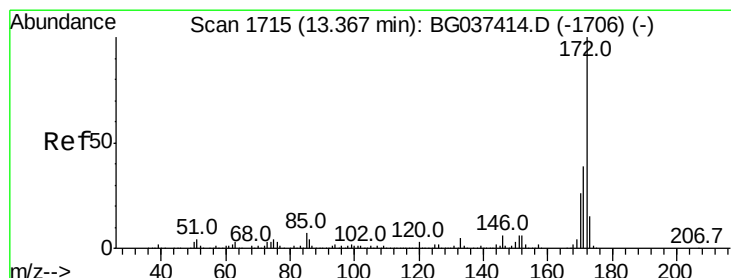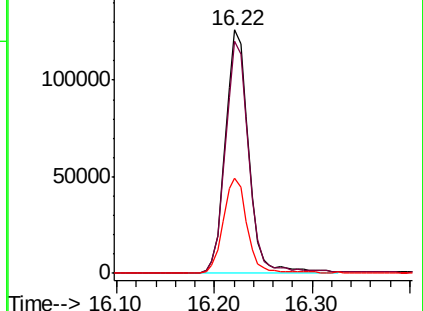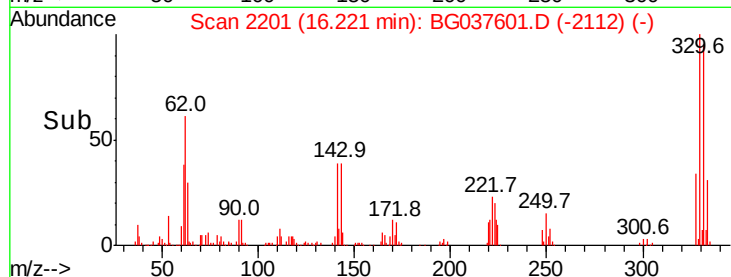

#45

2-Fluorobiphenyl

Concen: 77.467 ng

RT: 13.36 min Scan# 1714

Delta R.T. -0.01 min

Lab File: BG037601.D

Acq: 27 Oct 2018 4:17


Tgt Ion:172 Resp: 885136

Ion Ratio Lower Upper

172 100

171 38.7 31.0 46.4



170 25.7 20.2 30.2

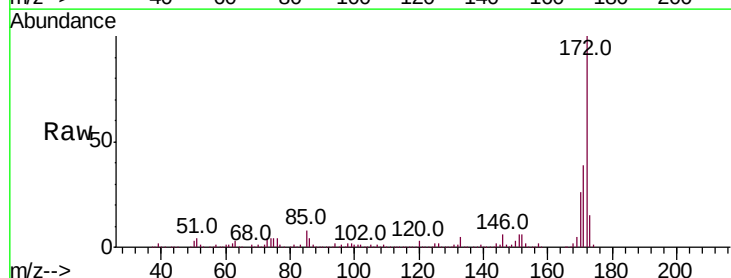


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

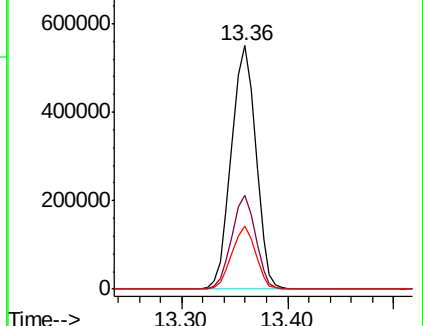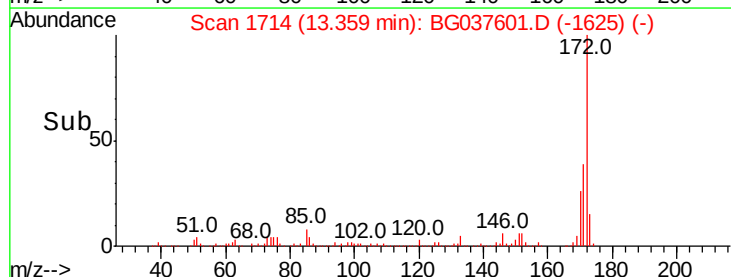

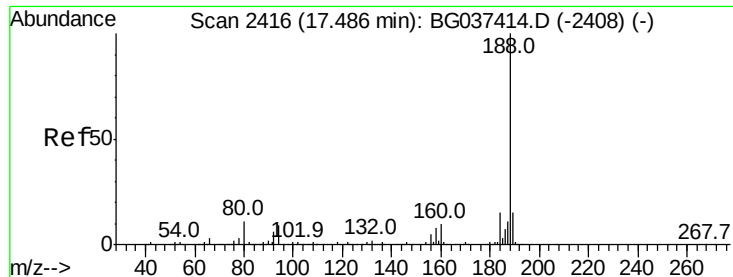

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.48 min Scan# 2416

Delta R.T. -0.00 min

Lab File: BG037601.D

Acq: 27 Oct 2018 4:17

Instrument :

BNA_G

ClientSampleId :

VB44949


Tot Ion:188 Resp: 422252

Ion Ratio Lower Upper

188 100

94 8.9 7.2 10.8




80 9.6 7.7 11.5

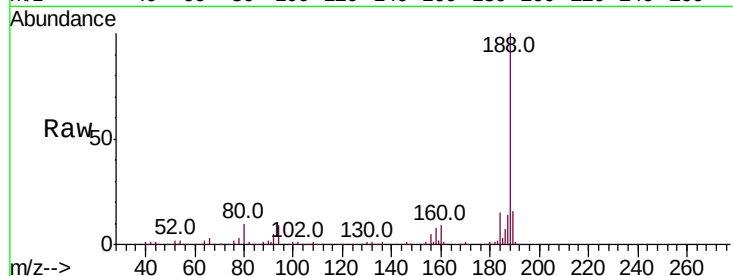

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

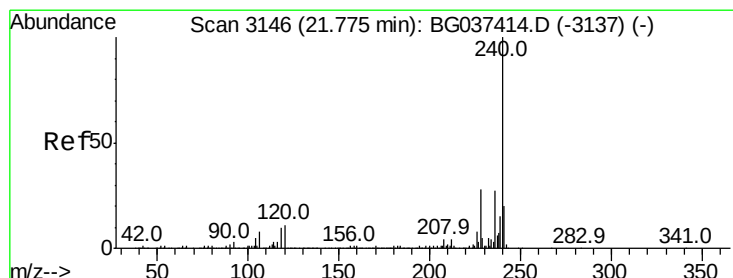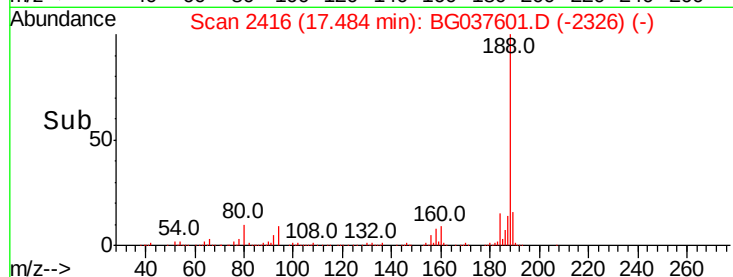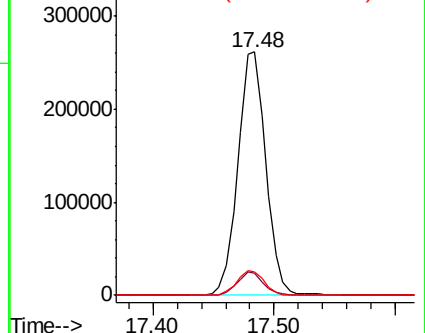

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.77 min Scan# 3145

Delta R.T. -0.01 min

Lab File: BG037601.D

Acq: 27 Oct 2018 4:17


Tgt Ion:240 Resp: 385311

Ion Ratio Lower Upper

240 100

120 10.7 8.1 12.1



236 26.2 21.4 32.0

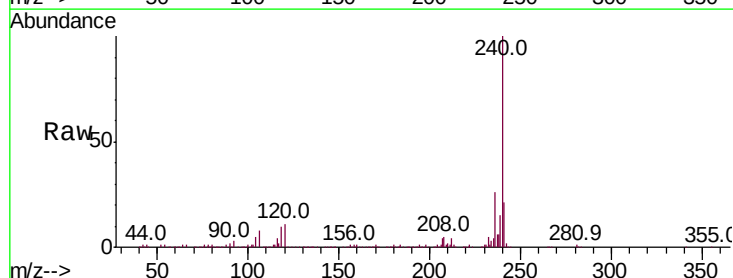


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

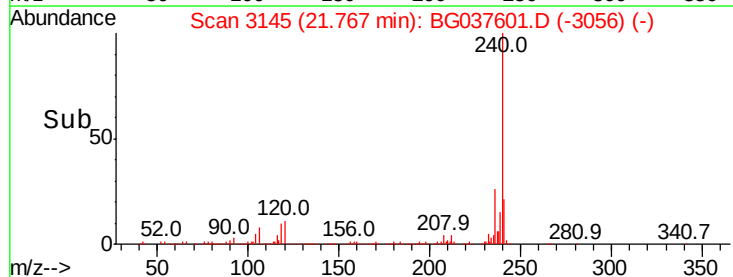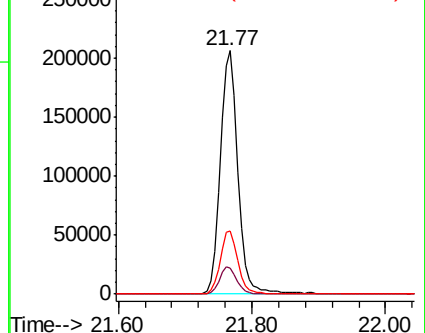

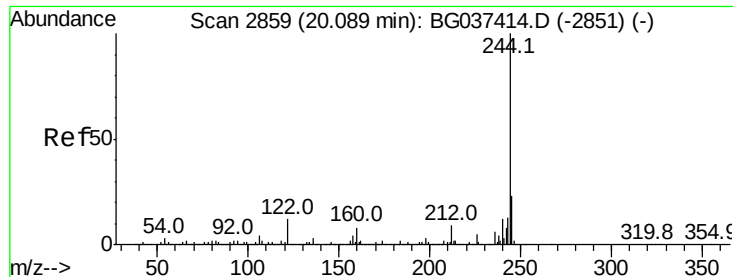

#79

Terphenyl-d14

Concen: 76.379 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BG037601.D

Acq: 27 Oct 2018 4:17

Instrument :

BNA_G

ClientSampleId :

VB44949


Tot Ion:244 Resp: 1377302

Ion Ratio Lower Upper

244 100

212 8.6 6.5 9.7




122 11.8 9.0 13.4

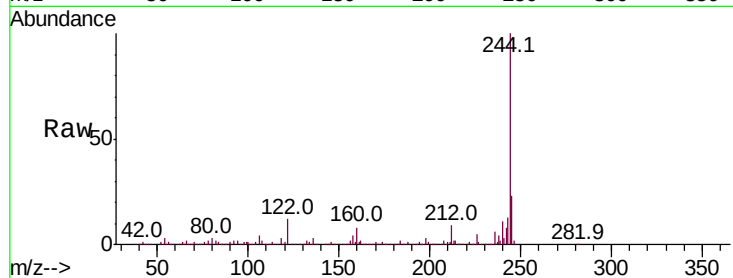

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

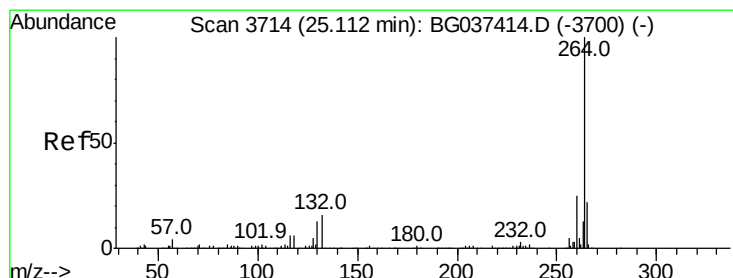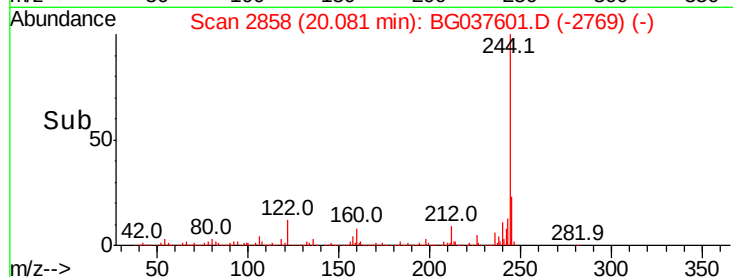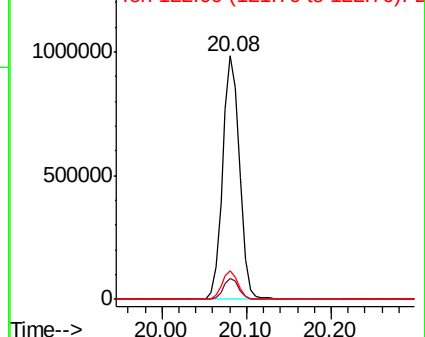

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.10 min Scan# 3713

Delta R.T. -0.01 min

Lab File: BG037601.D

Acq: 27 Oct 2018 4:17


Tgt Ion:264 Resp: 358525

Ion Ratio Lower Upper

264 100

260 24.2 18.2 27.4

265 20.9 17.9 26.9

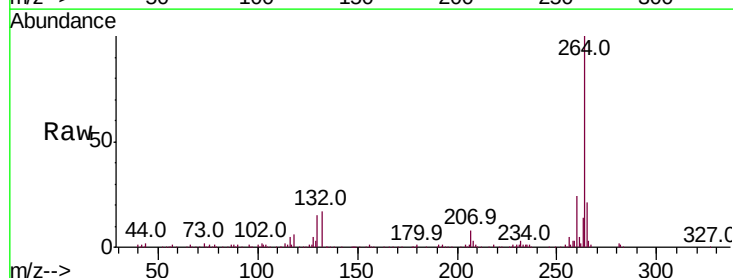

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

