

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102618\
 Data File : BG037598.D
 Acq On : 27 Oct 2018 2:20
 Operator : JU/SJ
 Sample : J5676-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB-1018-S-TCLP-GRID40

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.186	317	323	333	rVB	85317	141545	3.46%	0.718%
2	5.644	394	401	414	rBV	856443	1390198	33.99%	7.055%
3	7.243	666	673	689	rBV	800510	1408729	34.44%	7.150%
4	7.624	730	738	752	rBV	873039	1572490	38.44%	7.981%
5	8.100	809	819	826	rBV	189187	330899	8.09%	1.679%
6	8.424	867	874	883	rVB	651035	1162764	28.43%	5.901%
7	9.275	1010	1019	1029	rBV	568256	1058063	25.87%	5.370%
8	10.921	1291	1299	1307	rBV	265191	499782	12.22%	2.536%
9	13.359	1707	1714	1722	rBV	1563073	2516037	61.51%	12.769%
10	14.734	1940	1948	1959	rBV2	446194	754974	18.46%	3.832%
11	16.220	2194	2201	2217	rBV2	1127279	1841645	45.02%	9.347%
12	17.483	2408	2416	2424	rBV2	612652	994630	24.32%	5.048%
13	20.080	2852	2858	2875	rBV	3046973	4090301	100.00%	20.759%
14	21.767	3138	3145	3157	rBV2	569249	1034926	25.30%	5.252%
15	25.098	3701	3712	3735	rBV	260941	906858	22.17%	4.602%


Sum of corrected areas: 19703841

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102618\
Data File : BG037598.D
Acq On : 27 Oct 2018 2:20
Operator : JU/SJ
Sample : J5676-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB-1018-S-TCLP-GRID40

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

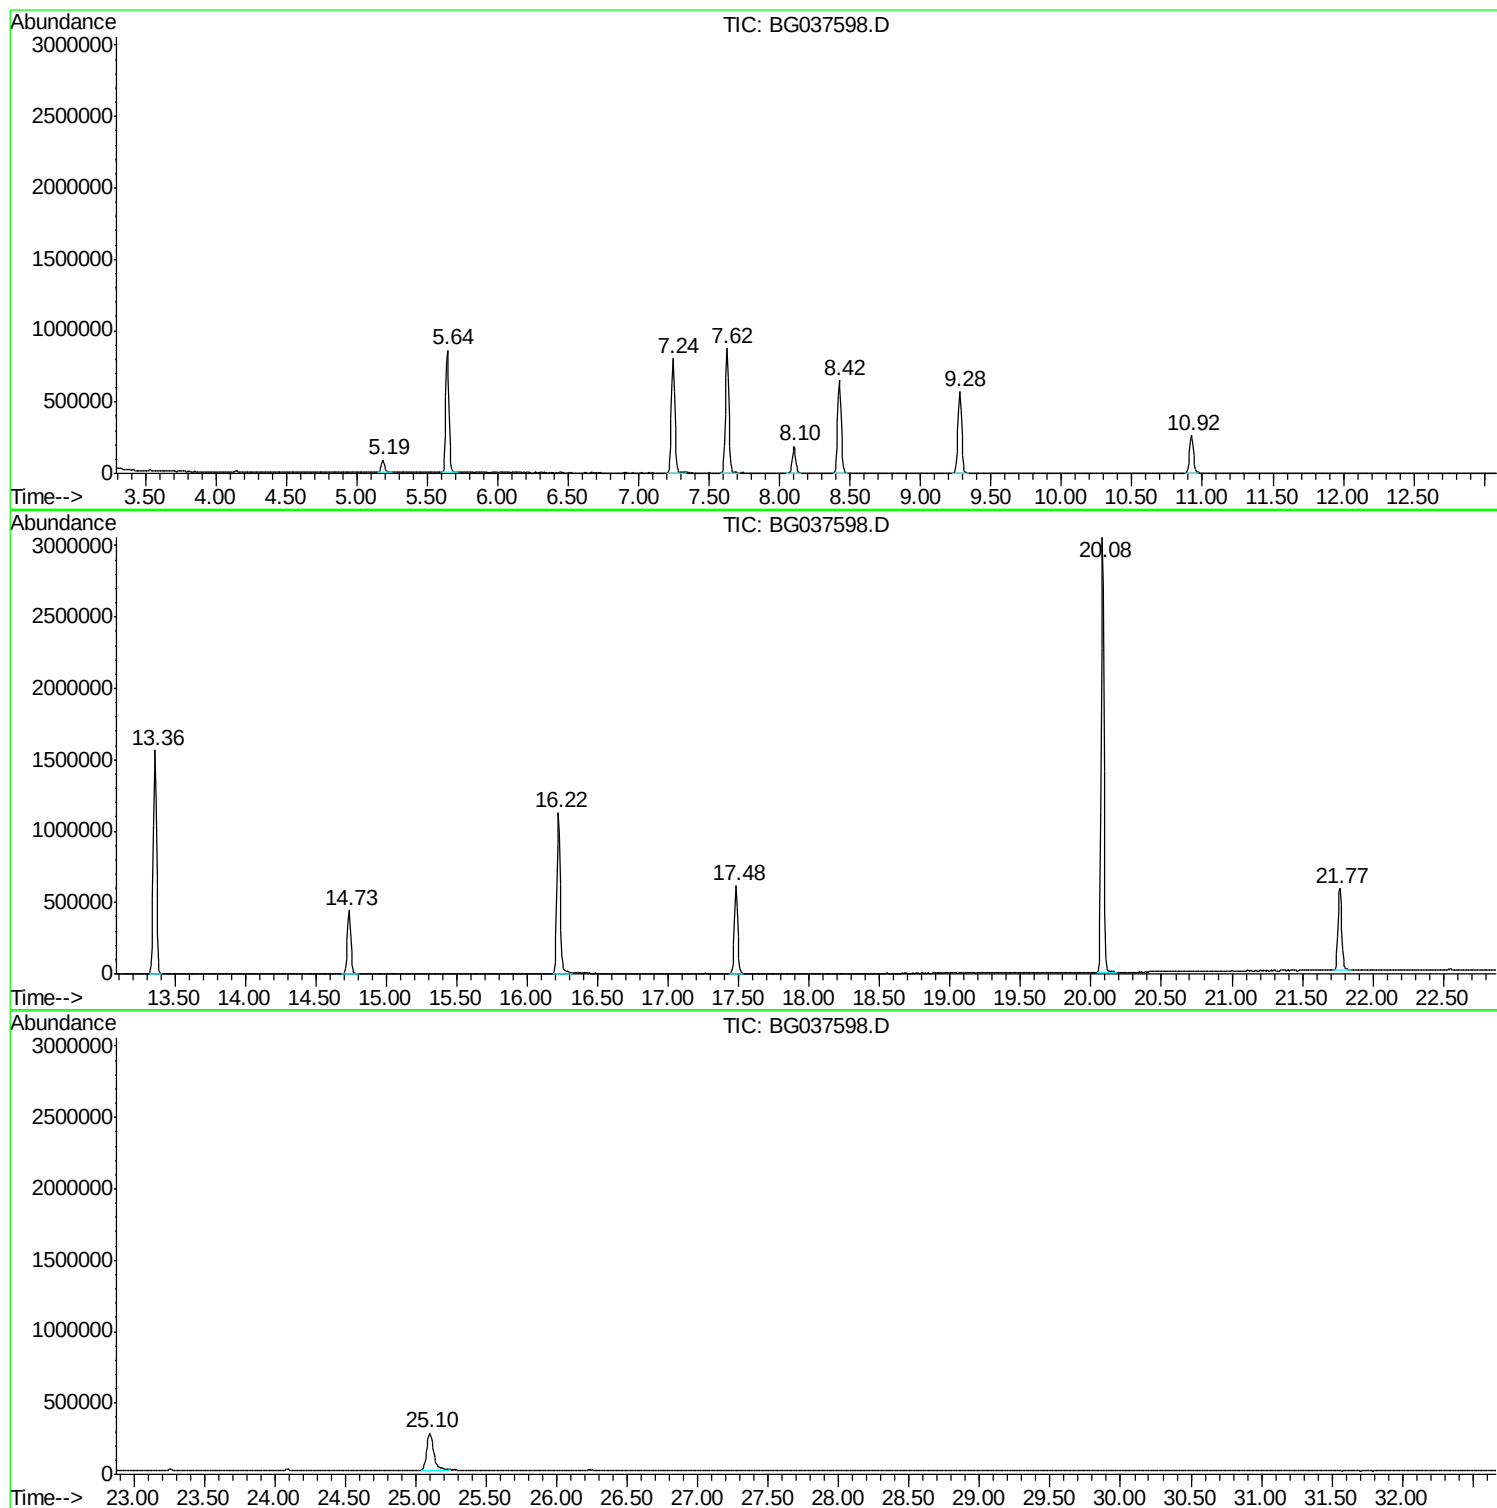

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102618\
Data_File : BG037598.D
Acq_On : 27 Oct 2018 2:200
Operator : JU/SJJ
Sample : J5676-011
Misc :
ALS_Vial : 18 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
CB-1018-S-TCLP-GRID40

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
