


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102618\
 Data File : BG037579.D
 Acq On : 26 Oct 2018 13:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

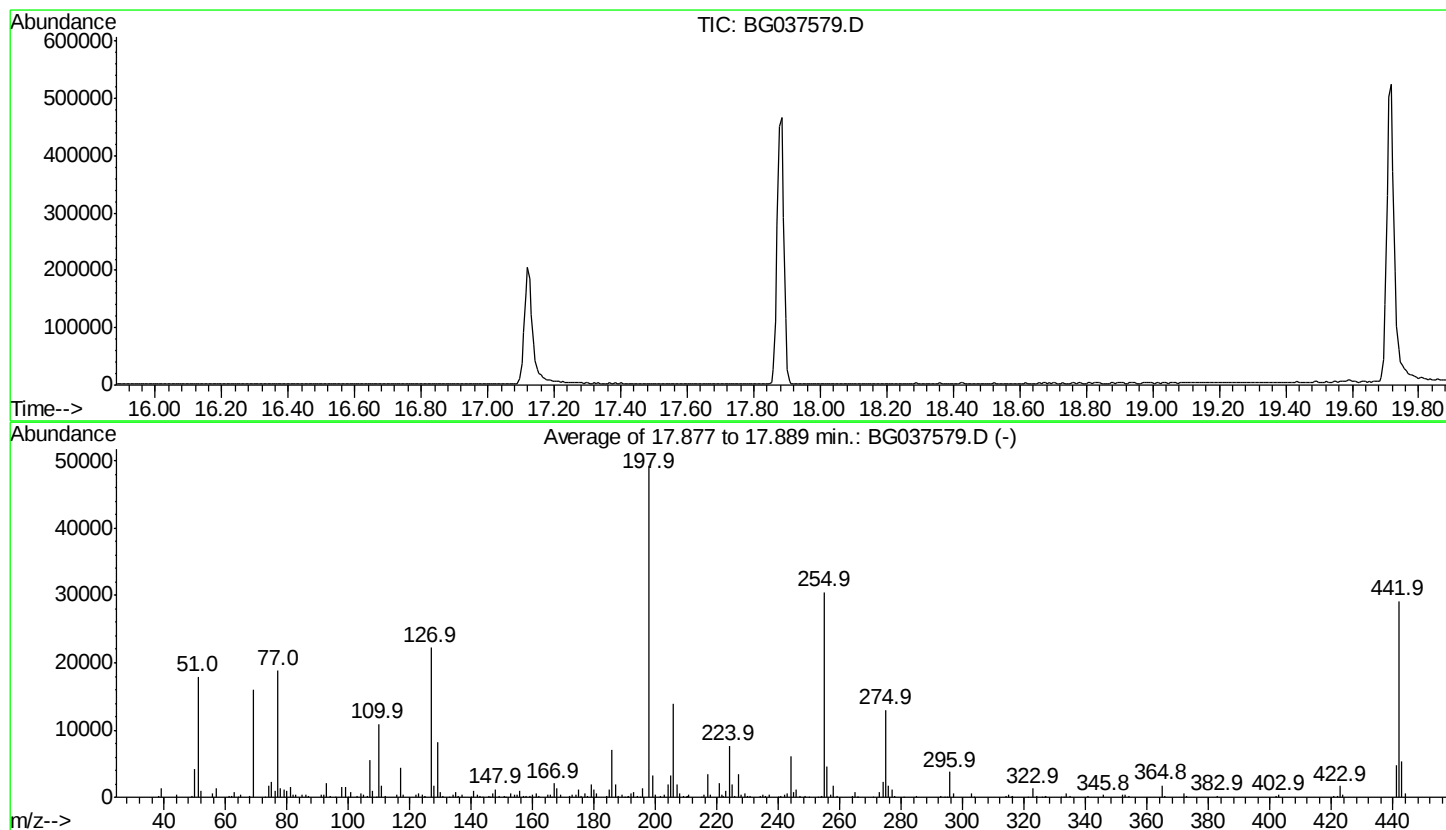

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	17957	PASS
68	69	0.00	2	1.2	197	PASS
69	198	0.00	100	32.3	15936	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.1	22269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49328	PASS
199	198	5	9	6.5	3189	PASS
275	198	10	60	26.4	13043	PASS
365	198	1	100	3.6	1793	PASS
441	198	0.01	100	9.7	4800	PASS
442	198	50	100	59.2	29208	PASS
443	442	15	24	18.4	5379	PASS