
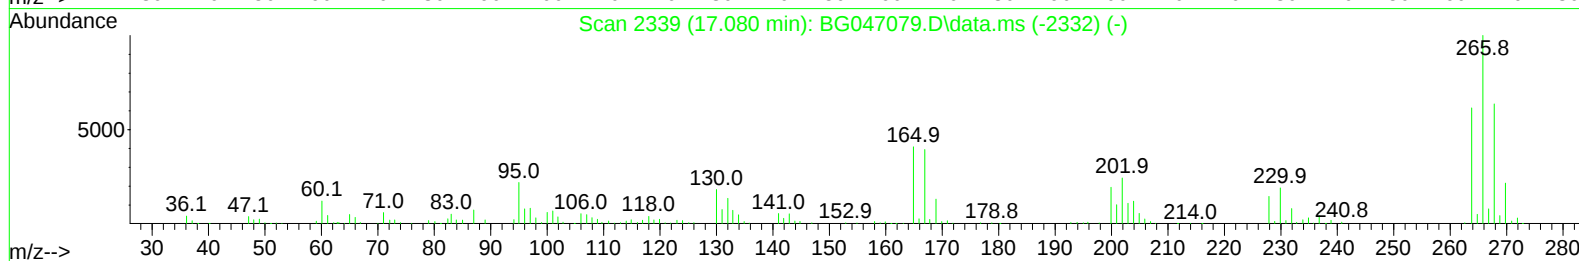
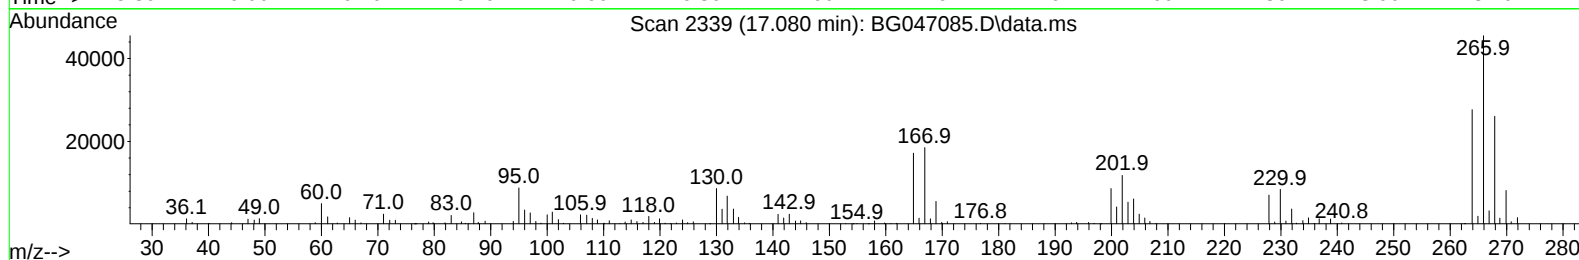


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102720\
Data File : BG047085.D
Acq On : 27 Oct 2020 8:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 02:24:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:55:38 2020
Response via : Initial Calibration

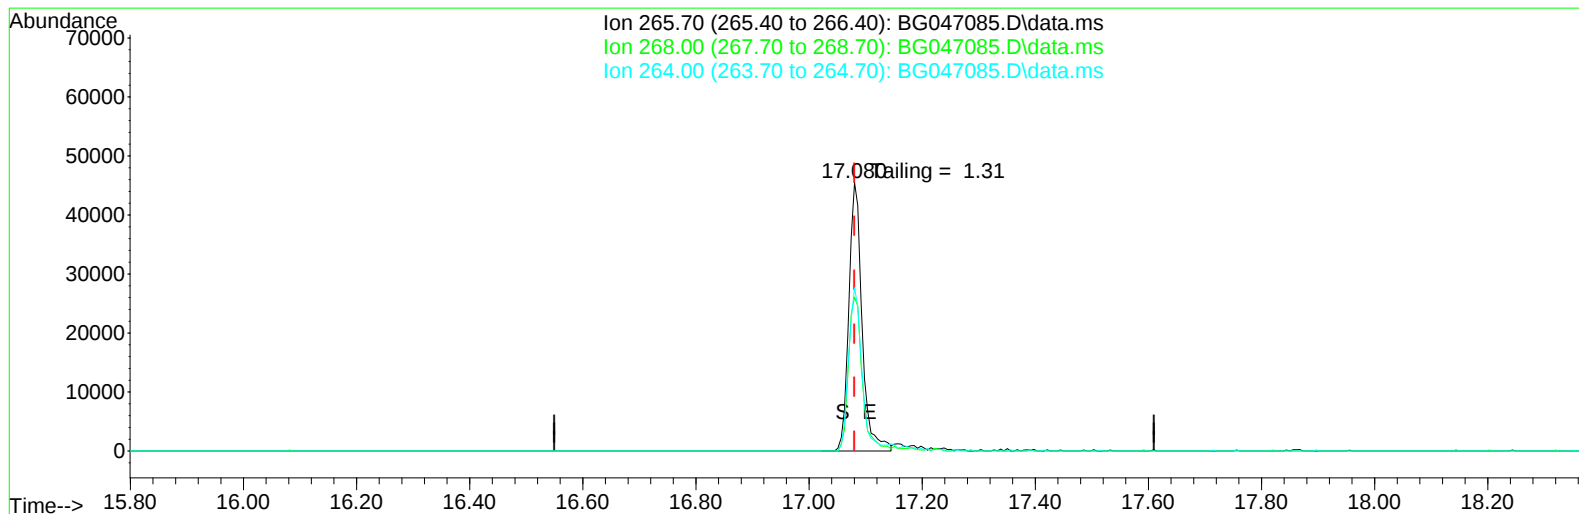

TIC: BG047085.D\data.ms

(70) Pentachlorophenol (C)




17.080min (+ 0.001) 21320.52 ng

response 74151

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.35
264.00	61.60	60.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102720\
Data File : BG047085.D
Acq On : 27 Oct 2020 8:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 02:24:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:55:38 2020
Response via : Initial Calibration

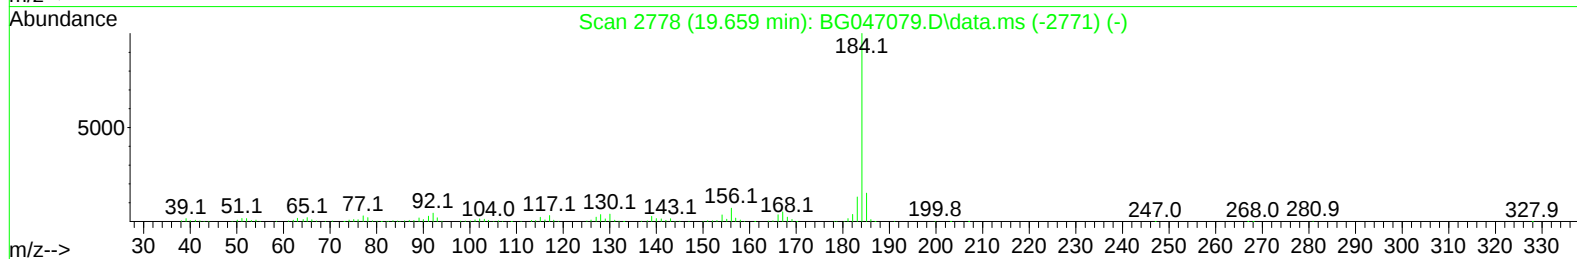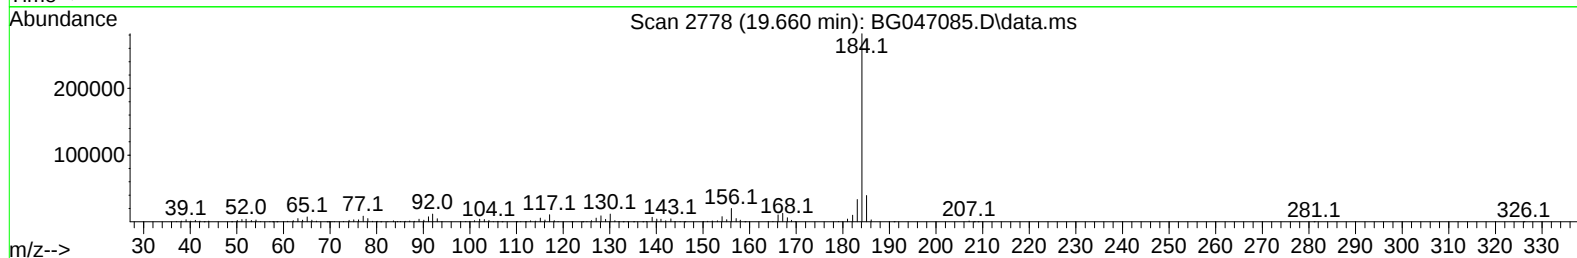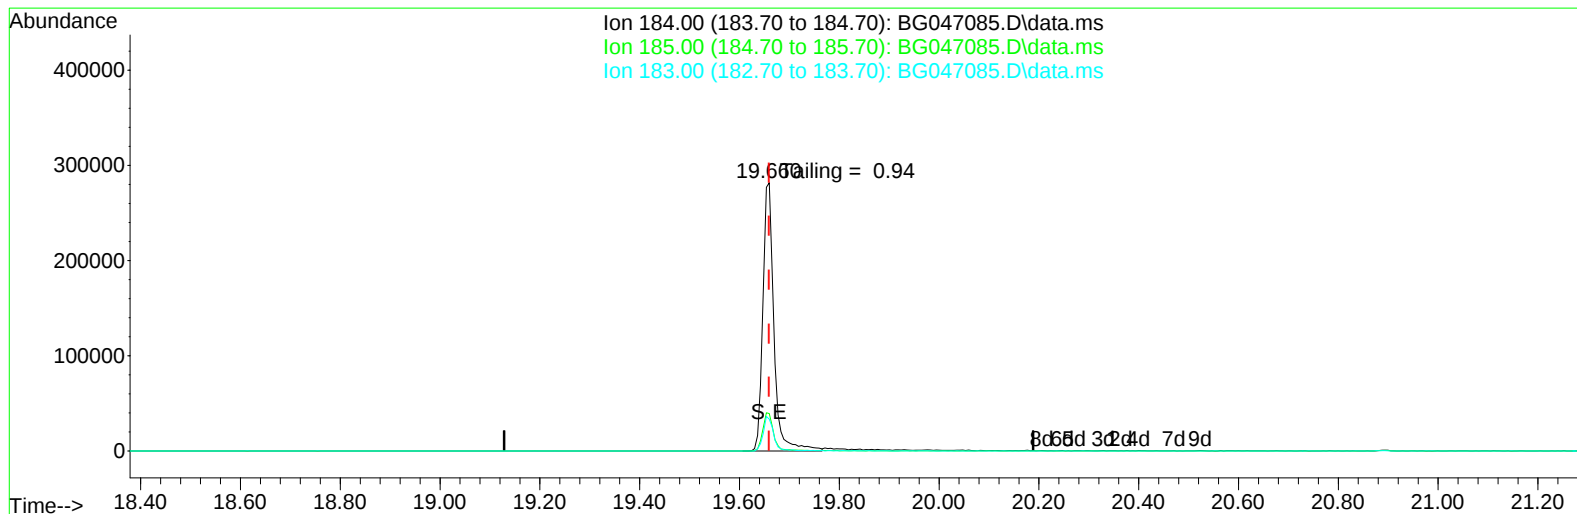

TIC: BG047085.D\data.ms

(77) Benzidine

19.660min (+ 0.001) 345238.98 ng m

response 465440

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	11.90
0.00	0.00	0.00