


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102720\
 Data File : BG047075.D
 Acq On : 26 Oct 2020 15:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 27 02:55:38 2020

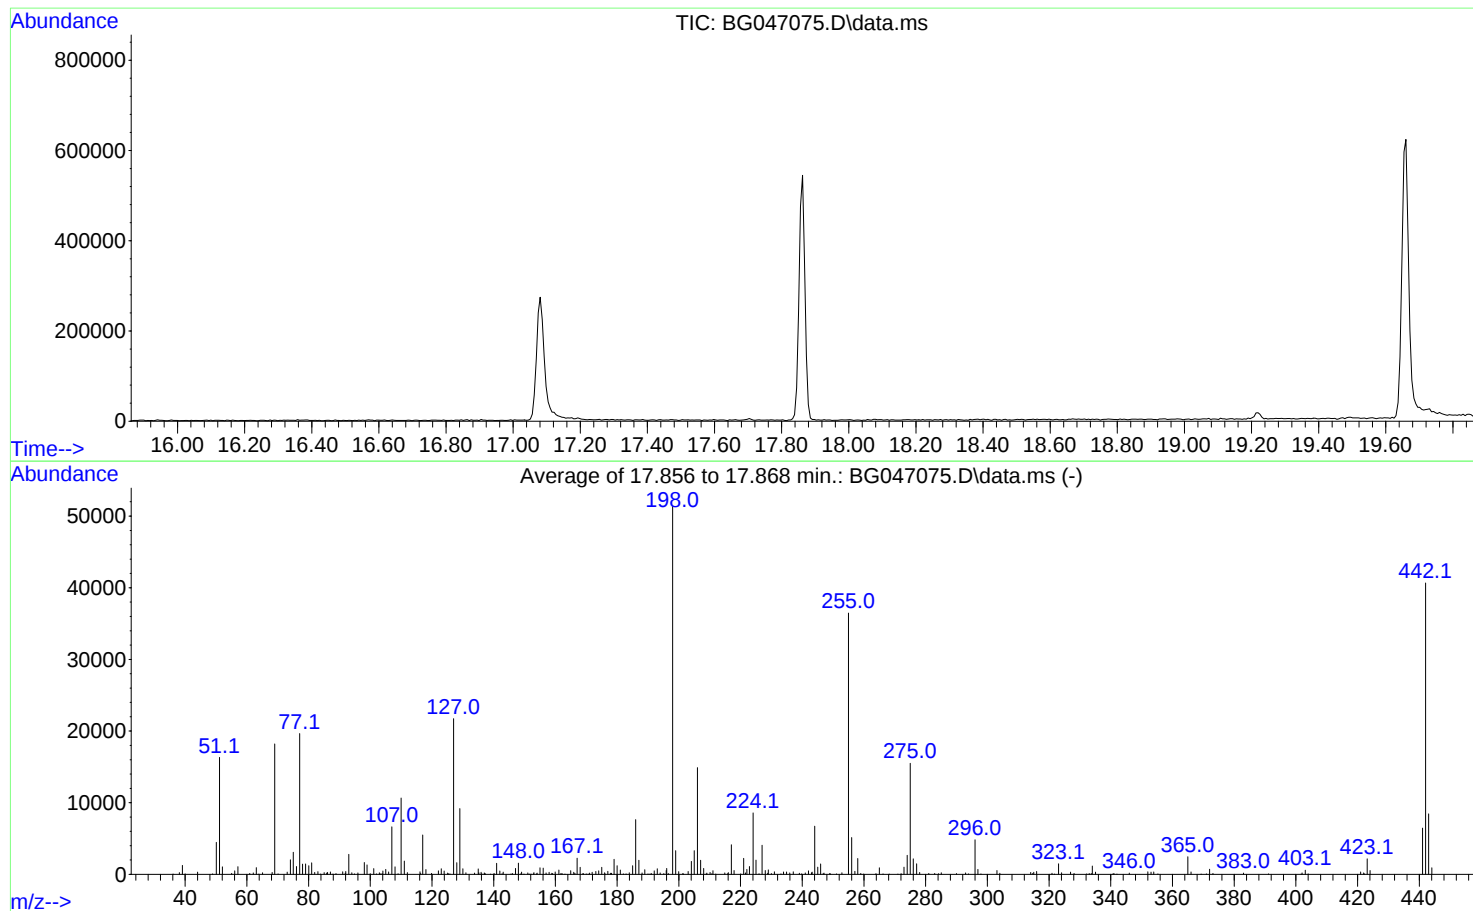

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	16324	PASS
68	69	0.00	2	1.5	276	PASS
69	198	0.00	100	35.5	18204	PASS
70	69	0.00	2	0.3	58	PASS
127	198	10	80	42.3	21718	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51341	PASS
199	198	5	9	6.4	3307	PASS
275	198	10	60	30.2	15505	PASS
365	198	1	100	4.8	2460	PASS
441	198	0.01	100	12.6	6464	PASS
442	198	50	100	79.2	40664	PASS
443	442	15	24	20.7	8436	PASS