

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050741.D
 Acq On : 27 Oct 2021 12:56
 Operator : CG/JU
 Sample : M4205-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.802	51	53	54	rBV2	1142	779	0.15%	0.019%
2	4.037	89	93	102	rBV	17967	31471	6.26%	0.757%
3	4.266	127	132	139	rBV	8442	13700	2.73%	0.329%
4	4.372	147	150	155	rVV4	2304	3631	0.72%	0.087%
5	4.431	158	160	162	rBV3	1161	1536	0.31%	0.037%
6	4.478	164	168	175	rVB6	2610	4321	0.86%	0.104%
7	4.583	184	186	193	rVB4	3151	5010	1.00%	0.120%
8	5.006	256	258	264	rVB4	1680	2448	0.49%	0.059%
9	5.300	302	308	313	rBV	5050	8091	1.61%	0.195%
10	6.381	490	492	494	rBV2	1017	915	0.18%	0.022%
11	6.610	528	531	537	rVB3	2402	3941	0.78%	0.095%
12	6.710	546	548	551	rBV3	858	887	0.18%	0.021%
13	6.781	558	560	562	rVB2	1257	973	0.19%	0.023%
14	6.816	562	566	569	rBV5	895	1259	0.25%	0.030%
15	6.839	569	570	575	rBV3	735	1139	0.23%	0.027%
16	6.886	575	578	579	rVV2	998	929	0.18%	0.022%
17	6.910	579	582	586	rVB4	2166	3123	0.62%	0.075%
18	7.268	641	643	647	rBV2	840	845	0.17%	0.020%
19	7.386	658	663	672	rBV2	33537	61405	12.22%	1.476%
20	7.562	687	693	699	rBV	27495	47463	9.44%	1.141%
21	7.674	709	712	716	rBV4	766	1056	0.21%	0.025%
22	7.774	723	729	737	rBV2	31406	58162	11.57%	1.398%
23	7.838	737	740	746	rVB4	1388	2228	0.44%	0.054%
24	7.885	746	748	754	rBV5	846	1114	0.22%	0.027%
25	8.250	802	810	817	rVB	100092	175441	34.91%	4.218%
26	8.537	855	859	861	rVV3	926	1294	0.26%	0.031%
27	8.943	922	928	940	rVB	32033	59437	11.83%	1.429%
28	9.078	946	951	956	rBV3	3162	5576	1.11%	0.134%
29	9.337	991	995	999	rBV3	713	890	0.18%	0.021%
30	9.419	1001	1009	1018	rVV	33837	61073	12.15%	1.468%
31	9.513	1021	1025	1027	rBV	750	802	0.16%	0.019%
32	10.147	1127	1133	1140	rVB2	27910	49265	9.80%	1.184%
33	10.453	1184	1185	1188	rBV	857	773	0.15%	0.019%
34	10.688	1219	1225	1235	rBV2	32295	63638	12.66%	1.530%
35	10.829	1243	1249	1253	rBV4	5152	10383	2.07%	0.250%
36	11.076	1283	1291	1305	rVB	146365	271970	54.11%	6.539%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050741.D
 Acq On : 27 Oct 2021 12:56
 Operator : CG/JU
 Sample : M4205-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

37	11.211	1305	1314	1323	rBV	32679	65461	13.02%	1.574%
38	12.721	1566	1571	1575	rVB3	1571	2831	0.56%	0.068%
39	12.815	1583	1587	1591	rBV4	513	911	0.18%	0.022%
40	12.932	1602	1607	1611	rBV4	1417	2562	0.51%	0.062%
41	13.667	1729	1732	1737	rVB4	1127	1635	0.33%	0.039%
42	13.737	1741	1744	1748	rBV2	667	967	0.19%	0.023%
43	13.861	1761	1765	1770	rBV3	2288	3138	0.62%	0.075%
44	13.914	1770	1774	1778	rVB3	688	896	0.18%	0.022%
45	14.196	1816	1822	1827	rVB3	1347	2288	0.46%	0.055%
46	14.266	1828	1834	1840	rVV	80278	118883	23.65%	2.858%
47	14.325	1840	1844	1846	rVB2	1161	1144	0.23%	0.028%
48	14.572	1879	1886	1893	rVB	86257	140329	27.92%	3.374%
49	14.736	1909	1914	1917	rBV3	945	1434	0.29%	0.034%
50	14.871	1930	1937	1945	rBV	234151	379403	75.49%	9.122%
51	15.059	1965	1969	1985	rBV3	18968	41642	8.29%	1.001%
52	15.271	2001	2005	2009	rBV3	2182	2788	0.55%	0.067%
53	15.582	2056	2058	2063	rVB3	725	862	0.17%	0.021%
54	15.682	2072	2075	2077	rBV	1653	1466	0.29%	0.035%
55	15.864	2099	2106	2112	rBV	110551	175567	34.93%	4.221%
56	15.976	2120	2125	2134	rBV2	22521	36563	7.27%	0.879%
57	16.563	2217	2225	2230	rBV5	4602	8633	1.72%	0.208%
58	16.734	2252	2254	2258	rBV2	880	965	0.19%	0.023%
59	17.069	2309	2311	2317	rVB2	880	1058	0.21%	0.025%
60	17.145	2323	2324	2327	rVB2	1052	930	0.19%	0.022%
61	17.339	2352	2357	2362	rBV3	2743	4345	0.86%	0.104%
62	17.386	2362	2365	2367	rVV3	1233	1367	0.27%	0.033%
63	17.409	2367	2369	2372	rVB4	1128	1299	0.26%	0.031%
64	17.480	2378	2381	2384	rBV3	771	802	0.16%	0.019%
65	17.621	2397	2405	2411	rBV	312061	480608	95.63%	11.555%
66	17.721	2416	2422	2428	rVV	123211	192444	38.29%	4.627%
67	17.791	2431	2434	2438	rVB3	1711	2123	0.42%	0.051%
68	17.968	2461	2464	2467	rBV	1000	1317	0.26%	0.032%
69	18.079	2480	2483	2486	rVB3	3552	3632	0.72%	0.087%
70	18.120	2488	2490	2493	rBV3	825	1133	0.23%	0.027%
71	18.255	2510	2513	2516	rVB4	4283	4715	0.94%	0.113%
72	18.361	2528	2531	2532	rBV2	917	776	0.15%	0.019%
73	18.385	2532	2535	2536	rVB	981	780	0.16%	0.019%
74	18.455	2543	2547	2548	rVB3	755	855	0.17%	0.021%
75	18.491	2548	2553	2555	rBV2	1489	2488	0.50%	0.060%
76	18.549	2558	2563	2570	rVB5	2566	5614	1.12%	0.135%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050741.D
 Acq On : 27 Oct 2021 12:56
 Operator : CG/JU
 Sample : M4205-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

77	18.608	2570	2573	2575	rBV3	1032	1190	0.24%	0.029%
78	18.684	2580	2586	2589	rVB5	2101	3966	0.79%	0.095%
79	18.726	2589	2593	2595	rBV4	1760	2508	0.50%	0.060%
80	18.761	2595	2599	2604	rBV3	4144	6851	1.36%	0.165%
81	18.872	2616	2618	2619	rVB2	1166	792	0.16%	0.019%
82	18.890	2619	2621	2624	rBV	1147	1100	0.22%	0.026%
83	18.925	2625	2627	2628	rVB	1490	840	0.17%	0.020%
84	19.002	2635	2640	2644	rBV5	5538	7326	1.46%	0.176%
85	19.066	2647	2651	2652	rBV3	2074	1681	0.33%	0.040%
86	19.154	2663	2666	2667	rBV3	1355	1202	0.24%	0.029%
87	19.213	2675	2676	2678	rBV2	1111	800	0.16%	0.019%
88	19.325	2694	2695	2697	rBV2	1215	807	0.16%	0.019%
89	19.389	2701	2706	2708	rBV2	6174	8866	1.76%	0.213%
90	19.442	2713	2715	2717	rBV2	1828	1128	0.22%	0.027%
91	19.519	2726	2728	2729	rBV3	2579	2256	0.45%	0.054%
92	19.624	2744	2746	2747	rBV2	1877	1372	0.27%	0.033%
93	19.666	2750	2753	2758	rVV	6407	9099	1.81%	0.219%
94	19.724	2762	2763	2766	rBV3	1723	2008	0.40%	0.048%
95	19.995	2799	2809	2817	rBV	175779	273060	54.33%	6.565%
96	20.488	2890	2893	2896	rBV3	7130	6809	1.35%	0.164%
97	20.988	2976	2978	2982	rVB5	7241	8466	1.68%	0.204%
98	21.922	3131	3137	3144	rBV	271288	468598	93.24%	11.266%
99	25.106	3672	3679	3691	rVB3	67732	192320	38.27%	4.624%
100	25.347	3711	3720	3732	rVB3	166695	502590	100.00%	12.084%




Sum of corrected areas: 4159257

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050741.D
Acq On : 27 Oct 2021 12:56
Operator : CG/JU
Sample : M4205-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

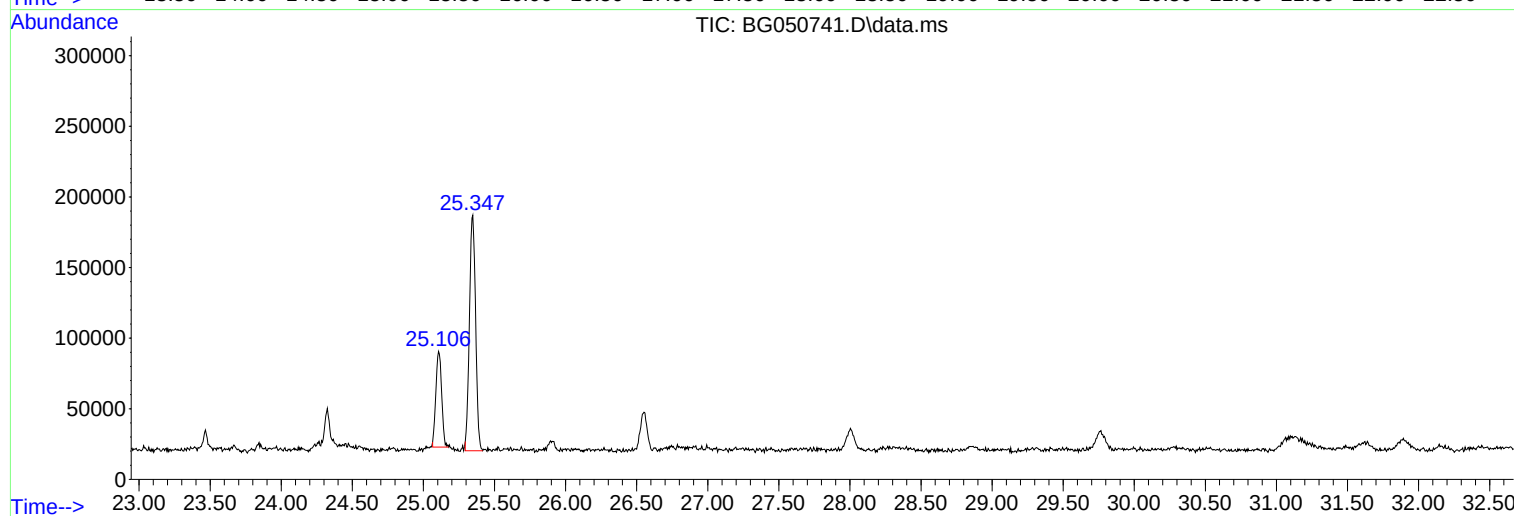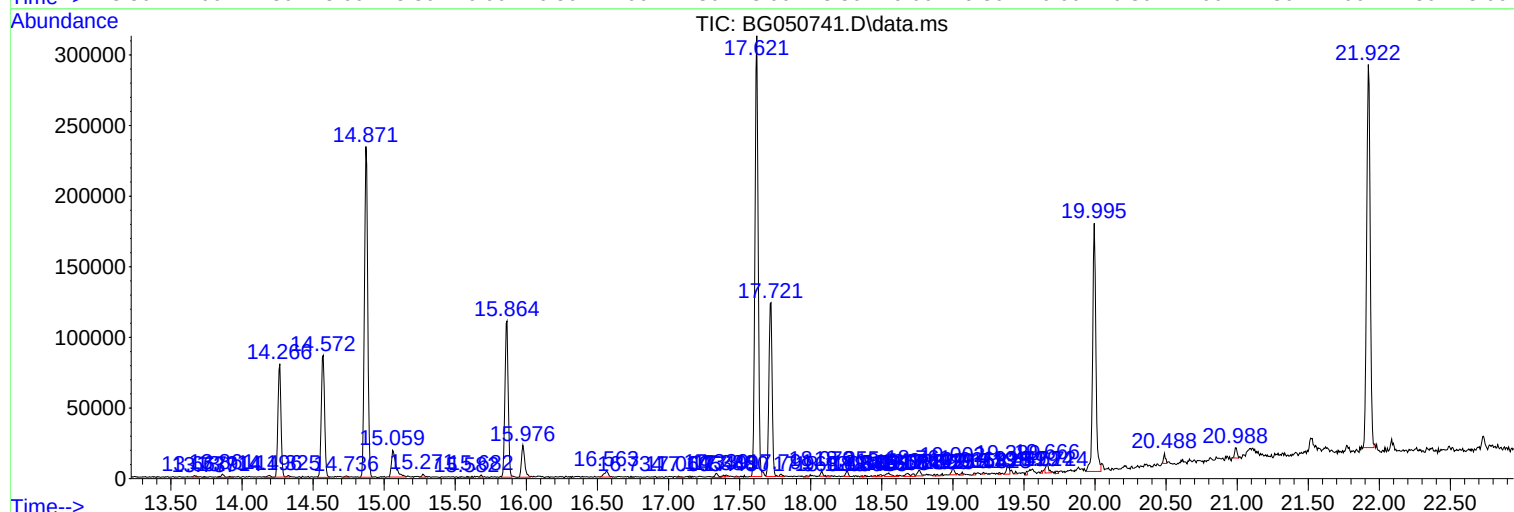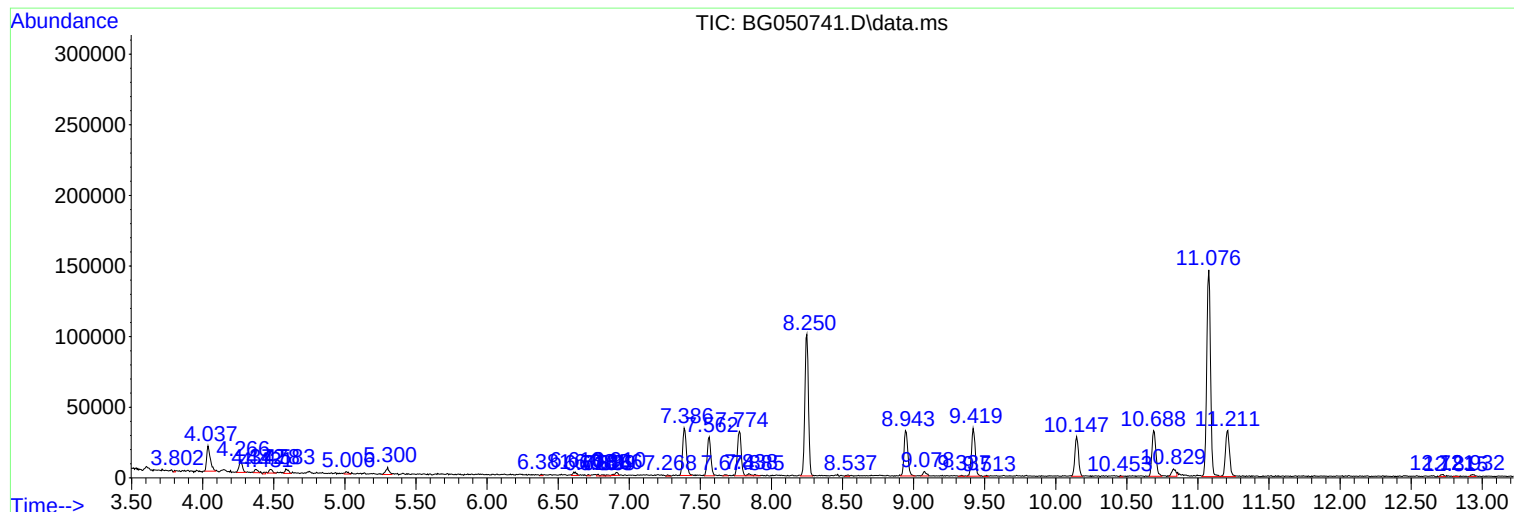

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050741.D
Acq On : 27 Oct 2021 12:56
Operator : CG/JU
Sample : M4205-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050741.D
Acq On : 27 Oct 2021 12:56
Operator : CG/JU
Sample : M4205-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc