

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050748.D
 Acq On : 27 Oct 2021 18:28
 Operator : CG/JU
 Sample : M4205-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.201	118	121	124	rBV3	1033	1535	0.23%	0.029%
2	4.266	126	132	139	rVB	7974	14335	2.19%	0.272%
3	4.371	145	150	155	rBV4	2243	3604	0.55%	0.068%
4	4.448	160	163	165	rBV4	1071	1585	0.24%	0.030%
5	4.477	165	168	172	rVB3	2027	2829	0.43%	0.054%
6	4.589	185	187	190	rBV2	729	1093	0.17%	0.021%
7	4.924	242	244	246	rBV3	842	1013	0.15%	0.019%
8	5.059	264	267	269	rVB3	817	941	0.14%	0.018%
9	5.294	302	307	312	rBV2	4237	6089	0.93%	0.115%
10	6.122	444	448	450	rBV3	645	902	0.14%	0.017%
11	6.616	527	532	535	rVB4	2032	3334	0.51%	0.063%
12	7.074	606	610	613	rVB3	756	1021	0.16%	0.019%
13	7.386	656	663	670	rBV	49150	86511	13.22%	1.639%
14	7.556	686	692	702	rVB	37860	67820	10.36%	1.285%
15	7.773	723	729	736	rVB	45355	82110	12.55%	1.555%
16	7.844	736	741	745	rVB5	1223	1990	0.30%	0.038%
17	8.243	803	809	817	rVB	128488	223820	34.20%	4.240%
18	8.943	918	928	938	rBV	55953	105745	16.16%	2.003%
19	9.013	938	940	944	rVV3	621	882	0.13%	0.017%
20	9.072	947	950	956	rVB2	1744	3291	0.50%	0.062%
21	9.172	963	967	970	rVB2	813	1093	0.17%	0.021%
22	9.418	1001	1009	1017	rVB	48427	89166	13.63%	1.689%
23	10.141	1124	1132	1139	rBV2	38665	72177	11.03%	1.367%
24	10.429	1176	1181	1183	rBV3	672	943	0.14%	0.018%
25	10.688	1216	1225	1236	rBV	48513	95570	14.61%	1.810%
26	11.070	1282	1290	1298	rBV	189398	351760	53.76%	6.663%
27	11.205	1306	1313	1326	rBV	55139	106609	16.29%	2.019%
28	11.757	1405	1407	1409	rBV2	644	787	0.12%	0.015%
29	14.260	1828	1833	1840	rVB	105685	162430	24.82%	3.077%
30	14.565	1879	1885	1892	rBV	125306	198717	30.37%	3.764%
31	14.871	1929	1937	1946	rVB	335686	514967	78.70%	9.755%
32	15.059	1963	1969	1979	rBV2	31367	64969	9.93%	1.231%
33	15.858	2099	2105	2113	rVB	162843	243817	37.26%	4.619%
34	15.970	2119	2124	2131	rBV2	32848	52735	8.06%	0.999%
35	16.105	2140	2147	2149	rBV4	1403	1865	0.29%	0.035%
36	17.215	2334	2336	2339	rBV3	828	772	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050748.D
 Acq On : 27 Oct 2021 18:28
 Operator : CG/JU
 Sample : M4205-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AZ8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

37	17.251	2339	2342	2346	rVV3	551	834	0.13%	0.016%
38	17.403	2364	2368	2372	rVB4	1148	1646	0.25%	0.031%
39	17.615	2398	2404	2412	rBV	404430	630318	96.33%	11.940%
40	17.715	2414	2421	2429	rVV	176344	265706	40.61%	5.033%
41	18.173	2497	2499	2502	rVB2	721	912	0.14%	0.017%
42	18.549	2562	2563	2567	rBV2	1094	777	0.12%	0.015%
43	18.731	2592	2594	2597	rBV2	815	877	0.13%	0.017%
44	19.201	2672	2674	2677	rBV3	935	847	0.13%	0.016%
45	19.242	2680	2681	2684	rVB2	1474	819	0.13%	0.016%
46	19.330	2695	2696	2699	rBV3	933	1120	0.17%	0.021%
47	19.407	2707	2709	2710	rBV2	1103	822	0.13%	0.016%
48	19.642	2746	2749	2751	rBV3	1530	1553	0.24%	0.029%
49	19.742	2765	2766	2768	rBV2	1177	788	0.12%	0.015%
50	19.824	2779	2780	2781	rBV	1525	805	0.12%	0.015%
51	19.994	2803	2809	2818	rVB	208971	300645	45.95%	5.695%
52	21.922	3130	3137	3143	rBV	347979	601033	91.85%	11.385%
53	25.106	3670	3679	3689	rVB3	88532	246309	37.64%	4.666%
54	25.341	3709	3719	3734	rVB3	214660	654358	100.00%	12.396%


Sum of corrected areas: 5278996

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050748.D
Acq On : 27 Oct 2021 18:28
Operator : CG/JU
Sample : M4205-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

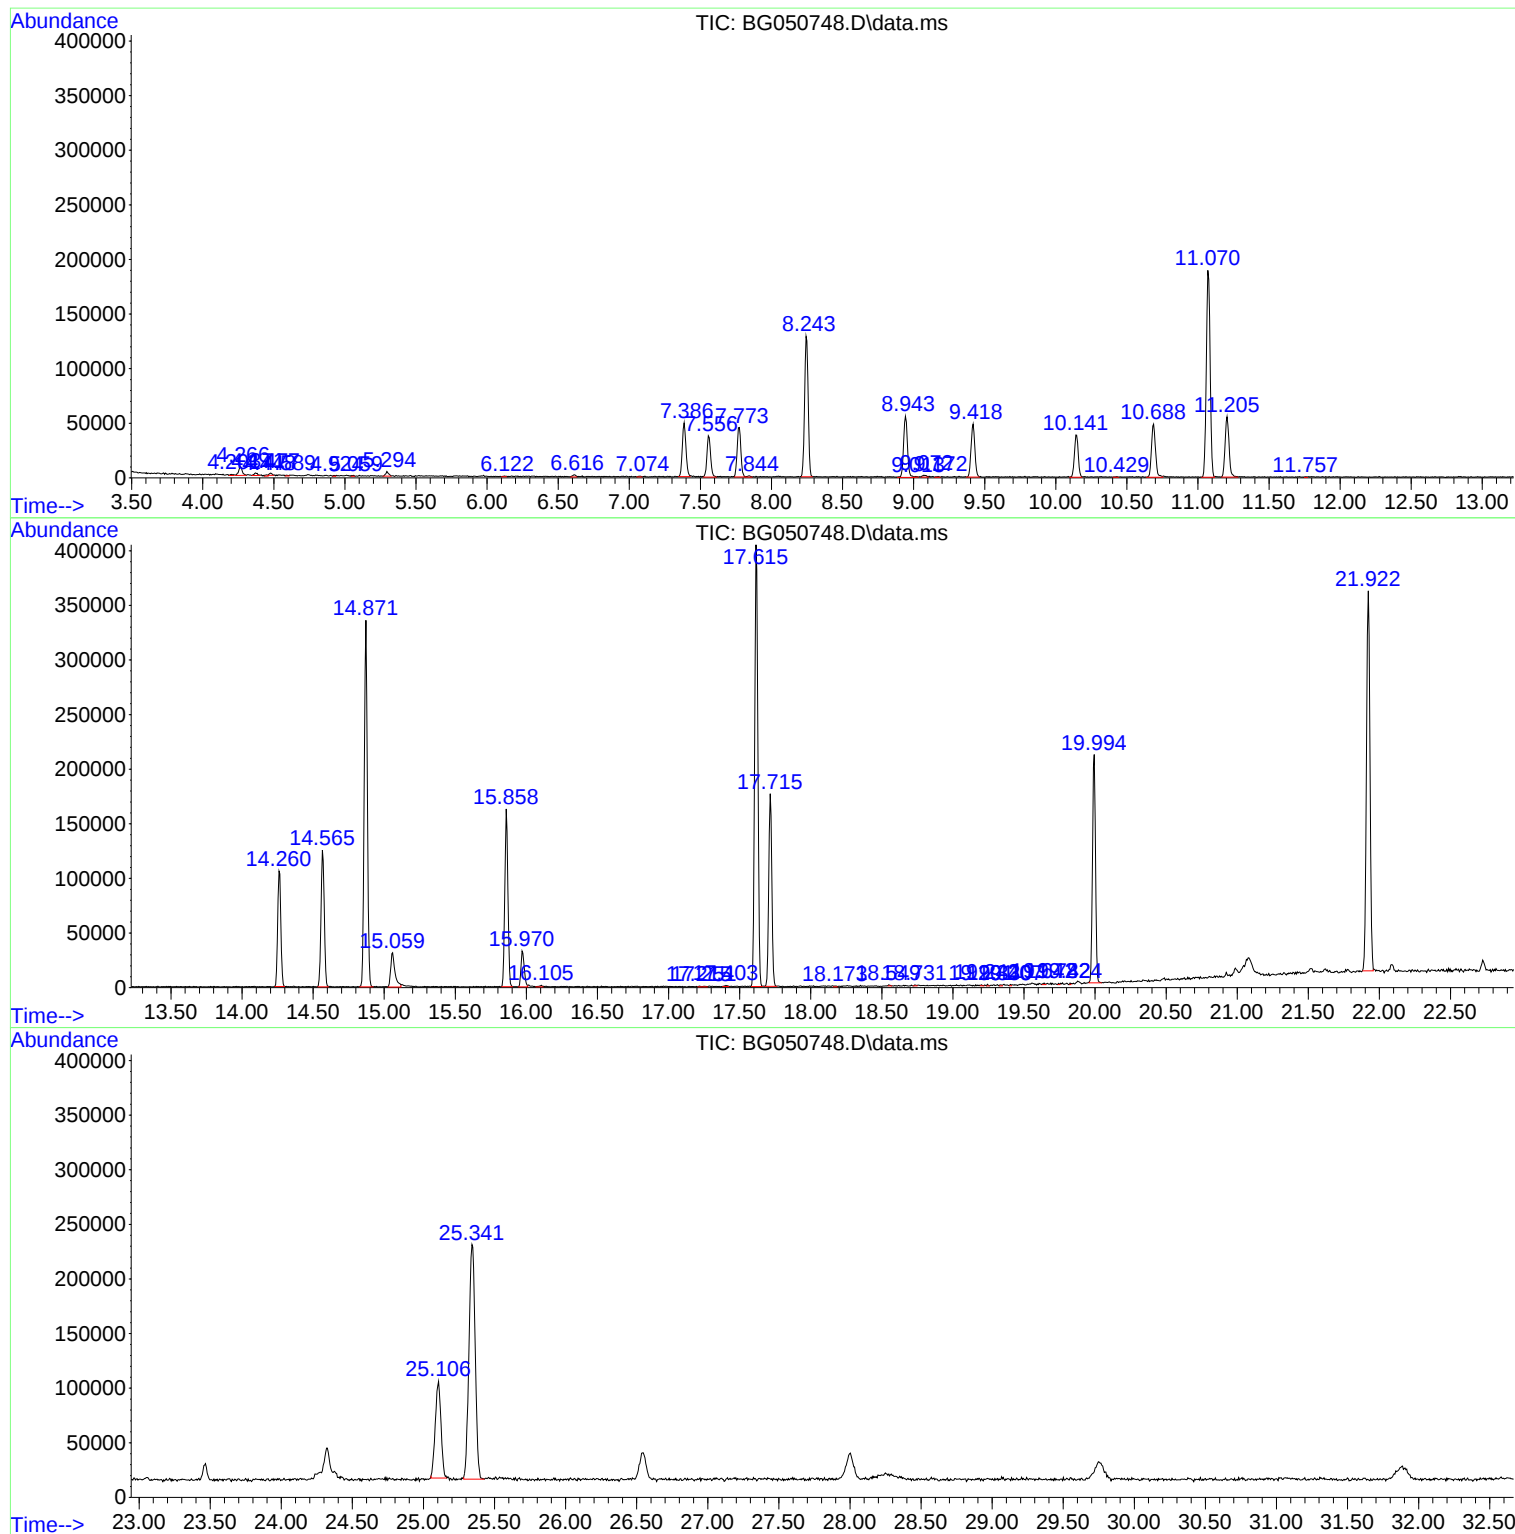

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050748.D
Acq On : 27 Oct 2021 18:28
Operator : CG/JU
Sample : M4205-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050748.D
Acq On : 27 Oct 2021 18:28
Operator : CG/JU
Sample : M4205-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------