

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050750.D
 Acq On : 27 Oct 2021 19:50
 Operator : CG/JU
 Sample : M4205-20
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B40

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.143	107	111	114	rVB4	2555	3681	0.59%	0.066%
2	4.261	127	131	137	rVB2	9055	15419	2.47%	0.277%
3	4.378	147	151	155	rVB5	2465	4276	0.68%	0.077%
4	4.484	164	169	171	rVB4	2388	3541	0.57%	0.064%
5	4.537	174	178	180	rBV3	871	1083	0.17%	0.019%
6	4.743	210	213	216	rBV4	1391	1864	0.30%	0.034%
7	5.295	302	307	313	rVB3	4748	6855	1.10%	0.123%
8	5.371	318	320	323	rBV3	774	1080	0.17%	0.019%
9	5.747	381	384	385	rBV2	782	753	0.12%	0.014%
10	6.100	442	444	447	rBV3	896	923	0.15%	0.017%
11	6.464	504	506	511	rBV2	1295	1388	0.22%	0.025%
12	6.517	513	515	519	rBV3	538	820	0.13%	0.015%
13	6.611	528	531	538	rVV4	2011	3359	0.54%	0.060%
14	6.670	538	541	545	rVB2	604	803	0.13%	0.014%
15	6.805	562	564	568	rBV2	727	1011	0.16%	0.018%
16	6.893	577	579	581	rBV	1268	1086	0.17%	0.020%
17	7.140	618	621	623	rVB2	825	813	0.13%	0.015%
18	7.387	656	663	673	rBV	56320	100622	16.11%	1.810%
19	7.557	685	692	700	rVB	44166	74257	11.89%	1.336%
20	7.769	722	728	736	rVV	54926	95233	15.25%	1.713%
21	7.845	736	741	744	rVB4	1132	1949	0.31%	0.035%
22	8.045	769	775	778	rBV3	621	1185	0.19%	0.021%
23	8.244	802	809	817	rBV	122217	207619	33.24%	3.734%
24	8.803	902	904	906	rBV	853	883	0.14%	0.016%
25	8.938	921	927	939	rVB	62229	114081	18.26%	2.052%
26	9.067	945	949	950	rBV3	1855	1916	0.31%	0.034%
27	9.414	1001	1008	1016	rVB	54176	101313	16.22%	1.822%
28	9.713	1056	1059	1063	rVB2	559	809	0.13%	0.015%
29	10.142	1126	1132	1142	rBV	45233	81540	13.05%	1.467%
30	10.495	1189	1192	1196	rVB	584	712	0.11%	0.013%
31	10.683	1218	1224	1235	rBV	58294	109029	17.45%	1.961%
32	10.777	1237	1240	1242	rVB2	1081	934	0.15%	0.017%
33	10.841	1248	1251	1254	rBV2	652	779	0.12%	0.014%
34	11.071	1283	1290	1298	rBV	177551	321381	51.45%	5.780%
35	11.206	1306	1313	1321	rBV	60538	116046	18.58%	2.087%
36	11.288	1326	1327	1331	rBV	620	715	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050750.D
 Acq On : 27 Oct 2021 19:50
 Operator : CG/JU
 Sample : M4205-20
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

37	11.699	1396	1397	1400	rBV	668	725	0.12%	0.013%
38	14.261	1827	1833	1841	rVB	126738	188338	30.15%	3.387%
39	14.566	1878	1885	1895	rBV	141607	226500	36.26%	4.074%
40	14.872	1930	1937	1945	rVB	292269	466779	74.73%	8.395%
41	15.054	1963	1968	1983	rBV3	33802	73746	11.81%	1.326%
42	15.277	2001	2006	2009	rVB4	2860	3553	0.57%	0.064%
43	15.859	2099	2105	2112	rBV	185674	280379	44.89%	5.043%
44	15.971	2120	2124	2132	rBV2	36334	58034	9.29%	1.044%
45	16.100	2139	2146	2151	rBV2	1348	2257	0.36%	0.041%
46	17.398	2363	2367	2371	rBV4	1074	1629	0.26%	0.029%
47	17.616	2397	2404	2410	rBV	373536	579404	92.76%	10.421%
48	17.657	2410	2411	2415	rVV	16980	17736	2.84%	0.319%
49	17.716	2415	2421	2431	rVV	203971	312053	49.96%	5.612%
50	17.792	2431	2434	2437	rVB2	2962	3422	0.55%	0.062%
51	18.021	2472	2473	2479	rVB3	739	764	0.12%	0.014%
52	18.074	2479	2482	2483	rBV	1071	838	0.13%	0.015%
53	18.250	2509	2512	2517	rBV3	1615	1764	0.28%	0.032%
54	18.491	2550	2553	2557	rBV2	2014	2380	0.38%	0.043%
55	18.544	2557	2562	2568	rVB5	2659	4731	0.76%	0.085%
56	18.597	2568	2571	2572	rBV	849	800	0.13%	0.014%
57	18.626	2572	2576	2577	rBV2	951	993	0.16%	0.018%
58	18.685	2581	2586	2591	rBV4	2807	5441	0.87%	0.098%
59	18.979	2634	2636	2642	rVB3	1539	2142	0.34%	0.039%
60	19.026	2642	2644	2646	rVB2	1027	1015	0.16%	0.018%
61	19.061	2648	2650	2651	rBV2	1020	781	0.13%	0.014%
62	19.232	2676	2679	2681	rBV2	1319	1732	0.28%	0.031%
63	19.273	2684	2686	2691	rVV3	1113	1267	0.20%	0.023%
64	19.537	2728	2731	2733	rBV4	1493	2184	0.35%	0.039%
65	19.561	2733	2735	2737	rVB2	1804	2003	0.32%	0.036%
66	19.661	2747	2752	2758	rVB	28423	38698	6.20%	0.696%
67	19.831	2779	2781	2782	rBV2	1315	864	0.14%	0.016%
68	19.878	2787	2789	2792	rBV2	3602	4103	0.66%	0.074%
69	19.990	2803	2808	2820	rVB	246049	394908	63.22%	7.102%
70	20.084	2822	2824	2825	rBV	1677	1152	0.18%	0.021%
71	21.923	3129	3137	3143	rBV	330286	590923	94.60%	10.628%
72	25.101	3670	3678	3688	rBV2	101582	281707	45.10%	5.067%
73	25.342	3709	3719	3732	rVB	206462	624637	100.00%	11.234%



Sum of corrected areas: 5560140

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050750.D
Acq On : 27 Oct 2021 19:50
Operator : CG/JU
Sample : M4205-20
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B40

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

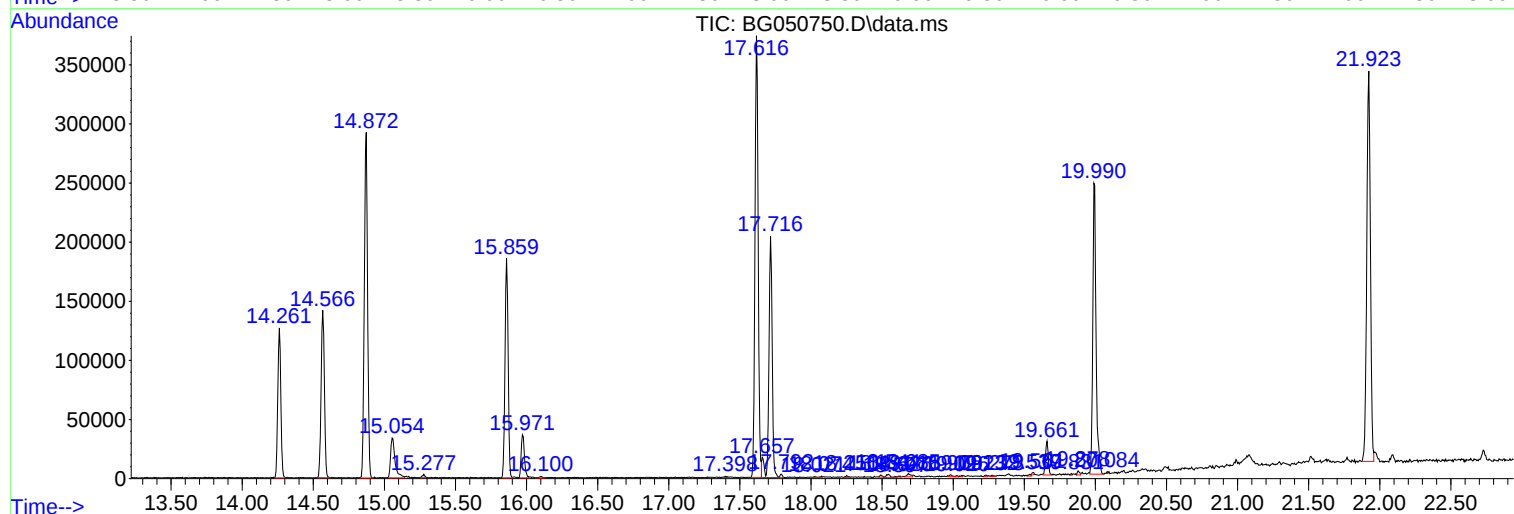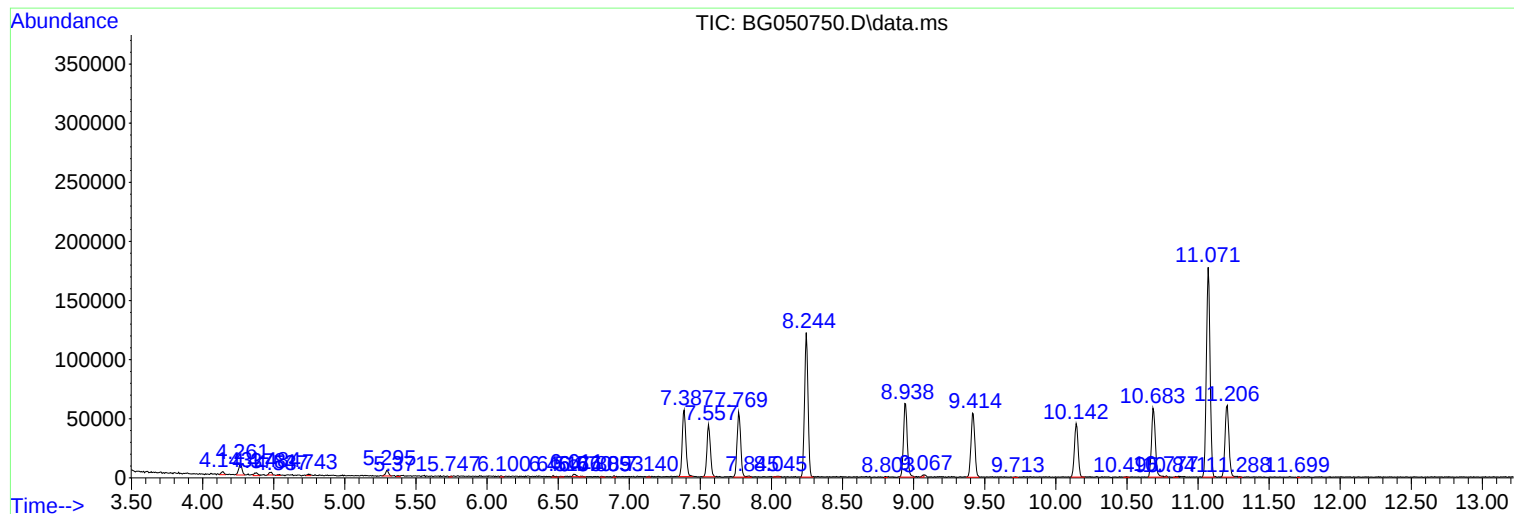

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050750.D
Acq On : 27 Oct 2021 19:50
Operator : CG/JU
Sample : M4205-20
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B40

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050750.D
Acq On : 27 Oct 2021 19:50
Operator : CG/JU
Sample : M4205-20
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B40

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------