

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050752.D
 Acq On : 27 Oct 2021 21:12
 Operator : CG/JU
 Sample : M4205-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.813	53	55	58	rBV3	833	875	0.14%	0.014%
2	3.878	65	66	70	rBV	1410	1403	0.23%	0.023%
3	4.042	91	94	103	rBV3	5380	10774	1.78%	0.175%
4	4.136	105	110	118	rVB2	2359	3832	0.63%	0.062%
5	4.265	127	132	138	rVB2	9011	14855	2.46%	0.242%
6	4.371	147	150	155	rVB3	2183	3058	0.51%	0.050%
7	4.477	164	168	173	rBV4	2683	3681	0.61%	0.060%
8	4.747	208	214	217	rVV4	1196	1836	0.30%	0.030%
9	4.806	221	224	227	rVB2	822	811	0.13%	0.013%
10	5.029	261	262	265	rVB2	901	763	0.13%	0.012%
11	5.059	265	267	270	rBV	865	1069	0.18%	0.017%
12	5.294	300	307	313	rBV2	4915	9015	1.49%	0.147%
13	5.382	320	322	325	rBV2	622	778	0.13%	0.013%
14	5.940	415	417	420	rVB3	644	730	0.12%	0.012%
15	6.075	437	440	443	rVB2	681	857	0.14%	0.014%
16	6.222	461	465	468	rBV3	917	1161	0.19%	0.019%
17	6.539	515	519	522	rBV3	782	864	0.14%	0.014%
18	6.616	526	532	539	rVV2	1957	3583	0.59%	0.058%
19	7.385	657	663	671	rBV	68573	124564	20.60%	2.026%
20	7.556	686	692	700	rBV	53623	93666	15.49%	1.524%
21	7.767	722	728	737	rBV	65960	117732	19.47%	1.915%
22	7.844	737	741	743	rBV3	1006	1170	0.19%	0.019%
23	8.043	773	775	780	rVB3	801	1033	0.17%	0.017%
24	8.243	802	809	819	rVB	114912	195370	32.31%	3.178%
25	8.461	841	846	850	rBV3	1206	1604	0.27%	0.026%
26	8.543	857	860	864	rVB2	573	873	0.14%	0.014%
27	8.672	881	882	888	rVB3	522	720	0.12%	0.012%
28	8.942	921	928	938	rBV2	72817	130066	21.51%	2.116%
29	9.072	944	950	956	rBV	2907	5244	0.87%	0.085%
30	9.207	971	973	979	rBV2	519	765	0.13%	0.012%
31	9.418	1001	1009	1016	rBV	69266	128284	21.22%	2.087%
32	9.788	1069	1072	1075	rBV	594	701	0.12%	0.011%
33	9.982	1104	1105	1108	rVB	872	715	0.12%	0.012%
34	10.141	1126	1132	1143	rVB	56549	105358	17.42%	1.714%
35	10.687	1218	1225	1235	rBV	72689	138611	22.92%	2.255%
36	10.817	1242	1247	1259	rBV2	9575	20412	3.38%	0.332%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050752.D
 Acq On : 27 Oct 2021 21:12
 Operator : CG/JU
 Sample : M4205-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

37	10.911	1261	1263	1266	rVV2	1170	1314	0.22%	0.021%
38	10.934	1266	1267	1270	rVB3	967	744	0.12%	0.012%
39	11.069	1283	1290	1299	rBV	168127	309690	51.22%	5.038%
40	11.204	1306	1313	1324	rBV	77960	147965	24.47%	2.407%
41	12.714	1563	1570	1575	rBV4	1678	3134	0.52%	0.051%
42	12.932	1603	1607	1612	rVB4	1457	2467	0.41%	0.040%
43	13.666	1730	1732	1735	rVB2	712	767	0.13%	0.012%
44	14.195	1818	1822	1827	rVB2	729	901	0.15%	0.015%
45	14.260	1827	1833	1843	rBV	160094	235818	39.00%	3.836%
46	14.565	1878	1885	1893	rBV	176501	284569	47.06%	4.629%
47	14.730	1909	1913	1916	rBV2	756	847	0.14%	0.014%
48	14.871	1930	1937	1945	rVB	282073	451388	74.65%	7.343%
49	15.053	1963	1968	1983	rBV2	43471	91551	15.14%	1.489%
50	15.276	2000	2006	2011	rVB3	2044	3559	0.59%	0.058%
51	15.676	2071	2074	2077	rVB	949	1021	0.17%	0.017%
52	15.858	2099	2105	2117	rVB	226494	353958	58.54%	5.758%
53	15.969	2119	2124	2135	rVV	46673	77576	12.83%	1.262%
54	16.099	2141	2146	2149	rVB2	1547	2420	0.40%	0.039%
55	16.563	2217	2225	2229	rBV5	2383	4823	0.80%	0.078%
56	17.139	2319	2323	2327	rBV3	1003	1705	0.28%	0.028%
57	17.203	2332	2334	2336	rBV	690	710	0.12%	0.012%
58	17.333	2351	2356	2359	rBV3	1031	1374	0.23%	0.022%
59	17.409	2365	2369	2371	rBV2	1289	1138	0.19%	0.019%
60	17.562	2393	2395	2397	rBV2	797	705	0.12%	0.011%
61	17.615	2398	2404	2415	rVV	357254	559614	92.55%	9.104%
62	17.714	2415	2421	2430	rVV2	251372	381154	63.04%	6.201%
63	17.791	2430	2434	2436	rVB4	4210	5247	0.87%	0.085%
64	17.985	2466	2467	2470	rBV	787	927	0.15%	0.015%
65	18.079	2479	2483	2486	rVB3	1553	2066	0.34%	0.034%
66	18.120	2489	2490	2496	rVV3	487	856	0.14%	0.014%
67	18.255	2508	2513	2517	rVB4	4042	4249	0.70%	0.069%
68	18.367	2530	2532	2535	rVB3	827	893	0.15%	0.015%
69	18.496	2550	2554	2557	rBV3	1413	1716	0.28%	0.028%
70	18.549	2558	2563	2565	rVV4	1467	2217	0.37%	0.036%
71	18.619	2573	2575	2577	rVB2	1362	718	0.12%	0.012%
72	18.684	2584	2586	2588	rVB2	1107	772	0.13%	0.013%
73	18.895	2620	2622	2626	rBV4	896	705	0.12%	0.011%
74	19.066	2648	2651	2653	rBV4	990	957	0.16%	0.016%
75	19.113	2657	2659	2661	rBV3	771	684	0.11%	0.011%
76	19.160	2666	2667	2670	rBV	1327	1186	0.20%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050752.D
 Acq On : 27 Oct 2021 21:12
 Operator : CG/JU
 Sample : M4205-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B10

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

77	19.277	2685	2687	2692	rBV4	1087	1533	0.25%	0.025%
78	19.383	2703	2705	2708	rBV4	2073	2736	0.45%	0.045%
79	19.412	2708	2710	2713	rVB3	2842	2433	0.40%	0.040%
80	19.559	2732	2735	2742	rVB5	3677	5884	0.97%	0.096%
81	19.630	2745	2747	2749	rVV3	1869	1659	0.27%	0.027%
82	19.659	2749	2752	2758	rVB	7499	10968	1.81%	0.178%
83	19.806	2775	2777	2778	rBV2	1049	858	0.14%	0.014%
84	19.877	2787	2789	2792	rBV4	2429	2486	0.41%	0.040%
85	19.994	2803	2809	2819	rVB	307121	461056	76.25%	7.500%
86	20.076	2819	2823	2824	rBV2	1494	1680	0.28%	0.027%
87	20.482	2890	2892	2900	rVB6	3675	5601	0.93%	0.091%
88	21.921	3130	3137	3149	rVB	322135	556628	92.06%	9.055%
89	24.318	3540	3545	3553	rVB4	26829	55927	9.25%	0.910%
90	25.100	3670	3678	3689	rVB2	129524	362062	59.88%	5.890%
91	25.341	3709	3719	3733	rVB	201435	604650	100.00%	9.836%




Sum of corrected areas: 6147099

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050752.D
Acq On : 27 Oct 2021 21:12
Operator : CG/JU
Sample : M4205-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

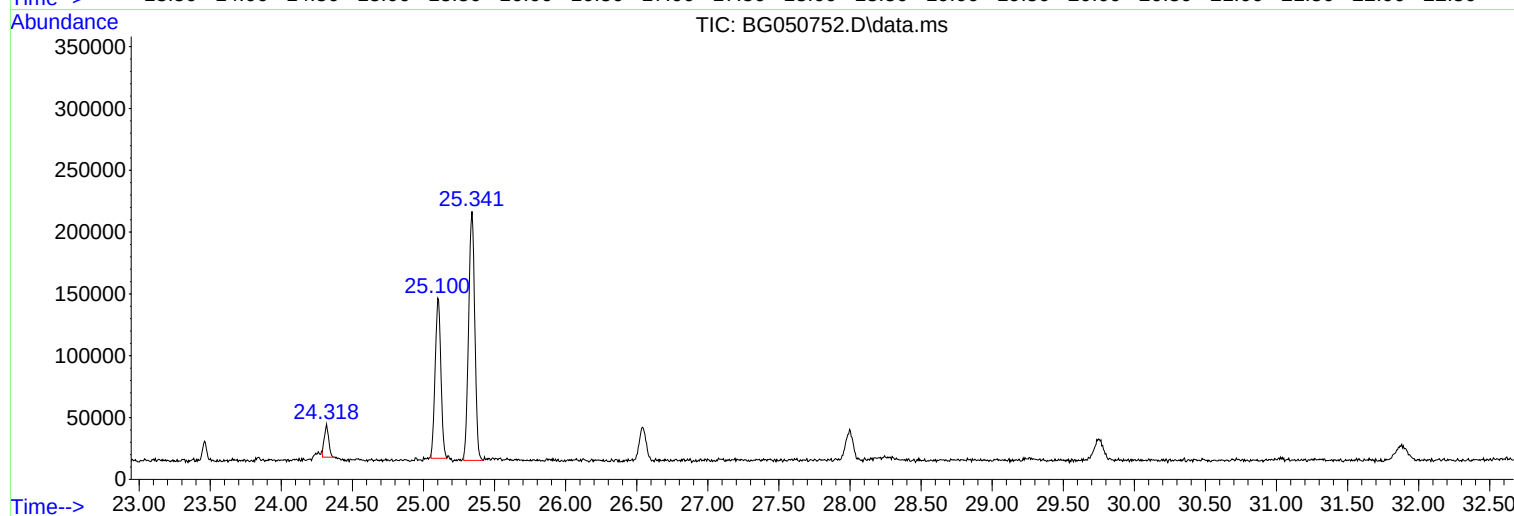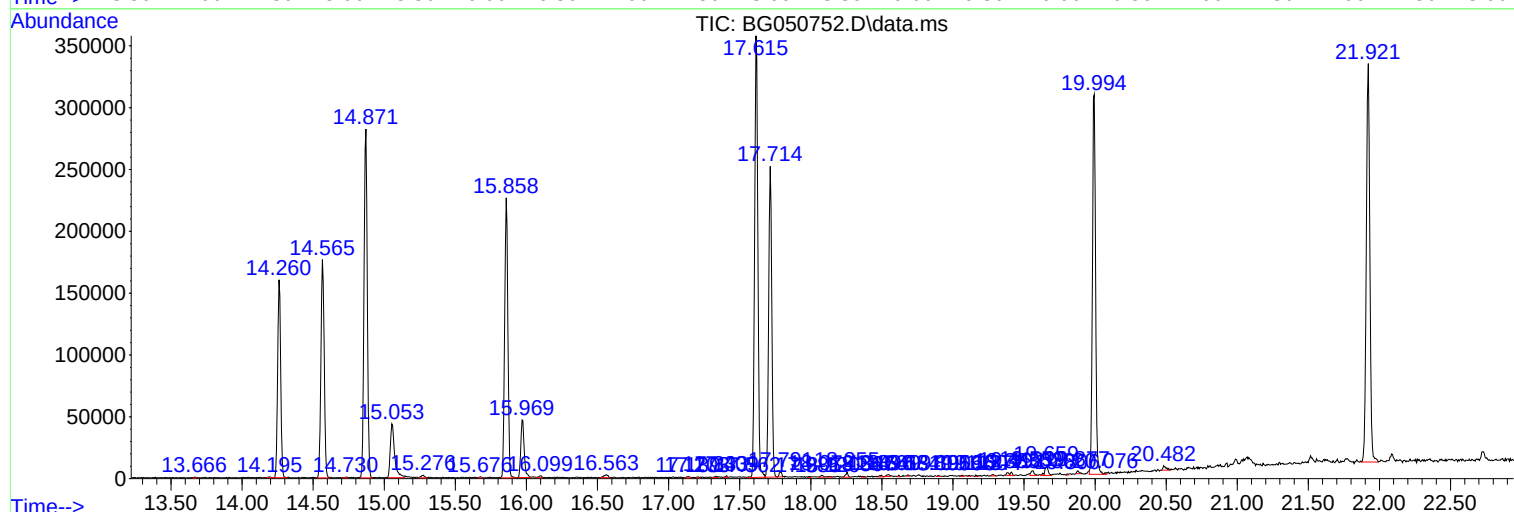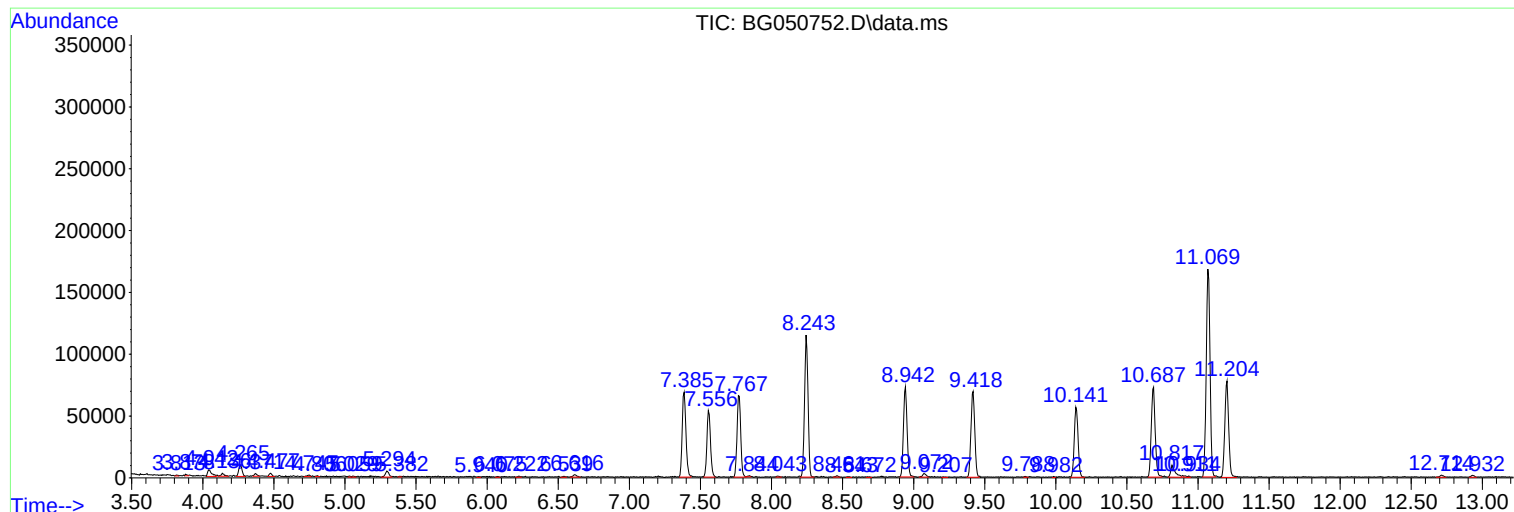

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050752.D
Acq On : 27 Oct 2021 21:12
Operator : CG/JU
Sample : M4205-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050752.D
Acq On : 27 Oct 2021 21:12
Operator : CG/JU
Sample : M4205-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
