

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050753.D
 Acq On : 27 Oct 2021 21:54
 Operator : CG/JU
 Sample : M4205-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050753.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.263	128	132	137	rVB	10030	16532	2.84%	0.316%
2	4.475	166	168	173	rVB3	2787	3781	0.65%	0.072%
3	4.745	211	214	219	rVB4	1693	2419	0.42%	0.046%
4	5.297	303	308	313	rBV3	4934	8524	1.46%	0.163%
5	5.944	417	418	421	rVB2	1012	689	0.12%	0.013%
6	6.613	528	532	536	rVB5	2573	4398	0.75%	0.084%
7	6.649	536	538	539	rBV2	820	810	0.14%	0.015%
8	7.195	627	631	633	rBV3	749	1052	0.18%	0.020%
9	7.383	656	663	672	rBV	54556	99665	17.11%	1.907%
10	7.489	677	681	682	rVB4	798	807	0.14%	0.015%
11	7.559	682	693	701	rBV	42757	76717	13.17%	1.468%
12	7.771	722	729	737	rVV	52666	90503	15.53%	1.731%
13	7.841	738	741	743	rVB2	1141	1228	0.21%	0.023%
14	8.012	767	770	773	rBV2	822	1162	0.20%	0.022%
15	8.047	773	776	779	rVV4	992	1411	0.24%	0.027%
16	8.247	803	810	819	rVB	111295	195304	33.52%	3.736%
17	8.364	827	830	833	rVB3	604	800	0.14%	0.015%
18	8.400	833	836	841	rBV4	669	1279	0.22%	0.024%
19	8.652	877	879	881	rVB	810	721	0.12%	0.014%
20	8.811	904	906	910	rVB3	756	691	0.12%	0.013%
21	8.881	915	918	920	rBV3	533	755	0.13%	0.014%
22	8.940	922	928	937	rBV	59631	106419	18.27%	2.036%
23	9.075	946	951	955	rBV3	2831	4875	0.84%	0.093%
24	9.416	1002	1009	1020	rVB	54412	96961	16.64%	1.855%
25	10.074	1119	1121	1124	rVB3	1003	809	0.14%	0.015%
26	10.145	1124	1133	1142	rBV	43559	80272	13.78%	1.536%
27	10.268	1153	1154	1159	rBV2	504	708	0.12%	0.014%
28	10.685	1218	1225	1234	rBV2	53276	102576	17.61%	1.962%
29	10.850	1248	1253	1256	rBV2	695	1032	0.18%	0.020%
30	11.073	1282	1291	1300	rBV	169414	301828	51.80%	5.774%
31	11.202	1306	1313	1322	rBV	58564	109342	18.77%	2.092%
32	11.326	1331	1334	1338	rVB3	687	894	0.15%	0.017%
33	11.631	1384	1386	1392	rVB3	442	686	0.12%	0.013%
34	12.083	1457	1463	1464	rBV3	880	1247	0.21%	0.024%
35	12.213	1482	1485	1489	rBV3	743	919	0.16%	0.018%
36	12.935	1606	1608	1612	rVB3	694	866	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050753.D
 Acq On : 27 Oct 2021 21:54
 Operator : CG/JU
 Sample : M4205-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

37	13.670	1731	1733	1737	rBV3	1040	1021	0.18%	0.020%
38	13.729	1741	1743	1745	rBV2	688	736	0.13%	0.014%
39	14.022	1791	1793	1798	rBV3	540	892	0.15%	0.017%
40	14.263	1826	1834	1840	rBV	116056	178305	30.60%	3.411%
41	14.569	1879	1886	1892	rBV	131471	213591	36.66%	4.086%
42	14.868	1929	1937	1946	rBV	273193	435264	74.71%	8.327%
43	15.056	1962	1969	1982	rBV2	34140	72789	12.49%	1.392%
44	15.274	2002	2006	2011	rVB5	2185	3481	0.60%	0.067%
45	15.485	2039	2042	2047	rVB	696	913	0.16%	0.017%
46	15.673	2070	2074	2078	rVB3	626	977	0.17%	0.019%
47	15.856	2098	2105	2112	rBV	170337	269261	46.22%	5.151%
48	15.973	2119	2125	2136	rVB2	34876	57888	9.94%	1.107%
49	16.091	2144	2145	2148	rBV4	1120	1198	0.21%	0.023%
50	16.555	2222	2224	2229	rVB4	1184	1392	0.24%	0.027%
51	16.790	2259	2264	2265	rVB2	566	701	0.12%	0.013%
52	17.054	2306	2309	2311	rBV2	726	684	0.12%	0.013%
53	17.301	2348	2351	2353	rVB	758	714	0.12%	0.014%
54	17.395	2364	2367	2371	rBV3	1135	1728	0.30%	0.033%
55	17.454	2374	2377	2379	rVB	1122	811	0.14%	0.016%
56	17.542	2389	2392	2395	rBV3	773	743	0.13%	0.014%
57	17.618	2398	2405	2415	rVV	358718	556531	95.52%	10.647%
58	17.718	2415	2422	2430	rVV2	191105	294482	50.54%	5.633%
59	17.789	2430	2434	2438	rVB	1829	2507	0.43%	0.048%
60	17.877	2446	2449	2450	rBV	689	686	0.12%	0.013%
61	17.947	2459	2461	2463	rVB	1073	738	0.13%	0.014%
62	18.012	2471	2472	2476	rVB3	900	836	0.14%	0.016%
63	18.047	2476	2478	2480	rBV	820	844	0.14%	0.016%
64	18.118	2487	2490	2491	rBV2	825	902	0.15%	0.017%
65	18.135	2491	2493	2495	rVB2	783	757	0.13%	0.014%
66	18.170	2495	2499	2500	rBV2	856	1015	0.17%	0.019%
67	18.253	2510	2513	2518	rVB5	1988	2805	0.48%	0.054%
68	18.546	2558	2563	2568	rBV3	1330	2508	0.43%	0.048%
69	18.687	2583	2587	2589	rBV4	1519	1763	0.30%	0.034%
70	18.764	2596	2600	2603	rBV4	1139	1483	0.25%	0.028%
71	18.834	2611	2612	2616	rBV2	750	848	0.15%	0.016%
72	18.870	2616	2618	2622	rBV2	783	1032	0.18%	0.020%
73	19.158	2664	2667	2670	rBV3	883	873	0.15%	0.017%
74	19.281	2686	2688	2692	rBV3	1233	1484	0.25%	0.028%
75	19.328	2694	2696	2698	rVV2	921	744	0.13%	0.014%
76	19.387	2703	2706	2708	rBV4	1645	2225	0.38%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050753.D
 Acq On : 27 Oct 2021 21:54
 Operator : CG/JU
 Sample : M4205-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AZ5

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

77	19.410	2708	2710	2711	rBV2	927	689	0.12%	0.013%
78	19.451	2715	2717	2719	rVB2	1204	870	0.15%	0.017%
79	19.492	2719	2724	2725	rBV2	1225	1827	0.31%	0.035%
80	19.663	2748	2753	2758	rVB	8284	13037	2.24%	0.249%
81	19.710	2758	2761	2763	rBV3	1268	1160	0.20%	0.022%
82	19.745	2765	2767	2771	rVV4	927	1106	0.19%	0.021%
83	19.810	2776	2778	2779	rVB2	1347	746	0.13%	0.014%
84	19.880	2787	2790	2791	rBV2	2896	2357	0.40%	0.045%
85	19.992	2803	2809	2819	rVB	242142	355181	60.96%	6.795%
86	20.244	2851	2852	2853	rBV	2757	1241	0.21%	0.024%
87	21.919	3130	3137	3144	rBV	318606	550181	94.43%	10.525%
88	25.104	3670	3679	3691	rVB2	98045	279492	47.97%	5.347%
89	25.339	3710	3719	3731	rVB2	196846	582626	100.00%	11.146%




Sum of corrected areas: 5227347

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050753.D
Acq On : 27 Oct 2021 21:54
Operator : CG/JU
Sample : M4205-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AZ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

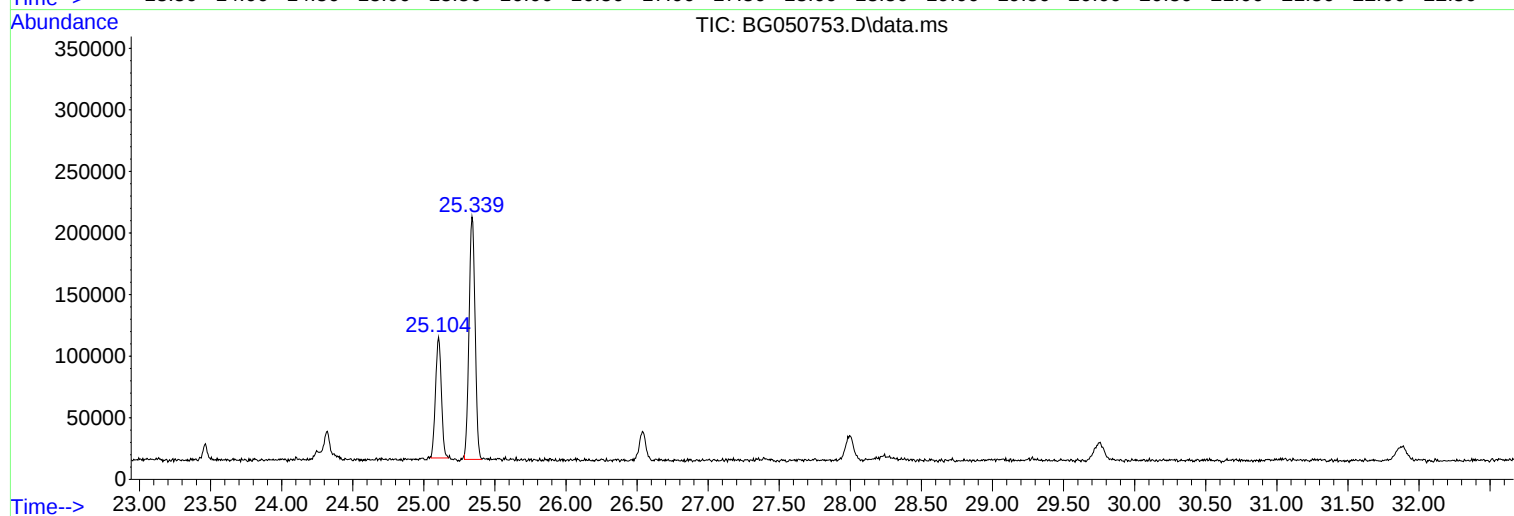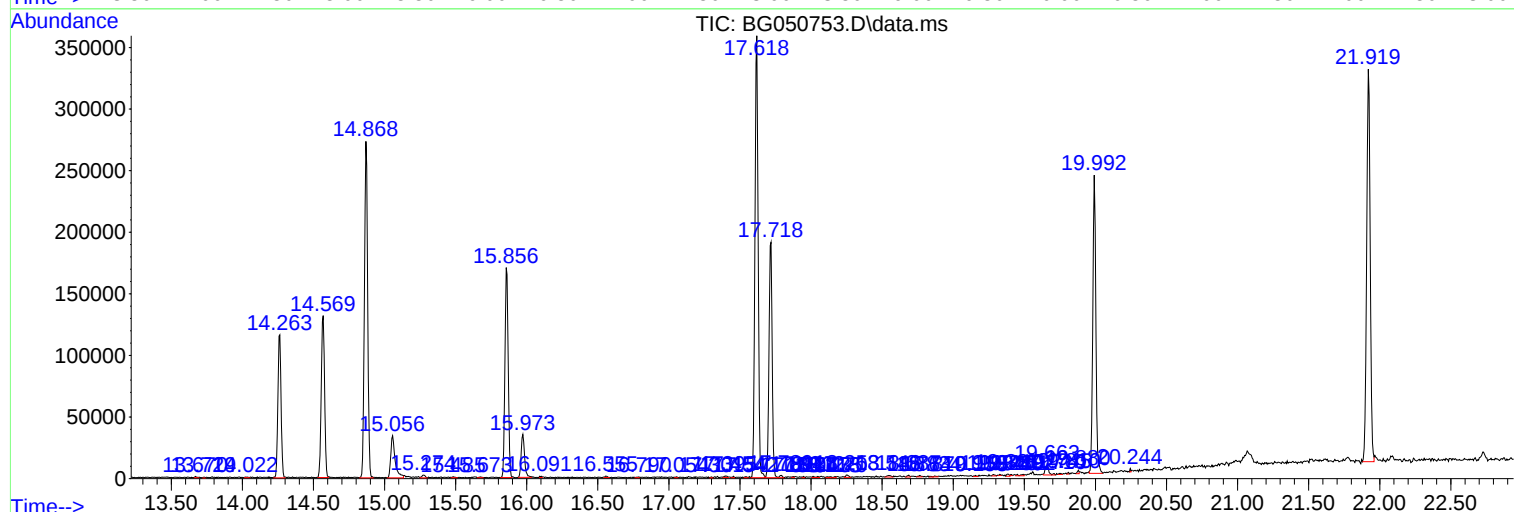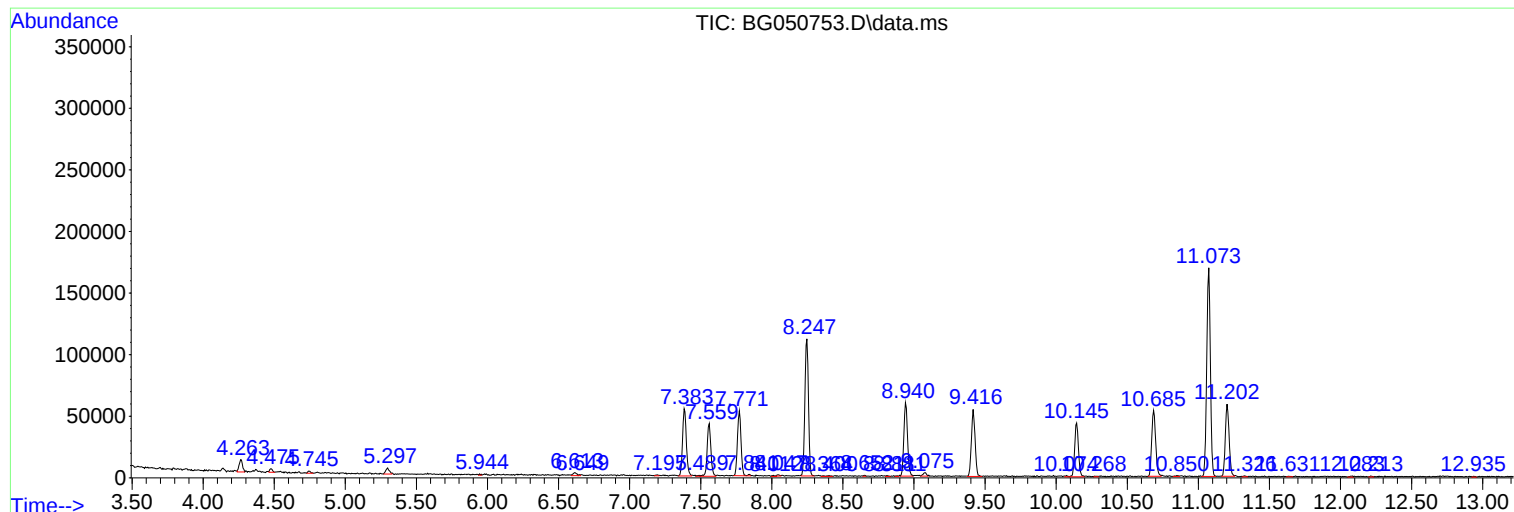

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050753.D
Acq On : 27 Oct 2021 21:54
Operator : CG/JU
Sample : M4205-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AZ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050753.D
Acq On : 27 Oct 2021 21:54
Operator : CG/JU
Sample : M4205-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AZ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------