

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050754.D
 Acq On : 27 Oct 2021 22:35
 Operator : CG/JU
 Sample : M4205-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B39

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.269	128	133	139	rVB	9288	15101	2.41%	0.288%
2	4.480	165	169	173	rVB4	3192	4855	0.77%	0.092%
3	4.980	252	254	255	rBV	1148	768	0.12%	0.015%
4	5.297	302	308	313	rBV3	4863	8001	1.28%	0.152%
5	6.126	446	449	453	rBV4	798	1109	0.18%	0.021%
6	6.613	529	532	538	rVB4	2244	3763	0.60%	0.072%
7	6.713	547	549	551	rBV2	822	727	0.12%	0.014%
8	7.301	648	649	652	rBV2	660	769	0.12%	0.015%
9	7.383	657	663	672	rVB	51492	93329	14.89%	1.778%
10	7.559	686	693	702	rBV	40067	70544	11.26%	1.344%
11	7.771	722	729	738	rVB	51121	87621	13.98%	1.669%
12	7.947	756	759	762	rBV2	678	891	0.14%	0.017%
13	8.041	772	775	778	rBV4	1090	1579	0.25%	0.030%
14	8.153	791	794	795	rBV2	775	735	0.12%	0.014%
15	8.247	803	810	819	rVB	119704	213710	34.10%	4.071%
16	8.464	844	847	848	rVB3	927	844	0.13%	0.016%
17	8.940	921	928	937	rBV	60155	108808	17.36%	2.073%
18	9.075	945	951	955	rVB4	1865	3361	0.54%	0.064%
19	9.416	1002	1009	1017	rBV	51844	92786	14.81%	1.768%
20	10.144	1127	1133	1142	rVB2	41209	74706	11.92%	1.423%
21	10.327	1162	1164	1167	rBV2	603	802	0.13%	0.015%
22	10.685	1218	1225	1235	rBV2	53423	98655	15.74%	1.879%
23	10.750	1235	1236	1242	rVB4	1099	1239	0.20%	0.024%
24	10.879	1254	1258	1261	rBV3	465	785	0.13%	0.015%
25	11.073	1282	1291	1299	rBV	175311	328779	52.46%	6.263%
26	11.202	1306	1313	1321	rBV	59654	113184	18.06%	2.156%
27	11.696	1393	1397	1400	rBV3	634	814	0.13%	0.016%
28	12.724	1570	1572	1575	rBV2	623	771	0.12%	0.015%
29	12.835	1589	1591	1595	rVB2	564	822	0.13%	0.016%
30	12.877	1595	1598	1602	rBV2	532	878	0.14%	0.017%
31	13.112	1635	1638	1642	rBV3	787	976	0.16%	0.019%
32	13.775	1750	1751	1757	rVB3	634	789	0.13%	0.015%
33	14.263	1826	1834	1841	rBV	113138	171794	27.41%	3.273%
34	14.563	1878	1885	1893	rBV	127975	208478	33.27%	3.972%
35	14.868	1929	1937	1944	rBV	297573	470345	75.05%	8.960%
36	15.056	1963	1969	1978	rBV	32067	65954	10.52%	1.256%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050754.D
 Acq On : 27 Oct 2021 22:35
 Operator : CG/JU
 Sample : M4205-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B39

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

37	15.144	1983	1984	1991	rVB3	1497	1989	0.32%	0.038%
38	15.585	2057	2059	2062	rBV2	650	742	0.12%	0.014%
39	15.855	2099	2105	2112	rVB	164506	257305	41.06%	4.902%
40	15.973	2119	2125	2133	rBV2	35404	55653	8.88%	1.060%
41	16.102	2143	2147	2149	rBV3	995	1393	0.22%	0.027%
42	17.407	2365	2369	2373	rBV3	1211	1279	0.20%	0.024%
43	17.501	2382	2385	2390	rBV4	619	943	0.15%	0.018%
44	17.618	2398	2405	2413	rBV	375706	585891	93.49%	11.161%
45	17.712	2415	2421	2430	rVB	180340	281426	44.91%	5.361%
46	18.112	2488	2489	2492	rBV	710	730	0.12%	0.014%
47	18.223	2504	2508	2511	rBV2	467	839	0.13%	0.016%
48	18.482	2549	2552	2554	rBV3	853	920	0.15%	0.018%
49	18.634	2577	2578	2582	rBV2	566	717	0.11%	0.014%
50	18.928	2625	2628	2632	rBV4	599	761	0.12%	0.014%
51	19.251	2680	2683	2684	rBV	1144	1080	0.17%	0.021%
52	19.404	2707	2709	2713	rVB2	1165	1354	0.22%	0.026%
53	19.557	2733	2735	2738	rVB3	2361	2131	0.34%	0.041%
54	19.880	2786	2790	2793	rBV3	2665	3220	0.51%	0.061%
55	19.992	2803	2809	2816	rBV	227498	324908	51.85%	6.190%
56	20.174	2838	2840	2841	rBV	1608	900	0.14%	0.017%
57	20.244	2850	2852	2854	rBV2	1830	1620	0.26%	0.031%
58	20.444	2884	2886	2887	rBV	1664	991	0.16%	0.019%
59	21.919	3130	3137	3146	rBV	337965	581784	92.84%	11.083%
60	25.103	3670	3679	3690	rVB	98310	264948	42.28%	5.047%
61	25.338	3709	3719	3732	rVB2	203943	626686	100.00%	11.939%




Sum of corrected areas: 5249282

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050754.D
Acq On : 27 Oct 2021 22:35
Operator : CG/JU
Sample : M4205-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B39

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

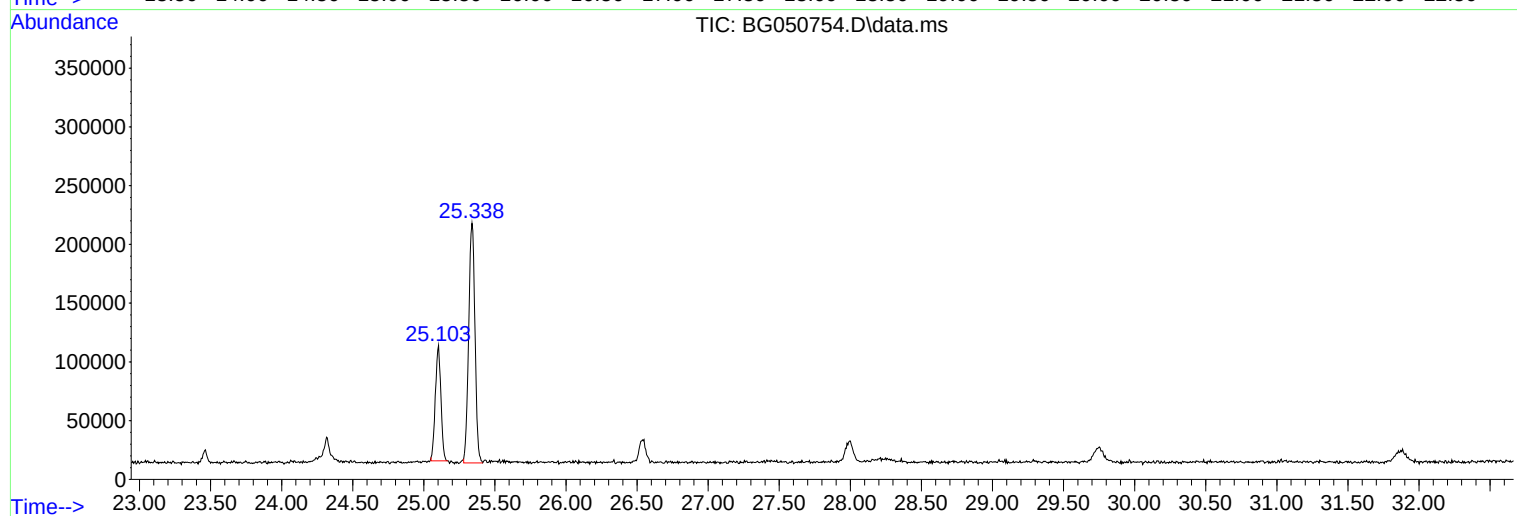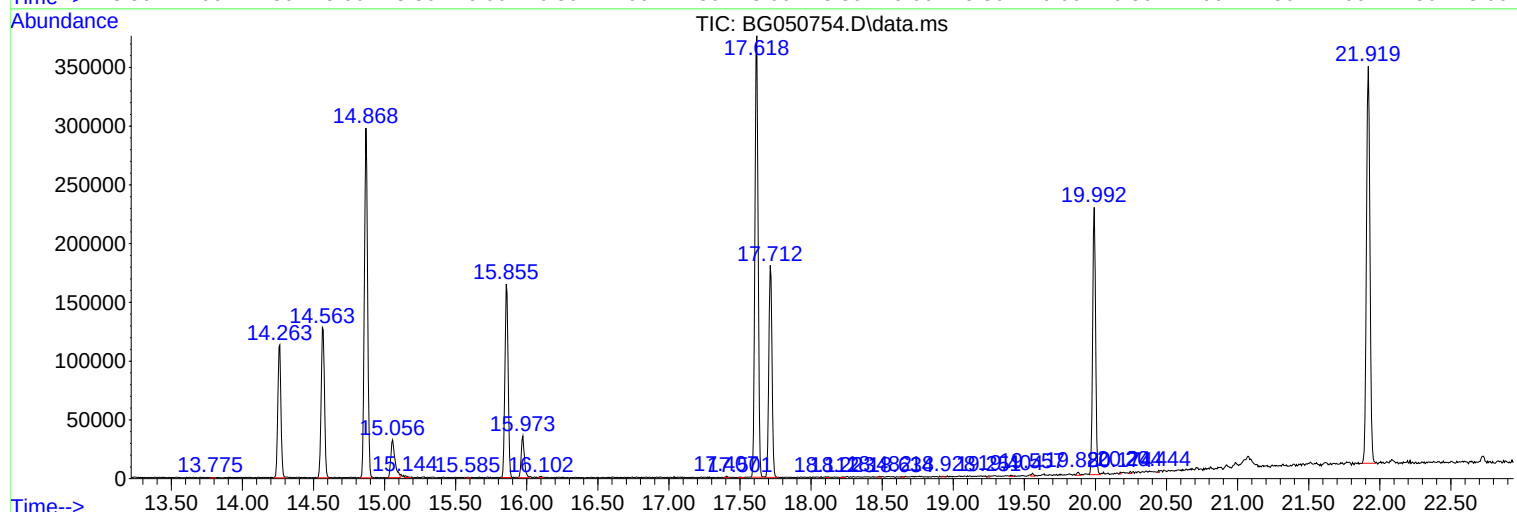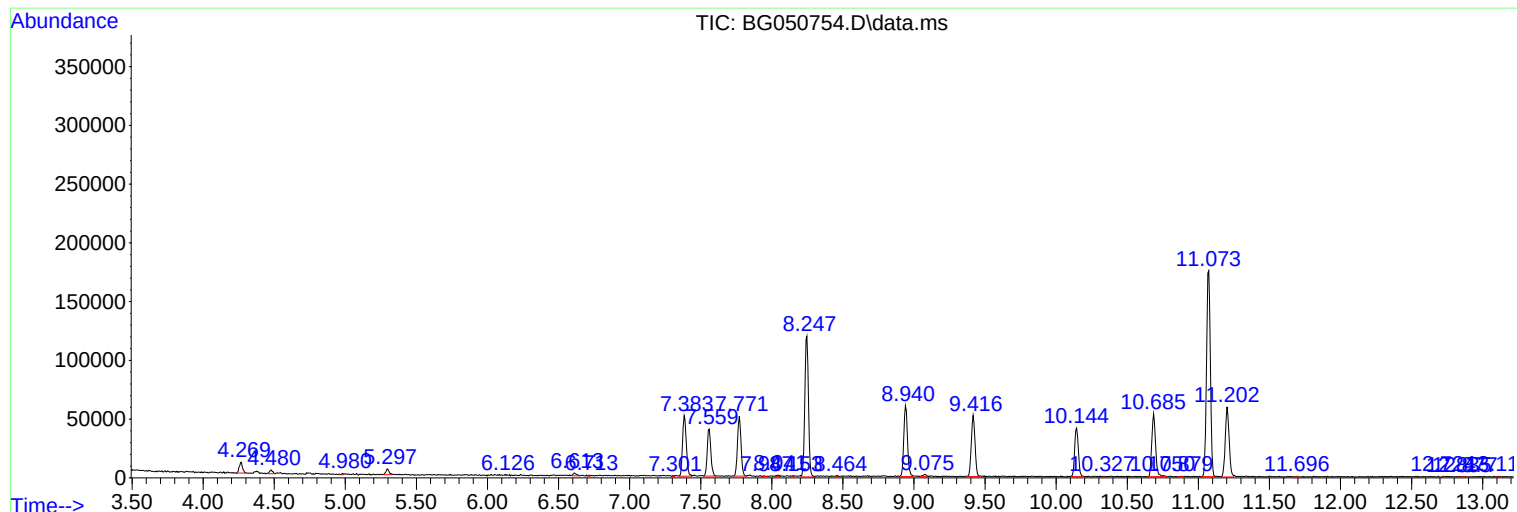

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050754.D
Acq On : 27 Oct 2021 22:35
Operator : CG/JU
Sample : M4205-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B39

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050754.D
Acq On : 27 Oct 2021 22:35
Operator : CG/JU
Sample : M4205-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B39

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------