

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050764.D
 Acq On : 28 Oct 2021 6:08
 Operator : CG/JU
 Sample : PB140136BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.600	15	19	25	rVV2	10755	17061	1.39%	0.137%
2	4.023	86	91	107	rBV	145940	264728	21.54%	2.128%
3	4.376	146	151	156	rVB2	3425	5650	0.46%	0.045%
4	7.384	655	663	676	rBV	178005	323354	26.31%	2.599%
5	7.555	683	692	703	rBV	136495	240759	19.59%	1.935%
6	7.766	721	728	739	rBV	169321	303390	24.68%	2.438%
7	8.242	803	809	817	rBV	130332	224062	18.23%	1.801%
8	8.935	920	927	936	rBV	205306	375391	30.54%	3.017%
9	9.417	999	1009	1021	rBV	169422	317628	25.84%	2.553%
10	10.140	1125	1132	1140	rVB	147538	267938	21.80%	2.153%
11	10.680	1216	1224	1234	rBV	188495	358665	29.18%	2.882%
12	10.768	1238	1239	1245	rVB3	1152	1493	0.12%	0.012%
13	11.068	1281	1290	1299	rBV	187583	343054	27.91%	2.757%
14	11.197	1306	1312	1324	rBV	202001	387075	31.49%	3.111%
15	12.643	1553	1558	1564	rVB	2778	5143	0.42%	0.041%
16	14.259	1827	1833	1840	rBV	428903	643085	52.32%	5.168%
17	14.564	1878	1885	1894	rVB	431079	698541	56.84%	5.614%
18	14.870	1930	1937	1944	rBV	301727	484827	39.45%	3.896%
19	15.052	1961	1968	1981	rBV	183566	330958	26.93%	2.660%
20	15.857	2098	2105	2115	rVB	584323	897956	73.06%	7.217%
21	15.968	2118	2124	2135	rBV	194473	301127	24.50%	2.420%
22	16.098	2142	2146	2152	rVB2	6448	7912	0.64%	0.064%
23	17.408	2362	2369	2373	rBV3	937	1634	0.13%	0.013%
24	17.613	2396	2404	2412	rBV	382205	604597	49.19%	4.859%
25	17.713	2414	2421	2432	rBV	706132	1070330	87.09%	8.602%
26	18.559	2562	2565	2570	rBV4	1309	2187	0.18%	0.018%
27	18.630	2572	2577	2578	rBV3	903	1324	0.11%	0.011%
28	19.558	2731	2735	2739	rBV4	8815	12702	1.03%	0.102%
29	19.629	2742	2747	2754	rBV2	8161	13782	1.12%	0.111%
30	19.881	2787	2790	2793	rBV5	2387	2839	0.23%	0.023%
31	19.993	2802	2809	2816	rBV	854264	1229046	100.00%	9.877%
32	20.222	2846	2848	2852	rBV4	1050	1435	0.12%	0.012%
33	20.569	2905	2907	2908	rBV2	2040	1506	0.12%	0.012%
34	20.669	2922	2924	2925	rBV2	2069	1255	0.10%	0.010%
35	20.921	2964	2967	2969	rBV4	2869	2640	0.21%	0.021%
36	20.992	2972	2979	2980	rVV6	4258	8888	0.72%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050764.D
 Acq On : 28 Oct 2021 6:08
 Operator : CG/JU
 Sample : PB140136BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

37	21.074	2983	2993	3002	rVB4	17210	67720	5.51%	0.544%
38	21.362	3040	3042	3045	rVB4	2158	1476	0.12%	0.012%
39	21.920	3130	3137	3144	rBV	350025	602768	49.04%	4.844%
40	22.073	3162	3163	3169	rVB5	2505	3475	0.28%	0.028%
41	22.220	3186	3188	3191	rBV4	1937	1503	0.12%	0.012%
42	22.725	3272	3274	3280	rVB5	5460	6981	0.57%	0.056%
43	22.925	3306	3308	3309	rVB2	2109	1269	0.10%	0.010%
44	22.984	3316	3318	3320	rBV3	2874	2453	0.20%	0.020%
45	23.459	3395	3399	3411	rVB9	9636	21481	1.75%	0.173%
46	23.565	3415	3417	3419	rVB2	2052	1706	0.14%	0.014%
47	23.877	3468	3470	3471	rVB	2956	1695	0.14%	0.014%
48	23.894	3471	3473	3474	rBV2	1990	1667	0.14%	0.013%
49	24.123	3510	3512	3513	rBV2	2488	1916	0.16%	0.015%
50	24.247	3526	3533	3535	rBV6	7827	15397	1.25%	0.124%
51	24.311	3540	3544	3553	rVB4	18607	48057	3.91%	0.386%
52	24.535	3580	3582	3583	rBV2	2337	1464	0.12%	0.012%
53	24.740	3616	3617	3619	rBV2	2526	1817	0.15%	0.015%
54	25.105	3668	3679	3691	rVB3	376133	1080006	87.87%	8.680%
55	25.340	3708	3719	3731	rVB2	207786	627611	51.06%	5.044%
56	25.510	3746	3748	3750	rBV2	2202	1407	0.11%	0.011%
57	25.915	3815	3817	3819	rBV3	2429	1798	0.15%	0.014%
58	26.186	3861	3863	3865	rBV3	2958	2127	0.17%	0.017%
59	26.221	3867	3869	3870	rBV3	2317	1677	0.14%	0.013%
60	26.385	3895	3897	3899	rBV2	1882	1600	0.13%	0.013%
61	26.538	3915	3923	3934	rVB4	19858	60036	4.88%	0.482%
62	26.644	3939	3941	3944	rVB4	2027	1533	0.12%	0.012%
63	27.989	4161	4170	4181	rVB5	17502	61469	5.00%	0.494%
64	28.900	4323	4325	4327	rBV3	2031	1608	0.13%	0.013%
65	29.018	4343	4345	4346	rBV2	1891	1271	0.10%	0.010%
66	29.705	4460	4462	4463	rBV2	4798	2765	0.22%	0.022%
67	29.740	4463	4468	4480	rVB10	12091	42348	3.45%	0.340%
68	29.917	4496	4498	4502	rBV4	2171	2510	0.20%	0.020%
69	30.334	4567	4569	4572	rBV3	2212	1641	0.13%	0.013%
70	30.921	4668	4669	4671	rBV2	2723	1882	0.15%	0.015%
71	31.615	4785	4787	4790	rBV3	2131	3040	0.25%	0.024%
72	31.814	4817	4821	4822	rBV3	3218	5030	0.41%	0.040%
73	32.138	4875	4876	4878	rBV2	2357	1362	0.11%	0.011%
74	32.173	4880	4882	4884	rBV3	2098	2067	0.17%	0.017%
75	32.625	4957	4959	4960	rBV2	2188	1326	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050764.D
Acq On : 28 Oct 2021 6:08
Operator : CG/JU
Sample : PB140136BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK136

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Title : SVOA CALIBRATION




Sum of corrected areas: 12442921

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050764.D
Acq On : 28 Oct 2021 6:08
Operator : CG/JU
Sample : PB140136BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

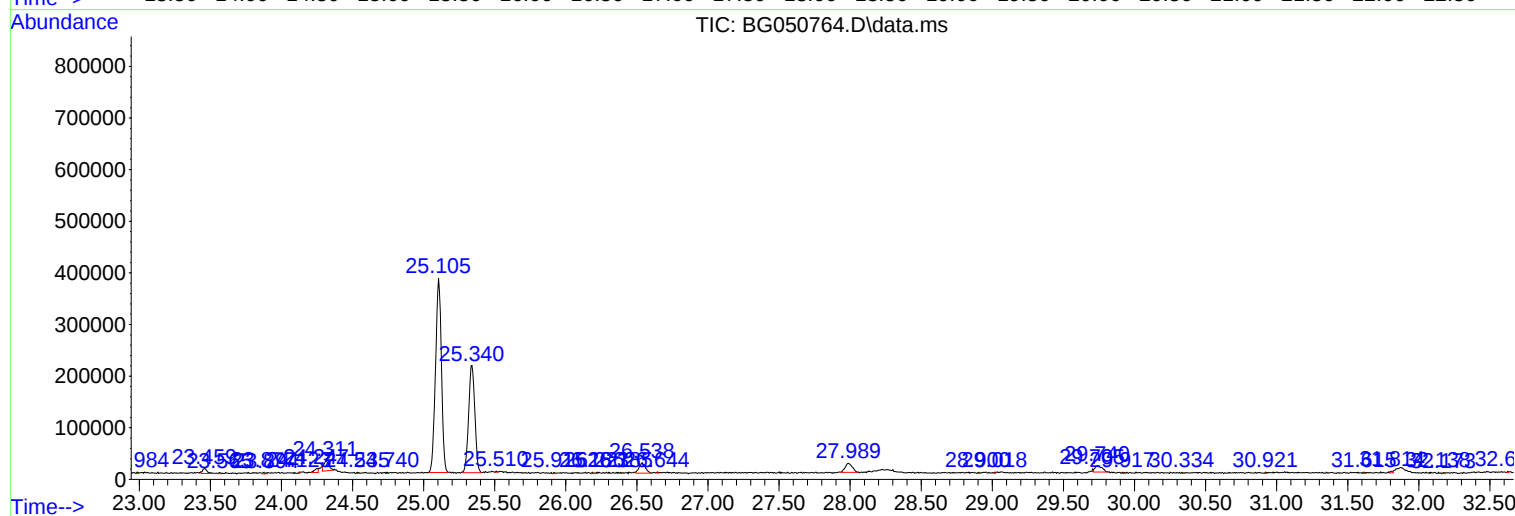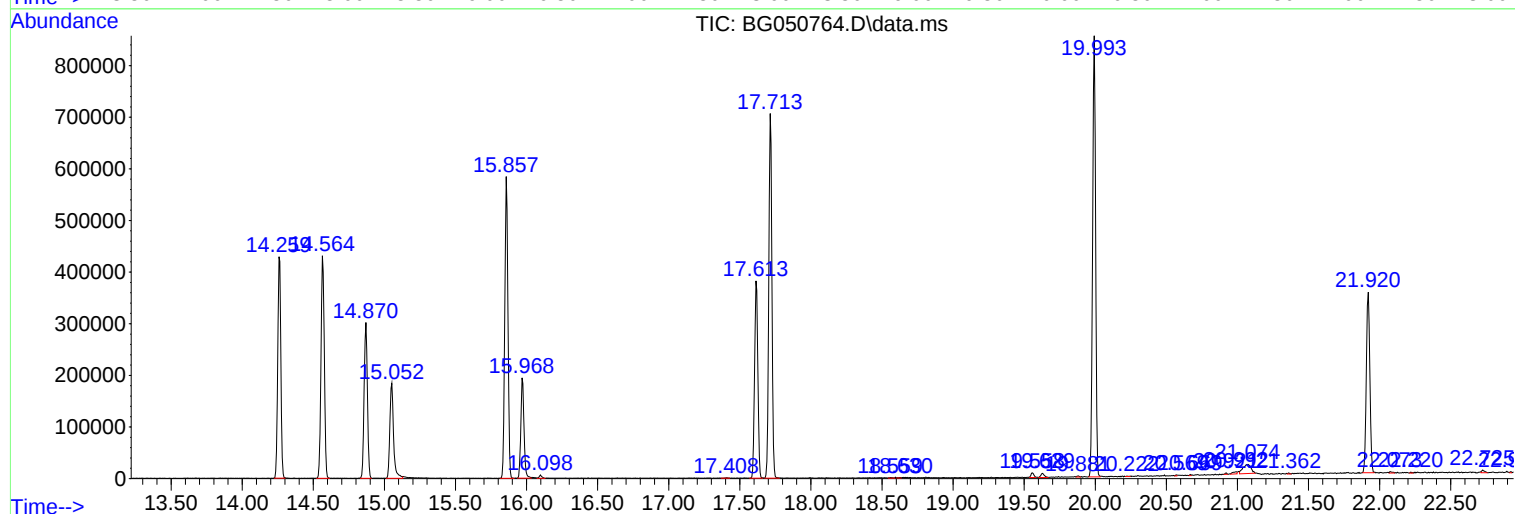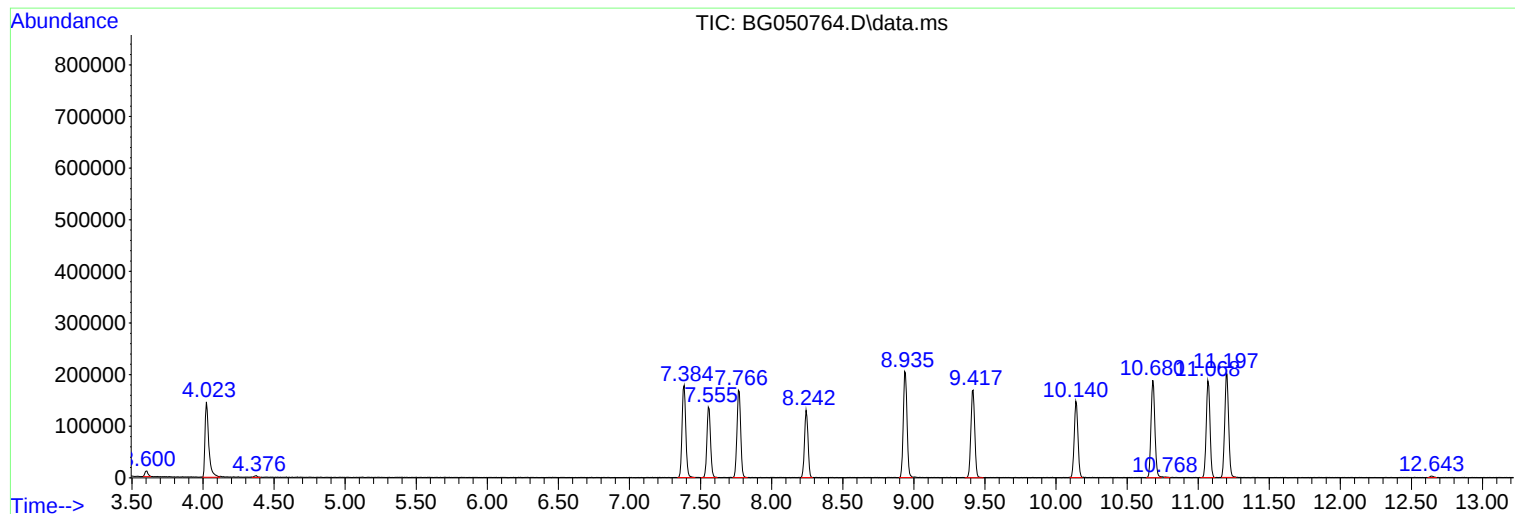

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050764.D
Acq On : 28 Oct 2021 6:08
Operator : CG/JU
Sample : PB140136BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK136










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(dodecyloxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.074	2.25 ng/ul	67720	Chrysene-d12	21.920

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(dodecyloxy)-	230	C14H30O2	004536-30-5	72
2			Batilol	344	C21H44O3	000544-62-7	64
3			Octadecane, 1-chloro-	288	C18H37Cl	003386-33-2	64
4			Pentacosane	352	C25H52	000629-99-2	64
5			Hexadecane, 1-chloro-	260	C16H33Cl	004860-03-1	64

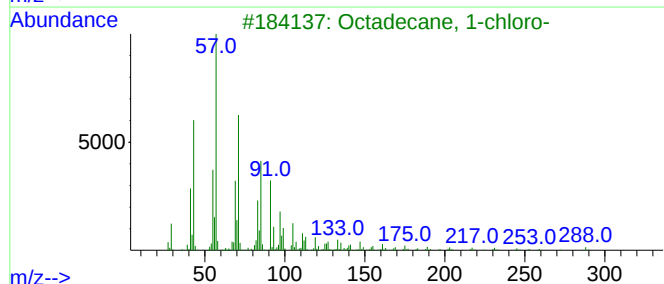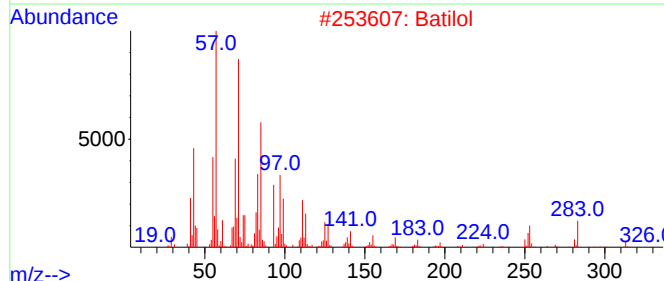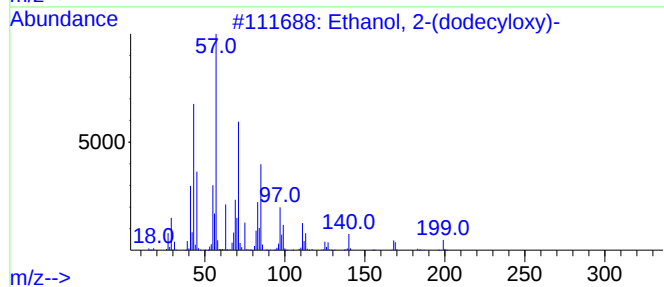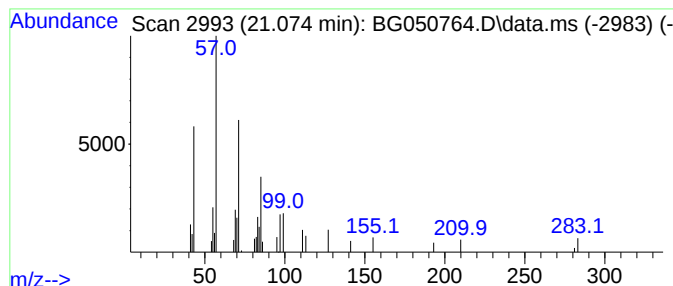

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050764.D
Acq On : 28 Oct 2021 6:08
Operator : CG/JU
Sample : PB140136BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(dod...	21.074	2.3	ng/ul	67720	5	21.920	602768	20.0