

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050773.D
 Acq On : 28 Oct 2021 12:18
 Operator : CG/JU
 Sample : M4215-16
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JDGF3

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.534	5	8	11	rBV3	634	1050	0.15%	0.018%
2	3.558	11	12	14	rVV3	858	900	0.12%	0.015%
3	3.599	17	19	24	rVV4	2553	3718	0.51%	0.062%
4	3.640	24	26	28	rVB2	1157	1025	0.14%	0.017%
5	3.899	64	70	71	rBV4	1438	2212	0.31%	0.037%
6	4.034	90	93	94	rBV3	1241	988	0.14%	0.017%
7	4.139	107	111	118	rBV3	5936	10504	1.45%	0.176%
8	4.210	121	123	127	rBV2	1306	1464	0.20%	0.025%
9	4.263	127	132	140	rVB	10847	17899	2.47%	0.300%
10	4.322	140	142	146	rBV3	1070	1539	0.21%	0.026%
11	4.374	148	151	157	rVB3	2077	2871	0.40%	0.048%
12	4.474	163	168	174	rVB5	2744	4234	0.59%	0.071%
13	4.527	174	177	179	rBV3	1052	1064	0.15%	0.018%
14	4.580	184	186	188	rBV3	1061	1000	0.14%	0.017%
15	4.739	212	213	218	rVB2	2052	2508	0.35%	0.042%
16	4.803	221	224	227	rVB3	952	963	0.13%	0.016%
17	4.921	243	244	247	rVV	1137	917	0.13%	0.015%
18	5.091	268	273	276	rBV3	1170	1660	0.23%	0.028%
19	5.185	285	289	294	rBV3	999	1876	0.26%	0.031%
20	5.297	303	308	313	rBV	5491	9258	1.28%	0.155%
21	5.391	321	324	325	rBV2	989	834	0.12%	0.014%
22	5.450	333	334	337	rVB	911	802	0.11%	0.013%
23	5.479	337	339	341	rBV2	974	1078	0.15%	0.018%
24	5.538	346	349	353	rBV4	1058	1046	0.14%	0.018%
25	5.655	366	369	372	rVB4	930	1203	0.17%	0.020%
26	6.531	516	518	520	rBV2	869	839	0.12%	0.014%
27	6.619	528	533	538	rBV2	2182	3385	0.47%	0.057%
28	6.725	549	551	554	rBV3	602	806	0.11%	0.014%
29	6.860	569	574	577	rVB2	592	1020	0.14%	0.017%
30	7.042	601	605	608	rBV2	556	826	0.11%	0.014%
31	7.130	618	620	624	rVB2	633	841	0.12%	0.014%
32	7.206	629	633	636	rBV3	1059	1672	0.23%	0.028%
33	7.383	656	663	675	rBV	71258	132748	18.34%	2.225%
34	7.559	686	693	700	rBV	57819	97542	13.48%	1.635%
35	7.770	723	729	737	rVV	70079	125157	17.29%	2.098%
36	7.847	737	742	745	rVB3	1418	2193	0.30%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050773.D
 Acq On : 28 Oct 2021 12:18
 Operator : CG/JU
 Sample : M4215-16
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JDGF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

37	8.035	771	774	781	rVB3	1440	2556	0.35%	0.043%
38	8.199	799	802	803	rBV2	1312	1161	0.16%	0.019%
39	8.246	803	810	818	rVB	123183	213799	29.54%	3.583%
40	8.329	821	824	825	rBV	874	850	0.12%	0.014%

41	8.464	842	847	850	rVB5	1989	3301	0.46%	0.055%
42	8.781	895	901	902	rBV5	1166	1797	0.25%	0.030%
43	8.893	918	920	922	rBV3	1327	1093	0.15%	0.018%
44	8.940	922	928	937	rVV	60640	110095	15.21%	1.845%
45	9.081	945	952	958	rBV4	3105	7545	1.04%	0.126%

46	9.157	964	965	971	rVB3	658	983	0.14%	0.016%
47	9.416	1001	1009	1017	rVB	71677	132236	18.27%	2.216%
48	9.504	1021	1024	1029	rVB3	820	1164	0.16%	0.020%
49	9.557	1029	1033	1036	rBV4	1243	1817	0.25%	0.030%
50	9.780	1066	1071	1074	rBV2	1069	1238	0.17%	0.021%

51	10.144	1124	1133	1143	rBV2	61192	112312	15.52%	1.882%
52	10.309	1158	1161	1165	rVB2	744	981	0.14%	0.016%
53	10.379	1171	1173	1178	rVB	612	903	0.12%	0.015%
54	10.685	1219	1225	1236	rVB2	76785	142763	19.73%	2.393%
55	10.755	1236	1237	1242	rVB3	1143	1245	0.17%	0.021%

56	10.820	1244	1248	1250	rBV2	1805	2621	0.36%	0.044%
57	11.072	1283	1291	1300	rBV	184346	335721	46.39%	5.627%
58	11.202	1305	1313	1325	rBV2	63698	129398	17.88%	2.169%
59	11.872	1423	1427	1430	rBV	783	1020	0.14%	0.017%
60	11.919	1432	1435	1438	rVB	982	1106	0.15%	0.019%

61	12.007	1447	1450	1452	rBV3	772	1051	0.15%	0.018%
62	12.130	1466	1471	1474	rBV4	577	795	0.11%	0.013%
63	12.212	1482	1485	1487	rBV3	765	860	0.12%	0.014%
64	13.470	1693	1699	1701	rBV3	1358	1649	0.23%	0.028%
65	13.528	1706	1709	1713	rBV2	954	1322	0.18%	0.022%

66	13.734	1741	1744	1745	rBV2	861	828	0.11%	0.014%
67	14.186	1817	1821	1823	rVB2	1224	1495	0.21%	0.025%
68	14.263	1827	1834	1844	rVB	168623	247849	34.25%	4.154%
69	14.404	1854	1858	1859	rBV2	765	1091	0.15%	0.018%
70	14.445	1863	1865	1868	rBV3	744	904	0.12%	0.015%

71	14.492	1871	1873	1876	rBV4	1208	1441	0.20%	0.024%
72	14.568	1879	1886	1893	rVB	188257	308527	42.63%	5.171%
73	14.651	1897	1900	1903	rBV4	909	991	0.14%	0.017%
74	14.674	1903	1904	1907	rVB2	1435	1216	0.17%	0.020%
75	14.739	1913	1915	1917	rVB2	1251	964	0.13%	0.016%

76	14.768	1917	1920	1923	rBV3	1094	1286	0.18%	0.022%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
 Data File : BG050773.D
 Acq On : 28 Oct 2021 12:18
 Operator : CG/JU
 Sample : M4215-16
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JDGF3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
 Title : SVOA CALIBRATION

77	14.798	1923	1925	1928	rBV3	1064	1150	0.16%	0.019%
78	14.874	1931	1938	1945	rBV	299535	495991	68.54%	8.313%
79	14.956	1947	1952	1954	rBV4	1365	1986	0.27%	0.033%
80	14.991	1957	1958	1960	rVB3	1655	799	0.11%	0.013%
81	15.056	1963	1969	1981	rBV2	43305	90776	12.54%	1.521%
82	15.185	1989	1991	1993	rBV3	1143	1223	0.17%	0.020%
83	15.215	1993	1996	1997	rBV3	1357	1515	0.21%	0.025%
84	15.273	2003	2006	2008	rBV4	3829	3957	0.55%	0.066%
85	15.438	2031	2034	2036	rBV4	1074	1519	0.21%	0.025%
86	15.555	2051	2054	2055	rBV3	1231	1630	0.23%	0.027%
87	15.661	2070	2072	2074	rBV3	1130	913	0.13%	0.015%
88	15.808	2096	2097	2099	rVB2	1815	965	0.13%	0.016%
89	15.861	2099	2106	2112	rBV	249576	391690	54.13%	6.565%
90	15.973	2119	2125	2133	rBV2	43081	73640	10.18%	1.234%
91	16.166	2156	2158	2160	rBV3	1678	1544	0.21%	0.026%
92	16.190	2160	2162	2163	rVB2	1551	1029	0.14%	0.017%
93	16.366	2190	2192	2193	rBV2	2156	1659	0.23%	0.028%
94	17.060	2309	2310	2311	rBV	3100	1717	0.24%	0.029%
95	17.142	2320	2324	2329	rBV7	9623	16865	2.33%	0.283%
96	17.618	2398	2405	2412	rBV	371663	588040	81.26%	9.856%
97	17.718	2416	2422	2429	rVV	249708	383351	52.97%	6.425%
98	19.997	2805	2810	2816	rVB	288556	423730	58.55%	7.102%
99	21.924	3133	3138	3144	rBV2	292391	537261	74.24%	9.005%
100	25.344	3713	3720	3731	rVB3	239589	723673	100.00%	12.129%




Sum of corrected areas: 5966239

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050773.D
Acq On : 28 Oct 2021 12:18
Operator : CG/JU
Sample : M4215-16
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JDGF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

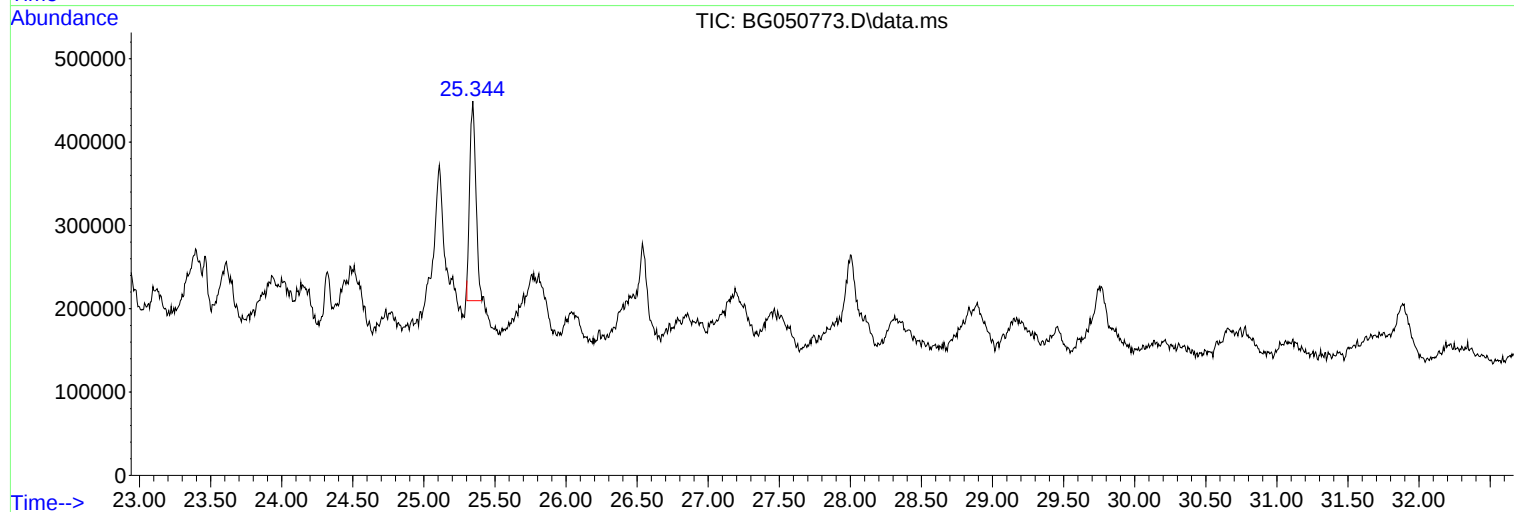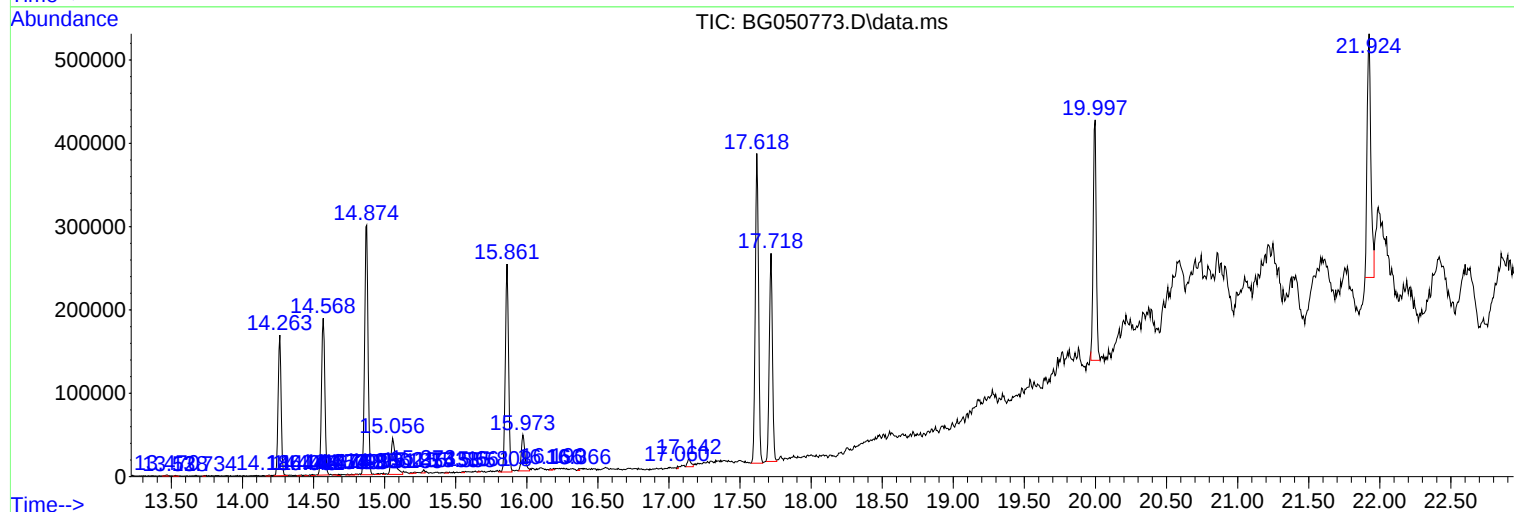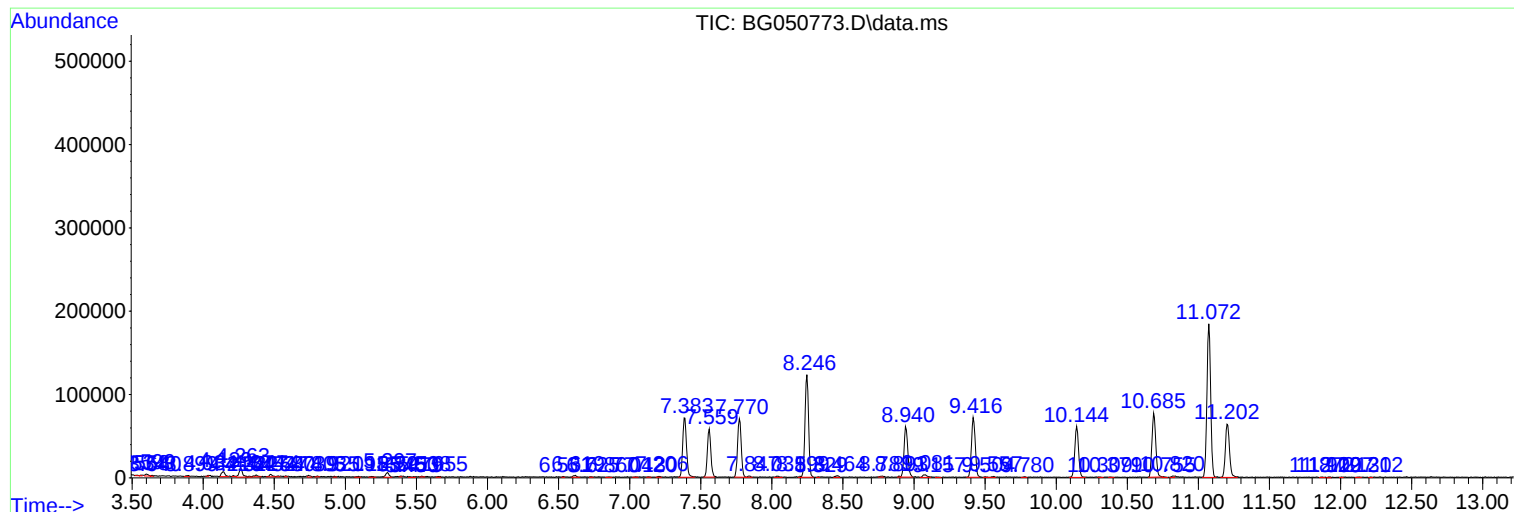

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050773.D
Acq On : 28 Oct 2021 12:18
Operator : CG/JU
Sample : M4215-16
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JDGF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102721\
Data File : BG050773.D
Acq On : 28 Oct 2021 12:18
Operator : CG/JU
Sample : M4215-16
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JDGF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
