

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102725\
 Data File : BG064587.D
 Acq On : 27 Oct 2025 14:41
 Operator : RC/JU
 Sample : PB170246BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB170246BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.747	445	452	462	rBV	1091986	1740834	36.42%	9.577%
2	7.351	716	725	734	rBV	917605	1591115	33.29%	8.753%
3	8.220	866	873	882	rBV	153710	257122	5.38%	1.414%
4	9.384	1061	1071	1083	rBV	512121	905686	18.95%	4.982%
5	11.046	1346	1354	1362	rVB	201292	359875	7.53%	1.980%
6	13.473	1758	1767	1774	rBV	1533719	2373773	49.66%	13.059%
7	14.842	1993	2000	2007	rVB	357540	565456	11.83%	3.111%
8	16.317	2244	2251	2265	rBV	1421837	2139132	44.75%	11.768%
9	17.574	2459	2465	2473	rBV	521061	807995	16.90%	4.445%
10	20.171	2900	2907	2913	rBV	3498601	4779783	100.00%	26.295%
11	21.851	3185	3193	3203	rBV2	555860	945093	19.77%	5.199%
12	23.690	3500	3506	3519	rVB4	41459	90085	1.88%	0.496%
13	24.848	3694	3703	3713	rVB5	49112	133780	2.80%	0.736%
14	25.194	3750	3762	3774	rBV	326197	943085	19.73%	5.188%
15	25.306	3774	3781	3789	rVB3	21960	58705	1.23%	0.323%
16	26.276	3935	3946	3959	rVB5	48563	180571	3.78%	0.993%
17	26.511	3981	3986	3997	rVB4	17983	52945	1.11%	0.291%
18	27.962	4222	4233	4235	rBV3	21322	48555	1.02%	0.267%
19	28.062	4240	4250	4265	rVB9	42916	204243	4.27%	1.124%




Sum of corrected areas: 18177833

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102725\
Data File : BG064587.D
Acq On : 27 Oct 2025 14:41
Operator : RC/JU
Sample : PB170246BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170246BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

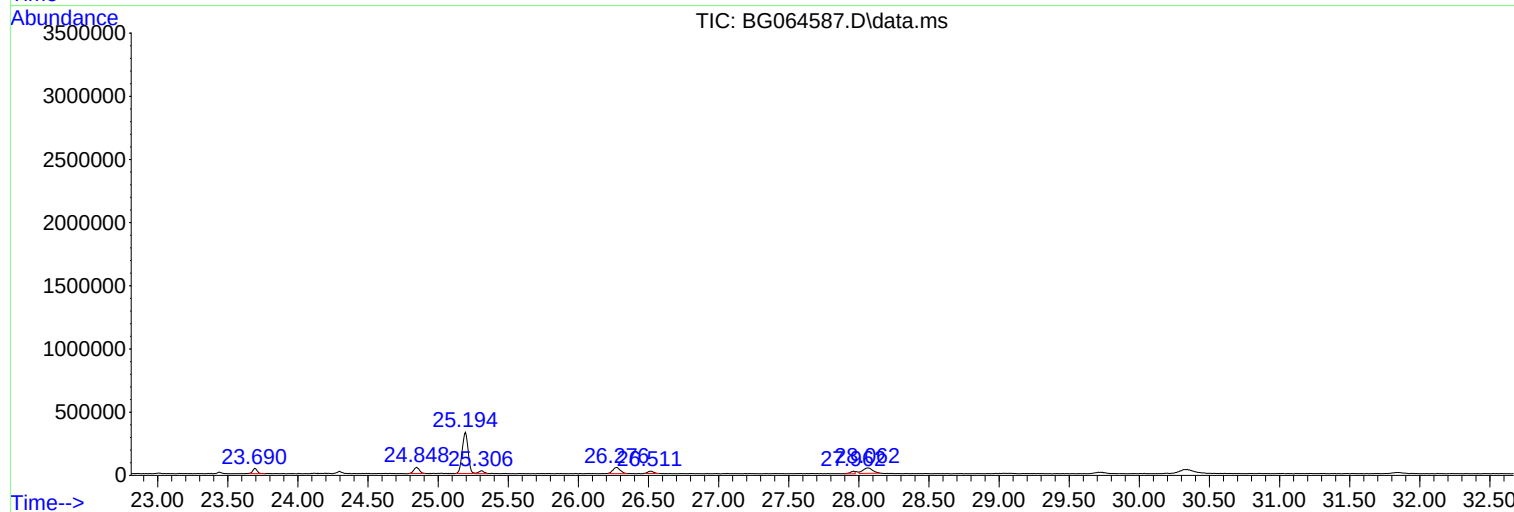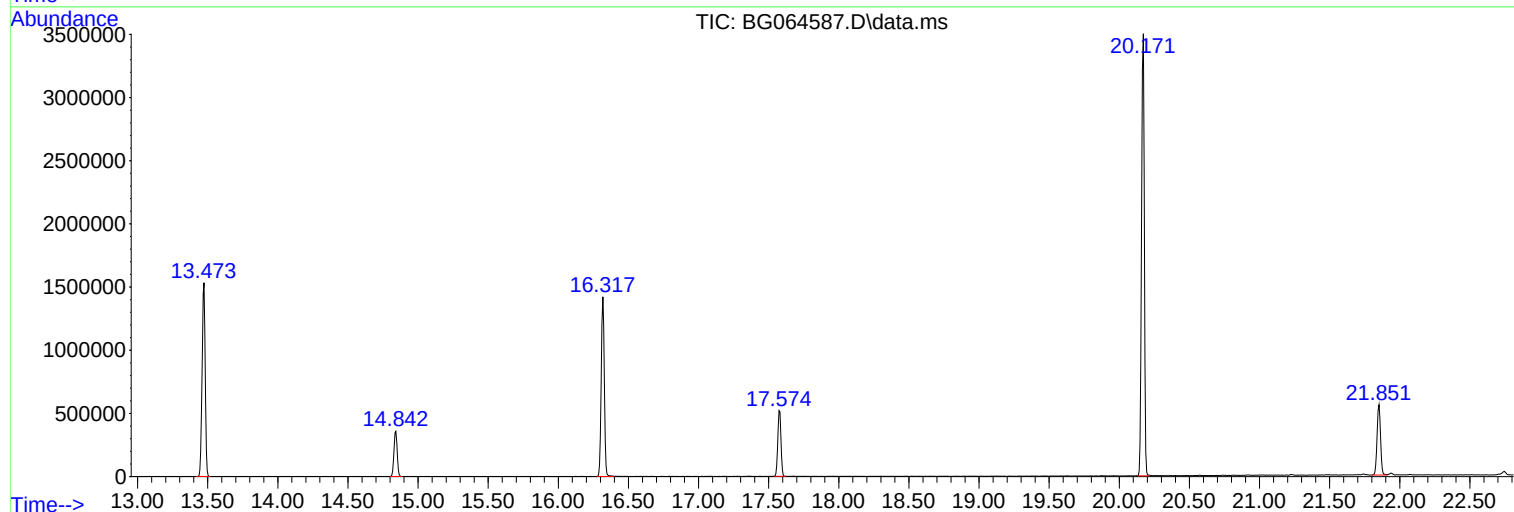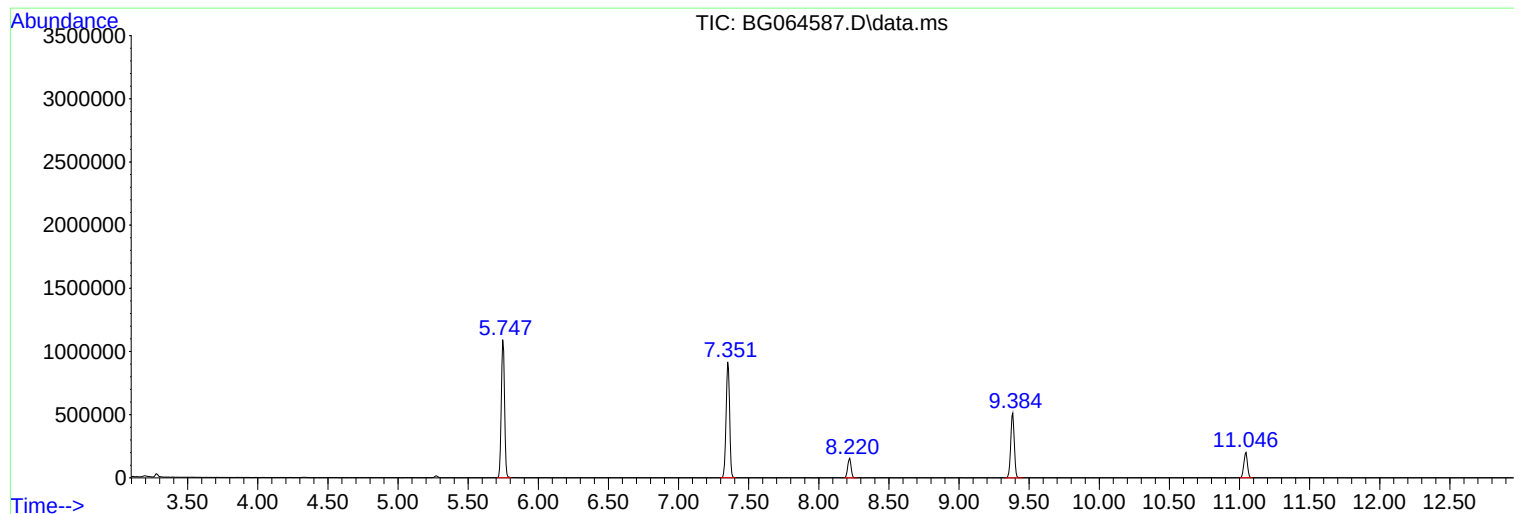

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102725\
Data File : BG064587.D
Acq On : 27 Oct 2025 14:41
Operator : RC/JU
Sample : PB170246BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170246BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102725\
Data File : BG064587.D
Acq On : 27 Oct 2025 14:41
Operator : RC/JU
Sample : PB170246BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170246BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------