
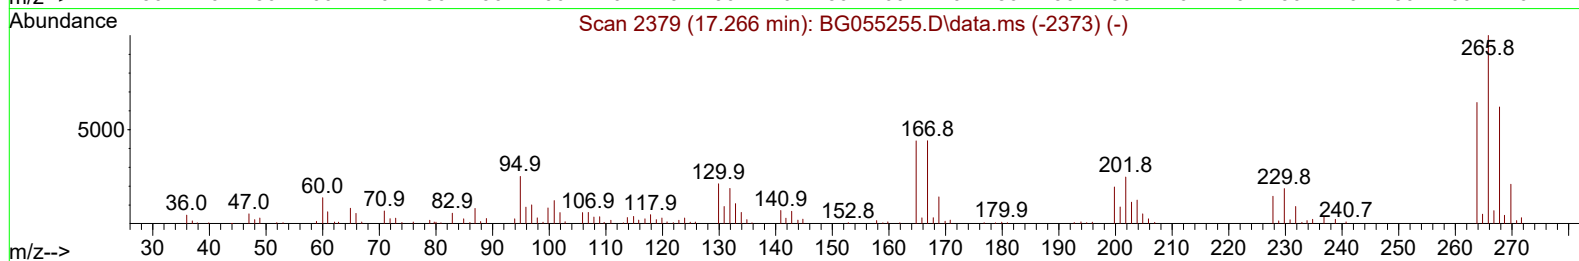
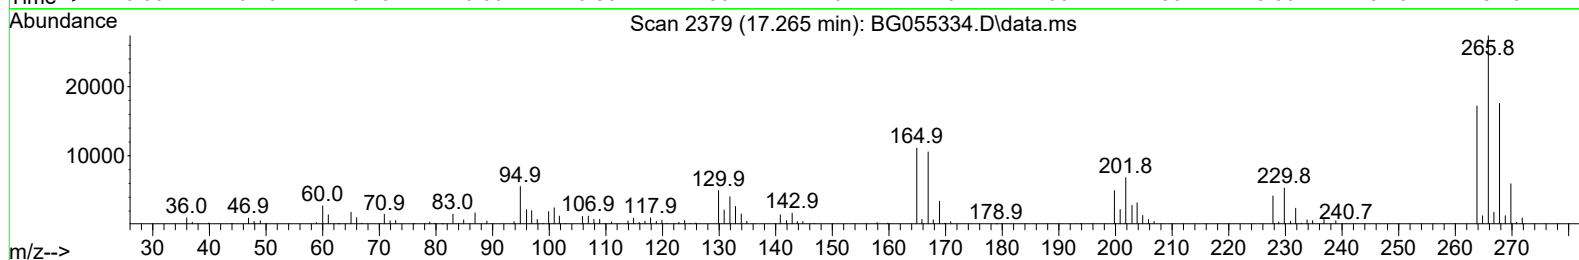


Quant Time: Oct 29 08:28:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 04:52:38 2022
Response via : Initial Calibration

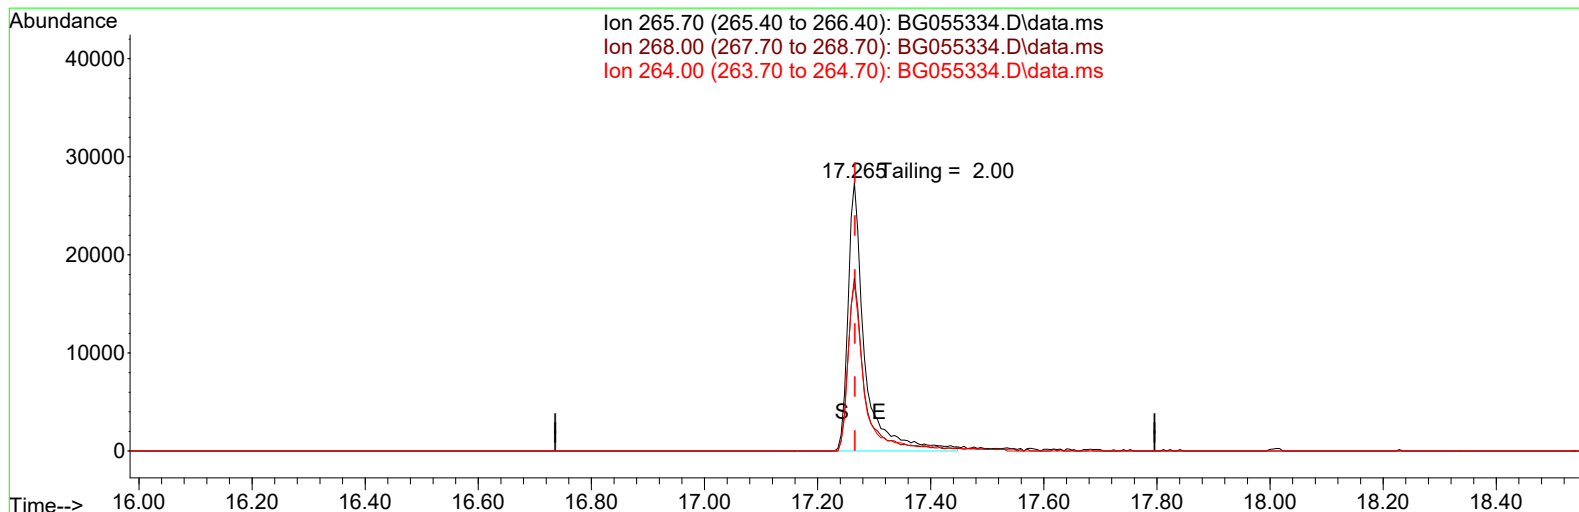

TIC: BG055334.D\data.ms

(70) Pentachlorophenol (C)




17.265min (-0.001) 24530.26 ng

response **57068**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	64.25
264.00	64.40	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
Data File : BG055334.D
Acq On : 28 Oct 2022 9:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 08:28:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 04:52:38 2022
Response via : Initial Calibration

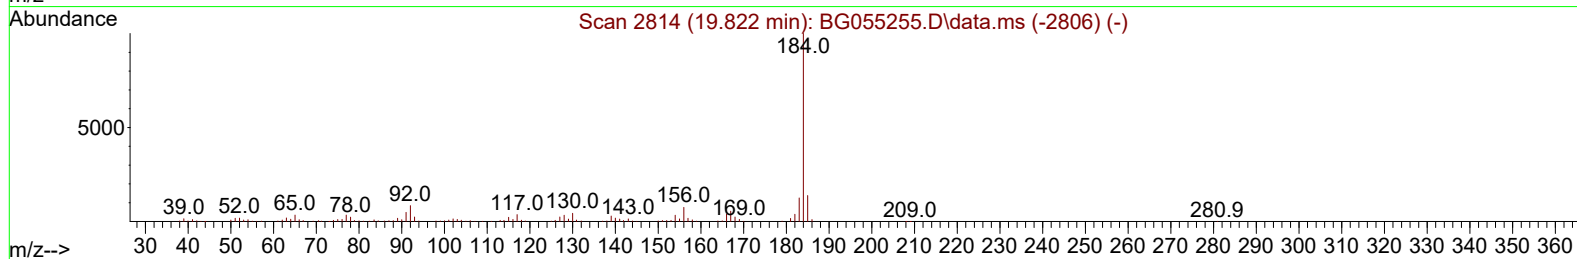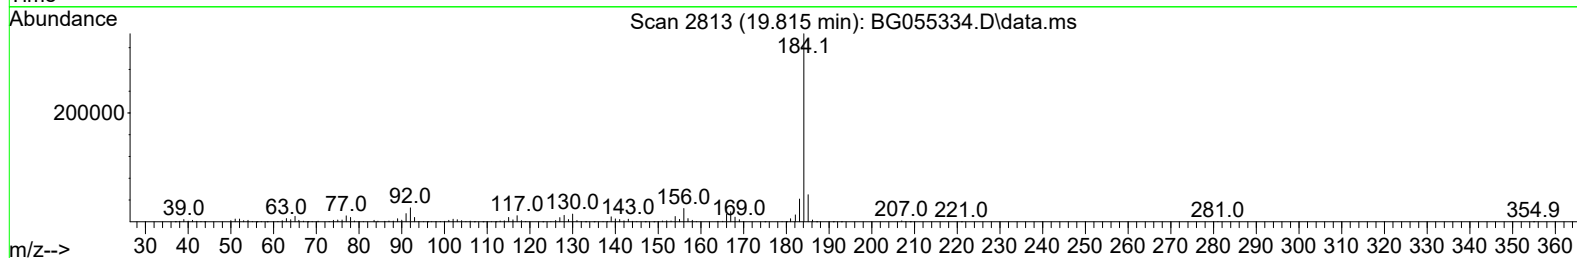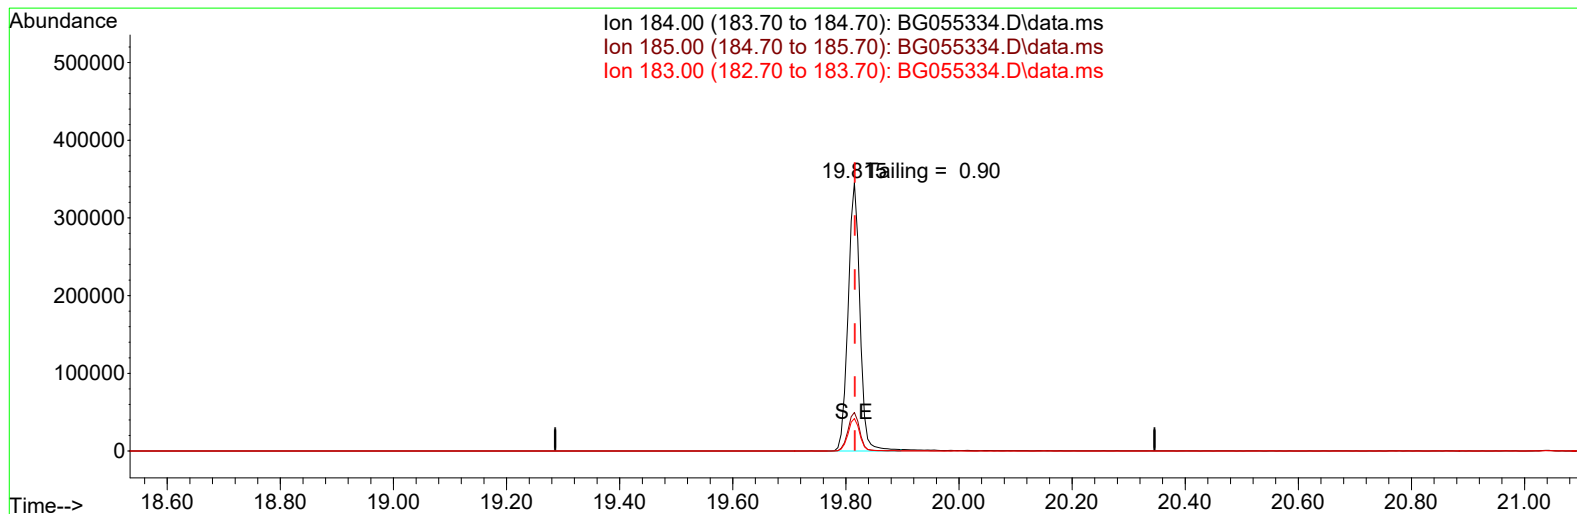

TIC: BG055334.D\data.ms

(77) Benzidine**19.815min (-0.001) 321399.72 ng****response 459138**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.39
183.00	12.50	12.13
0.00	0.00	0.00