
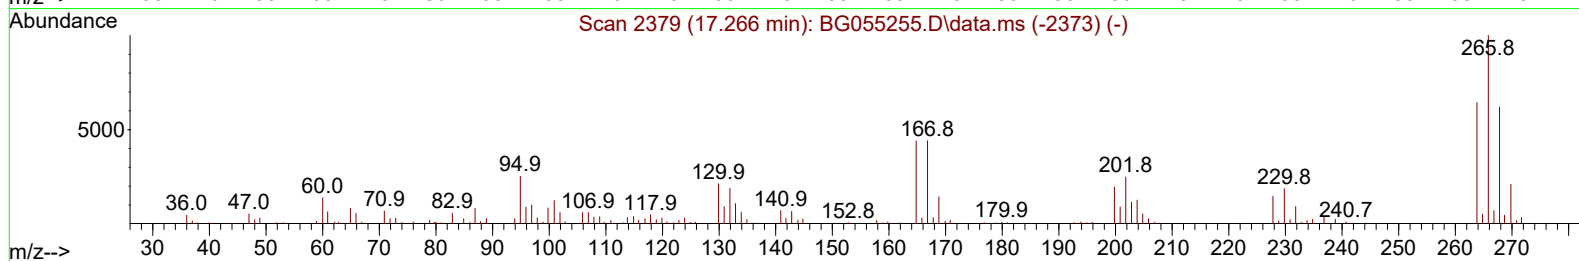
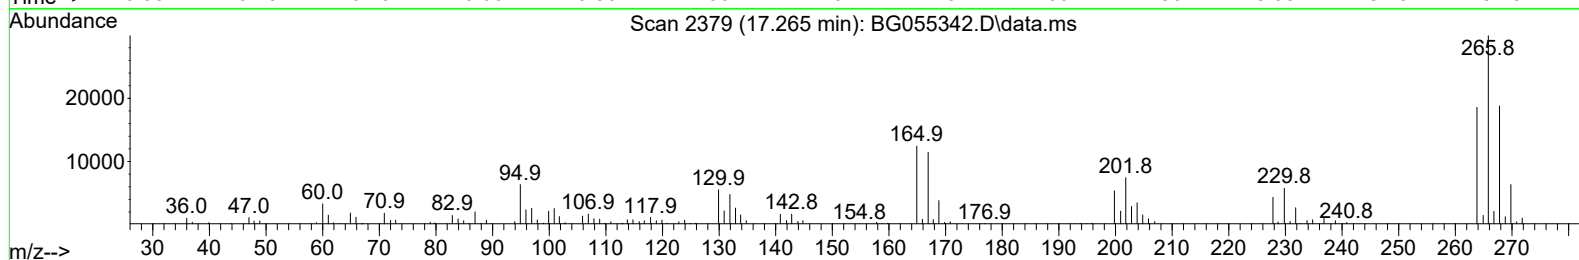


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
Data File : BG055342.D
Acq On : 28 Oct 2022 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 15:48:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

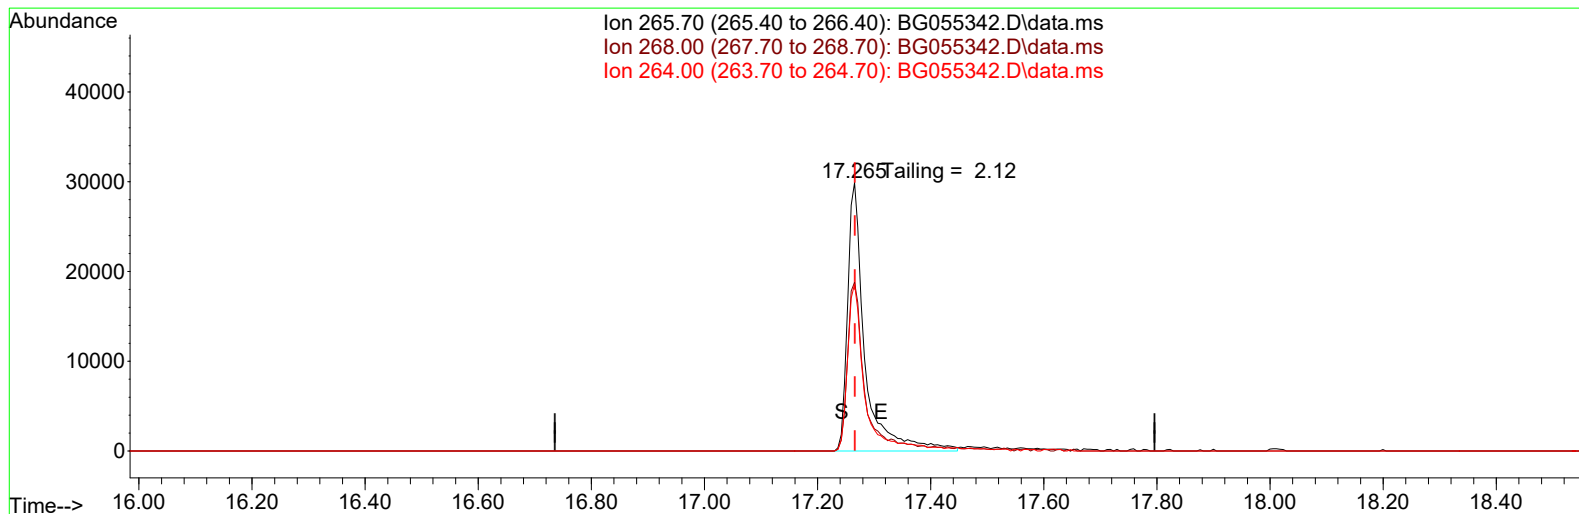

TIC: BG055342.D\data.ms

(70) Pentachlorophenol (C)




17.265min (-0.001) 27924.73 ng

response 63892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	62.83
264.00	64.40	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
Data File : BG055342.D
Acq On : 28 Oct 2022 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 15:48:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

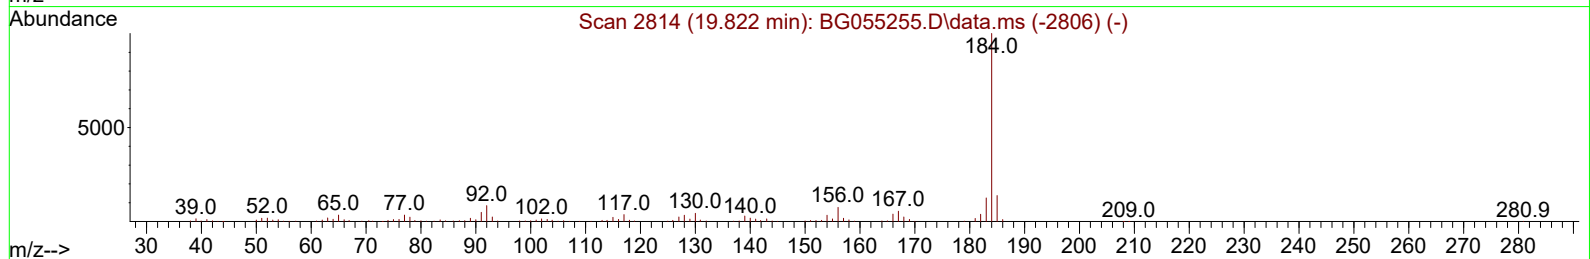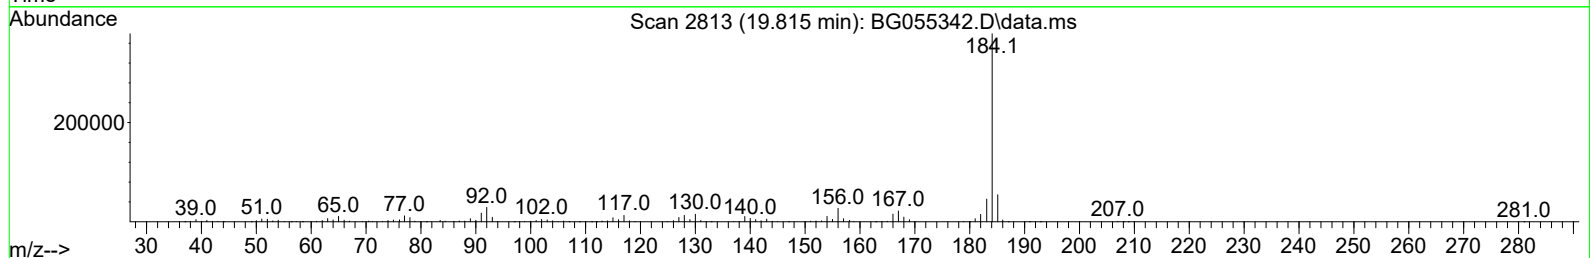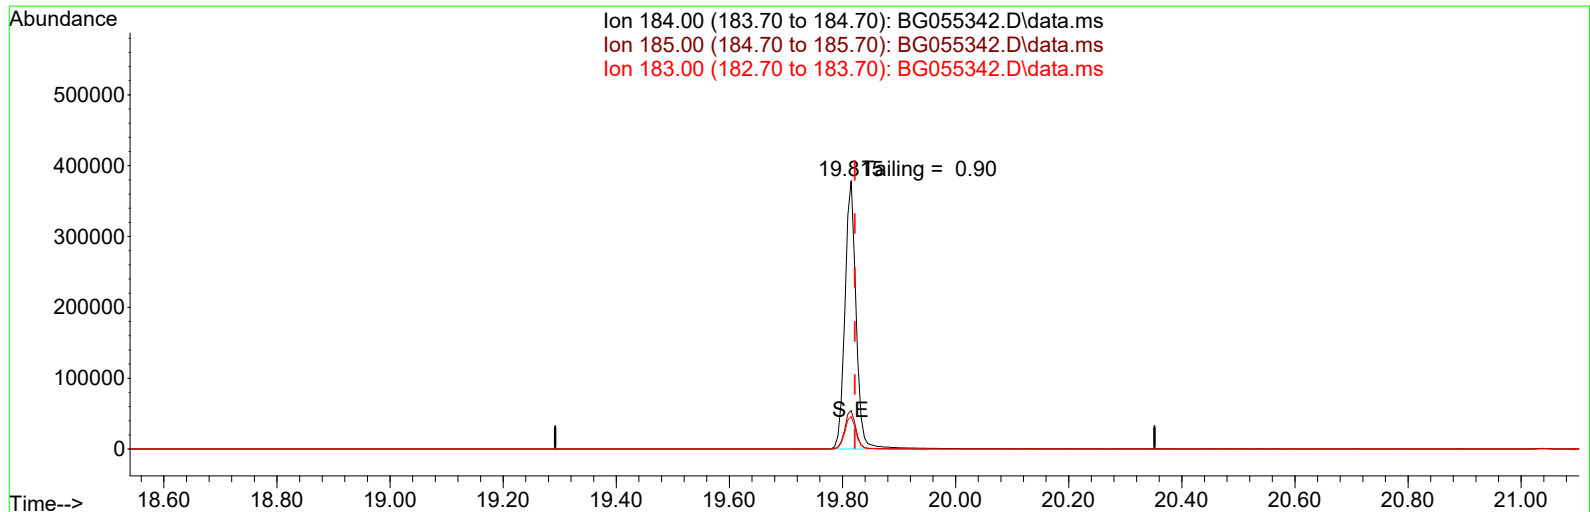

TIC: BG055342.D\data.ms

(77) Benzidine

19.815min (-0.007) 0.00 ng

response 525170

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.40
183.00	12.50	12.12
0.00	0.00	0.00