

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
 Data File : BG055352.D
 Acq On : 28 Oct 2022 22:07
 Operator : CG/JU
 Sample : N5226-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20221094-199-SITE-WATER

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.304	337	343	351	rVB	26761	41824	1.63%	0.465%
2	5.785	419	425	436	rBV	239201	388329	15.12%	4.319%
3	7.407	692	701	714	rBV	185073	329384	12.83%	3.663%
4	8.265	840	847	853	rBV	100190	170780	6.65%	1.899%
5	9.434	1039	1046	1060	rBV	325665	586365	22.84%	6.521%
6	11.091	1320	1328	1339	rBV	141494	254663	9.92%	2.832%
7	13.500	1731	1738	1754	rBV	966615	1499417	58.40%	16.676%
8	14.875	1965	1972	1981	rVB	239682	379586	14.78%	4.222%
9	16.355	2217	2224	2243	rBV	675413	1101549	42.90%	12.251%
10	17.607	2431	2437	2446	rBV	327892	487233	18.98%	5.419%
11	20.180	2869	2875	2882	rBV	2035261	2567694	100.00%	28.557%
12	21.490	3092	3098	3100	rBV6	12978	25705	1.00%	0.286%
13	21.884	3158	3165	3173	rVB2	330902	574013	22.36%	6.384%
14	25.268	3730	3741	3754	rBV2	199750	584964	22.78%	6.506%




Sum of corrected areas: 8991506

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
Data File : BG055352.D
Acq On : 28 Oct 2022 22:07
Operator : CG/JU
Sample : N5226-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20221094-199-SITE-WATER

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

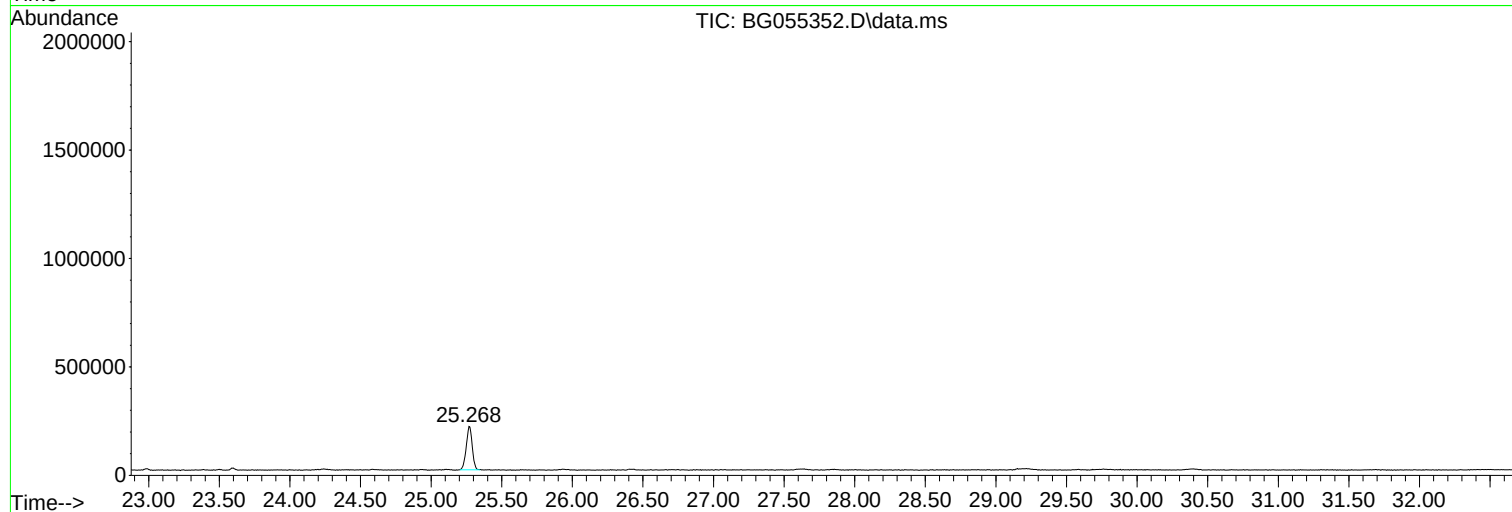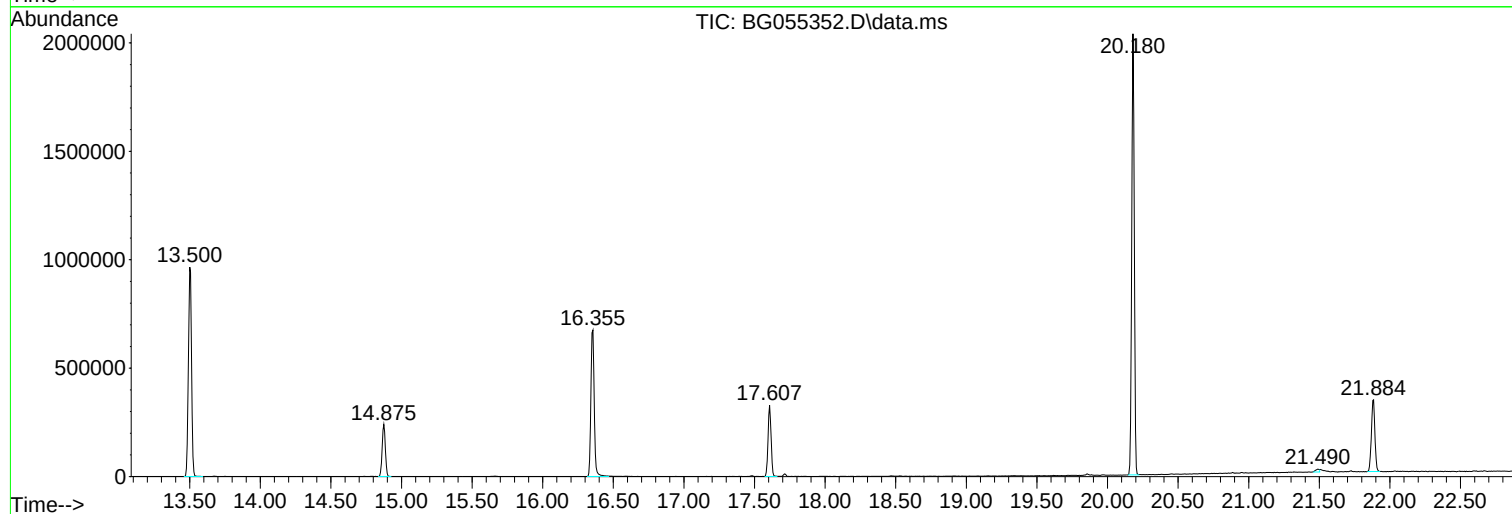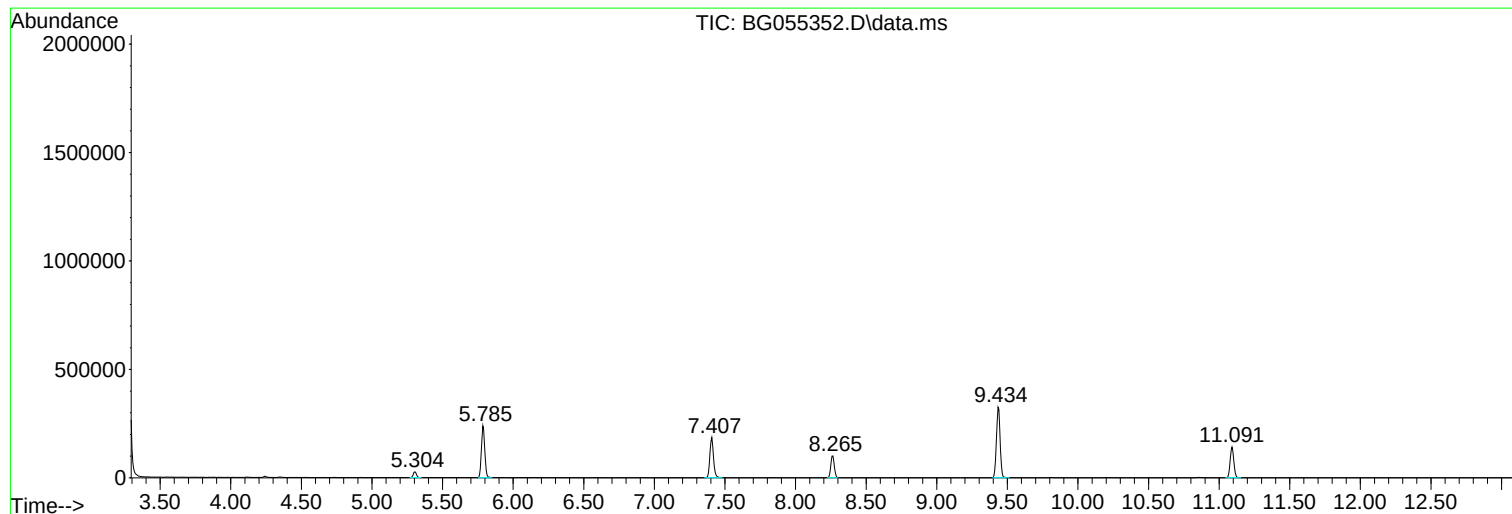

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
Data File : BG055352.D
Acq On : 28 Oct 2022 22:07
Operator : CG/JU
Sample : N5226-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20221094-199-SITE-WATER










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.304	4.90 ng	41824	1,4-Dichlorobenzene-d4	8.265

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	3-Hexanol	102	C6H14O	000623-37-0	33		
3	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	25		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		
5	(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9		

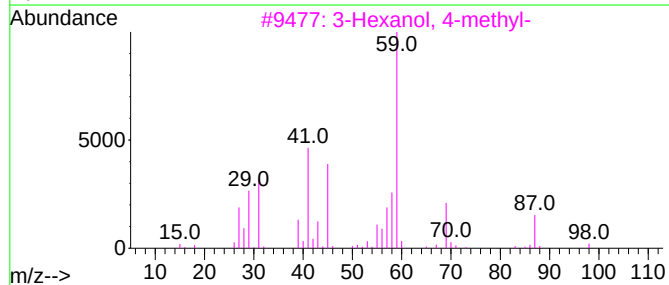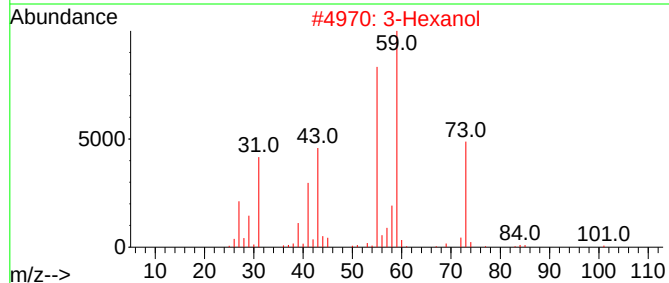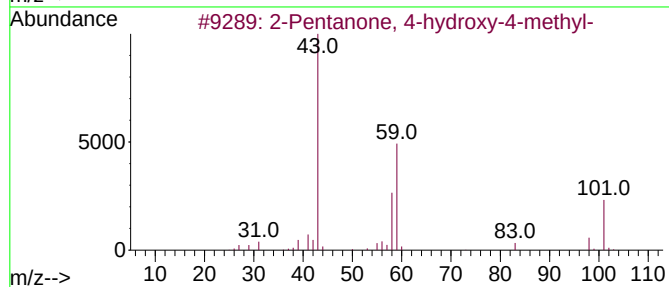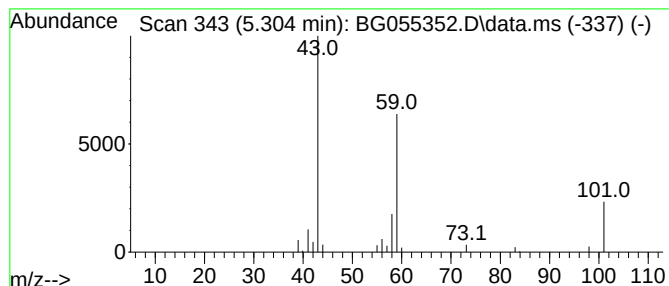

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
Data File : BG055352.D
Acq On : 28 Oct 2022 22:07
Operator : CG/JU
Sample : N5226-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20221094-199-SITE-WATER

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.304	4.9	ng	41824	1	8.265	170780	20.0