


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
 Data File : BG055334.D
 Acq On : 28 Oct 2022 9:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 29 04:52:38 2022

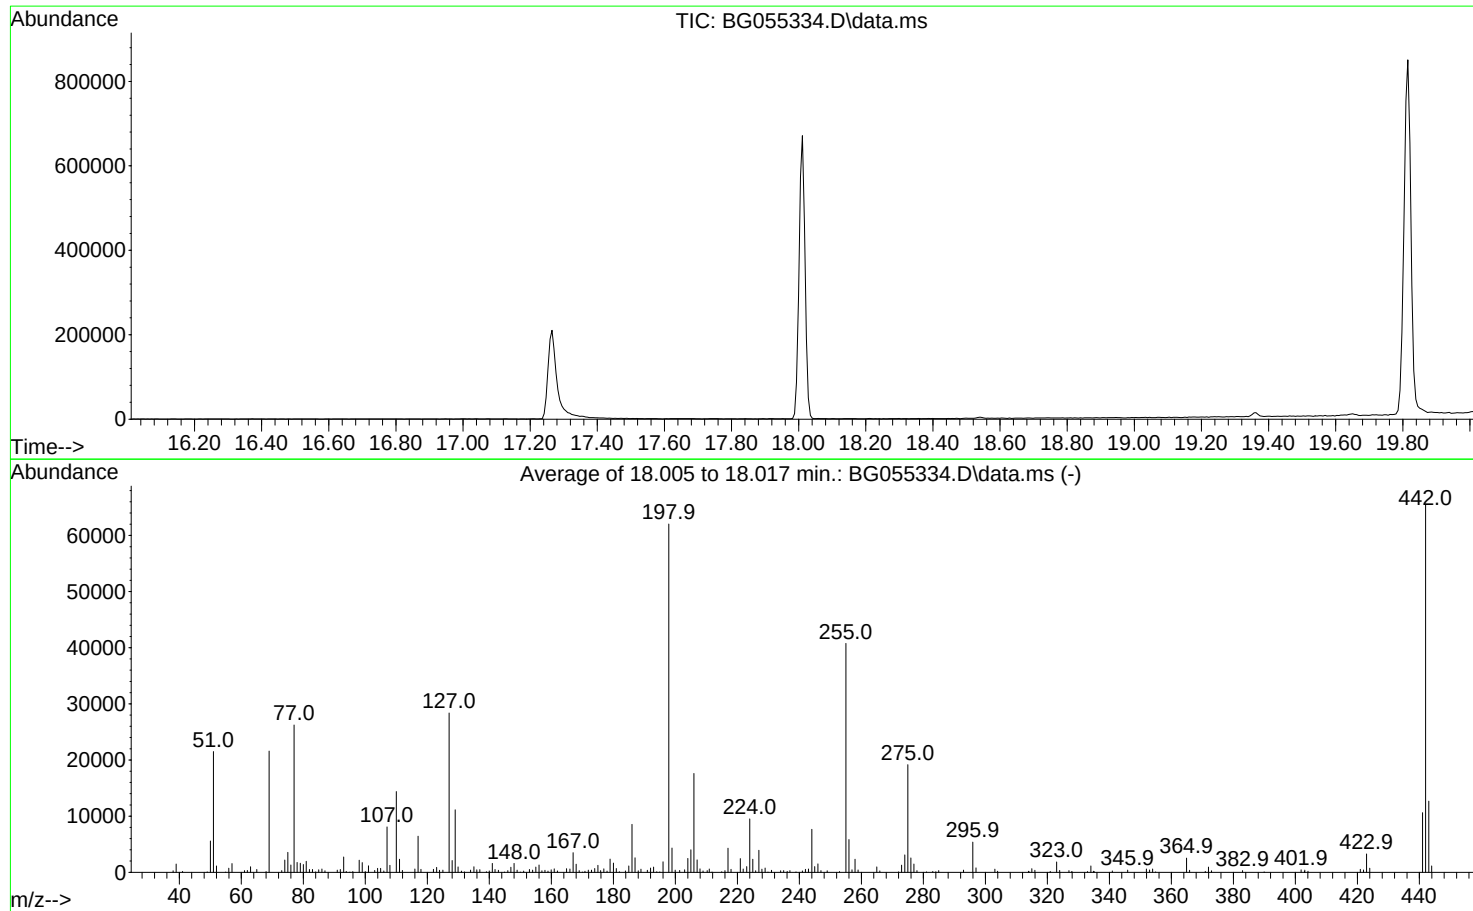




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	21495	PASS
68	69	0.00	2	0.6	129	PASS
69	198	0.00	100	34.8	21587	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	28379	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62032	PASS
199	198	5	9	7.0	4322	PASS
275	198	10	60	30.9	19181	PASS
365	198	1	100	4.1	2532	PASS
441	198	0.01	100	17.1	10626	PASS
442	442	50	100	100.0	65528	PASS
443	442	15	24	19.3	12669	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
Data File : BG055334.D
Acq On : 28 Oct 2022 9:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 29 08:28:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 04:52:38 2022
Response via : Initial Calibration

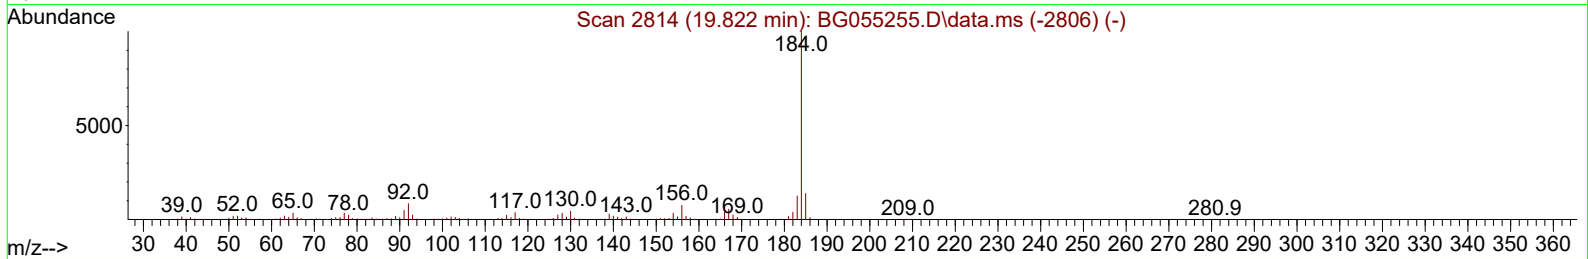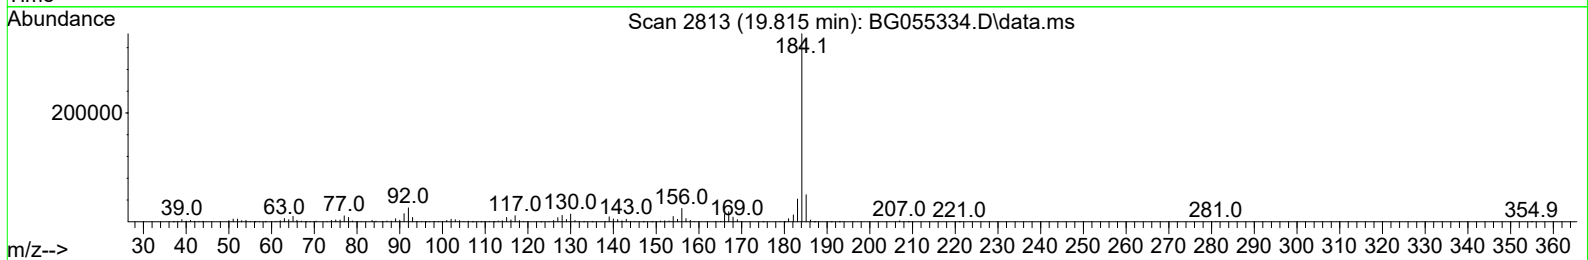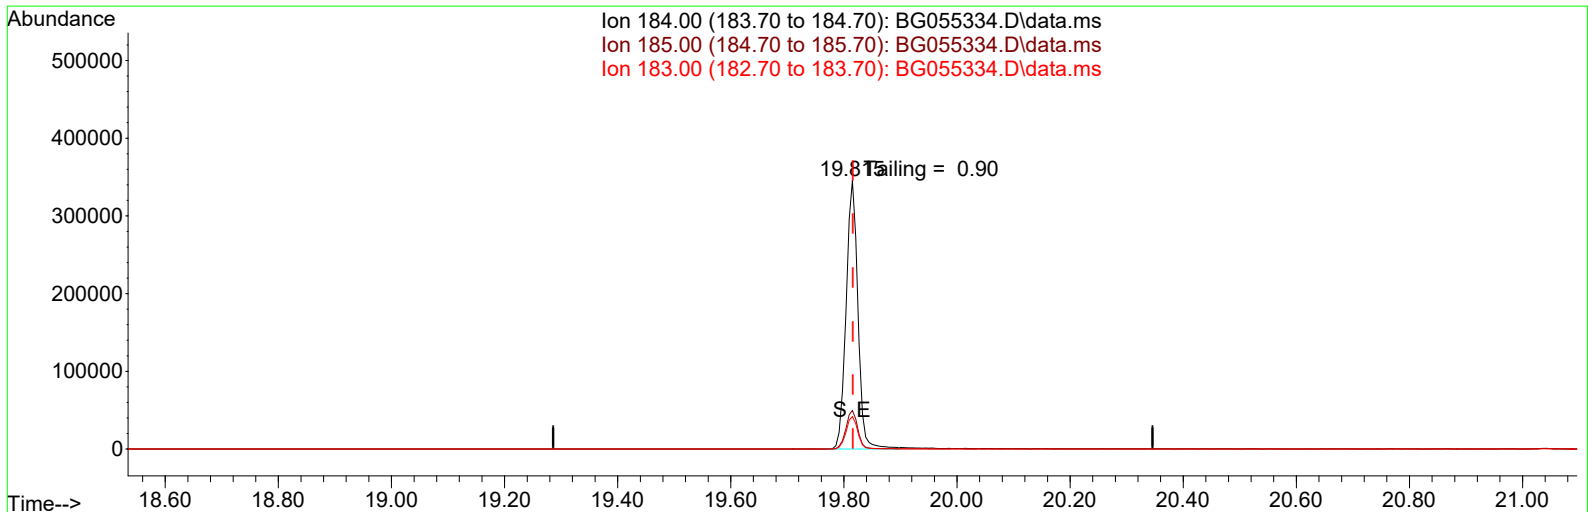

TIC: BG055334.D\data.ms

(77) Benzidine

19.815min (-0.001) 321399.72 ng

response 459138

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.39
183.00	12.50	12.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/28/2022	BNA_G	BG055334.D
Compound Name	Response	Retention Time
DDT	255229	21.037
DDD	4821	20.596
DDE	323	20.091
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5144	260373	1.98

Instrument :
BNA_G
ClientSampleId :
DFTPP