


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
 Data File : BG055342.D
 Acq On : 28 Oct 2022 15:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 29 04:52:38 2022

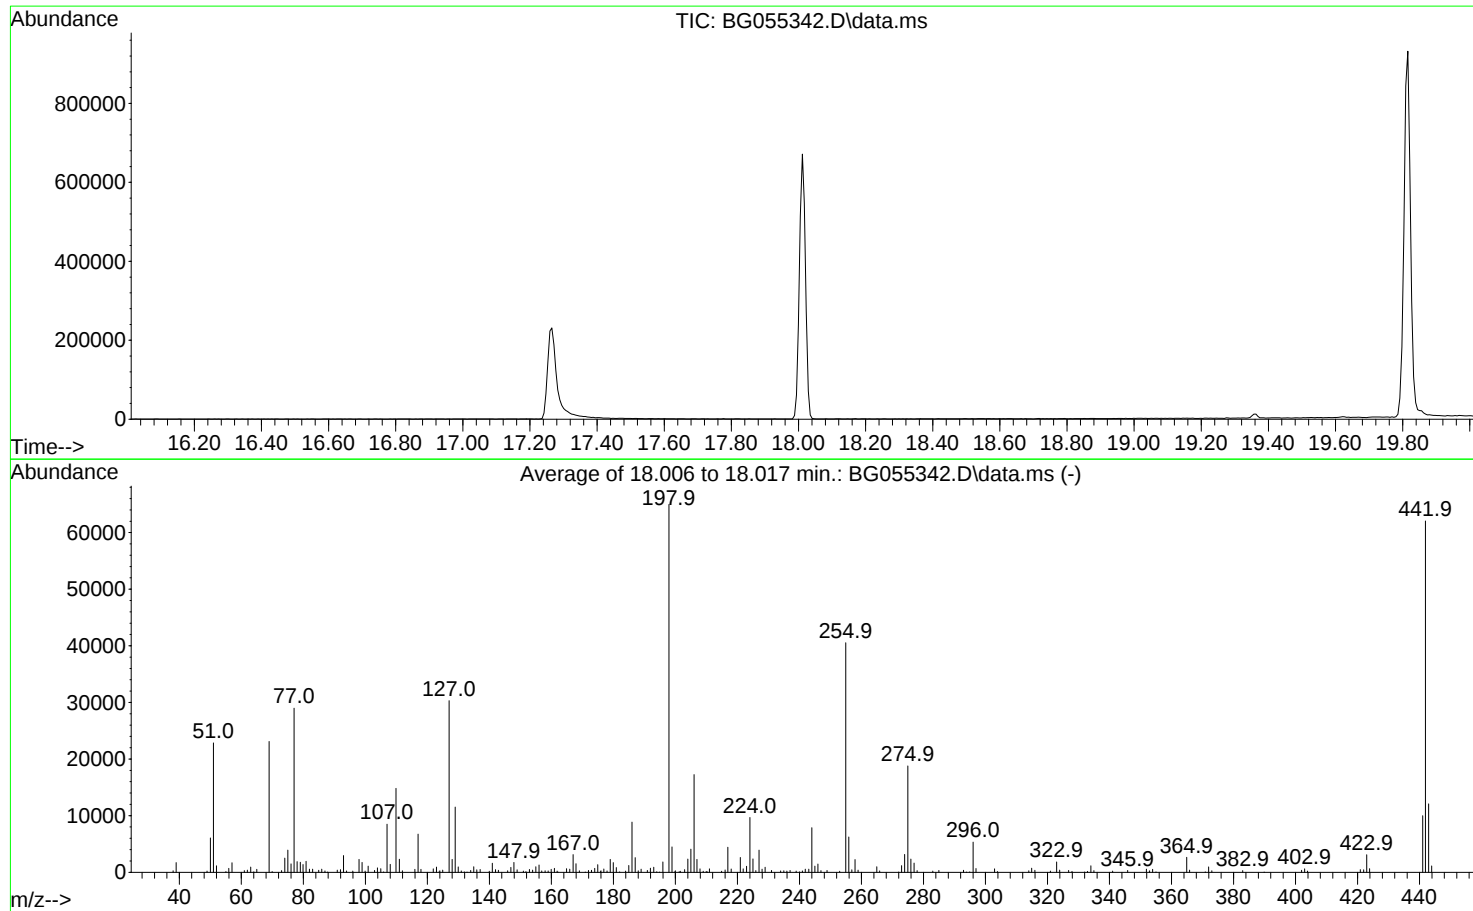




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	22837	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	23115	PASS
70	69	0.00	2	0.5	119	PASS
127	198	10	80	46.6	30304	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64971	PASS
199	198	5	9	6.9	4491	PASS
275	198	10	60	28.9	18786	PASS
365	198	1	100	4.1	2646	PASS
441	198	0.01	100	15.4	9981	PASS
442	442	50	100	100.0	62043	PASS
443	442	15	24	19.5	12077	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
Data File : BG055342.D
Acq On : 28 Oct 2022 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 28 15:48:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

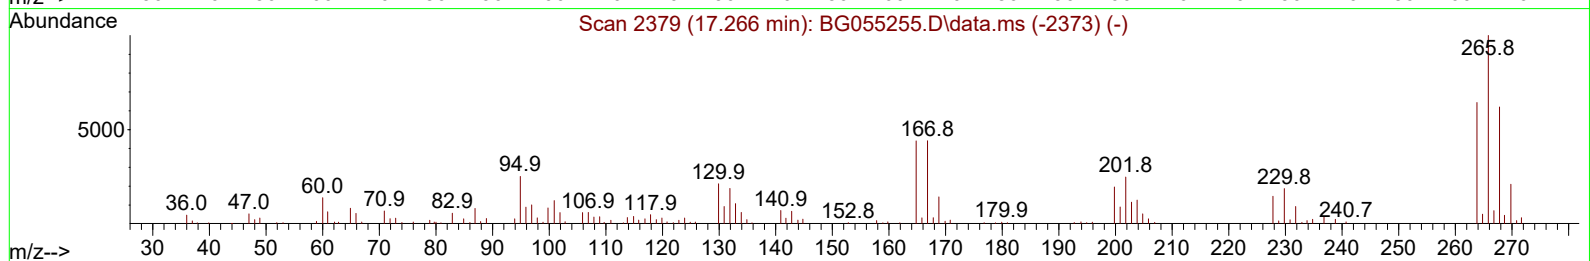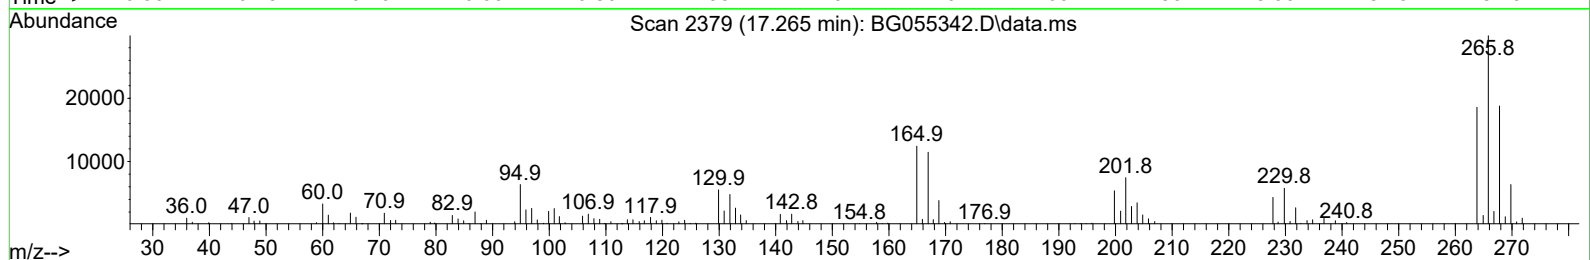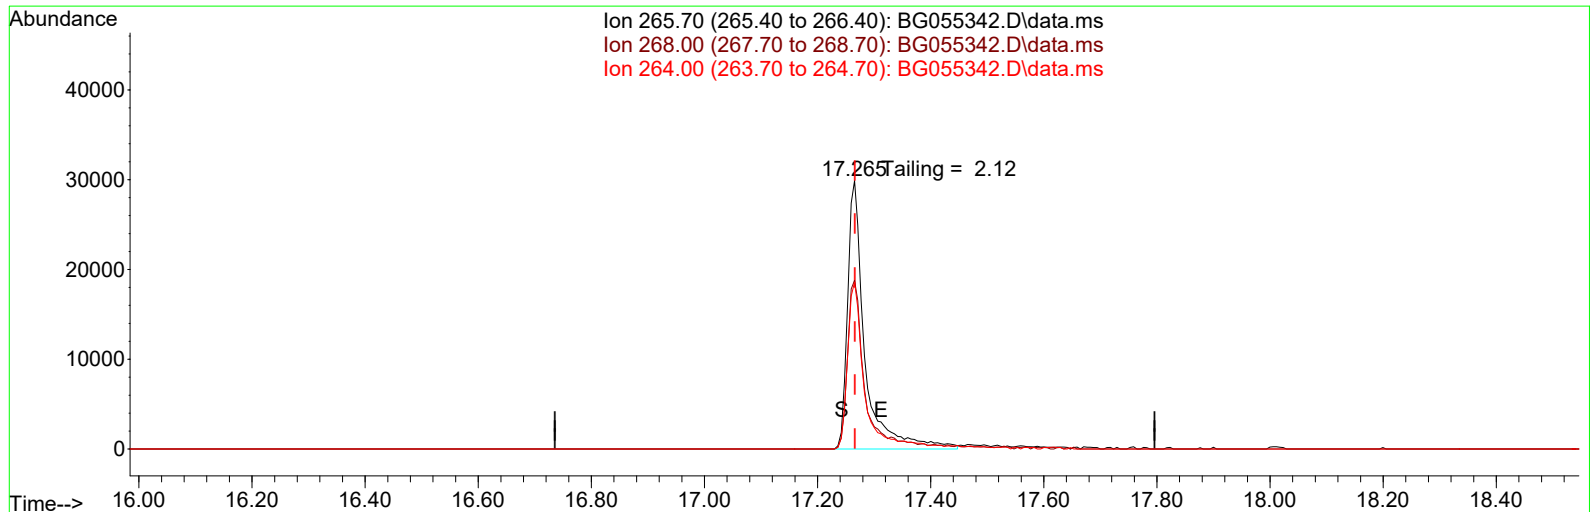

TIC: BG055342.D\data.ms

(70) Pentachlorophenol (C)

17.265min (-0.001) 27924.73 ng




response 63892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	62.83
264.00	64.40	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102822\
Data File : BG055342.D
Acq On : 28 Oct 2022 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 28 15:48:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

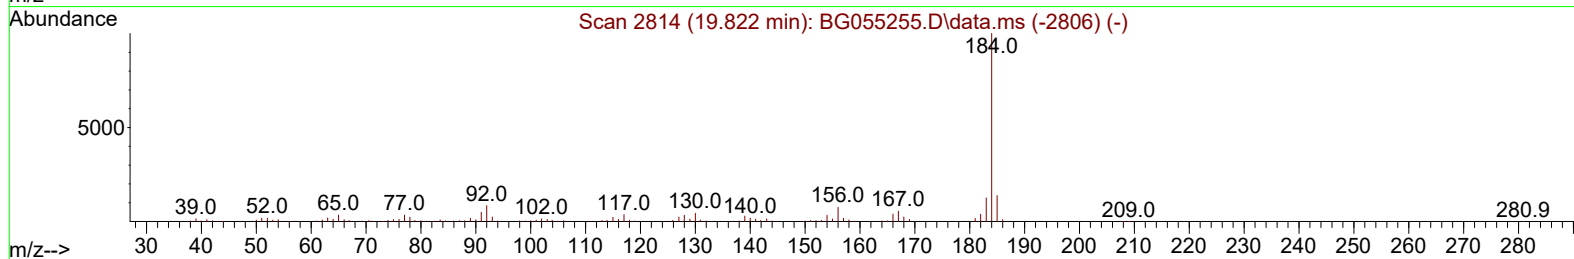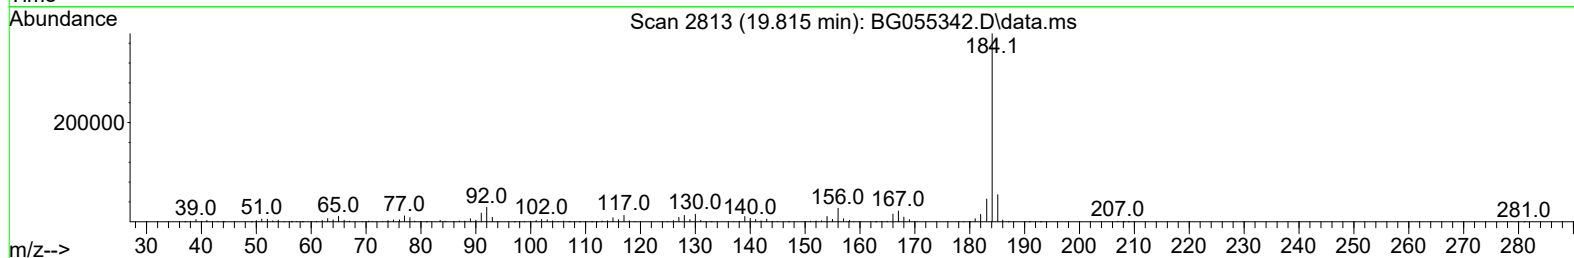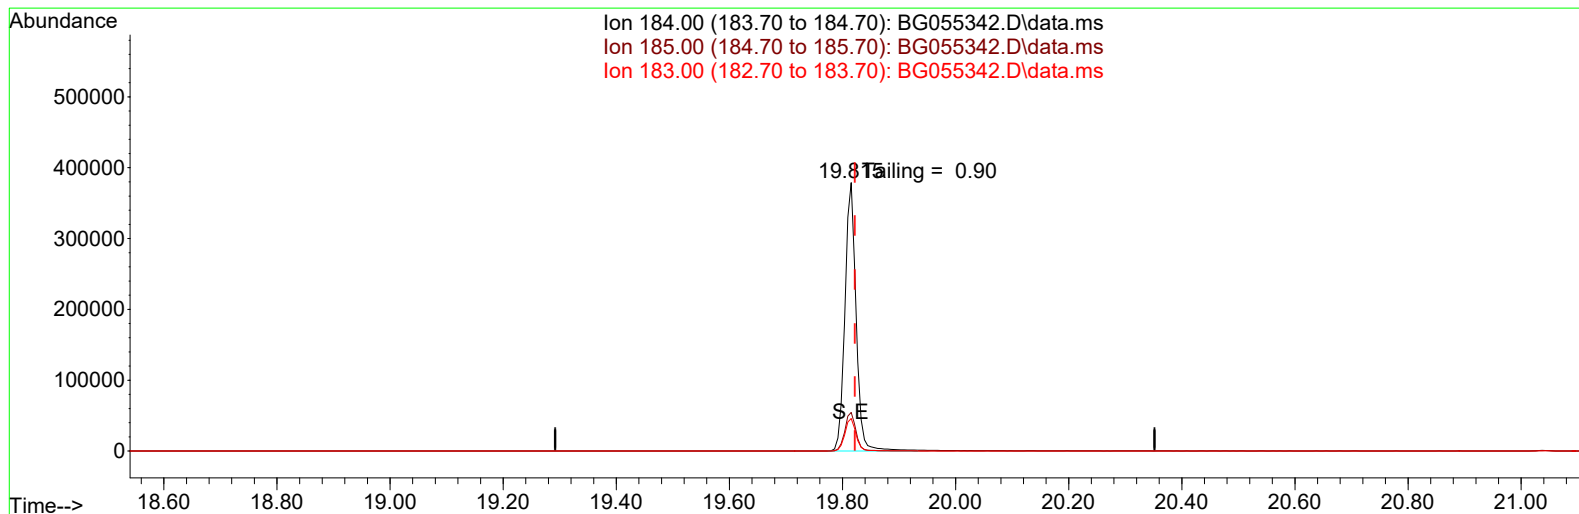

TIC: BG055342.D\data.ms

(77) Benzidine

19.815min (-0.007) 0.00 ng

response 525170

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.40
183.00	12.50	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/28/2022	BNA_G	BG055342.D
Compound Name	Response	Retention Time
DDT	251915	21.037
DDD	4915	20.591
DDE	346	20.091
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5261	257176	2.05

Instrument :
BNA_G
ClientSampleId :
DFTPP