

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059517.D
 Acq On : 28 Oct 2023 11:46
 Operator : MA/JU
 Sample : PB156455BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK455

Quant Time: Oct 30 02:12:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.366	152	72279	20.000	ng/ul	0.00
20) Naphthalene-d8	11.215	136	328300	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.993	164	183813	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.743	188	391292	20.000	ng/ul	0.00
79) Chrysene-d12	22.079	240	357310	20.000	ng/ul	# 0.00
88) Perylene-d12	25.692	264	389877	20.000	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.660	96	10213	5.287	ng/uL	0.00
4) Pyridine-d5	4.094	84	157419	29.160	ng/ul	0.00
7) Phenol-d5	7.467	99	219747	29.586	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.684	67	106545	31.231	ng/ul	0.00
11) 2-Chlorophenol-d4	7.872	132	179760	29.832	ng/ul	0.00
15) 4-Methylphenol-d8	9.041	113	169202	28.714	ng/ul	0.00
21) Nitrobenzene-d5	9.564	128	73763	31.599	ng/ul	0.00
24) 2-Nitrophenol-d4	10.281	143	76452	31.903	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.804	165	158029	29.931	ng/ul	0.00
31) 4-Chloroaniline-d4	11.350	131	268243	30.863	ng/ul	0.00
46) Dimethylphthalate-d6	14.388	166	527289	31.663	ng/ul	0.00
49) Acenaphthylene-d8	14.694	160	636537	32.571	ng/ul	0.00
54) 4-Nitrophenol-d4	15.146	143	81861	28.665	ng/ul	0.00
60) Fluorene-d10	15.980	176	443024	31.129	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.074	200	53844	29.057	ng/ul	0.00
73) Anthracene-d10	17.843	188	705297	33.271	ng/ul	0.00
81) Pyrene-d10	20.111	212	779613	31.390	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.440	264	732826	31.920	ng/ul	0.00
Target Compounds						
					Qvalue	
17) N-Nitroso-di-n-propyla...	9.041	70	4410	1.008	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059517.D
Acq On : 28 Oct 2023 11:46
Operator : MA/JU
Sample : PB156455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK455


Quant Time: Oct 30 02:12:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

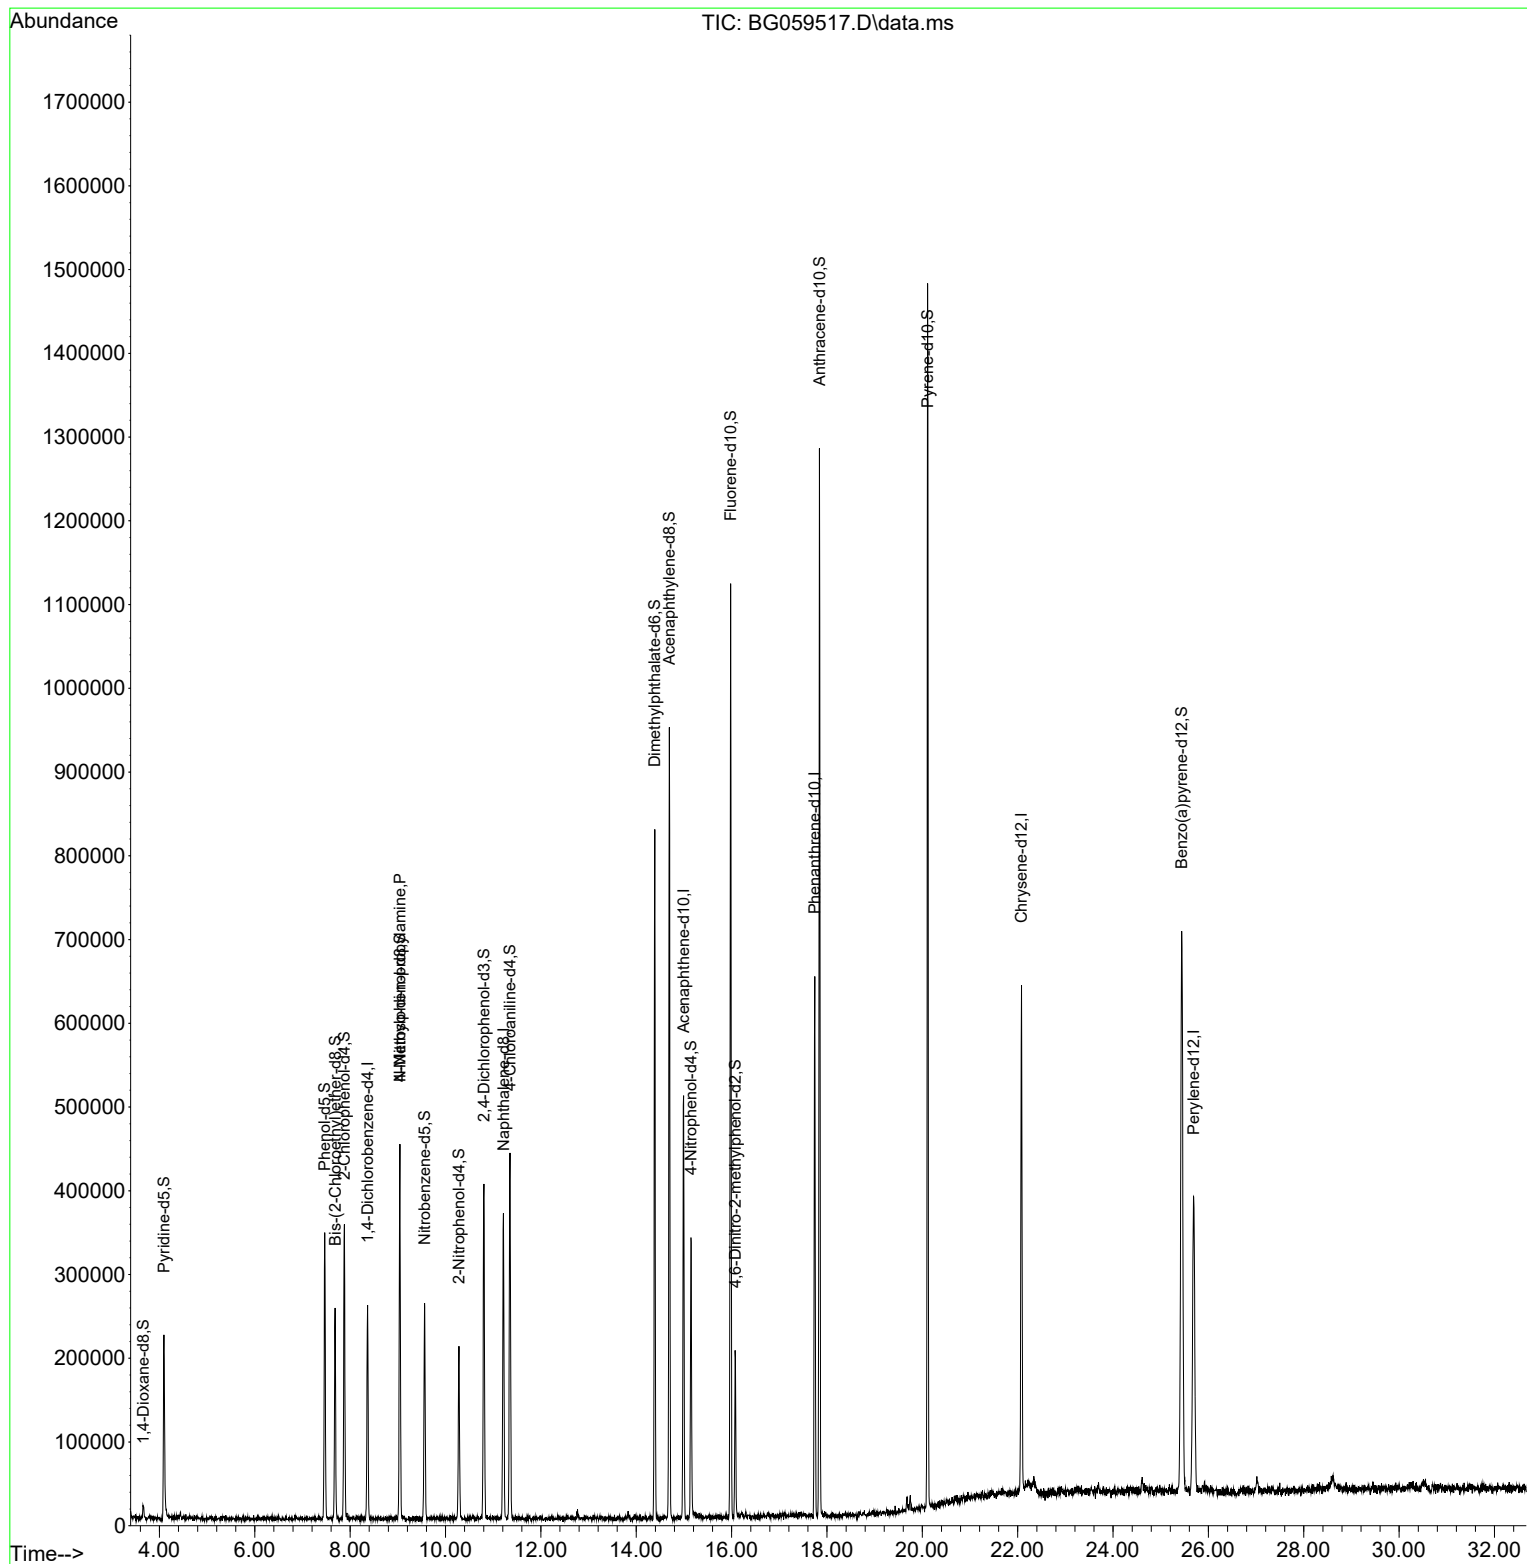

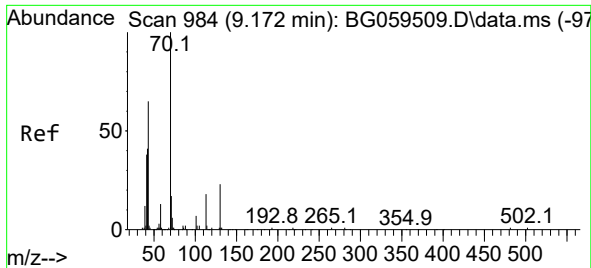

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.008 ng/ul
 RT: 9.041 min Scan# 90
 Delta R.T. -0.131 min
 Lab File: BG059517.D
 Acq: 28 Oct 2023 11:46

Instrument :
 BNA_G
 ClientSampleId :
 SBLK455

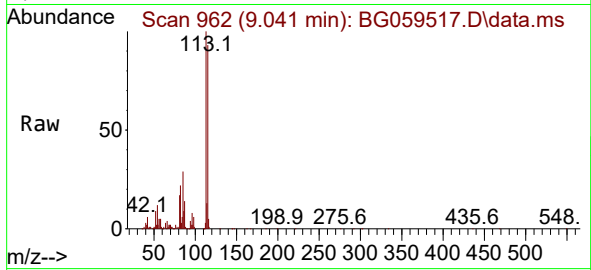

Tgt Ion:	70	Resp:	4410
Ion	Ratio	Lower	Upper
70	100		
42	239.6	33.8	50.8#
101	0.0	5.4	8.0#
130	0.0	18.2	27.4#

