

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059524.D
 Acq On : 28 Oct 2023 16:34
 Operator : MA/JU
 Sample : 04925-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCCX3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/31/2023
 Supervised By :mohammad ahmed 10/31/2023

Quant Time: Oct 30 02:44:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.362	152	64753	20.000	ng/ul	0.00
20) Naphthalene-d8	11.212	136	313845	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.990	164	187946	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.739	188	407603	20.000	ng/ul	0.00
79) Chrysene-d12	22.075	240	326984	20.000	ng/ul	0.00
88) Perylene-d12	25.689	264	367585	20.000	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.662	96	4679m	2.704	ng/uL	0.00
4) Pyridine-d5	4.091	84	9938m	2.055	ng/ul	0.00
7) Phenol-d5	7.463	99	126865	19.066	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.681	67	62753	20.532	ng/ul	0.00
11) 2-Chlorophenol-d4	7.874	132	105692	19.579	ng/ul	0.00
15) 4-Methylphenol-d8	9.038	113	81974	15.528	ng/ul	0.00
21) Nitrobenzene-d5	9.561	128	46577	20.872	ng/ul	0.00
24) 2-Nitrophenol-d4	10.277	143	50978	22.252	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.800	165	96040	19.028	ng/ul	0.00
31) 4-Chloroaniline-d4	11.347	131	80779	9.722	ng/ul	0.00
46) Dimethylphthalate-d6	14.384	166	319912	18.788	ng/ul	0.00
49) Acenaphthylene-d8	14.690	160	384216	19.227	ng/ul	0.00
54) 4-Nitrophenol-d4	15.148	143	52980	18.144	ng/ul	0.00
60) Fluorene-d10	15.977	176	284360	19.541	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.071	200	34978	18.121	ng/ul	-0.01
73) Anthracene-d10	17.839	188	434086m	19.658	ng/ul	0.00
81) Pyrene-d10	20.107	212	486248	21.394	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.430	264	438679	20.267	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	9.208	105	36855	4.429	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059524.D
Acq On : 28 Oct 2023 16:34
Operator : MA/JU
Sample : 04925-07
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
GCCX3

Quant Time: Oct 30 02:44:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/31/2023
Supervised By :mohammad ahmed 10/31/2023

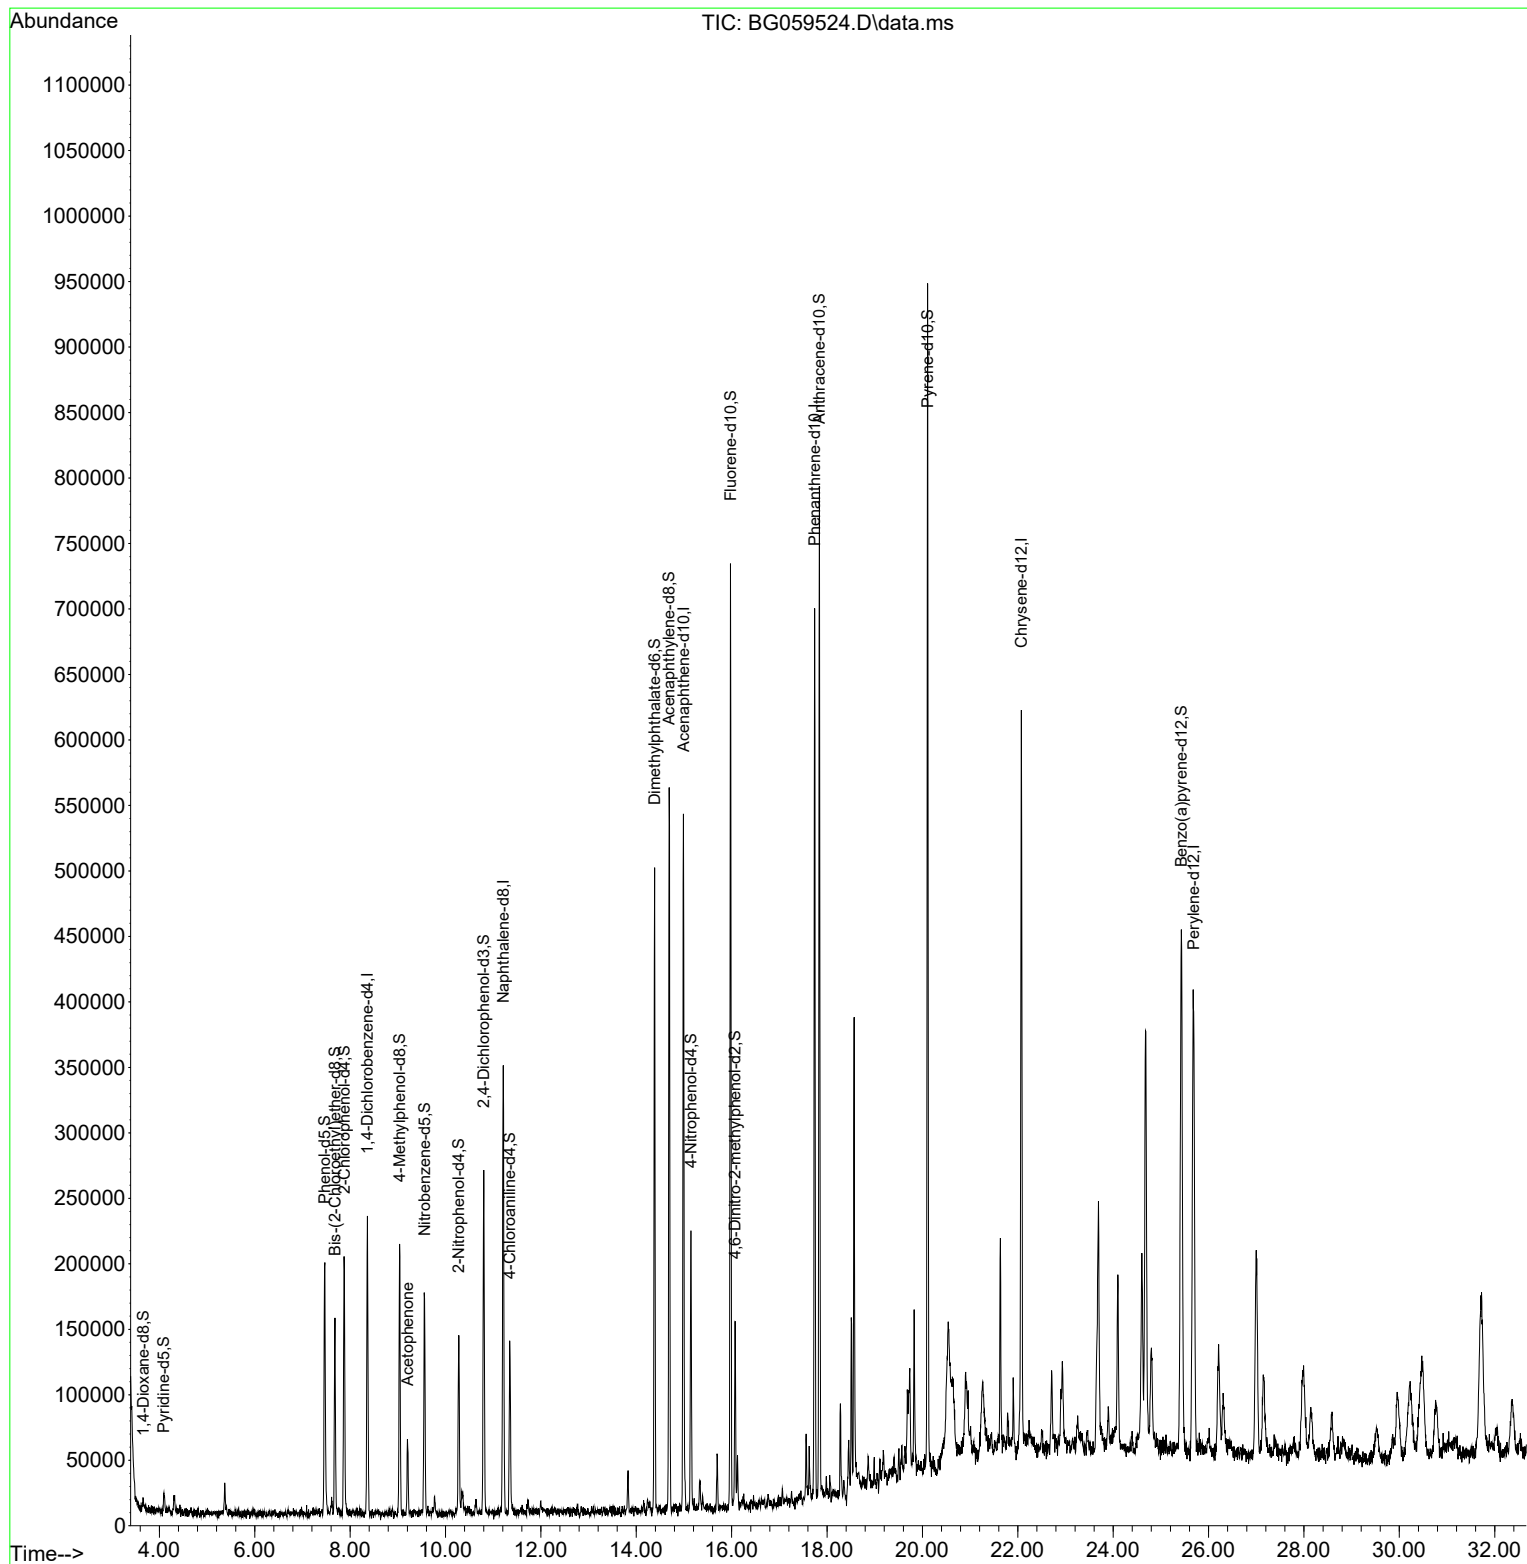

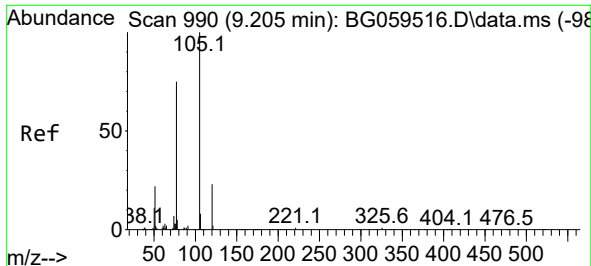

#16
 Acetophenone
 Concen: 4.429 ng/ul
 RT: 9.208 min Scan# 990
 Delta R.T. 0.001 min
 Lab File: BG059524.D
 Acq: 28 Oct 2023 16:34

Instrument :
 BNA_G
 ClientSampleId :
 GCCX3

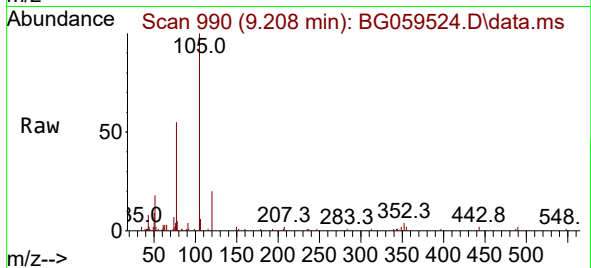

Tgt Ion:105 Resp: 3685
 Ion Ratio Lower Upper
 105 100
 77 55.5 59.6 89.4
 51 17.7 16.2 24.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/31/2023
 Supervised By :mohammad ahmed 10/31/2023

