

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059527.D
 Acq On : 28 Oct 2023 18:38
 Operator : MA/JU
 Sample : 04925-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCCX6

Quant Time: Oct 30 02:55:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.365	152	68216	20.000	ng/ul	0.00
20) Naphthalene-d8	11.209	136	313615	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.987	164	190270	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.737	188	381070	20.000	ng/ul	0.00
79) Chrysene-d12	22.073	240	325985	20.000	ng/ul	0.00
88) Perylene-d12	25.680	264	344942	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.659	96	4837	2.653	ng/uL	0.00
4) Pyridine-d5	4.100	84	11395	2.237	ng/ul	0.00
7) Phenol-d5	7.466	99	129585	18.486	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.678	67	58347	18.121	ng/ul	0.00
11) 2-Chlorophenol-d4	7.878	132	98858	17.383	ng/ul	0.00
15) 4-Methylphenol-d8	9.041	113	102531	18.436	ng/ul	0.00
21) Nitrobenzene-d5	9.558	128	43885	19.680	ng/ul	0.00
24) 2-Nitrophenol-d4	10.275	143	49469	21.610	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.804	165	92269	18.294	ng/ul	0.00
31) 4-Chloroaniline-d4	11.350	131	80100	9.647	ng/ul	0.00
46) Dimethylphthalate-d6	14.382	166	301408	17.485	ng/ul	0.00
49) Acenaphthylene-d8	14.693	160	371918	18.385	ng/ul	0.00
54) 4-Nitrophenol-d4	15.145	143	54054	18.286	ng/ul	0.00
60) Fluorene-d10	15.974	176	264550	17.958	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.074	200	36305	20.118	ng/ul	0.00
73) Anthracene-d10	17.836	188	382066	18.506	ng/ul	0.00
81) Pyrene-d10	20.110	212	428077	18.892	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.428	264	377571	18.588	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	9.205	105	41649	4.751	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059527.D
Acq On : 28 Oct 2023 18:38
Operator : MA/JU
Sample : 04925-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCCX6

Quant Time: Oct 30 02:55:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

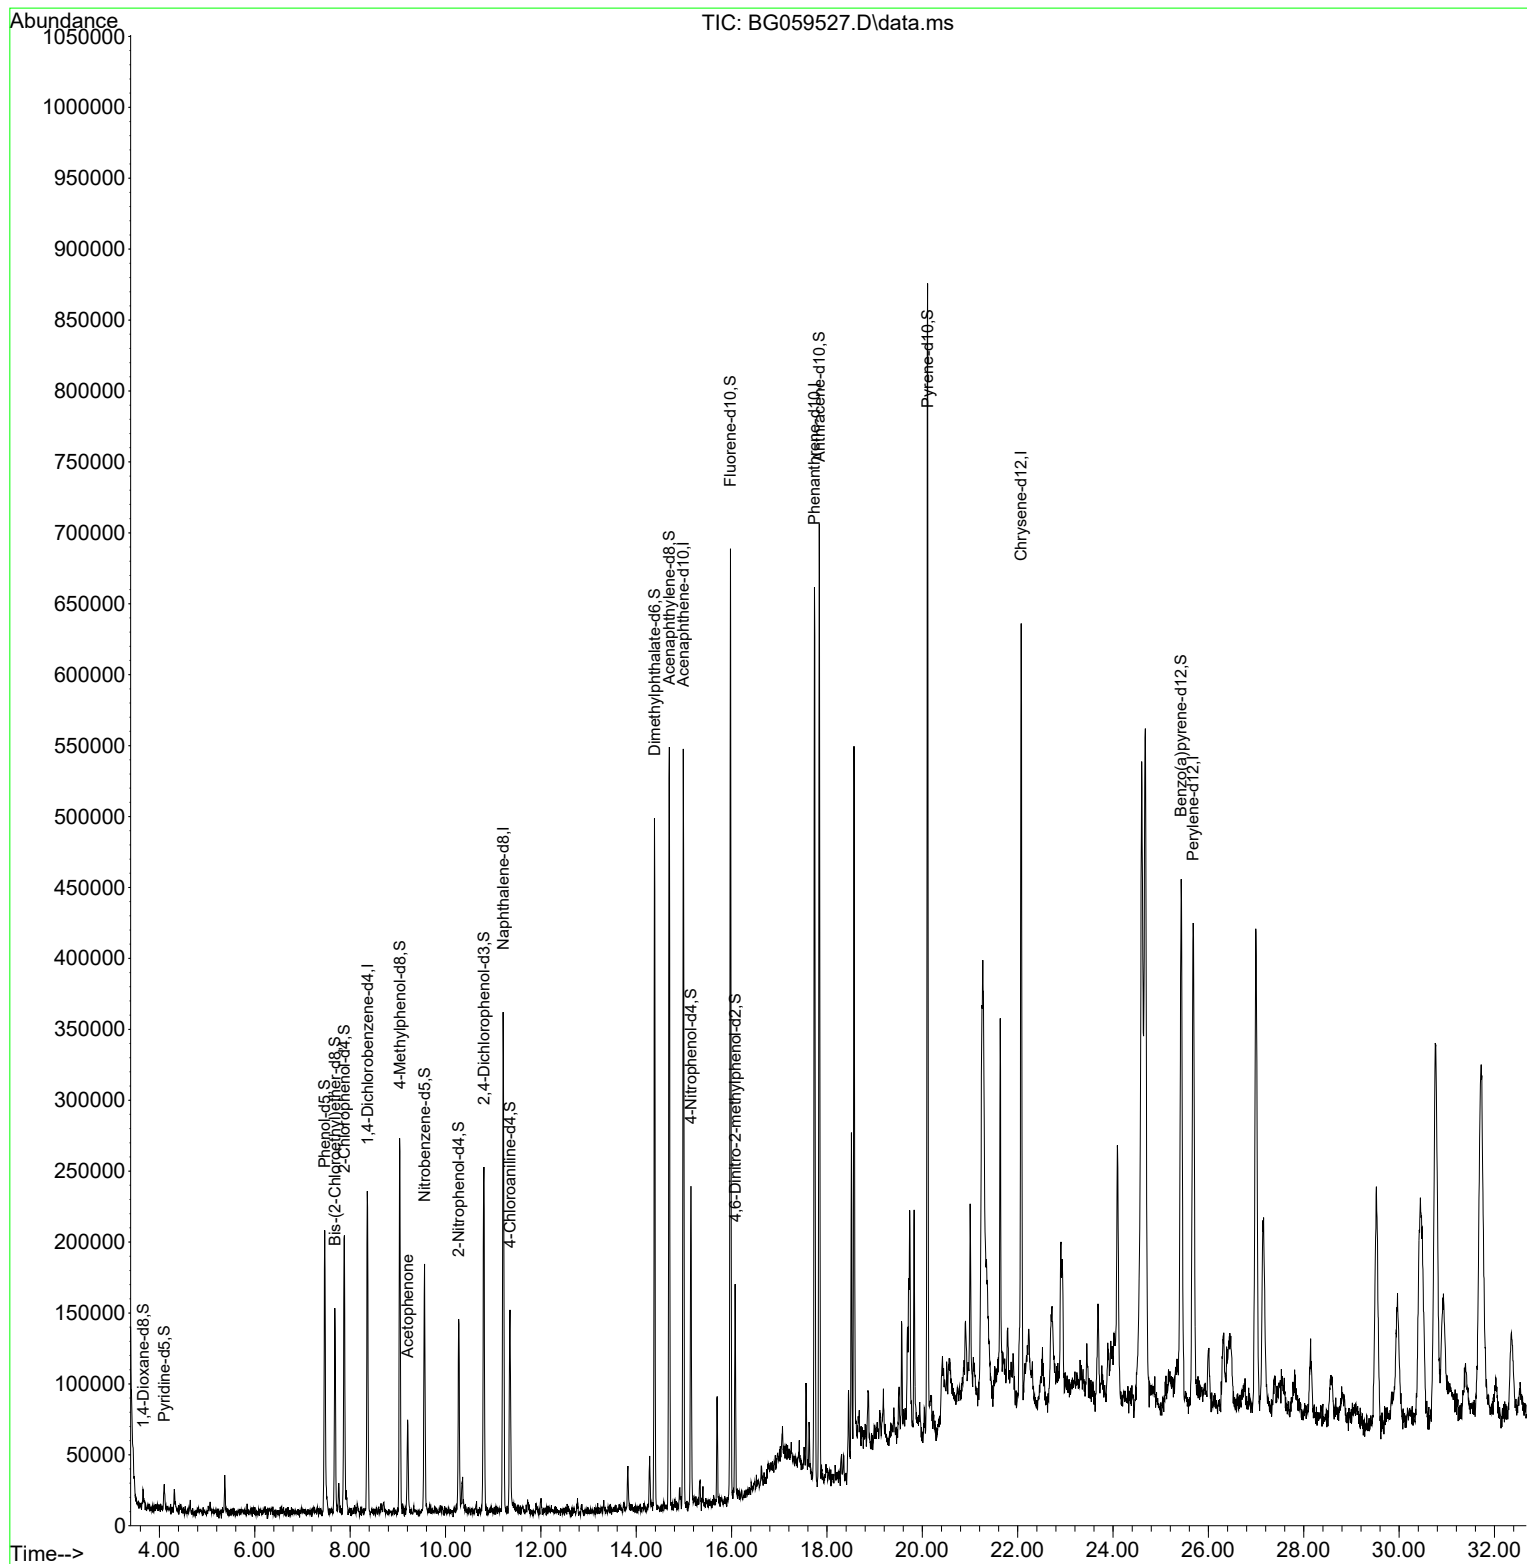

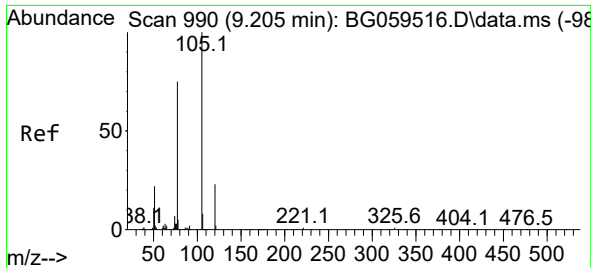

#16
 Acetophenone
 Concen: 4.751 ng/ul
 RT: 9.205 min Scan# 990
 Delta R.T. -0.002 min
 Lab File: BG059527.D
 Acq: 28 Oct 2023 18:38

Instrument :
 BNA_G
 ClientSampleId :
 GCCX6

Tgt Ion:	105	Resp:	41649
Ion Ratio	Lower	Upper	
105	100		
77	68.1	59.6	89.4
51	19.9	16.2	24.4

