

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059528.D
 Acq On : 28 Oct 2023 19:19
 Operator : MA/JU
 Sample : 04925-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCCY1

Quant Time: Oct 30 02:15:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.366	152	79620	20.000	ng/ul	0.00
20) Naphthalene-d8	11.210	136	376315	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.988	164	222922	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.737	188	441233	20.000	ng/ul	0.00
79) Chrysene-d12	22.073	240	348373	20.000	ng/ul	0.00
88) Perylene-d12	25.687	264	390162	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.654	96	3560	1.673	ng/uL	0.00
4) Pyridine-d5	4.100	84	15768	2.652	ng/ul	0.01
7) Phenol-d5	7.467	99	103380	12.635	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.678	67	45072	11.993	ng/ul	0.00
11) 2-Chlorophenol-d4	7.872	132	83598	12.594	ng/ul	0.00
15) 4-Methylphenol-d8	9.036	113	73825	11.373	ng/ul	0.00
21) Nitrobenzene-d5	9.553	128	38490	14.385	ng/ul	0.00
24) 2-Nitrophenol-d4	10.275	143	42573	15.499	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.798	165	78130	12.910	ng/ul	0.00
31) 4-Chloroaniline-d4	11.351	131	90864	9.121	ng/ul	0.00
46) Dimethylphthalate-d6	14.382	166	263556	13.050	ng/ul	0.00
49) Acenaphthylene-d8	14.694	160	313989	13.248	ng/ul	0.00
54) 4-Nitrophenol-d4	15.146	143	37676	10.878	ng/ul	0.00
60) Fluorene-d10	15.975	176	221387	12.827	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.075	200	28332	13.559	ng/ul	0.00
73) Anthracene-d10	17.837	188	331865	13.883	ng/ul	0.00
81) Pyrene-d10	20.105	212	349167	14.420	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.422	264	324155	14.109	ng/ul	-0.02
Target Compounds						
					Qvalue	
16) Acetophenone	9.206	105	21245	2.076	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059528.D
Acq On : 28 Oct 2023 19:19
Operator : MA/JU
Sample : 04925-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCCY1

Quant Time: Oct 30 02:15:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

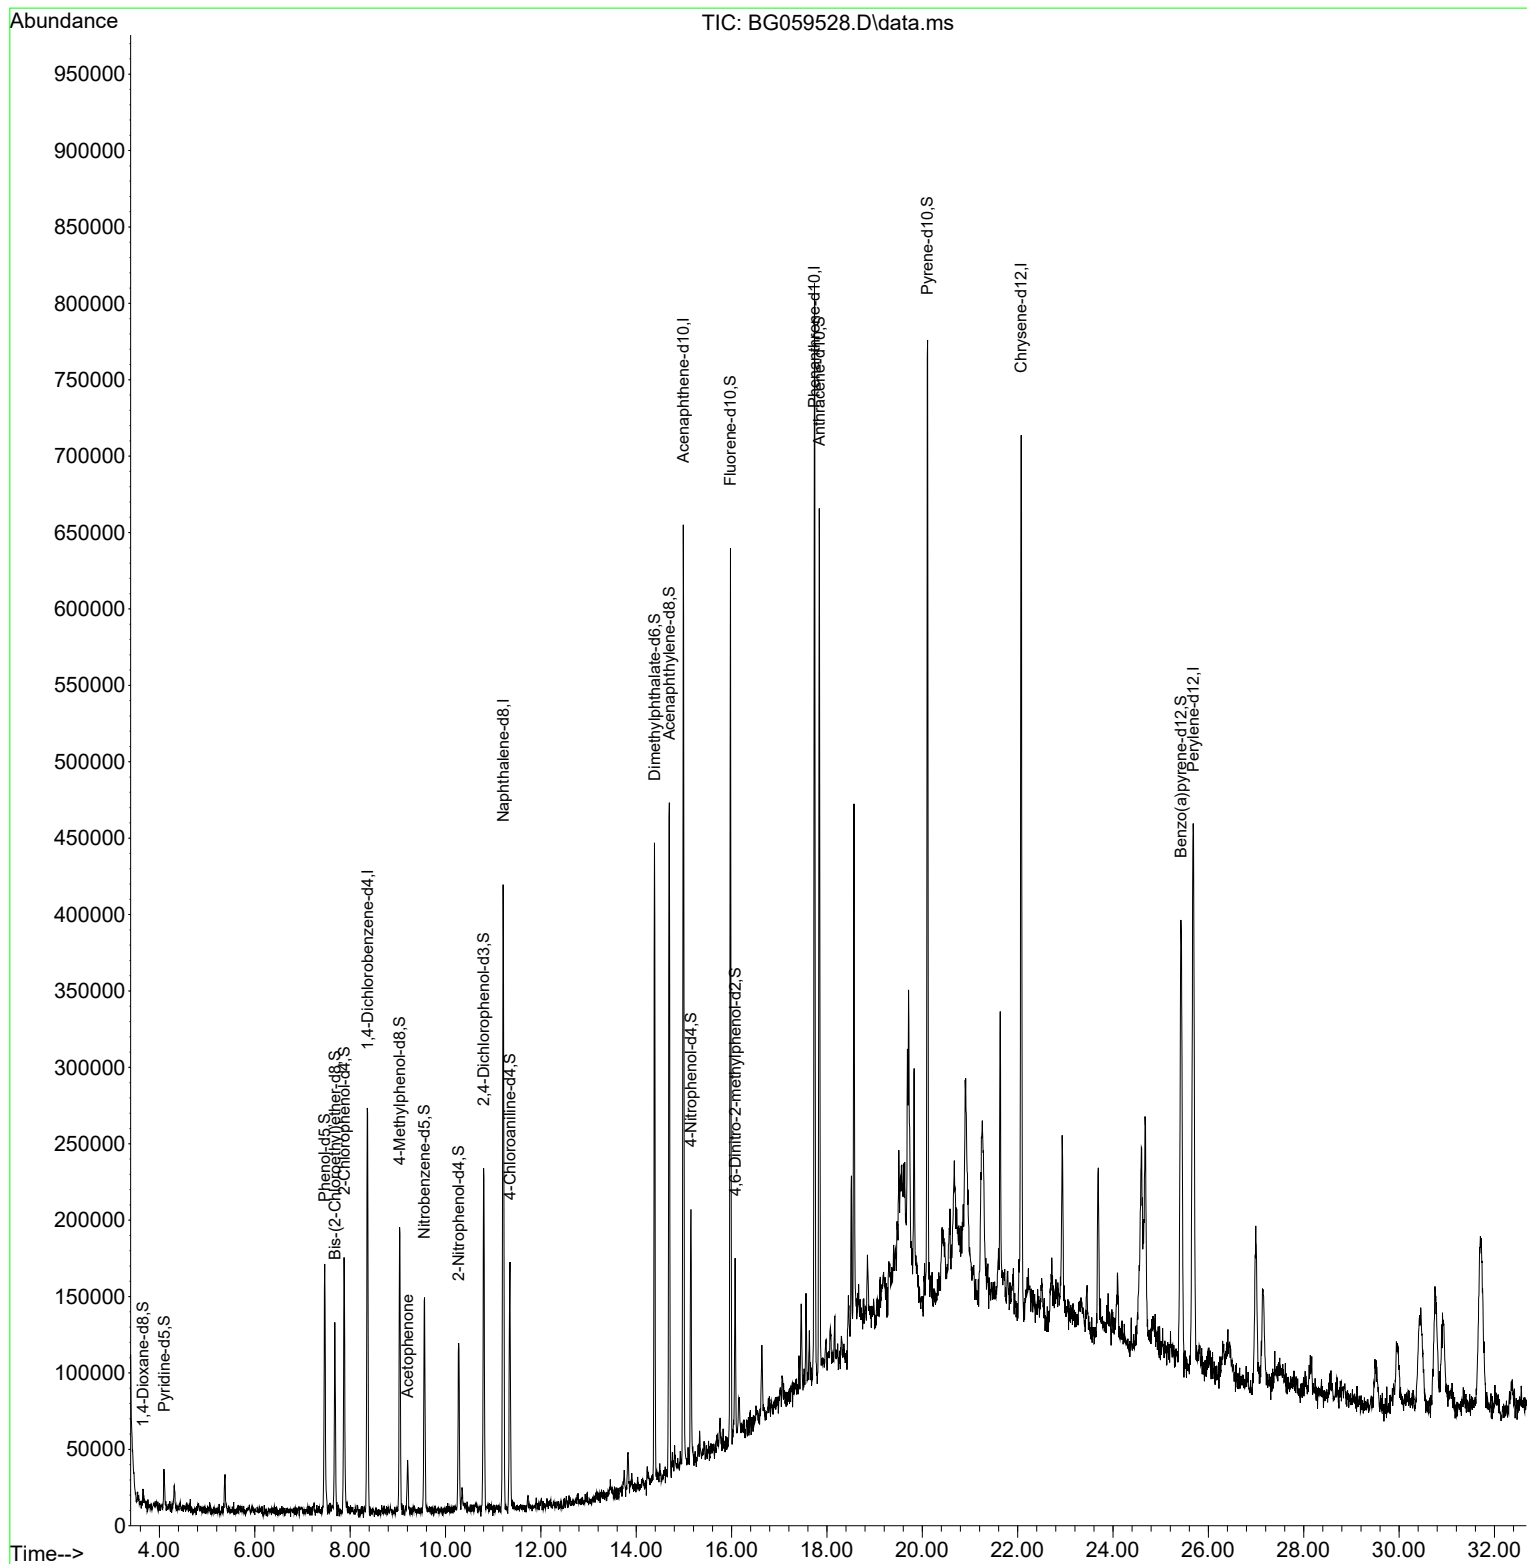

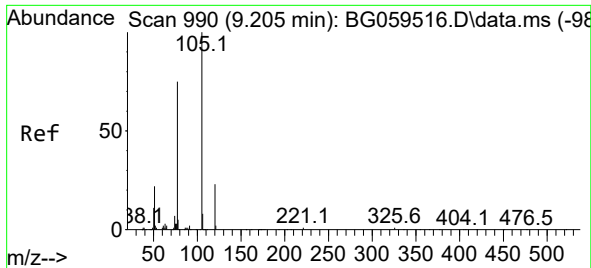

#16
 Acetophenone
 Concen: 2.076 ng/ul
 RT: 9.206 min Scan# 990
 Delta R.T. -0.001 min
 Lab File: BG059528.D
 Acq: 28 Oct 2023 19:19

Instrument :
 BNA_G
 ClientSampleId :
 GCCY1

Tgt Ion:	105	Resp:	21245
Ion Ratio	Lower	Upper	
105	100		
77	56.0	59.6	89.4#
51	20.3	16.2	24.4

