

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059538.D
 Acq On : 29 Oct 2023 2:51
 Operator : MA/JU
 Sample : 04925-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCCY4

Quant Time: Oct 30 02:17:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.361	152	57314	20.000	ng/ul	0.00
20) Naphthalene-d8	11.210	136	259094	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.988	164	166166	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.744	188	345025	20.000	ng/ul	0.00
79) Chrysene-d12	22.080	240	231394	20.000	ng/ul	0.00
88) Perylene-d12	25.693	264	274491	20.000	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.660	96	3942	2.573	ng/uL	0.00
4) Pyridine-d5	4.095	84	43996	10.278	ng/ul	0.00
7) Phenol-d5	7.468	99	123575	20.982	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.679	67	49837	18.423	ng/ul	0.00
11) 2-Chlorophenol-d4	7.879	132	98876	20.693	ng/ul	0.00
15) 4-Methylphenol-d8	9.042	113	104626	22.391	ng/ul	0.00
21) Nitrobenzene-d5	9.559	128	45985	24.961	ng/ul	0.00
24) 2-Nitrophenol-d4	10.282	143	51307	27.129	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.805	165	88398	21.215	ng/ul	0.00
31) 4-Chloroaniline-d4	11.351	131	120758	17.605	ng/ul	0.00
46) Dimethylphthalate-d6	14.383	166	312595	20.765	ng/ul	0.00
49) Acenaphthylene-d8	14.688	160	376552	21.314	ng/ul	0.00
54) 4-Nitrophenol-d4	15.153	143	56670	21.952	ng/ul	0.00
60) Fluorene-d10	15.975	176	276149	21.464	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.075	200	28453	17.414	ng/ul	0.00
73) Anthracene-d10	17.838	188	398650	21.327	ng/ul	0.00
81) Pyrene-d10	20.111	212	371107	23.073	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.441	264	348884	21.585	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	9.201	105	7832	1.063	ng/ul#	85
86) Bis(2-ethylhexyl)phtha...	21.909	149	33548	2.445	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059538.D
Acq On : 29 Oct 2023 2:51
Operator : MA/JU
Sample : 04925-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCCY4

Quant Time: Oct 30 02:17:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration




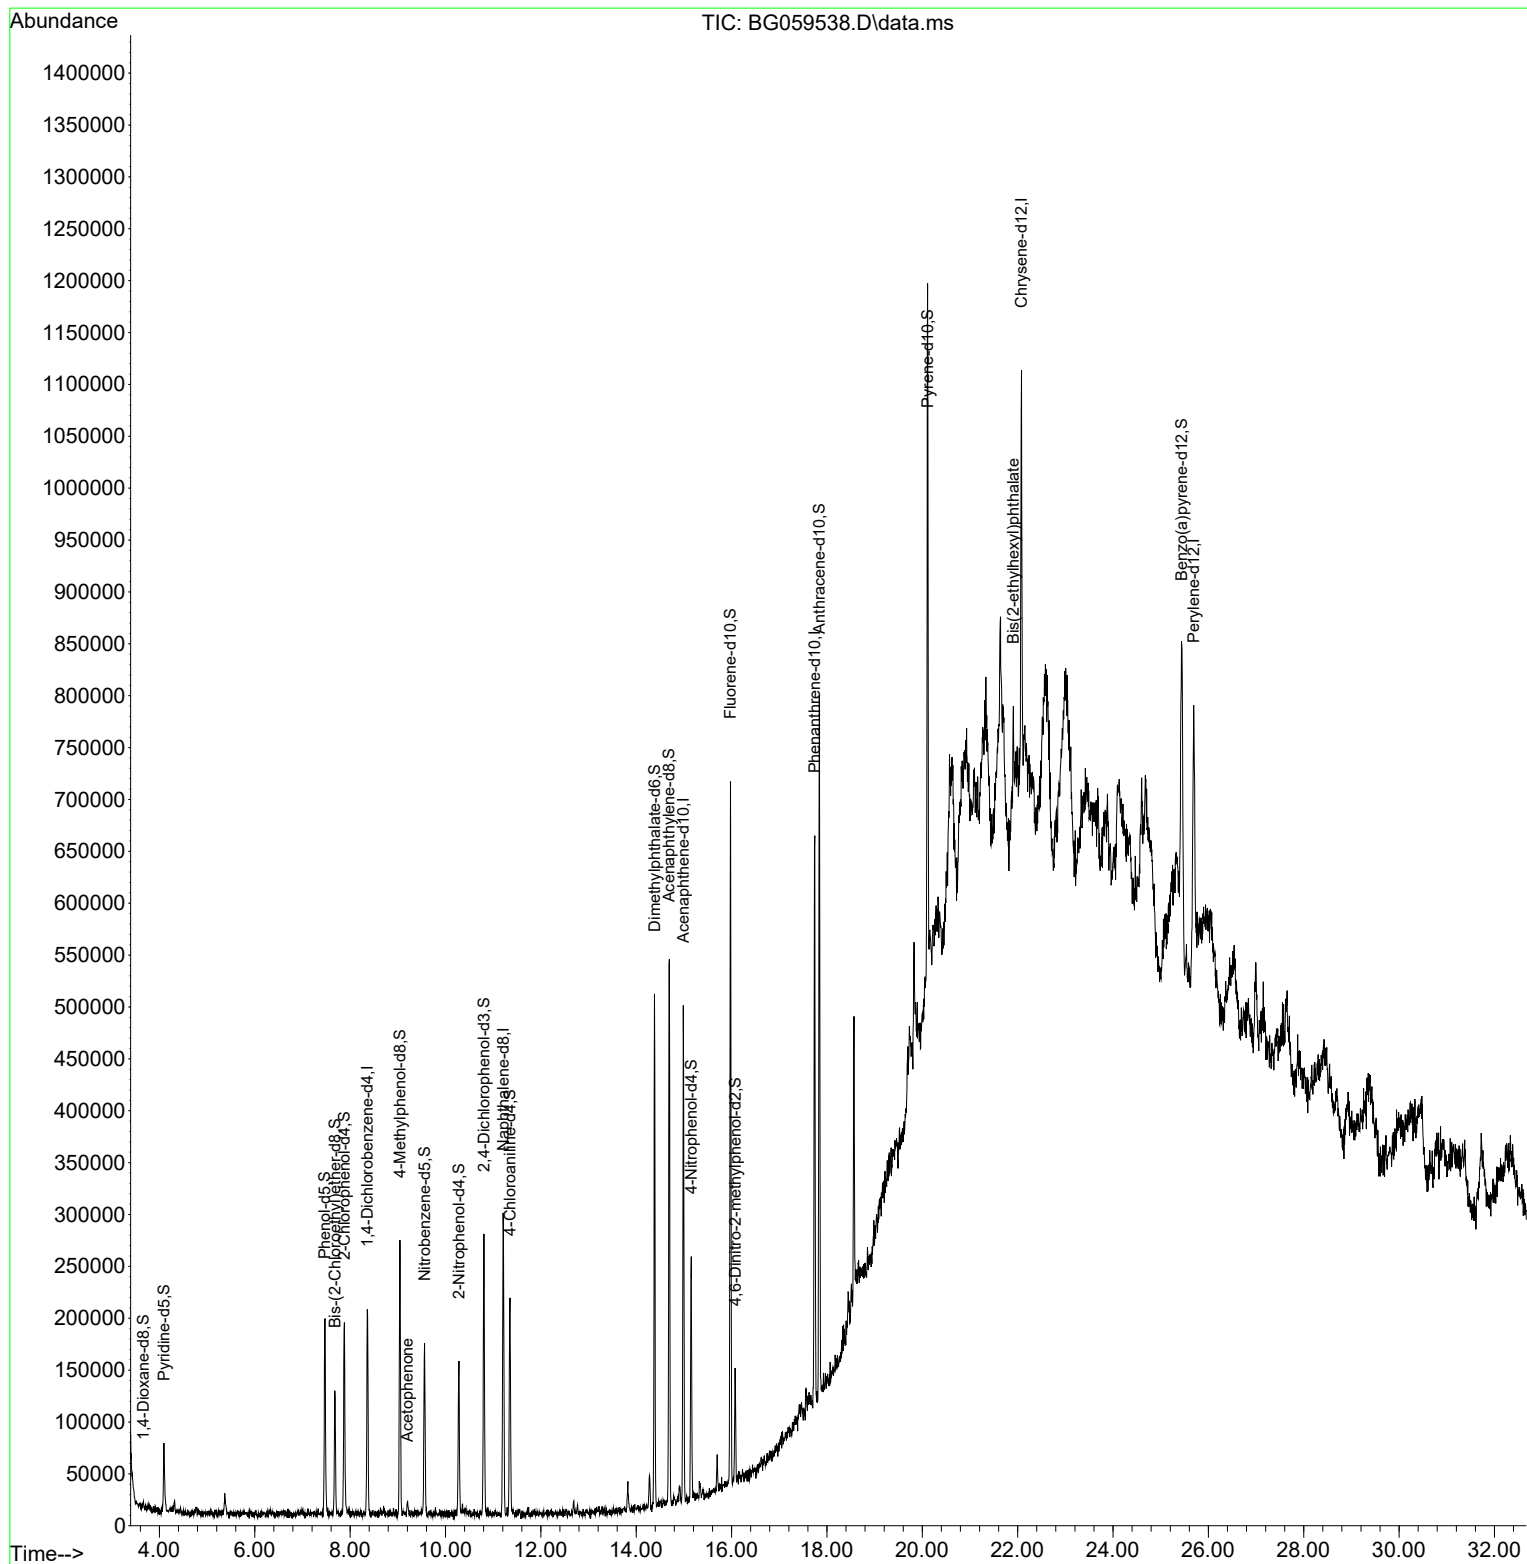


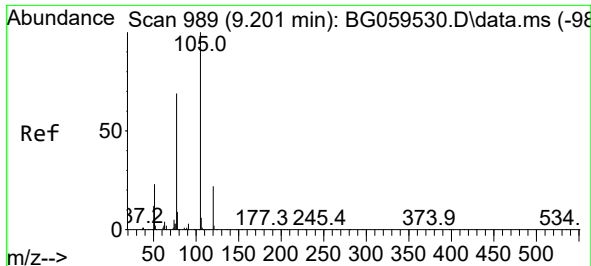

#16
Acetophenone
Concen: 1.063 ng/ul
RT: 9.201 min Scan# 91
Delta R.T. -0.007 min
Lab File: BG059538.D
Acq: 29 Oct 2023 2:51

Instrument :
BNA_G
ClientSampleId :
GCCY4

Tgt Ion:105 Resp: 7832
Ion Ratio Lower Upper
105 100
77 60.7 59.6 89.4
51 24.5 16.2 24.4#

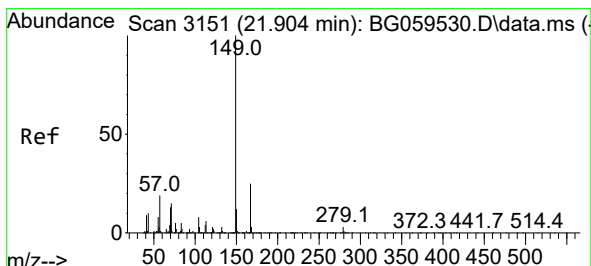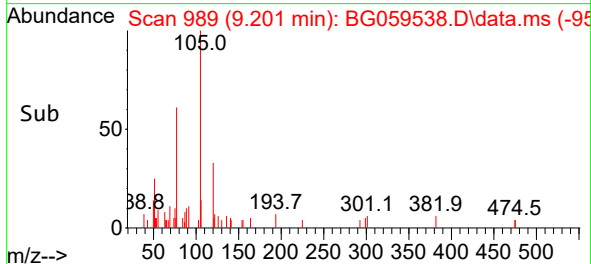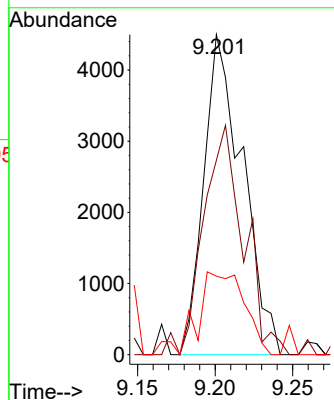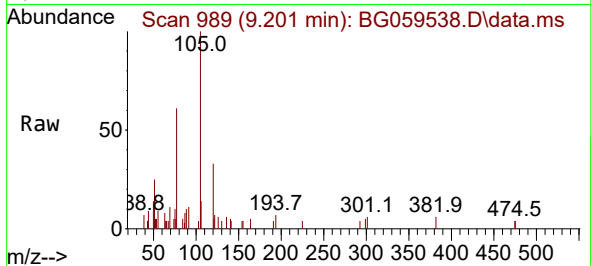

#86
Bis(2-ethylhexyl)phthalate
Concen: 2.445 ng/ul
RT: 21.909 min Scan# 3152
Delta R.T. -0.007 min
Lab File: BG059538.D
Acq: 29 Oct 2023 2:51

Tgt Ion:149 Resp: 33548
Ion Ratio Lower Upper
149 100
167 20.5 19.4 29.2
279 2.4 2.2 3.4

