

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059517.D
 Acq On : 28 Oct 2023 11:46
 Operator : MA/JU
 Sample : PB156455BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK455

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.460	9	12	17	rBV4	4360	8782	0.42%	0.040%
2	3.654	41	45	46	rBV2	15410	14751	0.70%	0.067%
3	4.094	114	120	128	rBV	221955	395951	18.92%	1.790%
4	4.441	177	179	184	rVB3	9758	12665	0.61%	0.057%
5	4.482	184	186	189	rBV	3991	4719	0.23%	0.021%
6	4.735	228	229	231	rBV2	6774	4676	0.22%	0.021%
7	4.893	251	256	257	rVB2	5125	5097	0.24%	0.023%
8	4.958	265	267	271	rBV2	3551	5691	0.27%	0.026%
9	5.181	303	305	309	rVV3	5653	7549	0.36%	0.034%
10	5.281	320	322	324	rBV2	5027	5065	0.24%	0.023%
11	5.346	330	333	338	rVB3	3712	6971	0.33%	0.032%
12	5.751	398	402	404	rBV	5814	7501	0.36%	0.034%
13	5.810	410	412	416	rBV3	5315	7027	0.34%	0.032%
14	5.939	430	434	438	rBV	3056	4922	0.24%	0.022%
15	6.063	454	455	457	rBV	5390	4631	0.22%	0.021%
16	6.174	471	474	477	rVB3	3930	5125	0.24%	0.023%
17	6.204	477	479	483	rBV	5098	7193	0.34%	0.033%
18	6.321	496	499	501	rBV2	3986	4948	0.24%	0.022%
19	6.374	507	508	513	rBV	5753	6558	0.31%	0.030%
20	6.838	584	587	590	rBV2	6408	5843	0.28%	0.026%
21	7.338	669	672	673	rVB	5358	4603	0.22%	0.021%
22	7.467	685	694	706	rBV	342827	590573	28.22%	2.671%
23	7.684	724	731	738	rVB	252341	419191	20.03%	1.896%
24	7.878	756	764	771	rVV	353294	616191	29.44%	2.786%
25	7.931	771	773	777	rVB	8117	6217	0.30%	0.028%
26	8.066	795	796	801	rVB	4390	4702	0.22%	0.021%
27	8.184	814	816	820	rVB	6654	7259	0.35%	0.033%
28	8.213	820	821	823	rBV	5727	4974	0.24%	0.022%
29	8.366	838	847	855	rBV	257021	445348	21.28%	2.014%
30	8.442	859	860	863	rBV	4548	4649	0.22%	0.021%
31	9.041	954	962	970	rVV	448157	745904	35.64%	3.373%
32	9.412	1024	1025	1030	rVB	6510	7659	0.37%	0.035%
33	9.453	1030	1032	1034	rBV	6726	6317	0.30%	0.029%
34	9.558	1041	1050	1059	rBV	260258	479724	22.92%	2.169%
35	9.817	1091	1094	1099	rVV2	5149	8712	0.42%	0.039%
36	10.187	1154	1157	1159	rVV2	5061	4540	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059517.D
 Acq On : 28 Oct 2023 11:46
 Operator : MA/JU
 Sample : PB156455BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK455

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	10.281	1166	1173	1179	rBV2	203786	349848	16.72%	1.582%
38	10.804	1255	1262	1269	rBV	398614	732629	35.01%	3.313%
39	11.215	1324	1332	1339	rBV	364436	643920	30.77%	2.912%
40	11.350	1347	1355	1363	rBV	437410	826574	39.49%	3.738%

41	11.721	1416	1418	1421	rBV	4994	4813	0.23%	0.022%
42	12.220	1499	1503	1505	rBV	5758	7702	0.37%	0.035%
43	12.261	1509	1510	1514	rBV	4193	4672	0.22%	0.021%
44	12.473	1544	1546	1548	rBV	5202	4526	0.22%	0.020%
45	12.766	1593	1596	1600	rBV4	11756	16783	0.80%	0.076%

46	13.190	1666	1668	1671	rVB	5003	4658	0.22%	0.021%
47	13.348	1692	1695	1696	rVB	5674	5720	0.27%	0.026%
48	13.383	1699	1701	1706	rVV	3500	5474	0.26%	0.025%
49	13.648	1741	1746	1747	rBV	4714	5196	0.25%	0.023%
50	13.771	1765	1767	1770	rBV	5557	5344	0.26%	0.024%

51	13.830	1773	1777	1779	rVV3	10743	13483	0.64%	0.061%
52	13.848	1779	1780	1784	rVV3	6420	5653	0.27%	0.026%
53	13.900	1786	1789	1791	rBV	4362	6389	0.31%	0.029%
54	14.388	1865	1872	1878	rBV	824386	1180097	56.39%	5.336%
55	14.694	1914	1924	1932	rBV	945480	1467587	70.12%	6.636%

56	14.993	1967	1975	1982	rVB	505683	824716	39.41%	3.729%
57	15.146	1994	2001	2009	rBV	335362	546647	26.12%	2.472%
58	15.534	2063	2067	2068	rVB	6522	7261	0.35%	0.033%
59	15.598	2072	2078	2079	rBV	4290	7460	0.36%	0.034%
60	15.692	2092	2094	2097	rBV3	4896	5454	0.26%	0.025%

61	15.792	2109	2111	2114	rVB2	5175	4718	0.23%	0.021%
62	15.892	2125	2128	2129	rBV	5878	4897	0.23%	0.022%
63	15.980	2135	2143	2150	rBV	1117238	1692342	80.86%	7.653%
64	16.074	2154	2159	2167	rVV2	198933	308837	14.76%	1.397%
65	16.192	2177	2179	2181	rBV2	3927	4720	0.23%	0.021%

66	16.298	2190	2197	2200	rBV4	8308	12683	0.61%	0.057%
67	16.339	2203	2204	2206	rBV	4882	4841	0.23%	0.022%
68	16.439	2218	2221	2224	rBV	4368	6818	0.33%	0.031%
69	16.509	2232	2233	2238	rVB	4992	7431	0.36%	0.034%
70	16.550	2238	2240	2241	rBV2	5952	4563	0.22%	0.021%

71	16.750	2271	2274	2276	rBV2	7406	9951	0.48%	0.045%
72	16.826	2286	2287	2290	rBV2	5126	6471	0.31%	0.029%
73	17.009	2316	2318	2319	rBV	6818	4797	0.23%	0.022%
74	17.103	2332	2334	2336	rBV	7846	9303	0.44%	0.042%
75	17.408	2383	2386	2387	rBV3	7879	9031	0.43%	0.041%

76	17.743	2437	2443	2451	rBV	647686	1013431	48.42%	4.583%
----	--------	------	------	------	-----	--------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059517.D
 Acq On : 28 Oct 2023 11:46
 Operator : MA/JU
 Sample : PB156455BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK455

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

77	17.843	2453	2460	2467	rBV	1275988	1911948	91.35%	8.646%
78	18.254	2526	2530	2533	rBV4	5187	6878	0.33%	0.031%
79	18.284	2533	2535	2538	rBV2	3670	4759	0.23%	0.022%
80	18.336	2542	2544	2546	rBV	4848	5056	0.24%	0.023%
81	18.389	2551	2553	2557	rVB2	6536	6933	0.33%	0.031%
82	18.671	2598	2601	2602	rBV2	6295	6579	0.31%	0.030%
83	19.030	2659	2662	2663	rBV	4251	5227	0.25%	0.024%
84	19.277	2703	2704	2707	rBV3	7415	6014	0.29%	0.027%
85	19.335	2712	2714	2719	rBV4	4601	7105	0.34%	0.032%
86	19.429	2728	2730	2733	rVB3	10713	8181	0.39%	0.037%
87	19.682	2768	2773	2775	rBV4	17807	24992	1.19%	0.113%
88	19.747	2780	2784	2787	rVB4	18047	25080	1.20%	0.113%
89	20.052	2835	2836	2839	rBV2	7285	8625	0.41%	0.039%
90	20.111	2840	2846	2852	rVV2	1461525	2092920	100.00%	9.464%
91	20.316	2877	2881	2882	rBV3	6285	8035	0.38%	0.036%
92	20.669	2939	2941	2942	rBV2	10543	5697	0.27%	0.026%
93	20.687	2942	2944	2946	rVV3	7897	5727	0.27%	0.026%
94	20.787	2959	2961	2963	rBV3	7307	6387	0.31%	0.029%
95	20.957	2988	2990	2992	rBV	10969	8550	0.41%	0.039%
96	22.079	3174	3181	3189	rBV	603275	1076797	51.45%	4.869%
97	23.642	3445	3447	3448	rBV2	11754	11077	0.53%	0.050%
98	25.440	3742	3753	3765	rVB4	665854	2057930	98.33%	9.306%
99	25.687	3785	3795	3808	rVB2	352641	1133432	54.16%	5.125%
100	27.949	4178	4180	4182	rBV3	11274	10986	0.52%	0.050%




Sum of corrected areas: 22114583

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059517.D
Acq On : 28 Oct 2023 11:46
Operator : MA/JU
Sample : PB156455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK455

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

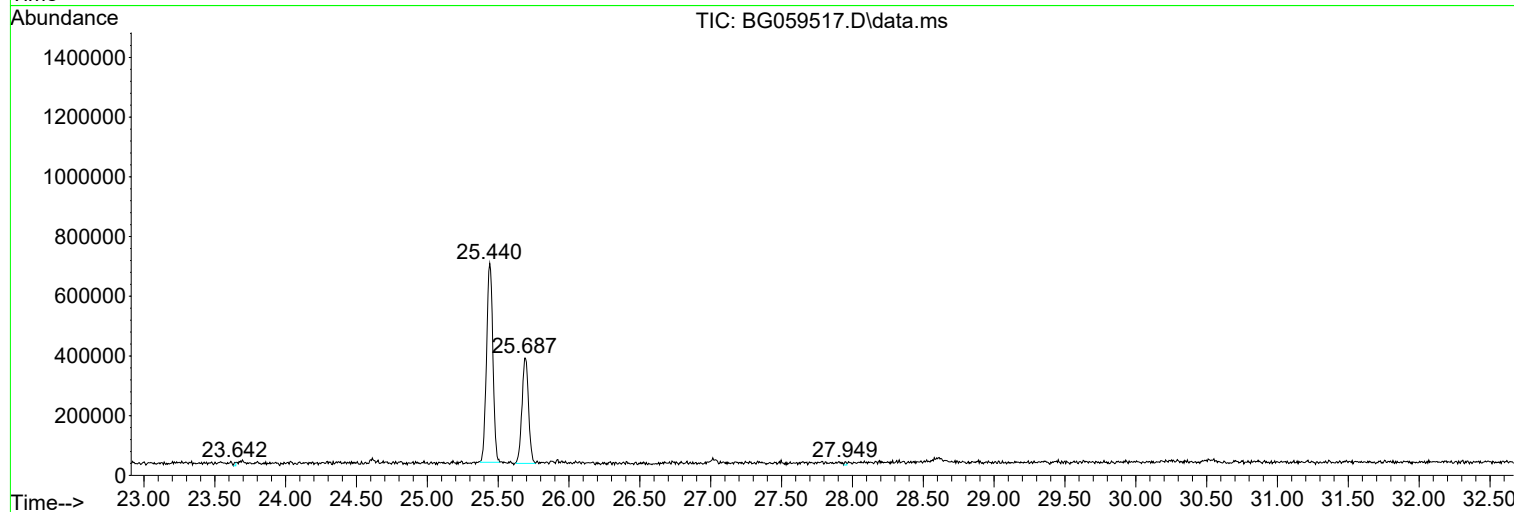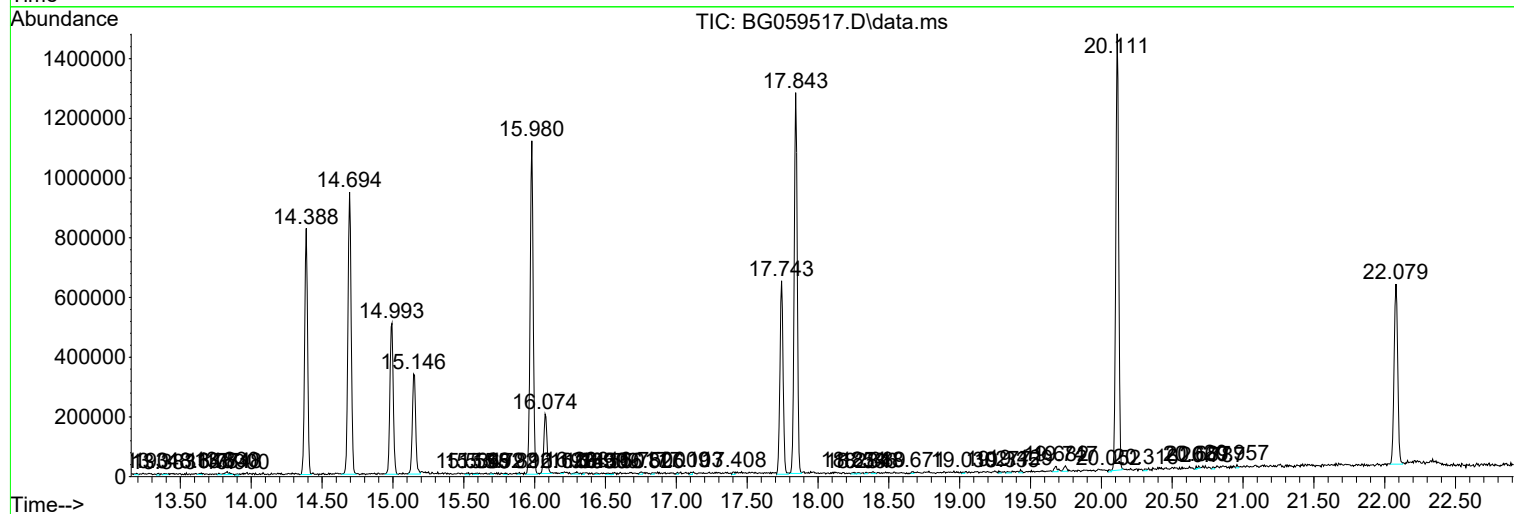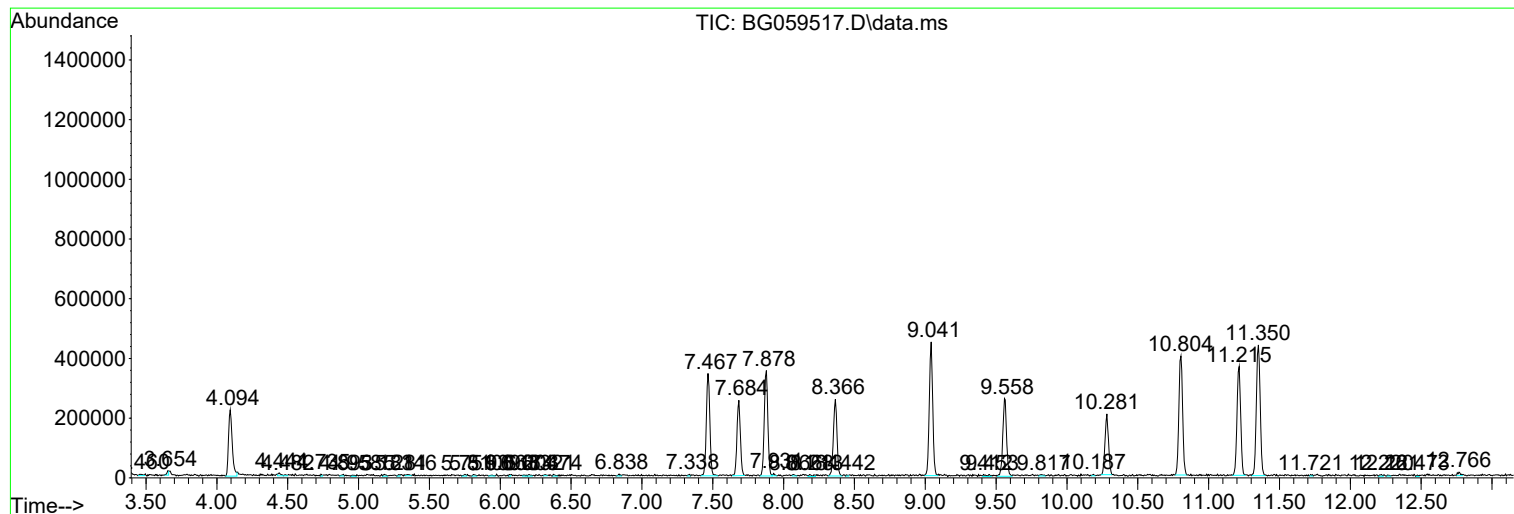

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059517.D
Acq On : 28 Oct 2023 11:46
Operator : MA/JU
Sample : PB156455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK455

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059517.D
Acq On : 28 Oct 2023 11:46
Operator : MA/JU
Sample : PB156455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK455

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc