

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059531.D
 Acq On : 28 Oct 2023 22:04
 Operator : MA/JU
 Sample : PB156455BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK455

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.954	94	96	100	rBV3	6831	7974	0.37%	0.035%
2	4.095	114	120	130	rBV	211985	374490	17.49%	1.643%
3	4.430	174	177	180	rBV4	10450	11170	0.52%	0.049%
4	4.964	266	268	271	rBV2	5400	6327	0.30%	0.028%
5	6.134	463	467	470	rBV2	4376	7249	0.34%	0.032%
6	6.709	562	565	568	rBV2	4567	7405	0.35%	0.032%
7	6.827	583	585	588	rVB	6781	5992	0.28%	0.026%
8	7.021	616	618	623	rBV	3947	7106	0.33%	0.031%
9	7.467	686	694	704	rBV	344087	619469	28.93%	2.717%
10	7.597	715	716	721	rVB	4556	5991	0.28%	0.026%
11	7.679	723	730	738	rVV	242261	410962	19.19%	1.803%
12	7.873	755	763	772	rBV	354255	615998	28.77%	2.702%
13	8.360	840	846	854	rVB2	235470	421397	19.68%	1.849%
14	9.036	955	961	969	rBV	441903	785780	36.69%	3.447%
15	9.483	1036	1037	1041	rVB2	5393	5854	0.27%	0.026%
16	9.559	1041	1050	1057	rBV3	296720	586717	27.40%	2.574%
17	9.929	1110	1113	1115	rBV2	7624	8143	0.38%	0.036%
18	10.000	1123	1125	1127	rBV	5578	5994	0.28%	0.026%
19	10.276	1165	1172	1179	rBV	252197	463198	21.63%	2.032%
20	10.799	1255	1261	1270	rVB	429611	786651	36.74%	3.451%
21	11.210	1321	1331	1339	rBV	338749	637094	29.75%	2.795%
22	11.345	1347	1354	1362	rVB	429547	786375	36.72%	3.450%
23	11.797	1430	1431	1434	rBV	5659	6600	0.31%	0.029%
24	11.985	1460	1463	1466	rBV2	4664	5932	0.28%	0.026%
25	12.126	1485	1487	1491	rBV	4733	6345	0.30%	0.028%
26	12.555	1558	1560	1562	rVB	8367	6174	0.29%	0.027%
27	12.579	1562	1564	1567	rBV	5856	6144	0.29%	0.027%
28	12.649	1572	1576	1577	rBV	5919	6317	0.29%	0.028%
29	12.973	1629	1631	1634	rVB2	7782	8099	0.38%	0.036%
30	13.296	1683	1686	1687	rBV2	6451	6302	0.29%	0.028%
31	13.825	1773	1776	1781	rVB2	14279	20132	0.94%	0.088%
32	14.383	1865	1871	1880	rVB	875727	1229638	57.42%	5.394%
33	14.688	1916	1923	1930	rBV2	947856	1486992	69.44%	6.523%
34	14.988	1967	1974	1980	rVB2	545420	845376	39.48%	3.708%
35	15.064	1985	1987	1991	rBV	5996	7932	0.37%	0.035%
36	15.146	1994	2001	2009	rBV	446533	705734	32.96%	3.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
 Data File : BG059531.D
 Acq On : 28 Oct 2023 22:04
 Operator : MA/JU
 Sample : PB156455BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK455

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	15.293	2023	2026	2027	rBV	6445	6458	0.30%	0.028%
38	15.893	2126	2128	2130	rBV	6479	6150	0.29%	0.027%
39	15.975	2135	2142	2150	rBV	1189965	1786081	83.41%	7.835%
40	16.075	2153	2159	2165	rVB	285628	437436	20.43%	1.919%
41	16.727	2267	2270	2273	rBV2	6089	8990	0.42%	0.039%
42	17.009	2317	2318	2323	rBV4	7567	11314	0.53%	0.050%
43	17.738	2435	2442	2448	rVB	719348	1086697	50.75%	4.767%
44	17.837	2452	2459	2465	rBV2	1341049	2013294	94.02%	8.832%
45	18.061	2495	2497	2500	rBV4	7063	5771	0.27%	0.025%
46	18.313	2539	2540	2543	rBV2	6754	7153	0.33%	0.031%
47	18.719	2606	2609	2611	rBV3	7869	8444	0.39%	0.037%
48	19.577	2753	2755	2757	rBV2	9439	7625	0.36%	0.033%
49	19.665	2766	2770	2776	rBV5	22058	39895	1.86%	0.175%
50	20.105	2840	2845	2853	rVB	1482933	2141399	100.00%	9.394%
51	22.074	3174	3180	3186	rVB	596144	1065996	49.78%	4.676%
52	25.429	3742	3751	3762	rVB2	706717	2112898	98.67%	9.269%
53	25.681	3786	3794	3808	rVB3	375505	1135199	53.01%	4.980%




Sum of corrected areas: 22795853

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059531.D
Acq On : 28 Oct 2023 22:04
Operator : MA/JU
Sample : PB156455BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK455

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

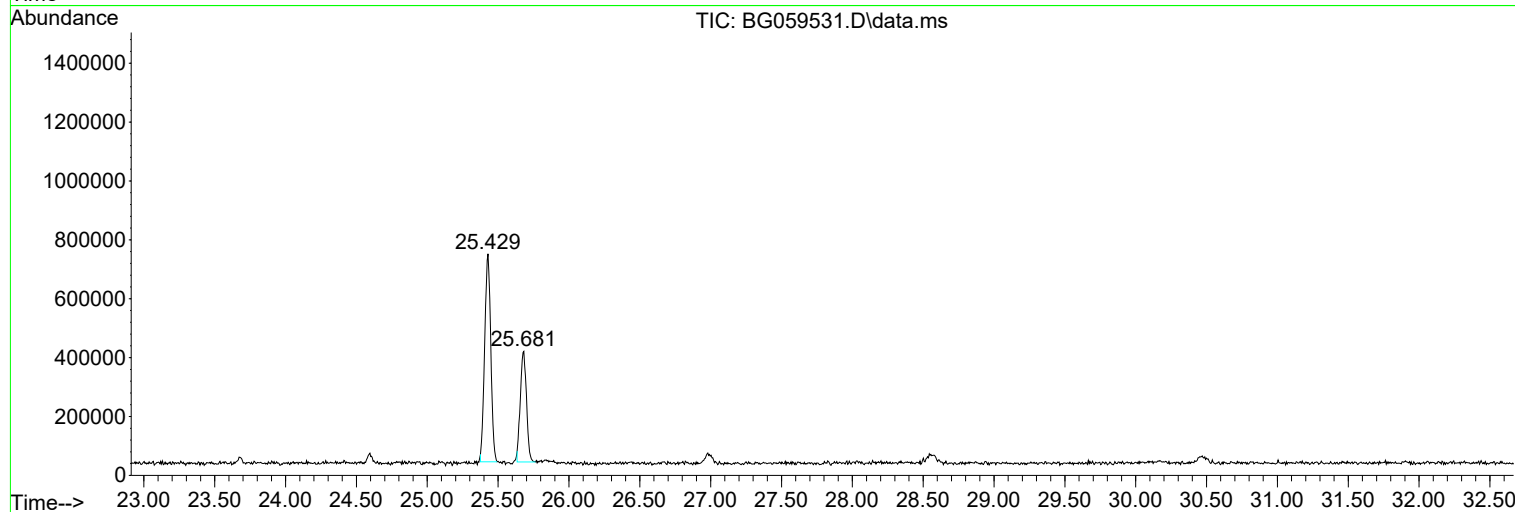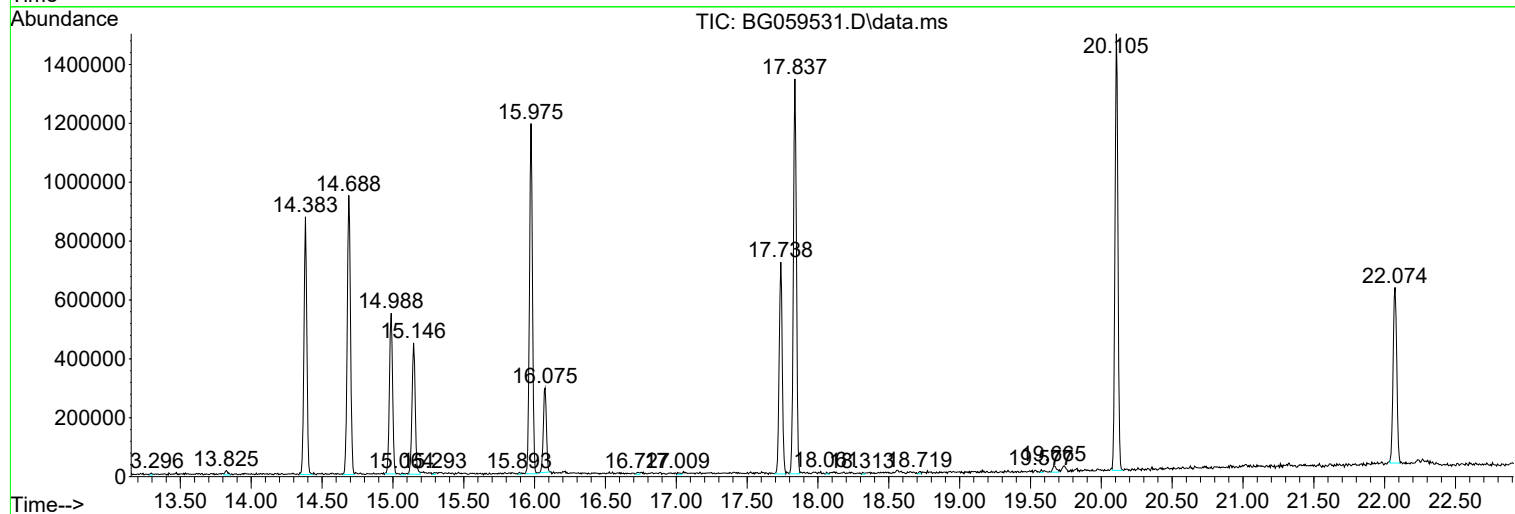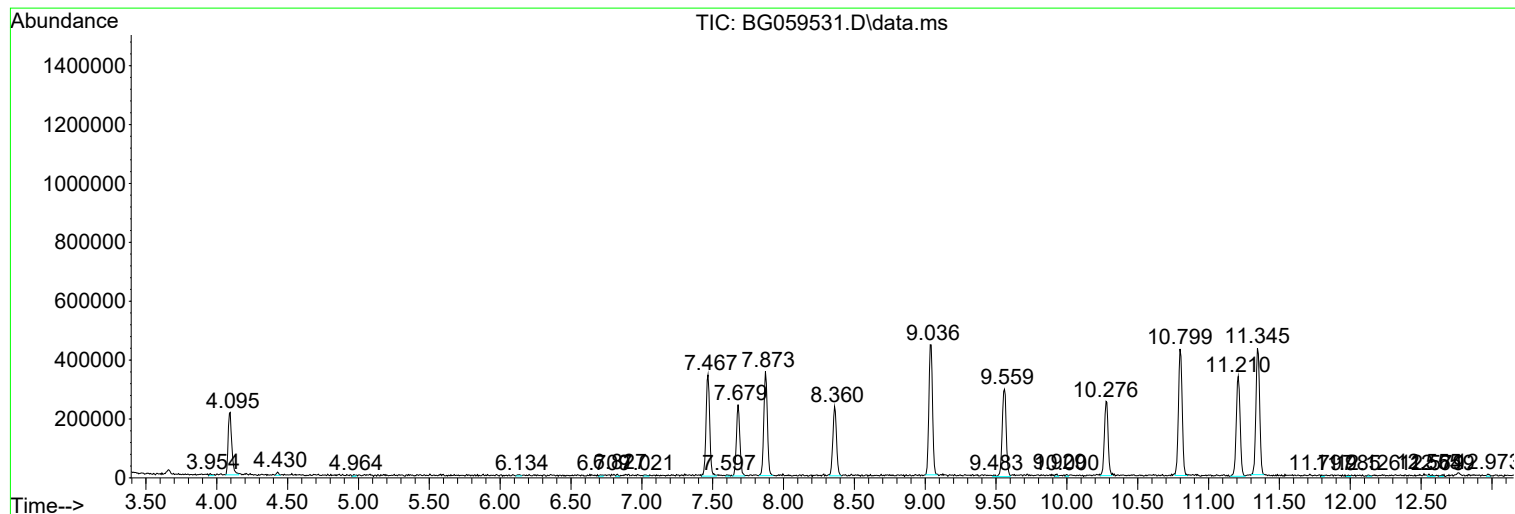

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059531.D
Acq On : 28 Oct 2023 22:04
Operator : MA/JU
Sample : PB156455BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK455

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102823\
Data File : BG059531.D
Acq On : 28 Oct 2023 22:04
Operator : MA/JU
Sample : PB156455BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK455

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------